

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN013125\  
 Data File : VN085612.D  
 Acq On : 31 Jan 2025 19:17  
 Operator : JC\MD  
 Sample : PB166357ZHE#17  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 25 Sample Multiplier: 1


Instrument :  
 MSVOA\_N  
 ClientSampleId :


Quant Time: Jan 31 22:34:20 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011425W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Jan 15 02:16:08 2025  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response            | Conc   | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|--------|--------|----------|
| -----                         |                |      |                     |        |        |          |
| Internal Standards            |                |      |                     |        |        |          |
| 1) Pentafluorobenzene         | 8.224          | 168  | 161151              | 50.000 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.100          | 114  | 329996              | 50.000 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.865         | 117  | 302646              | 50.000 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.788         | 152  | 103424              | 50.000 | ug/l   | 0.00     |
|                               |                |      |                     |        |        |          |
| System Monitoring Compounds   |                |      |                     |        |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.577          | 65   | 152506              | 58.627 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 117.260% |        |        |          |
| 35) Dibromofluoromethane      | 8.165          | 113  | 114752              | 50.124 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 100.240% |        |        |          |
| 50) Toluene-d8                | 10.565         | 98   | 423069              | 52.012 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 104.020% |        |        |          |
| 62) 4-Bromofluorobenzene      | 12.847         | 95   | 118167              | 42.469 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 77 - 121 |      | Recovery = 84.940%  |        |        |          |
|                               |                |      |                     |        |        |          |
| Target Compounds              |                |      |                     |        | Qvalue |          |
| 11) Tert butyl alcohol        | 5.518          | 59   | 177                 | 0.594  | ug/l # | 71       |
| 16) Acetone                   | 4.430          | 43   | 40716               | 48.442 | ug/l   | 96       |
| 18) Methyl Acetate            | 5.030          | 43   | 3419                | 1.338  | ug/l # | 65       |
| 20) Methylene Chloride        | 5.277          | 84   | 3367                | 1.618  | ug/l # | 82       |
| 25) 2-Butanone                | 7.506          | 43   | 4840                | 3.913  | ug/l   | 99       |
| 29) Tetrahydrofuran           | 7.841          | 42   | 223                 | 0.284  | ug/l # | 34       |
| 30) Chloroform                | 7.971          | 83   | 1425                | 0.363  | ug/l   | 91       |
| 31) Cyclohexane               | 8.224          | 56   | 4585                | 1.389  | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 8.218          | 75   | 14595               | 4.542  | ug/l # | 51       |
| 37) Ethyl Acetate             | 7.571          | 43   | 3754                | 1.158  | ug/l # | 81       |
| 38) Carbon Tetrachloride      | 8.224          | 117  | 18389               | 4.999  | ug/l # | 18       |
| 43) Isopropyl Acetate         | 8.688          | 43   | 261757              | 50.370 | ug/l # | 77       |
| 45) 1,2-Dichloropropane       | 9.735          | 63   | 2036                | 0.826  | ug/l # | 43       |
| 48) Methyl methacrylate       | 9.741          | 41   | 149748              | 64.033 | ug/l # | 46       |
| 49) 1,4-Dioxane               | 9.741          | 88   | 120                 | 3.047  | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.447         | 43   | 12250               | 4.062  | ug/l # | 75       |
| 53) t-1,3-Dichloropropene     | 10.729         | 75   | 947                 | 0.276  | ug/l   | 96       |
| 54) cis-1,3-Dichloropropene   | 10.359         | 75   | 45731               | 12.497 | ug/l # | 74       |
| 56) Ethyl methacrylate        | 10.988         | 69   | 2323                | 2.530  | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 11.206         | 76   | 7253                | 1.884  | ug/l # | 43       |
| 59) 2-Hexanone                | 11.200         | 43   | 89929               | 42.383 | ug/l # | 58       |
| 71) Bromoform                 | 12.841         | 173  | 799                 | 0.459  | ug/l # | 1        |
| 74) N-amyl acetate            | 12.482         | 43   | 2238                | 0.713  | ug/l # | 42       |
| 76) 1,2,3-Trichloropropane    | 12.847         | 75   | 67514               | 32.117 | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.847         | 75   | 67514               | 86.895 | ug/l # | 3        |
| -----                         |                |      |                     |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 31 22:34:20 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011425W.M  
Quant Title : SW846 8260  
QLast Update : Wed Jan 15 02:16:08 2025  
Response via : Initial Calibration




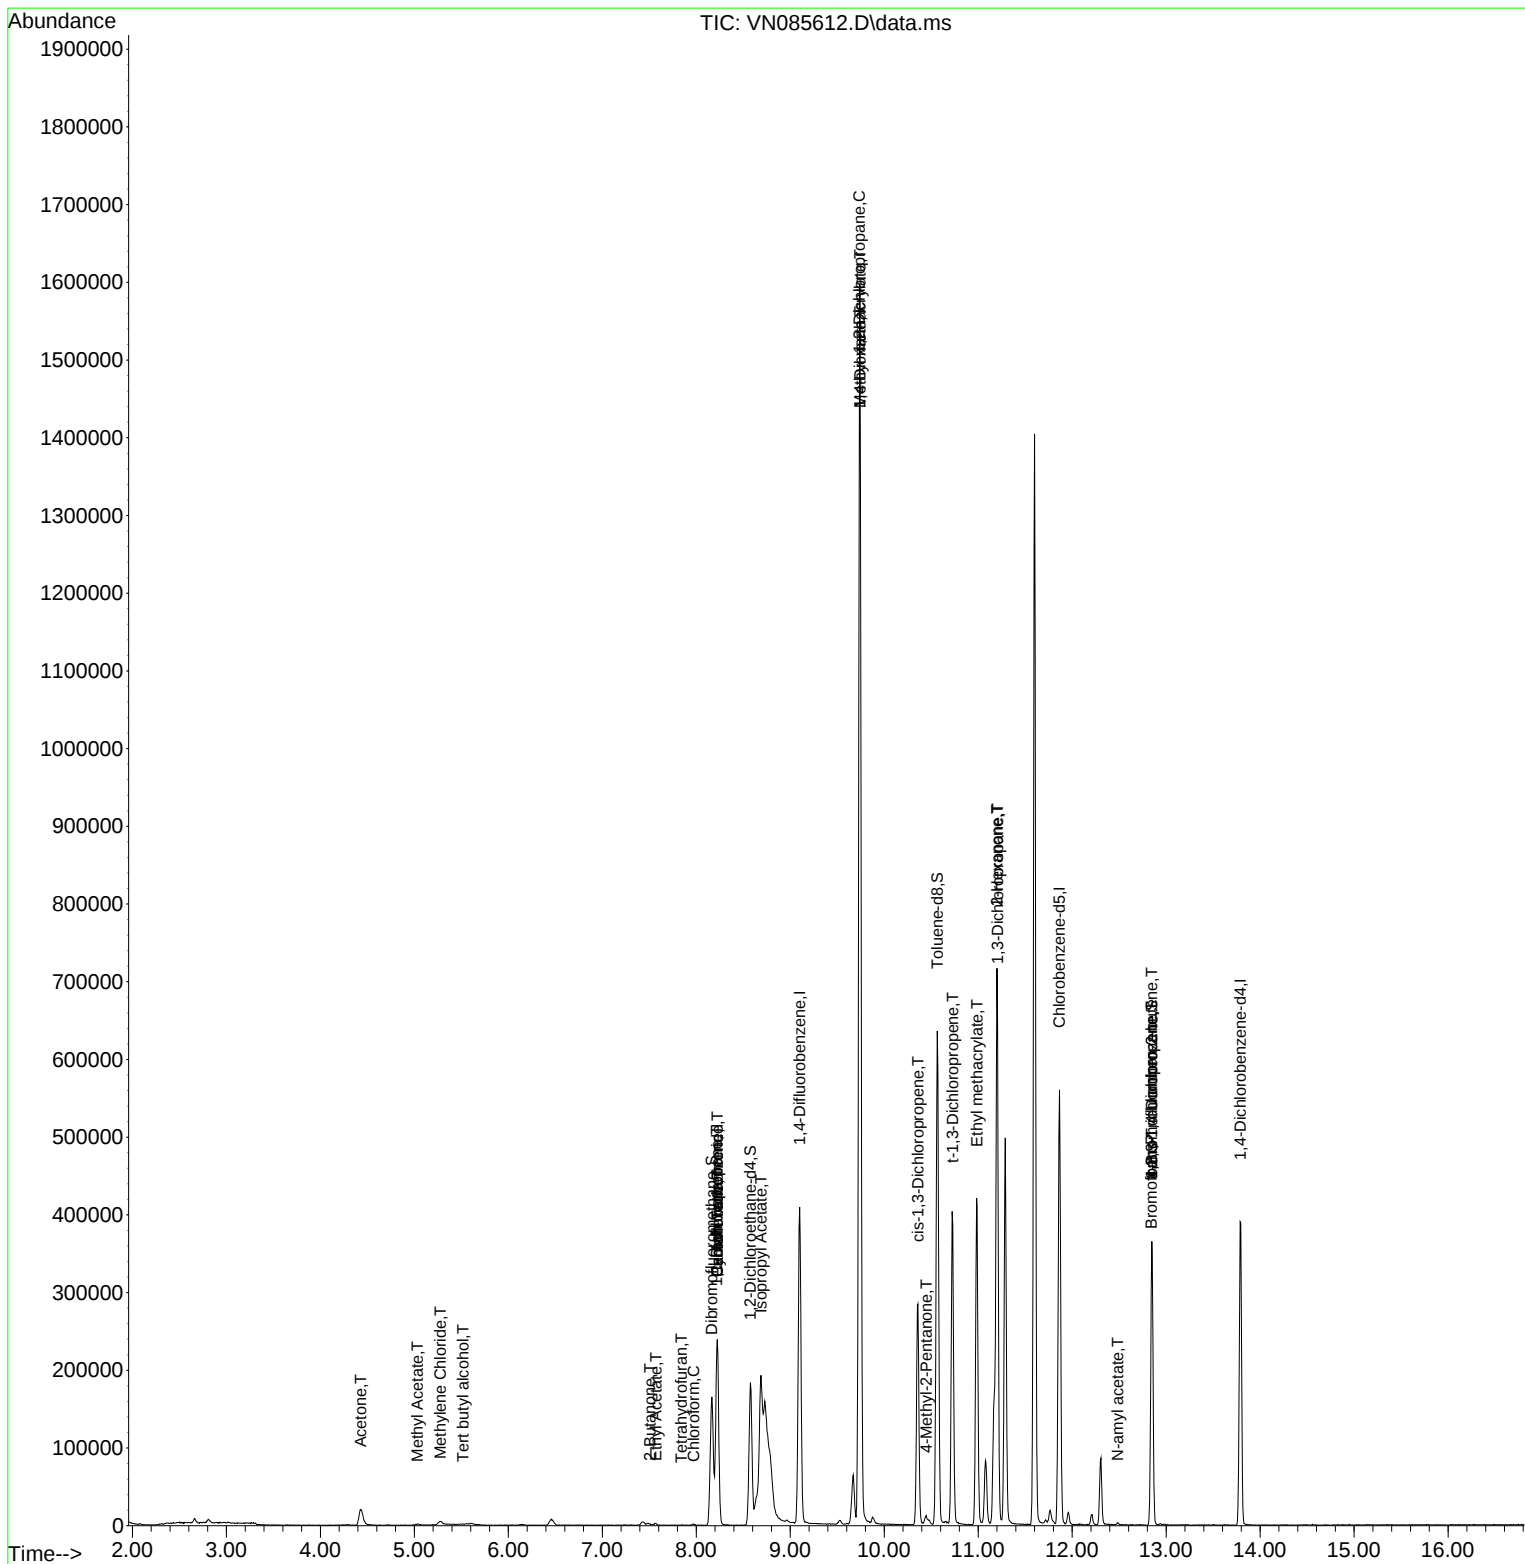




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:168 Resp: 161151  
Ion Ratio Lower Upper  
168 100  
99 61.9 53.6 80.4

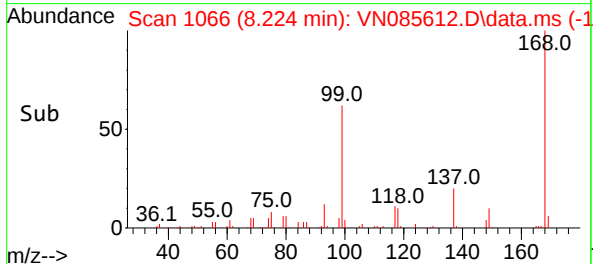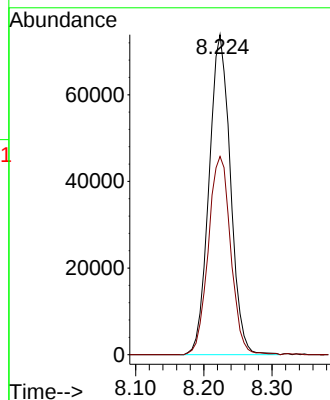

#11  
Tert butyl alcohol  
Concen: 0.594 ug/l  
RT: 5.518 min Scan# 606  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 59 Resp: 177  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.6 13.0#


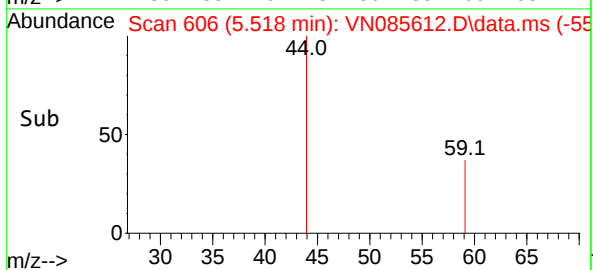
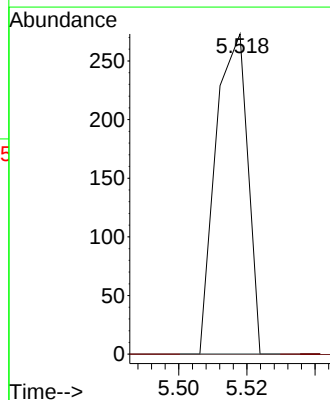
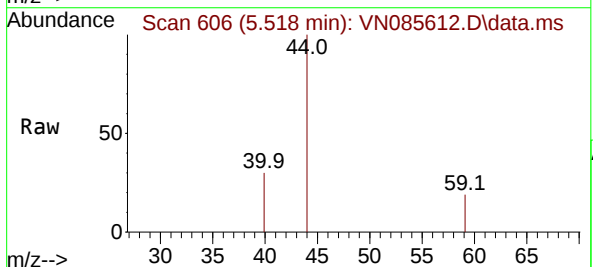




#16  
Acetone  
Concen: 48.442 ug/l  
RT: 4.430 min Scan# 419  
Delta R.T. 0.012 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 40716  
Ion Ratio Lower Upper  
43 100  
58 27.7 23.8 35.6

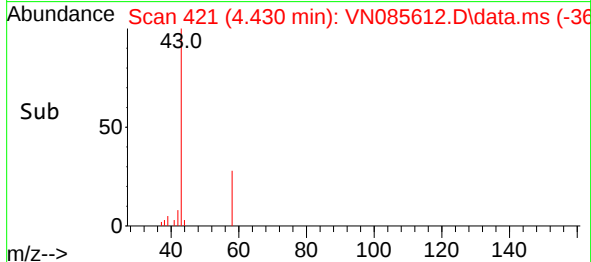

#18  
Methyl Acetate  
Concen: 1.338 ug/l  
RT: 5.030 min Scan# 523  
Delta R.T. 0.012 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17


Tgt Ion: 43 Resp: 3419  
Ion Ratio Lower Upper  
43 100  
74 6.0 18.6 28.0#

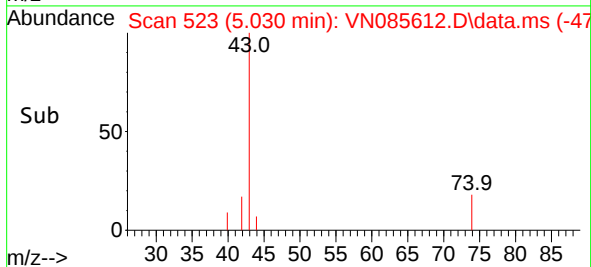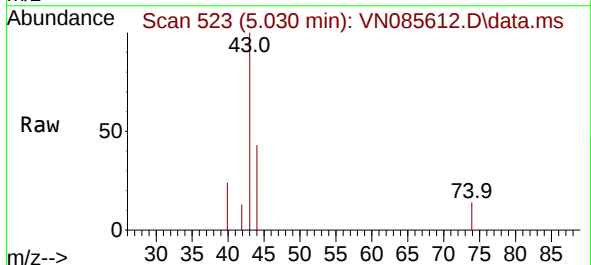






#20  
Methylene Chloride  
Concen: 1.618 ug/l  
RT: 5.277 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 84 Resp: 3367  
Ion Ratio Lower Upper  
84 100  
49 112.1 104.1 156.1  
51 30.0 31.0 46.4#  
86 44.7 51.9 77.9#

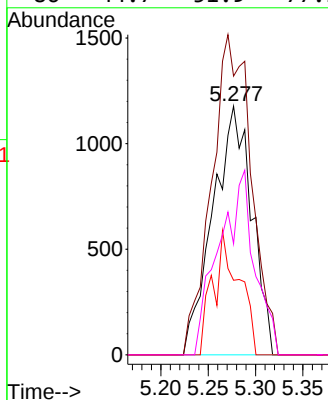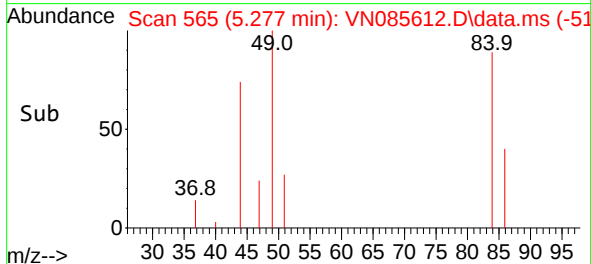

#25  
2-Butanone  
Concen: 3.913 ug/l  
RT: 7.506 min Scan# 944  
Delta R.T. 0.029 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 43 Resp: 4840  
Ion Ratio Lower Upper  
43 100  
72 24.8 20.2 30.4

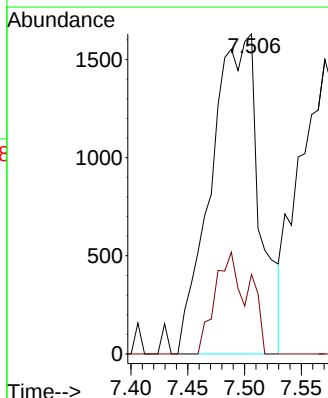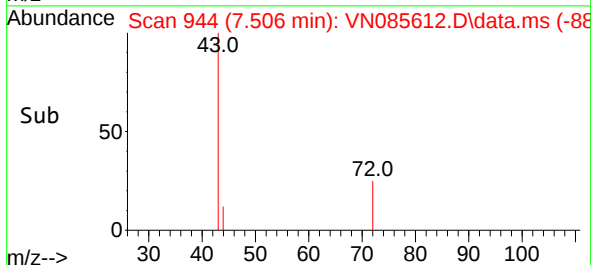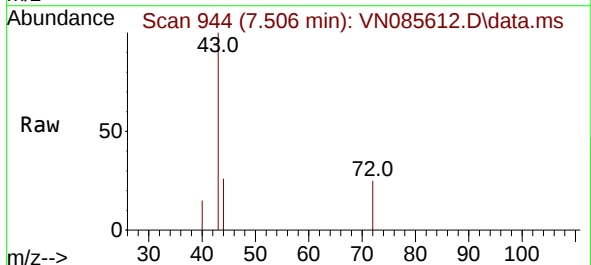

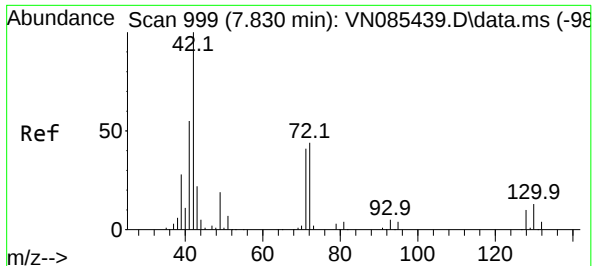

#29

Tetrahydrofuran

Concen: 0.284 ug/l

RT: 7.841 min Scan# 1001

Delta R.T. 0.012 min


Lab File: VN085612.D

Acq: 31 Jan 2025 19:17




Instrument :

MSVOA\_N

ClientSampleId :

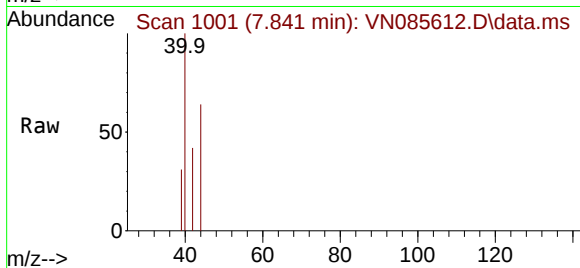

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 223   |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 0.0   | 34.2  | 51.2# |
| 71       | 0.0   | 32.5  | 48.7# |

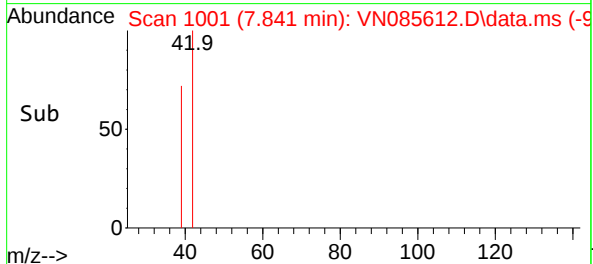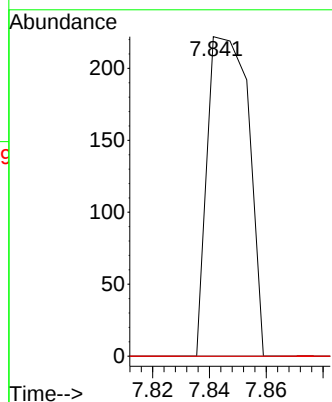

#30

Chloroform

Concen: 0.363 ug/l




RT: 7.971 min Scan# 1023


Delta R.T. 0.012 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 83    | Resp: | 1425  |
| Ion      | Ratio | Lower | Upper |
| 83       | 100   |       |       |
| 85       | 57.7  | 51.8  | 77.6  |

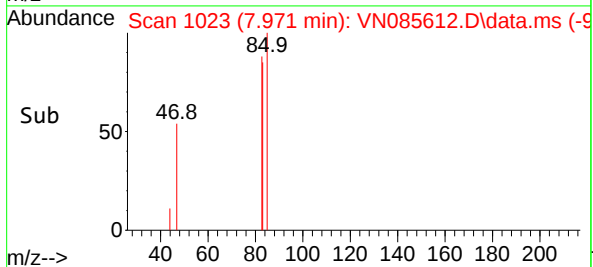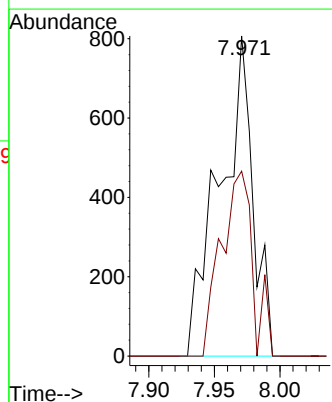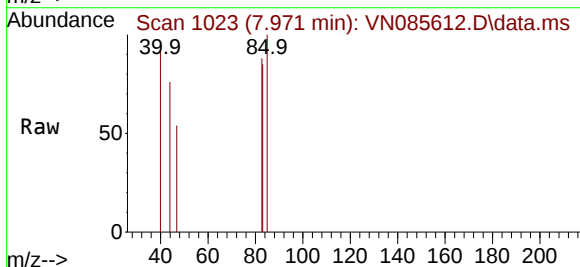



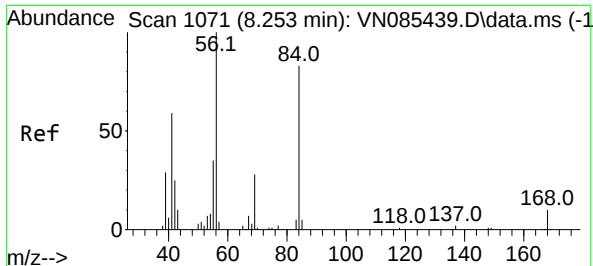


#31  
Cyclohexane  
Concen: 1.389 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.029 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 56 Resp: 4585  
Ion Ratio Lower Upper  
56 100  
69 169.1 22.2 33.4#  
84 123.7 66.4 99.6#

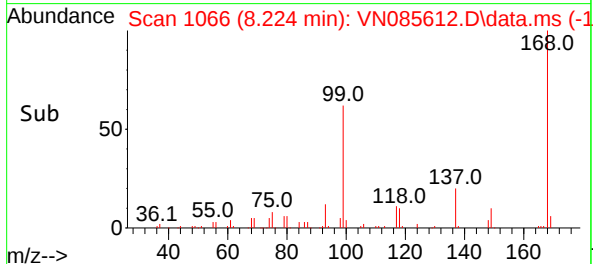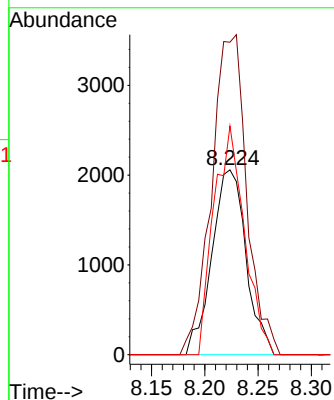

#33  
1,2-Dichloroethane-d4  
Concen: 58.627 ug/l  
RT: 8.577 min Scan# 1126  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 65 Resp: 152506  
Ion Ratio Lower Upper  
65 100  
67 51.3 0.0 101.6

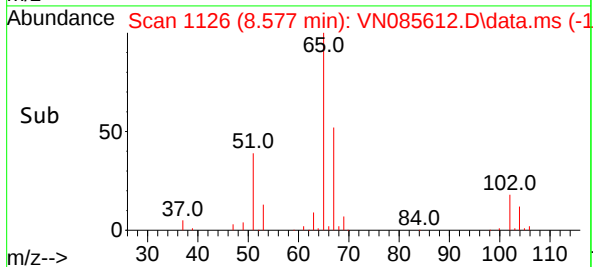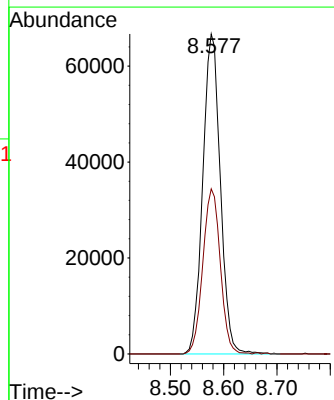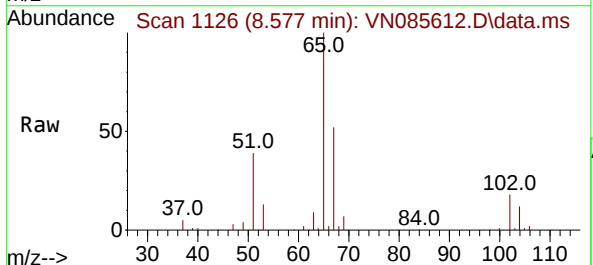

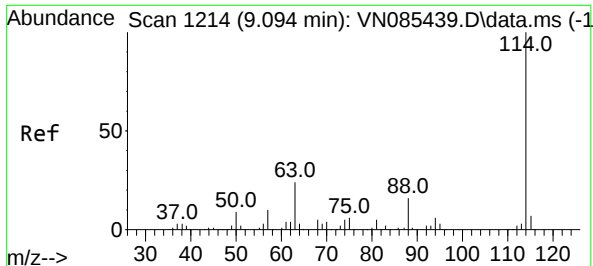

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion:114 Resp: 329996

Ion Ratio Lower Upper

114 100

63 23.2 0.0 47.6

88 16.2 0.0 32.6

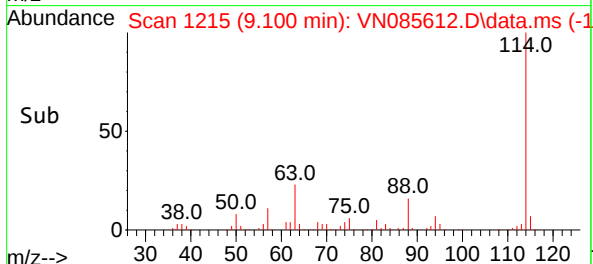

#35

Dibromofluoromethane

Concen: 50.124 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17




Tgt Ion:113 Resp: 114752


Ion Ratio Lower Upper

113 100

111 103.2 82.7 124.1

192 17.6 14.3 21.5

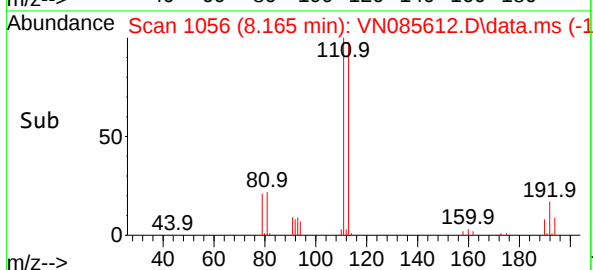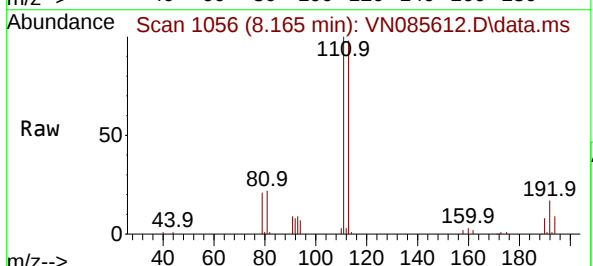



#36

1,1-Dichloropropene

Concen: 4.542 ug/l

RT: 8.218 min Scan# 1

Delta R.T. -0.147 min


Lab File: VN085612.D

Acq: 31 Jan 2025 19:17




Instrument :

MSVOA\_N

ClientSampleId :



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 75    | Resp: | 14595 |
| Ion      | Ratio | Lower | Upper |
| 75       | 100   |       |       |
| 110      | 9.1   | 16.5  | 49.5# |
| 77       | 0.0   | 24.4  | 36.6# |

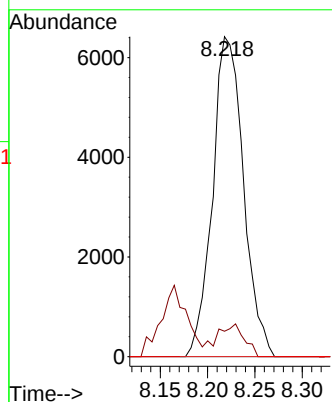

#37

Ethyl Acetate

Concen: 1.158 ug/l




RT: 7.571 min Scan# 955


Delta R.T. 0.018 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 3754  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 61       | 4.7   | 10.9  | 16.3# |
| 70       | 4.1   | 7.5   | 11.3# |

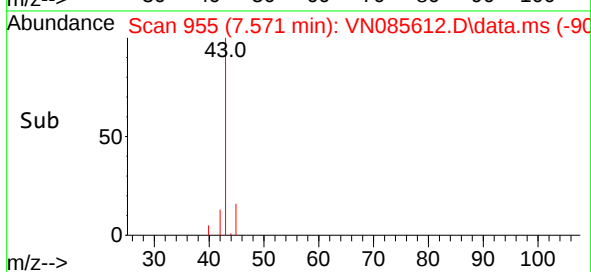






#38  
Carbon Tetrachloride  
Concen: 4.999 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.135 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion:117 Resp: 18389  
Ion Ratio Lower Upper  
117 100  
119 6.8 75.4 113.2#  
121 0.0 24.6 37.0#

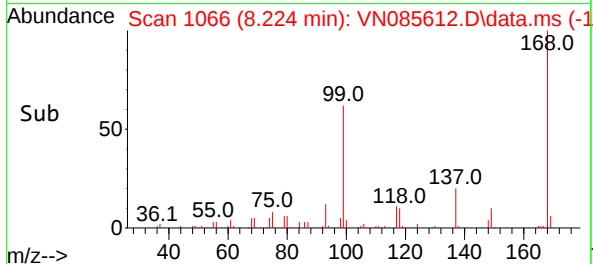

#43  
Isopropyl Acetate  
Concen: 50.370 ug/l  
RT: 8.688 min Scan# 1145  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 43 Resp: 261757  
Ion Ratio Lower Upper  
43 100  
61 12.2 20.7 31.1#  
87 6.9 9.8 14.8#

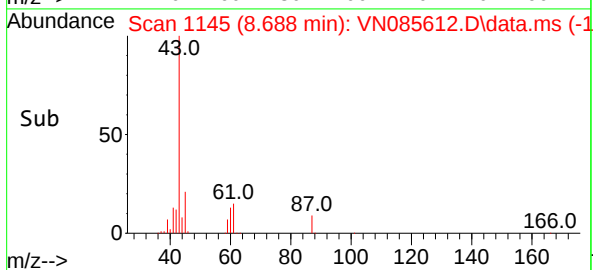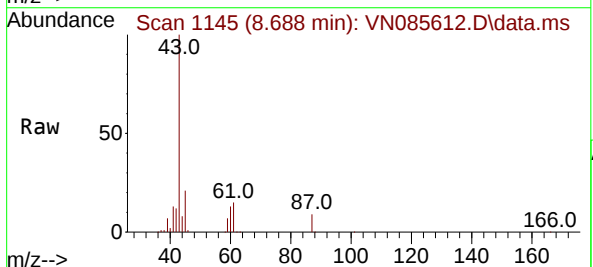

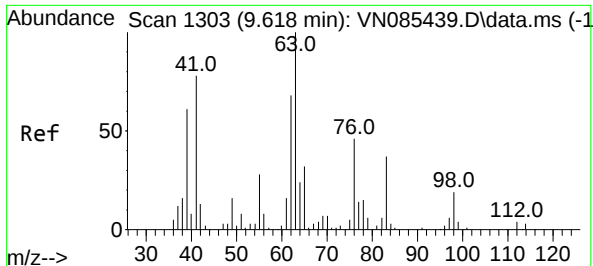

#45

1,2-Dichloropropane

Concen: 0.826 ug/l

RT: 9.735 min Scan# 1

Delta R.T. 0.118 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 63 Resp: 2036

Ion Ratio Lower Upper

63 100

65 0.0 25.6 38.4#

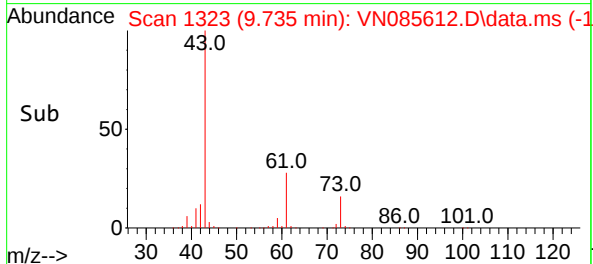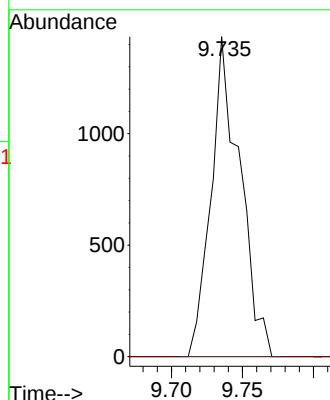

#48

Methyl methacrylate

Concen: 64.033 ug/l

RT: 9.741 min Scan# 1324

Delta R.T. 0.064 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17




Tgt Ion: 41 Resp: 149748


Ion Ratio Lower Upper

41 100

69 0.1 64.7 97.1#

39 57.2 49.0 73.6



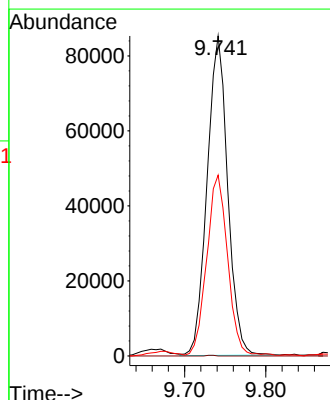
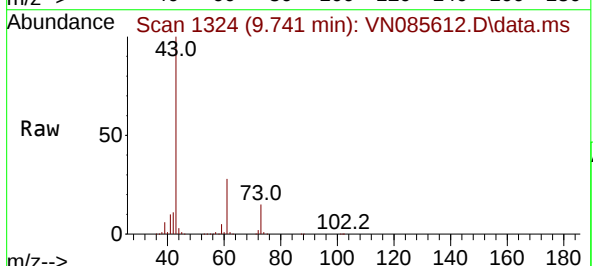




#49  
1,4-Dioxane  
Concen: 3.047 ug/l  
RT: 9.741 min Scan# 1324  
Delta R.T. 0.053 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 88 Resp: 120  
Ion Ratio Lower Upper  
88 100  
43 1221743.3 26.6 39.8#  
58 6767.5 59.5 89.3#

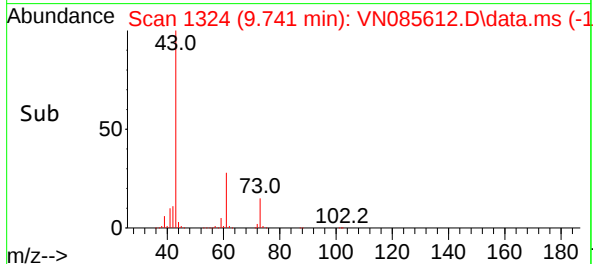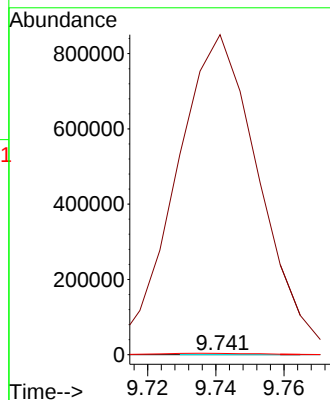

#50  
Toluene-d8  
Concen: 52.012 ug/l  
RT: 10.565 min Scan# 1464  
Delta R.T. -0.000 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 98 Resp: 423069  
Ion Ratio Lower Upper  
98 100  
100 63.5 52.2 78.4


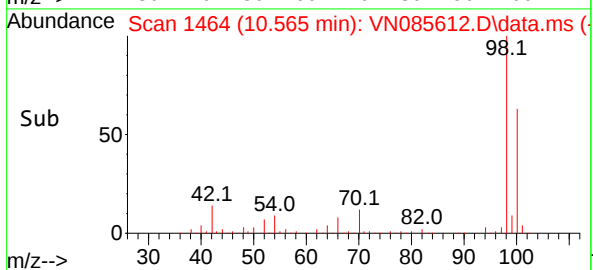
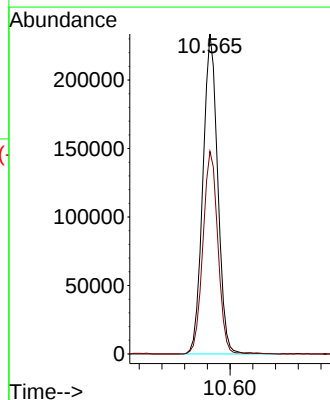
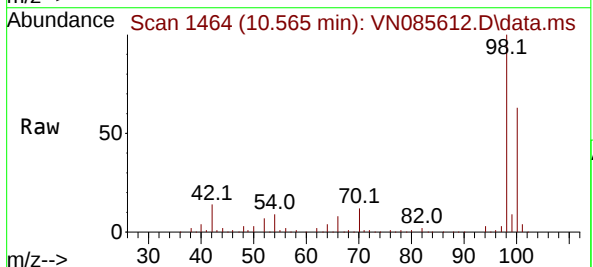




#51  
4-Methyl-2-Pentanone  
Concen: 4.062 ug/l  
RT: 10.447 min Scan# 1443  
Delta R.T. 0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 12250  
Ion Ratio Lower Upper  
43 100  
58 22.9 30.5 45.7#

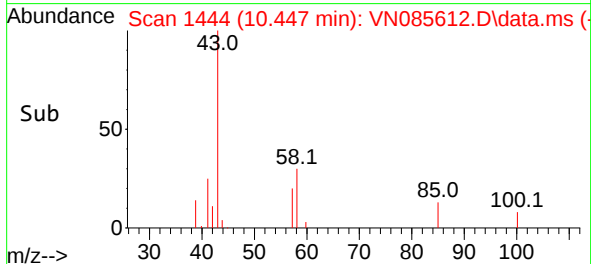

#53  
t-1,3-Dichloropropene  
Concen: 0.276 ug/l  
RT: 10.729 min Scan# 1492  
Delta R.T. -0.106 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 75 Resp: 947  
Ion Ratio Lower Upper  
75 100  
77 27.3 23.5 35.3


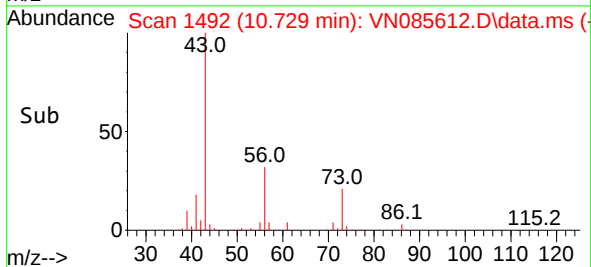

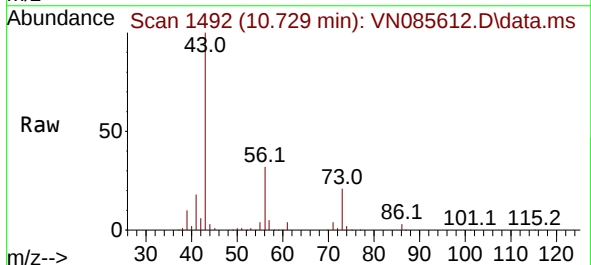




#54  
 cis-1,3-Dichloropropene  
 Concen: 12.497 ug/l  
 RT: 10.359 min Scan# 1429  
 Delta R.T. 0.053 min  
 Lab File: VN085612.D  
 Acq: 31 Jan 2025 19:17




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 75 Resp: 45731  
 Ion Ratio Lower Upper  
 75 100  
 77 0.9 25.0 37.4#  
 39 47.5 43.1 64.7

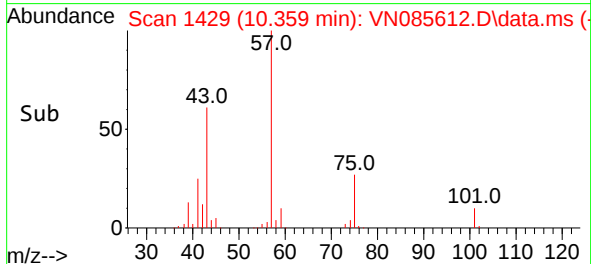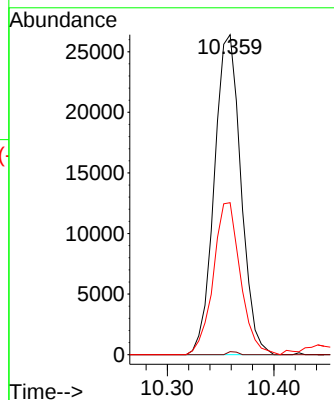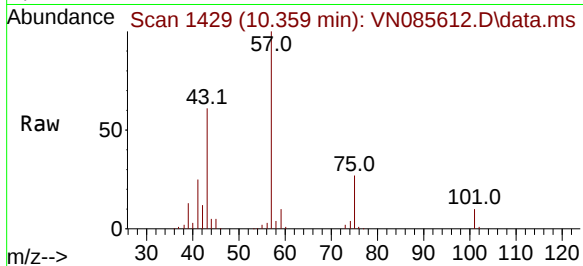

#56  
 Ethyl methacrylate  
 Concen: 2.530 ug/l  
 RT: 10.988 min Scan# 1536  
 Delta R.T. 0.117 min  
 Lab File: VN085612.D  
 Acq: 31 Jan 2025 19:17

Tgt Ion: 69 Resp: 2323  
 Ion Ratio Lower Upper  
 69 100  
 41 3691.6 54.6 82.0#  
 39 1773.1 32.4 48.6#

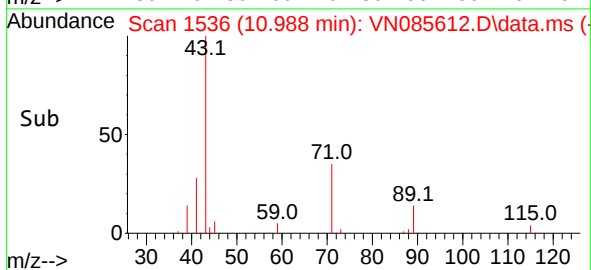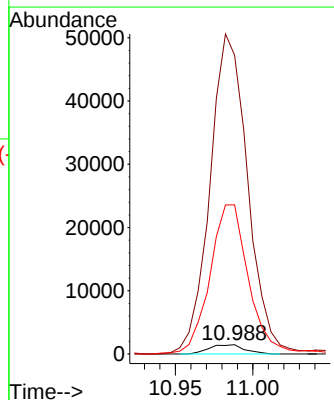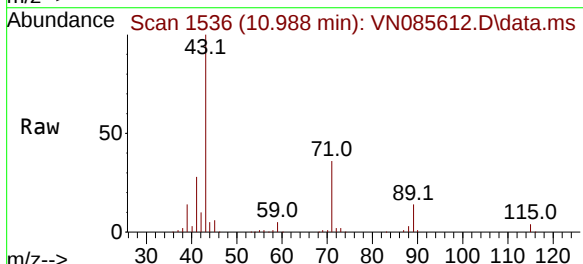

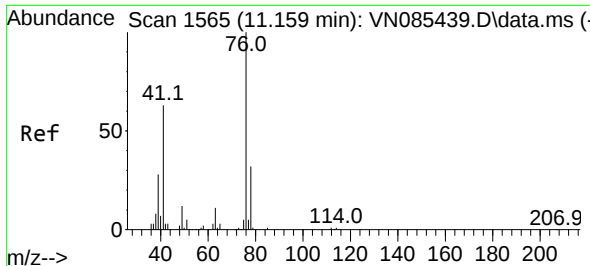

#57

1,3-Dichloropropane

Concen: 1.884 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.047 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 76 Resp: 7253

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

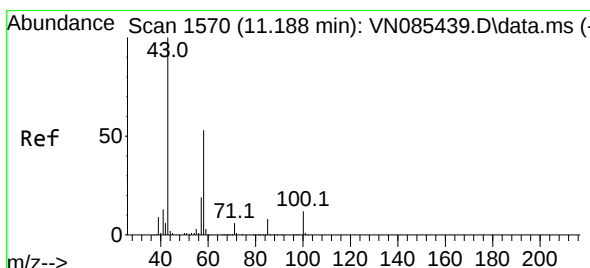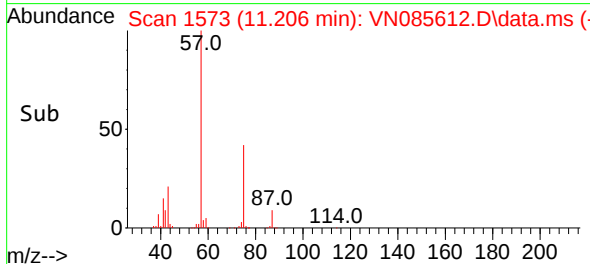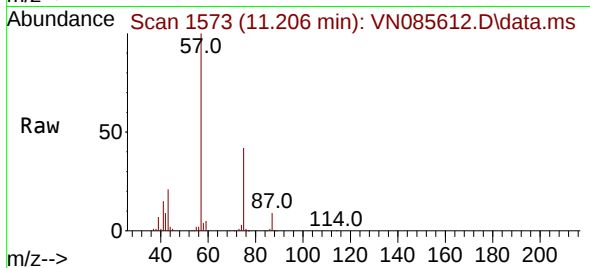

#59

2-Hexanone

Concen: 42.383 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.012 min

Lab File: VN085612.D




Acq: 31 Jan 2025 19:17


Tgt Ion: 43 Resp: 89929

Ion Ratio Lower Upper

43 100

58 22.6 26.2 78.6#


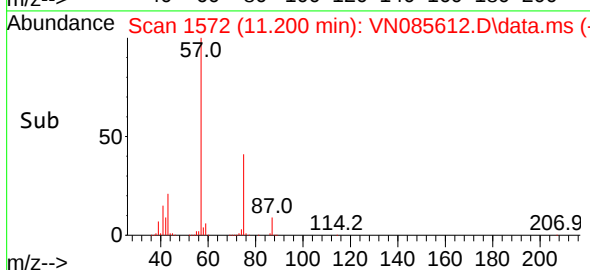

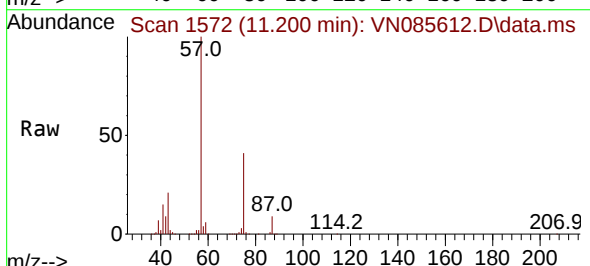




#62  
4-Bromofluorobenzene  
Concen: 42.469 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.000 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 95 Resp: 118167  
Ion Ratio Lower Upper  
95 100  
174 76.2 0.0 145.0  
176 72.4 0.0 142.4

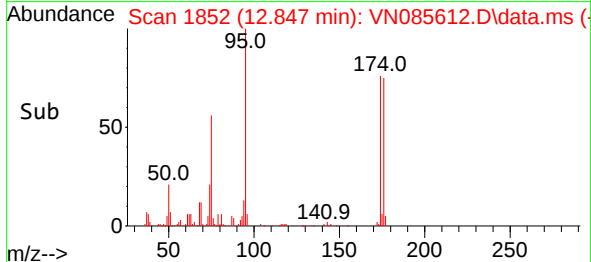

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 1685  
Delta R.T. -0.000 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17

Tgt Ion: 117 Resp: 302646  
Ion Ratio Lower Upper  
117 100  
82 61.5 48.6 72.8  
119 33.1 26.6 39.8

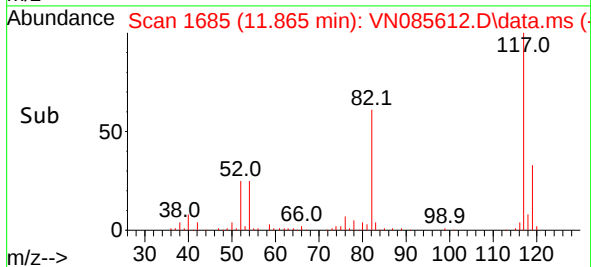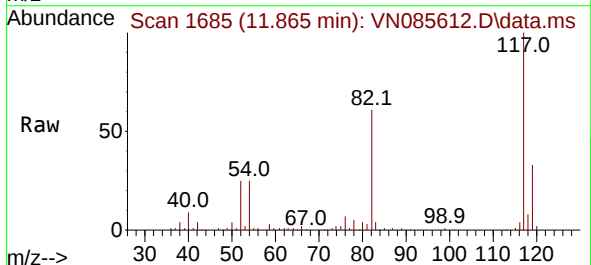



#71

Bromoform

Concen: 0.459 ug/l

RT: 12.841 min Scan# 1806

Delta R.T. 0.265 min


Lab File: VN085612.D

Acq: 31 Jan 2025 19:17

Instrument :

MSVOA\_N

ClientSampleId :






Tgt Ion:173 Resp: 799

Ion Ratio Lower Upper

173 100

175 594.7 24.4 73.2#

254 0.0 0.0 0.0

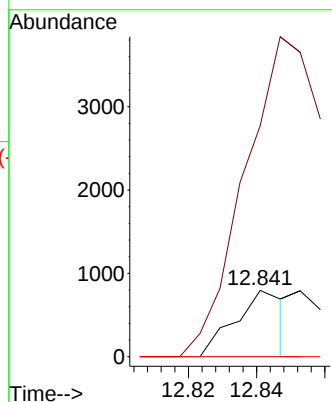

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. -0.000 min

Lab File: VN085612.D

Acq: 31 Jan 2025 19:17




Tgt Ion:152 Resp: 103424


Ion Ratio Lower Upper

152 100

115 61.7 31.1 93.3

150 155.9 0.0 343.6


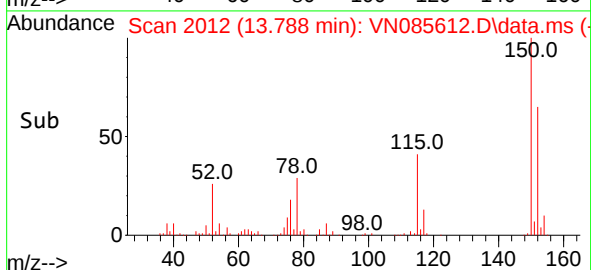






#74  
N-amy1 acetate  
Concen: 0.713 ug/l  
RT: 12.482 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17




Instrument :  
MSVOA\_N  
ClientSampleId :


|             |             |
|-------------|-------------|
| Tgt Ion: 43 | Resp: 2238  |
| Ion Ratio   | Lower Upper |
| 43 100      |             |
| 70 0.0      | 34.0 51.0#  |
| 55 0.0      | 21.4 32.2#  |
| 61 0.0      | 19.0 28.4#  |

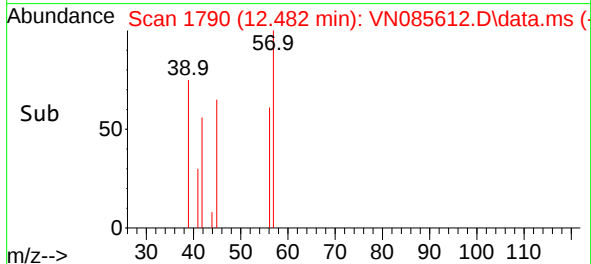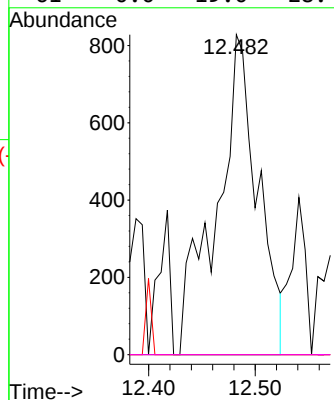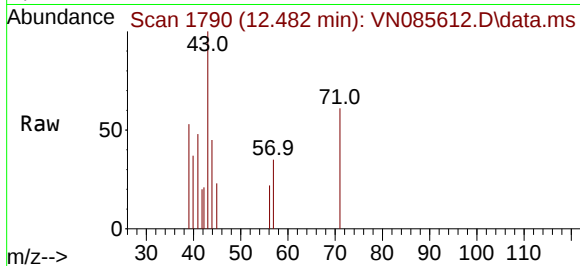

#76  
1,2,3-Trichloropropane  
Concen: 32.117 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.141 min  
Lab File: VN085612.D  
Acq: 31 Jan 2025 19:17


|             |              |
|-------------|--------------|
| Tgt Ion: 75 | Resp: 67514  |
| Ion Ratio   | Lower Upper  |
| 75 100      |              |
| 77 1.0      | 109.7 329.2# |

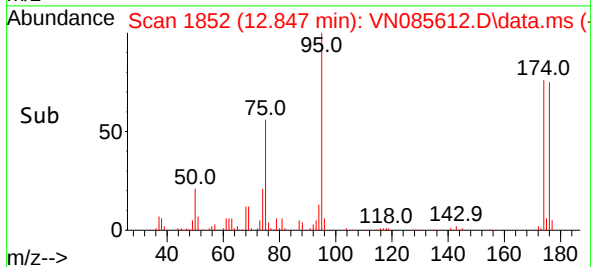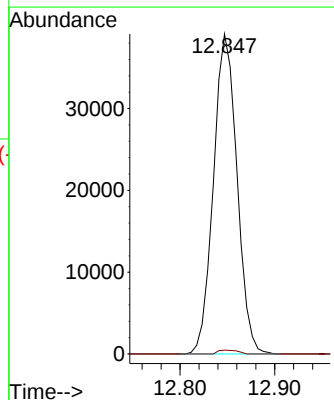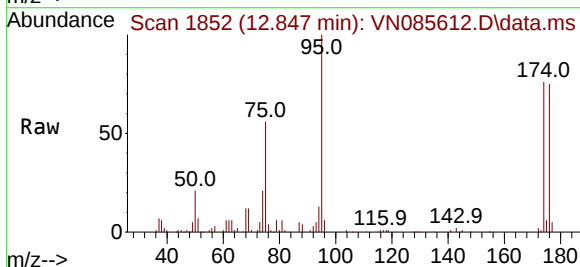



#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 86.895 ug/l  
 RT: 12.847 min Scan# 11  
 Delta R.T. 0.112 min  
 Lab File: VN085612.D  
 Acq: 31 Jan 2025 19:17

Instrument :  
 MSVOA\_N  
 ClientSampleId :

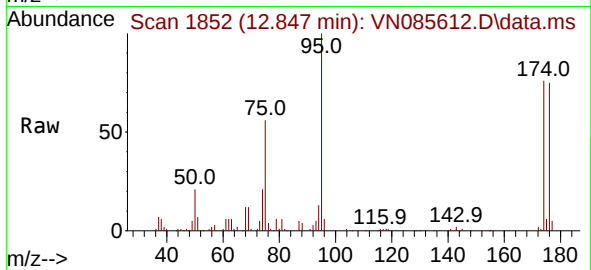

Tgt Ion: 75 Resp: 67514  
 Ion Ratio Lower Upper  
 75 100  
 53 0.1 95.6 143.4#  
 89 0.1 37.0 55.6#

