

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013125\
 Data File : VN085613.D
 Acq On : 31 Jan 2025 19:41
 Operator : JC\MD
 Sample : PB166357ZHE#01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB166357ZHE#01

Quant Time: Jan 31 22:34:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 15 02:16:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	165752	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	344120	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	324187	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	112034	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	160166	59.862	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	119.720%		
35) Dibromofluoromethane	8.165	113	118851	49.784	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.560%		
50) Toluene-d8	10.565	98	444373	52.389	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	104.780%		
62) 4-Bromofluorobenzene	12.847	95	130963	45.136	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	90.280%		
Target Compounds						
16) Acetone	4.430	43	33178	38.378	ug/l	97
20) Methylene Chloride	5.265	84	3322	1.552	ug/l #	78
30) Chloroform	7.965	83	6392	1.583	ug/l	99
43) Isopropyl Acetate	8.688	43	261992	48.346	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013125\
Data File : VN085613.D
Acq On : 31 Jan 2025 19:41
Operator : JC\MD
Sample : PB166357ZHE#01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB166357ZHE#01


Quant Time: Jan 31 22:34:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 02:16:08 2025
Response via : Initial Calibration

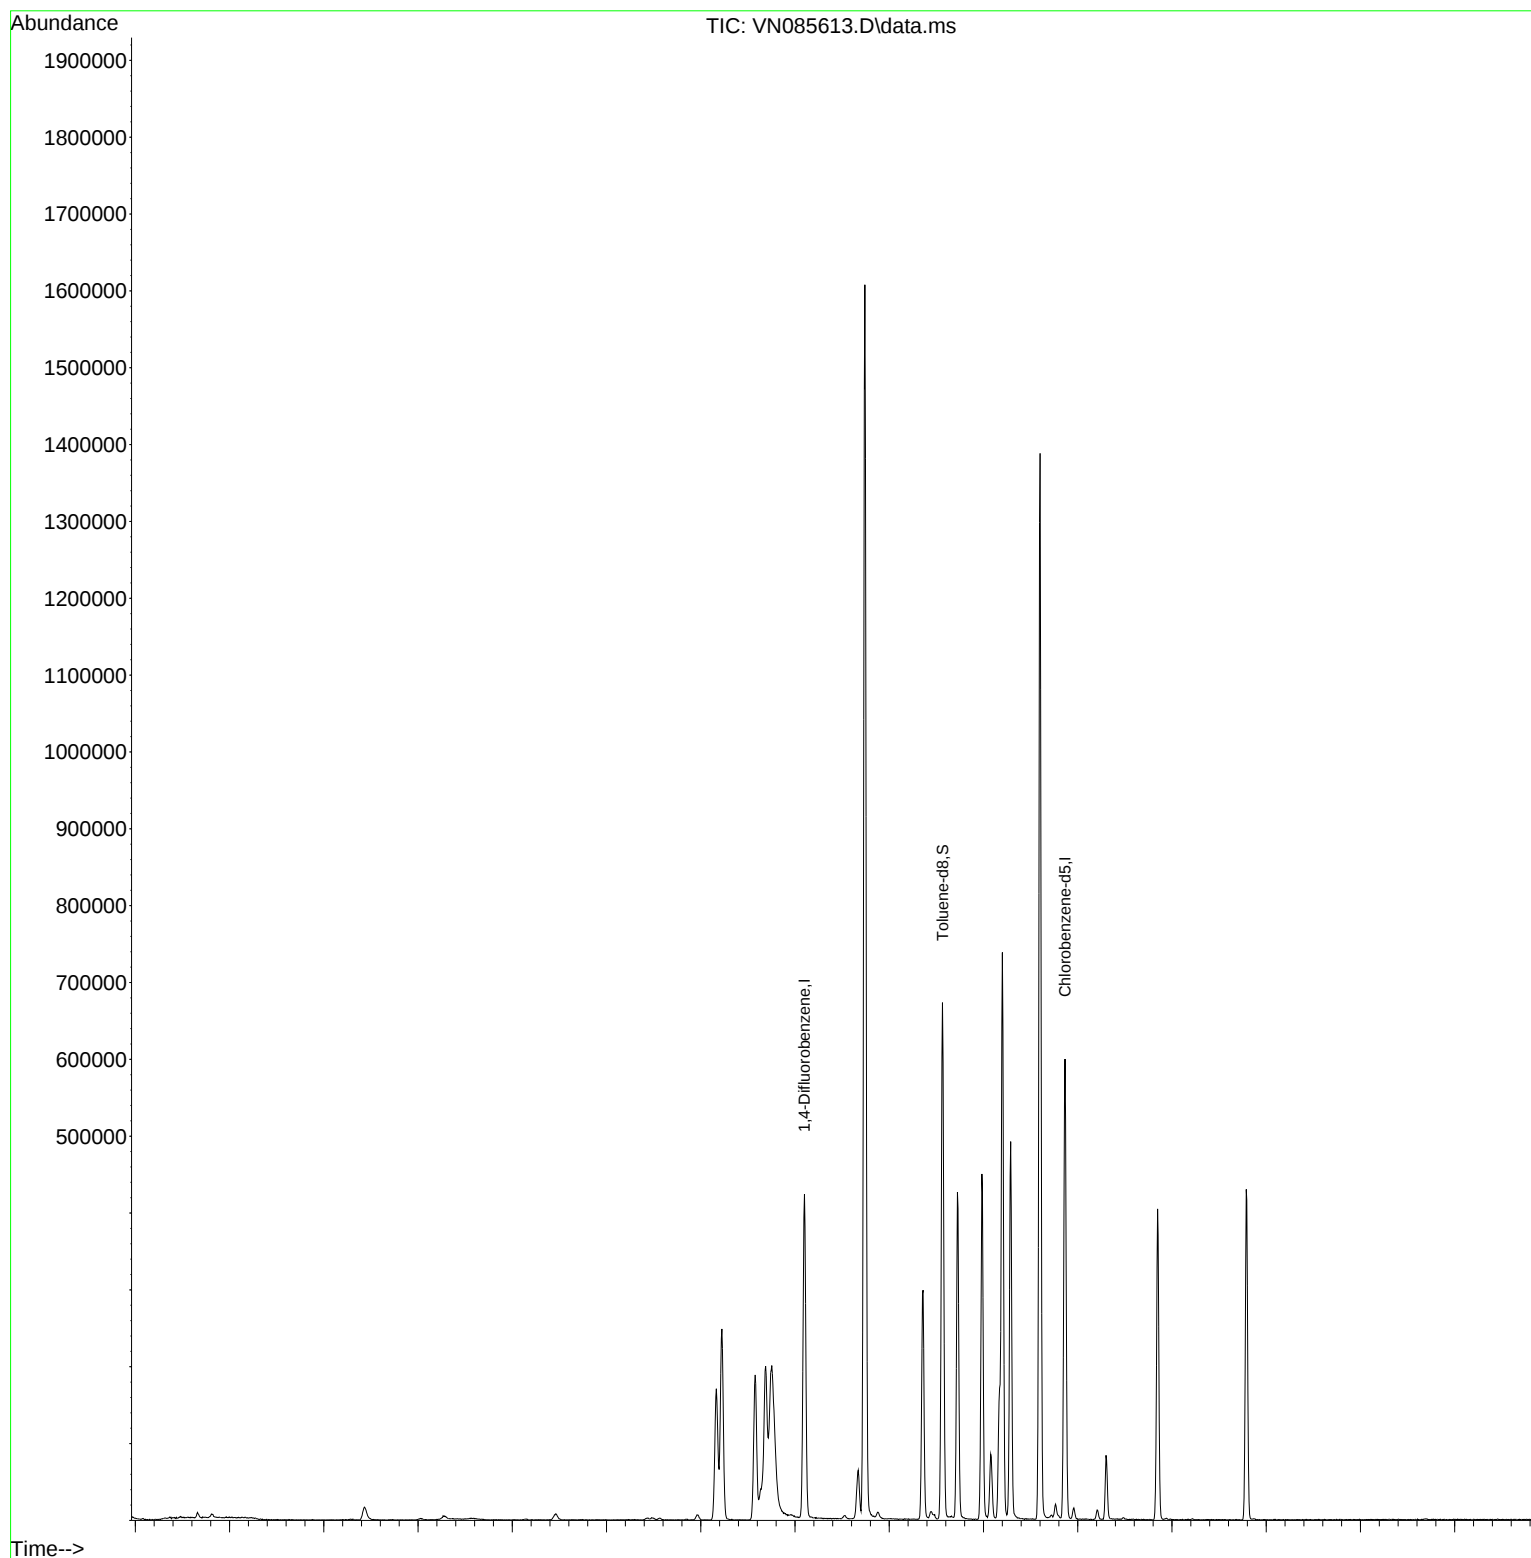



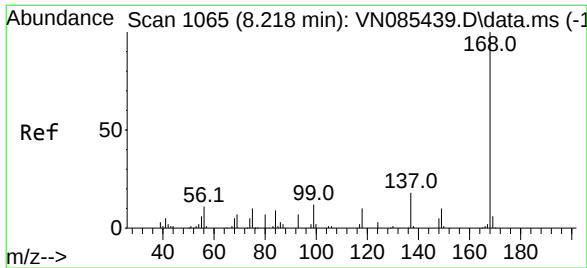


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085613.D
Acq: 31 Jan 2025 19:41

Instrument :
MSVOA_N
ClientSampleId :
PB166357ZHE#01



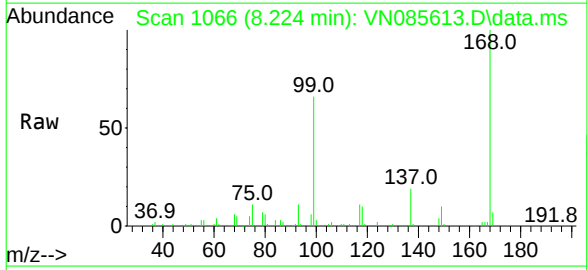



Tgt Ion:168 Resp: 165752
Ion Ratio Lower Upper
168 100
99 66.3 53.6 80.4

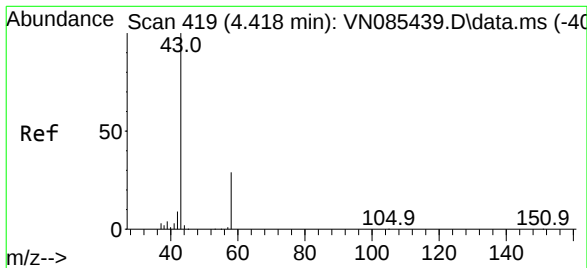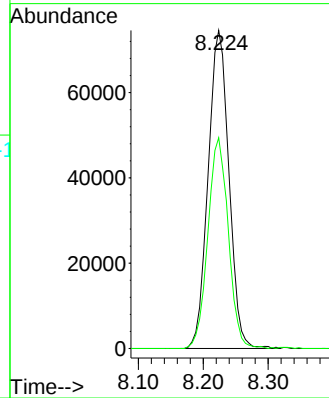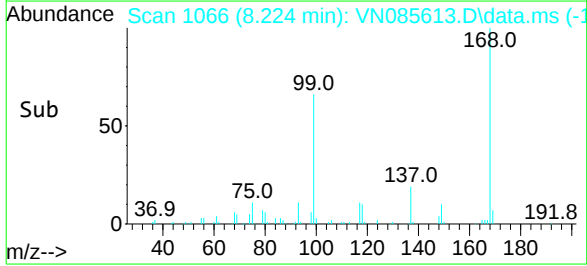

#16
Acetone
Concen: 38.378 ug/l
RT: 4.430 min Scan# 421
Delta R.T. 0.012 min
Lab File: VN085613.D
Acq: 31 Jan 2025 19:41

Tgt Ion: 43 Resp: 33178
Ion Ratio Lower Upper
43 100
58 28.1 23.8 35.6

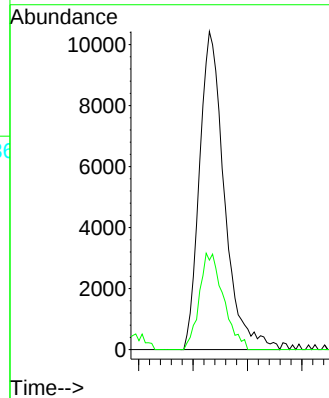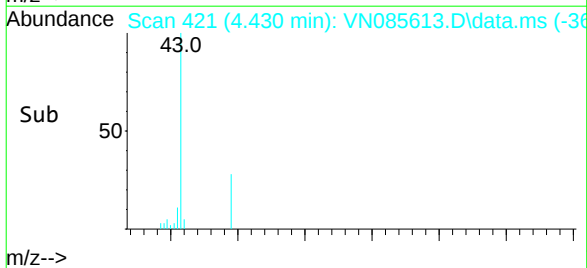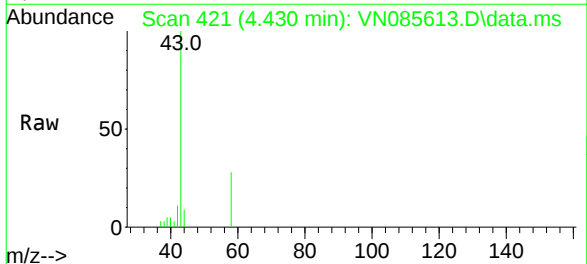

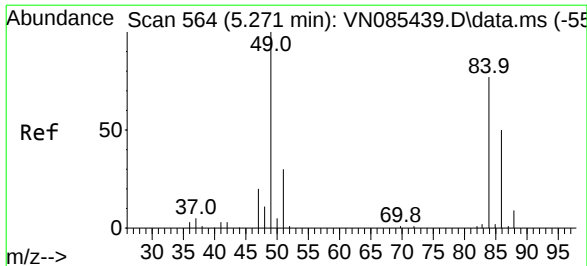

#20

Methylene Chloride

Concen: 1.552 ug/l

RT: 5.265 min Scan# 56

Delta R.T. -0.006 min

Lab File: VN085613.D


Acq: 31 Jan 2025 19:41

Instrument :




MSVOA_N

ClientSampleId :

PB166357ZHE#01

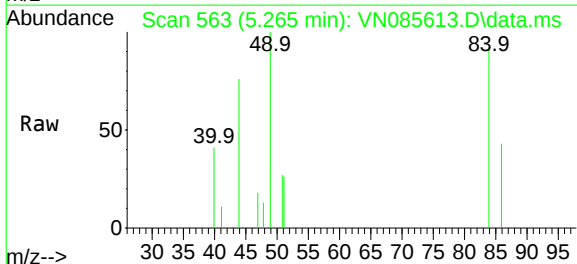

Tgt Ion:	84	Resp:	3322
Ion	Ratio	Lower	Upper
84	100		
49	108.5	104.1	156.1
51	57.4	31.0	46.4#
86	46.3	51.9	77.9#

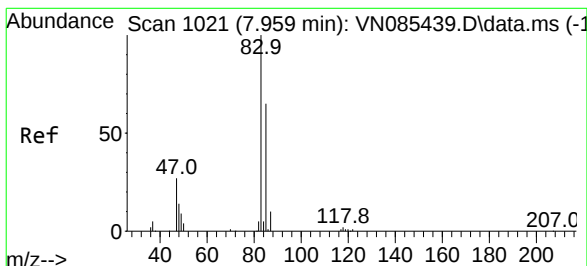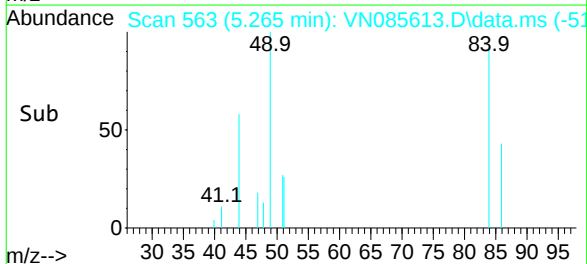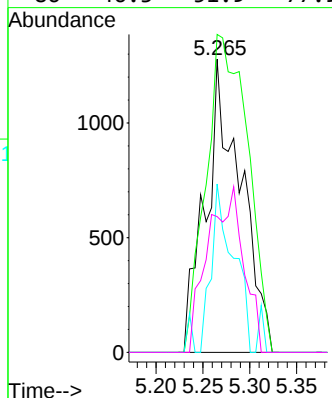

#30

Chloroform

Concen: 1.583 ug/l




RT: 7.965 min Scan# 1022


Delta R.T. 0.006 min

Lab File: VN085613.D

Acq: 31 Jan 2025 19:41

Tgt Ion:	83	Resp:	6392
Ion	Ratio	Lower	Upper
83	100		
85	65.9	51.8	77.6


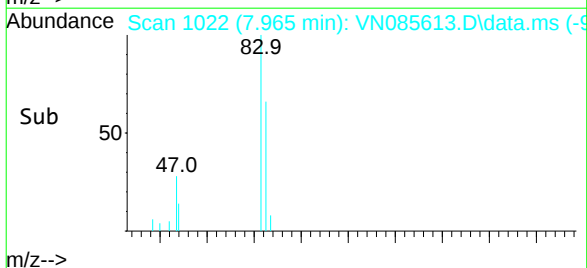
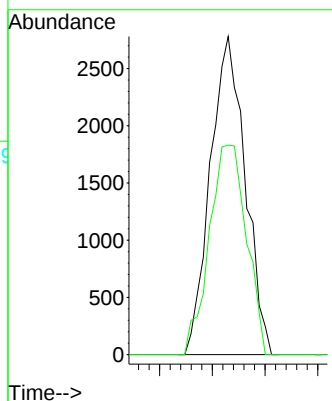
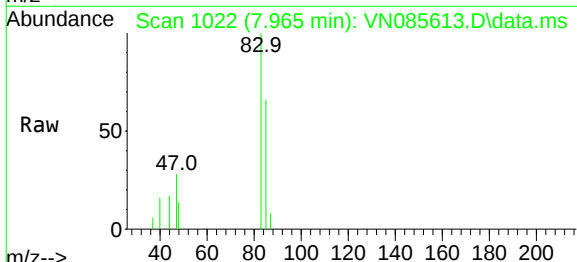


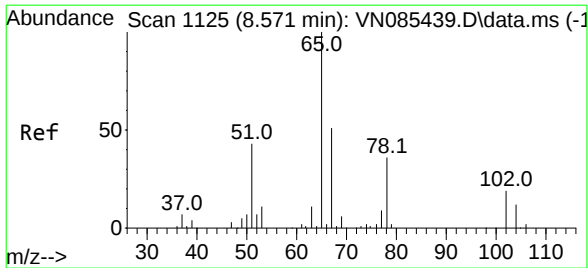

#33
1,2-Dichloroethane-d4
Concen: 59.862 ug/l
RT: 8.577 min Scan# 111
Delta R.T. 0.006 min
Lab File: VN085613.D
Acq: 31 Jan 2025 19:41




Instrument :
MSVOA_N
ClientSampleId :
PB166357ZHE#01


Tgt Ion: 65 Resp: 160166
Ion Ratio Lower Upper
65 100
67 50.3 0.0 101.6

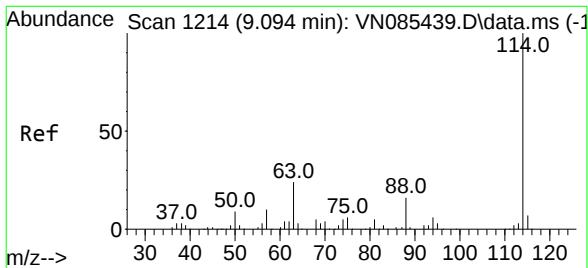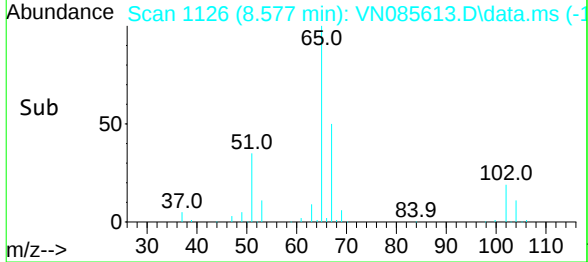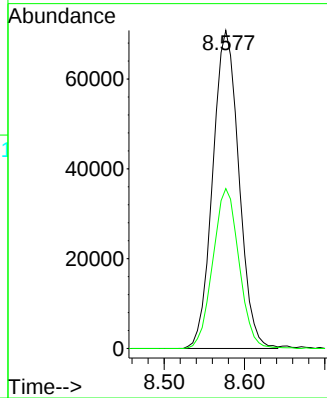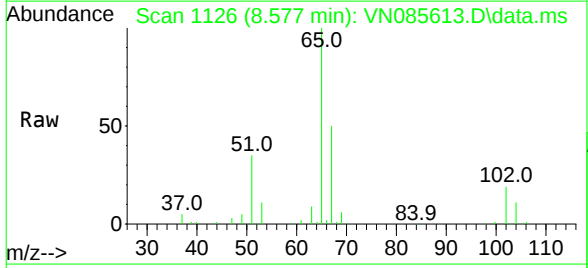

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 1215
Delta R.T. 0.006 min
Lab File: VN085613.D
Acq: 31 Jan 2025 19:41

Tgt Ion: 114 Resp: 344120
Ion Ratio Lower Upper
114 100
63 22.8 0.0 47.6
88 15.4 0.0 32.6


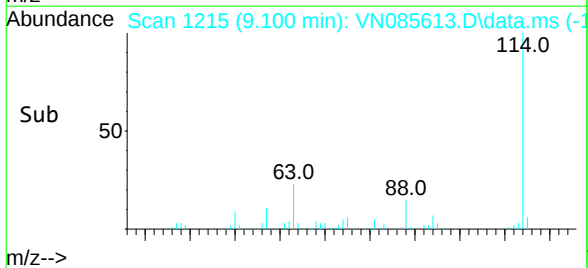
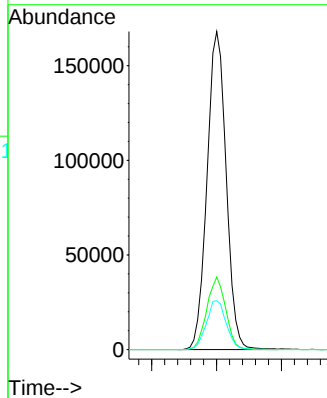
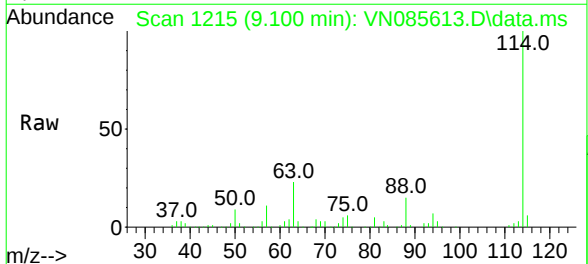


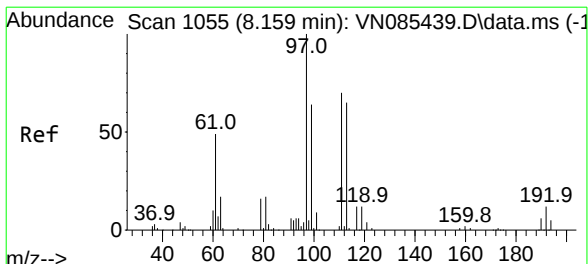

#35
 Dibromofluoromethane
 Concen: 49.784 ug/l
 RT: 8.165 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VN085613.D
 Acq: 31 Jan 2025 19:41




Instrument :
 MSVOA_N
 ClientSampleId :
 PB166357ZHE#01


Tgt Ion:	113	Resp:	118851
Ion	Ratio	Lower	Upper
113	100		
111	104.6	82.7	124.1
192	17.6	14.3	21.5

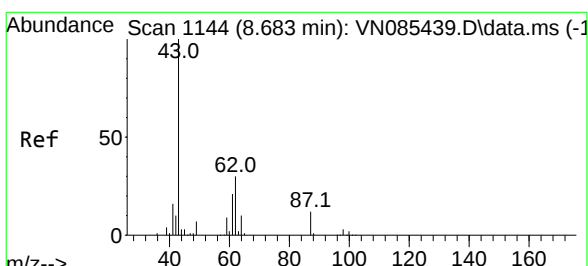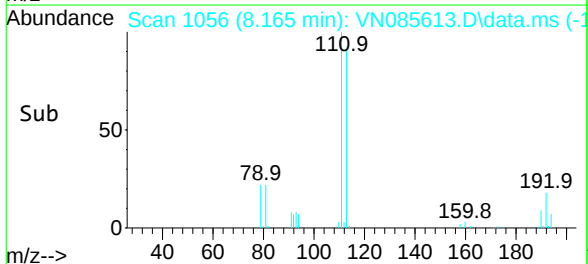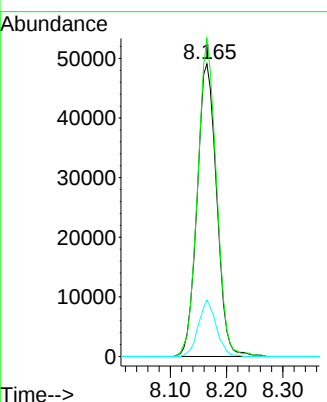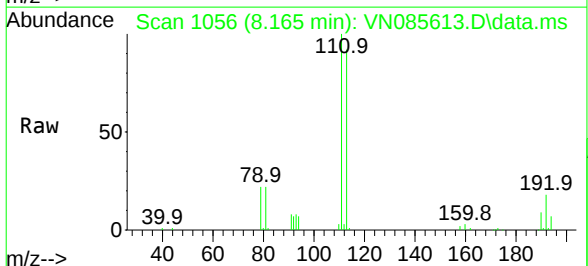

#43
 Isopropyl Acetate
 Concen: 48.346 ug/l
 RT: 8.688 min Scan# 1145
 Delta R.T. 0.006 min
 Lab File: VN085613.D
 Acq: 31 Jan 2025 19:41

Tgt Ion:	43	Resp:	261992
Ion	Ratio	Lower	Upper
43	100		
61	11.7	20.7	31.1#
87	7.3	9.8	14.8#

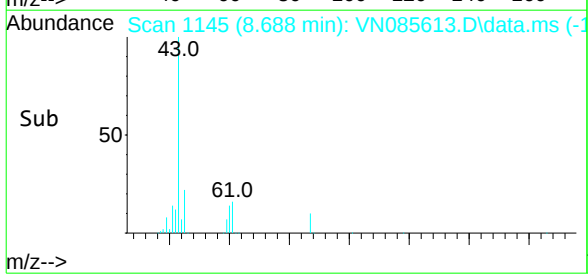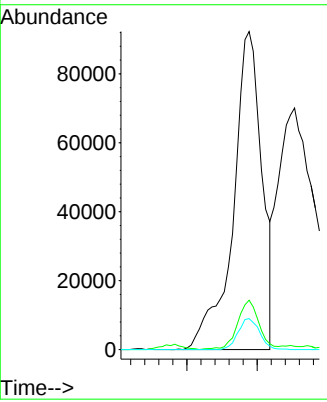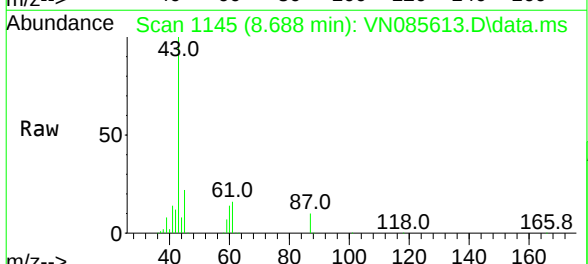

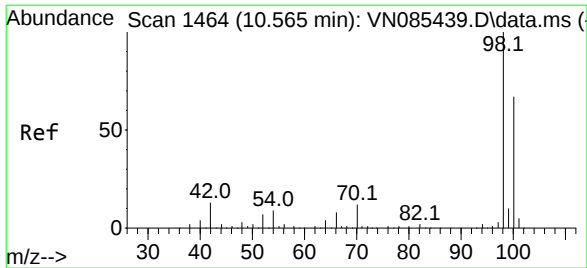

#50

Toluene-d8

Concen: 52.389 ug/l

RT: 10.565 min Scan# 14

Delta R.T. 0.000 min

Lab File: VN085613.D

Acq: 31 Jan 2025 19:41

Instrument :

MSVOA_N

ClientSampleId :





PB166357ZHE#01

Tgt Ion: 98 Resp: 444373

Ion Ratio Lower Upper

98 100

100 64.1 52.2 78.4

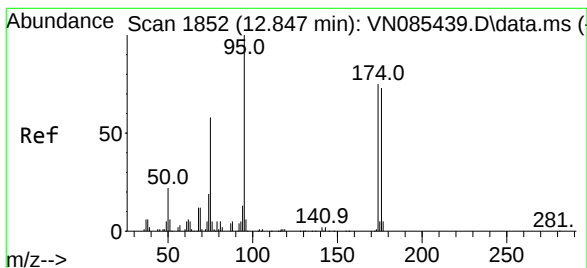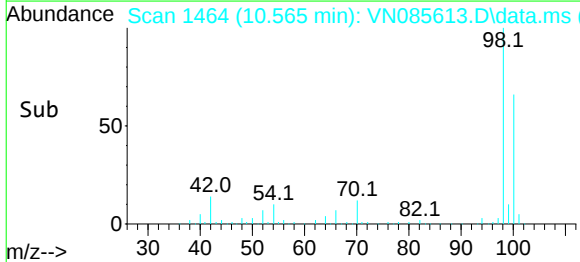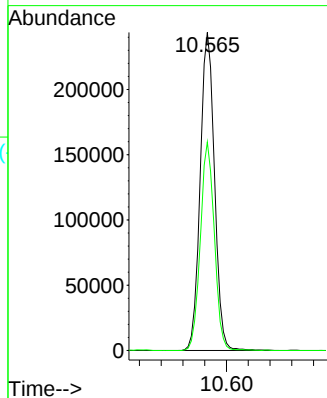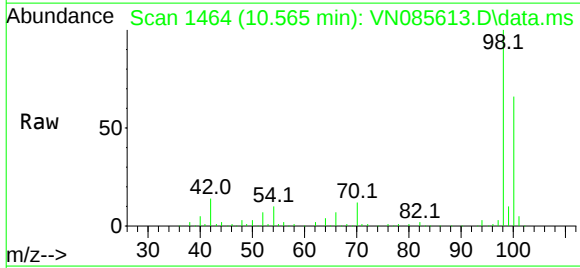

#62

4-Bromofluorobenzene

Concen: 45.136 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.000 min

Lab File: VN085613.D

Acq: 31 Jan 2025 19:41




Tgt Ion: 95 Resp: 130963


Ion Ratio Lower Upper

95 100

174 74.4 0.0 145.0

176 69.8 0.0 142.4

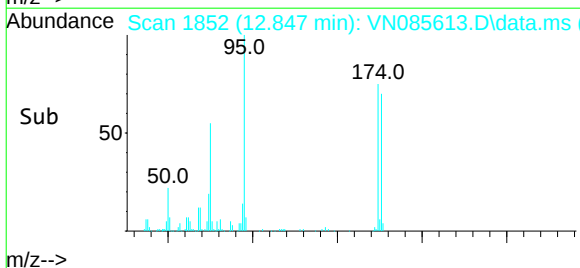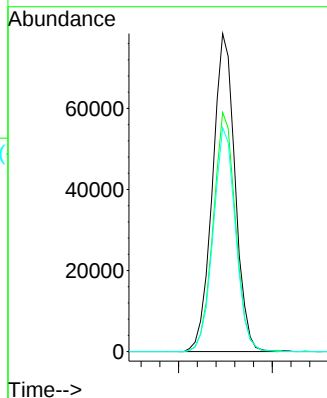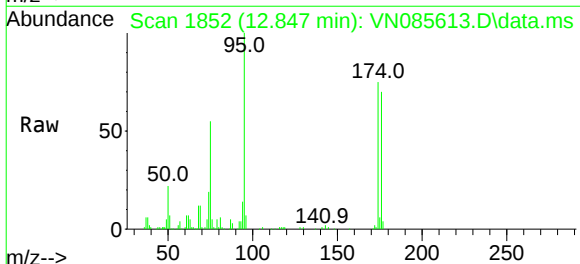

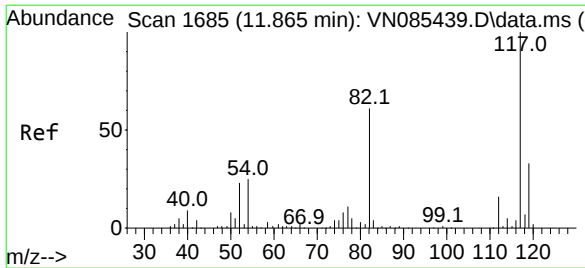

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 16

Delta R.T. 0.000 min

Lab File: VN085613.D

Acq: 31 Jan 2025 19:41

Instrument :

MSVOA_N

ClientSampleId :

PB166357ZHE#01





Tgt Ion:117 Resp: 324187

Ion Ratio Lower Upper

117 100

82 60.1 48.6 72.8

119 32.3 26.6 39.8

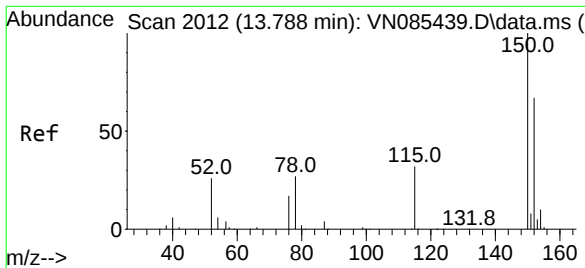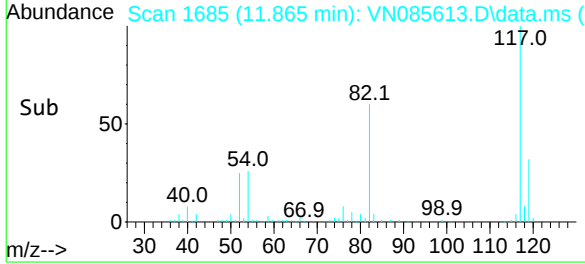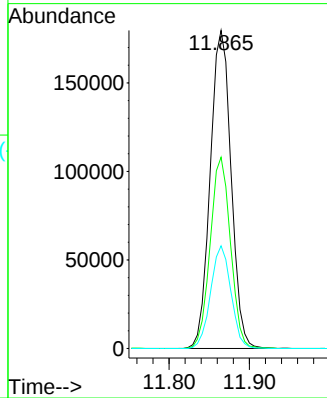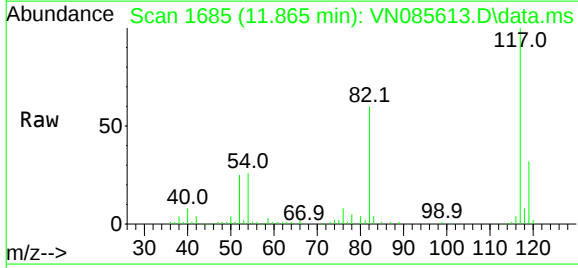

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.006 min

Lab File: VN085613.D

Acq: 31 Jan 2025 19:41

Tgt Ion:152 Resp: 112034

Ion Ratio Lower Upper

152 100

115 62.0 31.1 93.3

150 158.8 0.0 343.6

