


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020119\
Data File : VN053572.D
Acq On : 1 Feb 2019 12:53
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

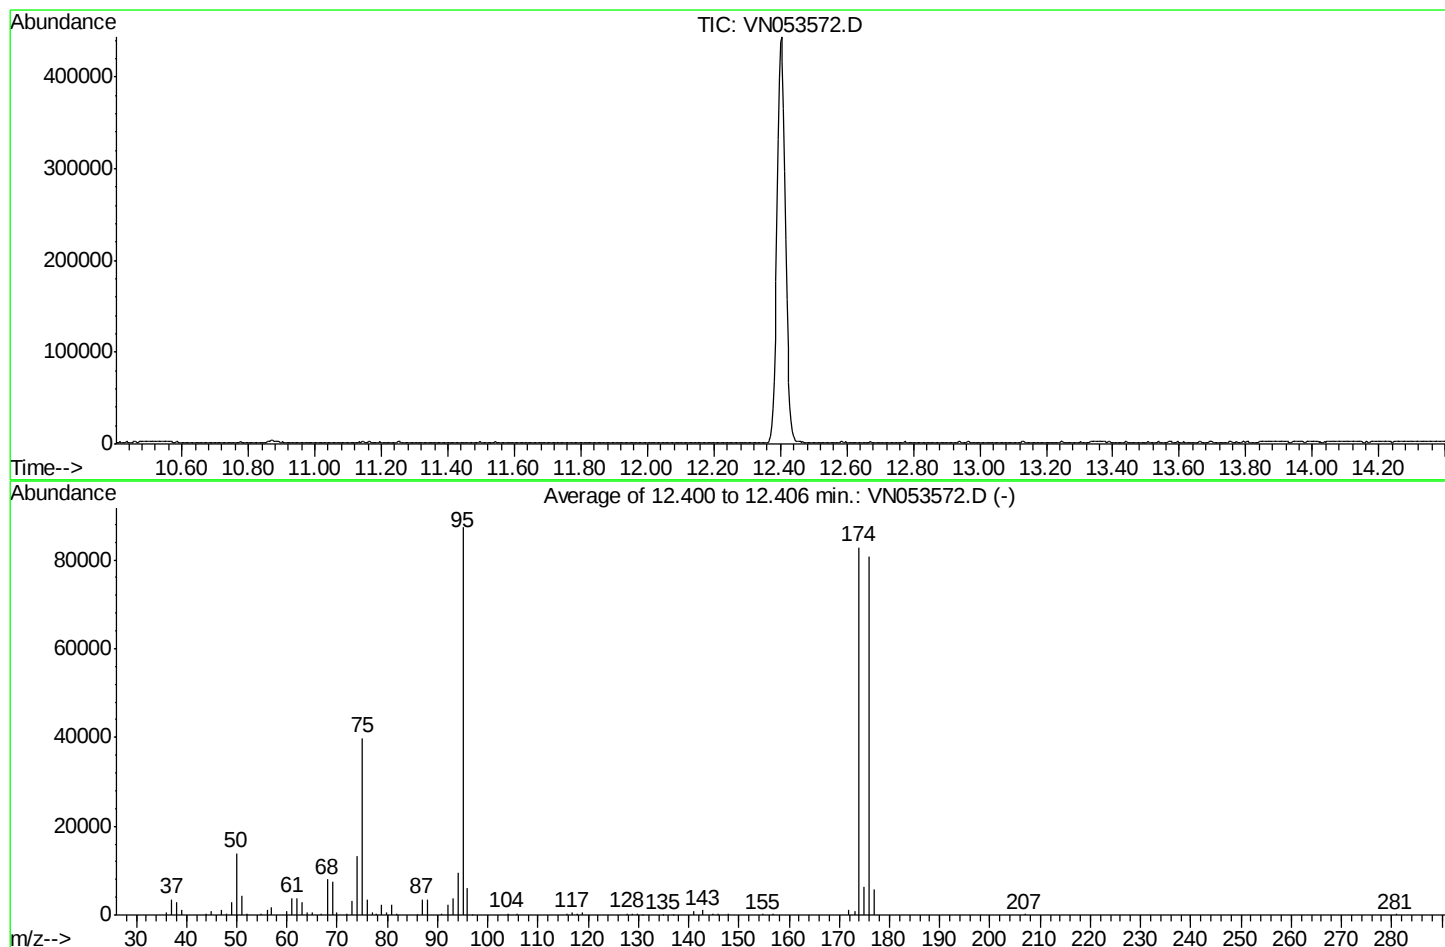

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13872	PASS
75	95	30	60	45.7	39904	PASS
95	95	100	100	100.0	87317	PASS
96	95	5	9	6.9	6058	PASS
173	174	0.00	2	1.1	916	PASS
174	95	50	100	94.8	82792	PASS
175	174	5	9	7.5	6245	PASS
176	174	95	101	97.3	80594	PASS
177	176	5	9	7.0	5677	PASS