


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020122\
Data File : VN070867.D
Acq On : 1 Feb 2022 10:19
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Title : SW846 8260
Last Update : Tue Jan 18 13:32:07 2022

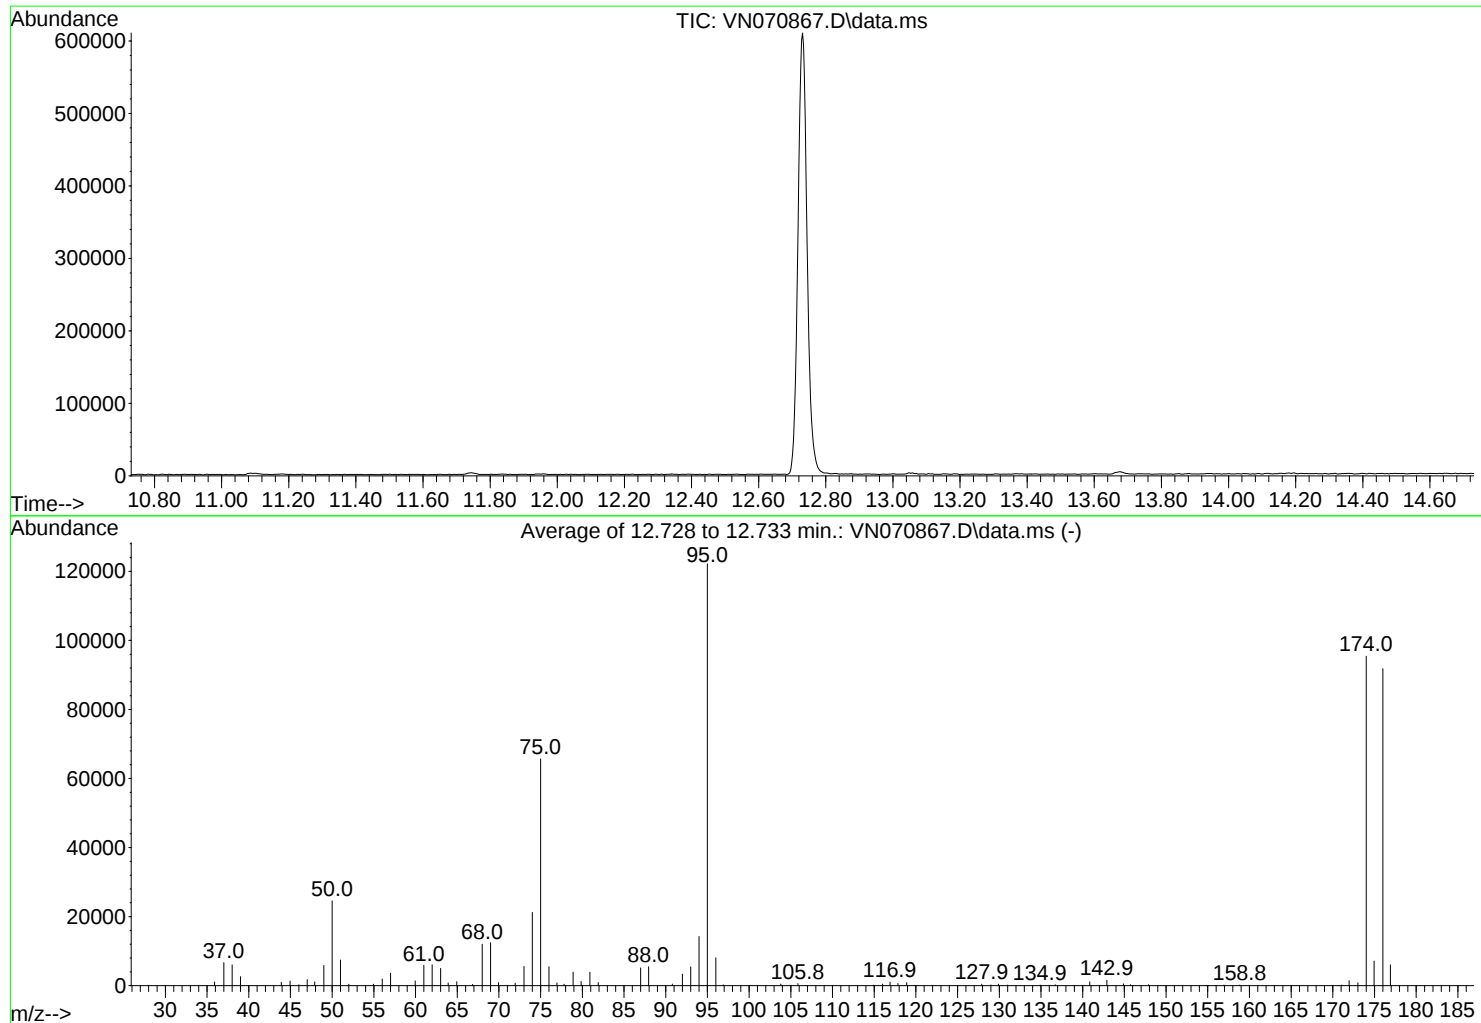

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	24565	PASS
75	95	30	60	53.7	65656	PASS
95	95	100	100	100.0	122179	PASS
96	95	5	9	6.6	8072	PASS
173	174	0.00	2	0.9	817	PASS
174	95	50	100	78.1	95437	PASS
175	174	5	9	7.5	7130	PASS
176	174	95	101	96.2	91824	PASS
177	176	5	9	6.6	6038	PASS