
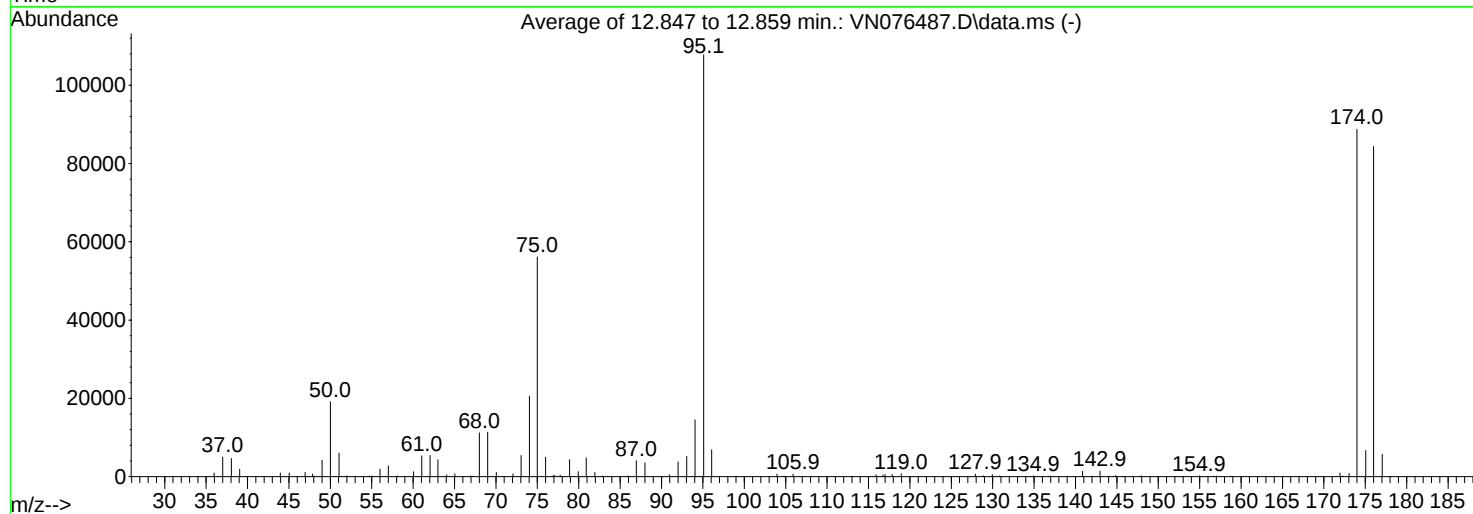


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020123\
Data File : VN076487.D
Acq On : 01 Feb 2023 09:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

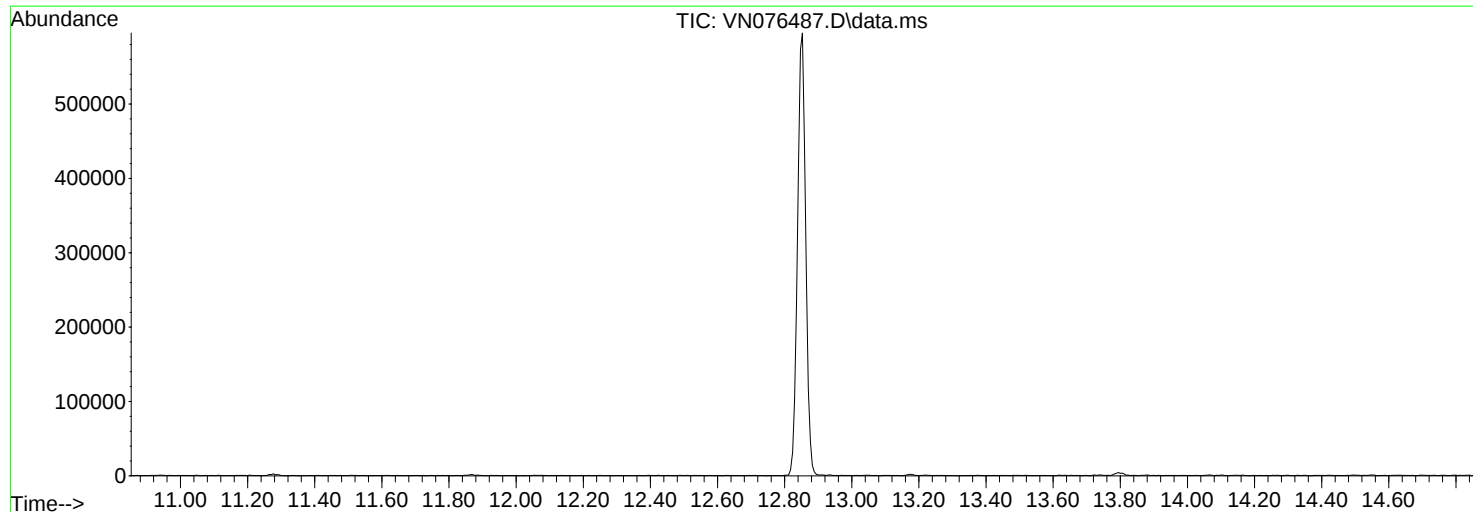

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	19121	PASS
75	95	30	60	52.1	56117	PASS
95	95	100	100	100.0	107765	PASS
96	95	5	9	6.4	6853	PASS
173	174	0.00	2	0.9	810	PASS
174	95	50	100	82.3	88736	PASS
175	174	5	9	7.5	6677	PASS
176	174	95	101	95.0	84317	PASS
177	176	5	9	6.7	5685	PASS

Average of 12.847 to 12.859 min.: VN076487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	943	49.00	4230	62.05	5423	74.05	2055
37.00	4981	50.00	19121	63.00	4319	75.00	5611
38.05	4631	51.05	5992	64.05	447	76.00	494
39.05	1874	52.00	248	65.05	692	76.90	23
39.90	74	54.75	176	66.90	198	77.05	371
43.95	948	55.05	179	67.20	131	77.75	374
45.05	945	56.00	1928	68.00	11188	78.90	4319
46.00	75	57.00	2733	69.00	11378	79.95	1274
46.95	1078	58.10	149	70.05	1057	80.90	4793
47.85	646	60.05	1267	72.05	685	81.95	1064
48.10	182	61.05	5298	73.05	5384	82.90	177

Average of 12.847 to 12.859 min.: VN076487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.95	213	104.85	137	129.95	554	147.90	248
86.95	4093	105.90	661	130.85	149	153.00	56
88.00	3563	112.90	100	134.90	223	154.95	255
90.95	508	114.80	60	136.80	79	156.70	105
92.00	3771	115.90	496	136.95	158	157.05	152
93.05	5168	116.75	440	140.85	1389	158.80	69
94.05	14513	117.00	541	142.00	115	171.95	961
95.10	107765	117.85	557	142.95	1430	172.30	155
96.05	6853	118.95	745	143.95	128	173.05	810
97.00	89	127.90	606	144.85	280	174.00	88736
103.95	602	128.85	246	145.80	129	175.05	6677

Average of 12.847 to 12.859 min.: VN076487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	84317						
177.05	5685						
177.90	71						
178.10	75						

Instrument :

MSVOA_N

ClientSampleId :

BFB