
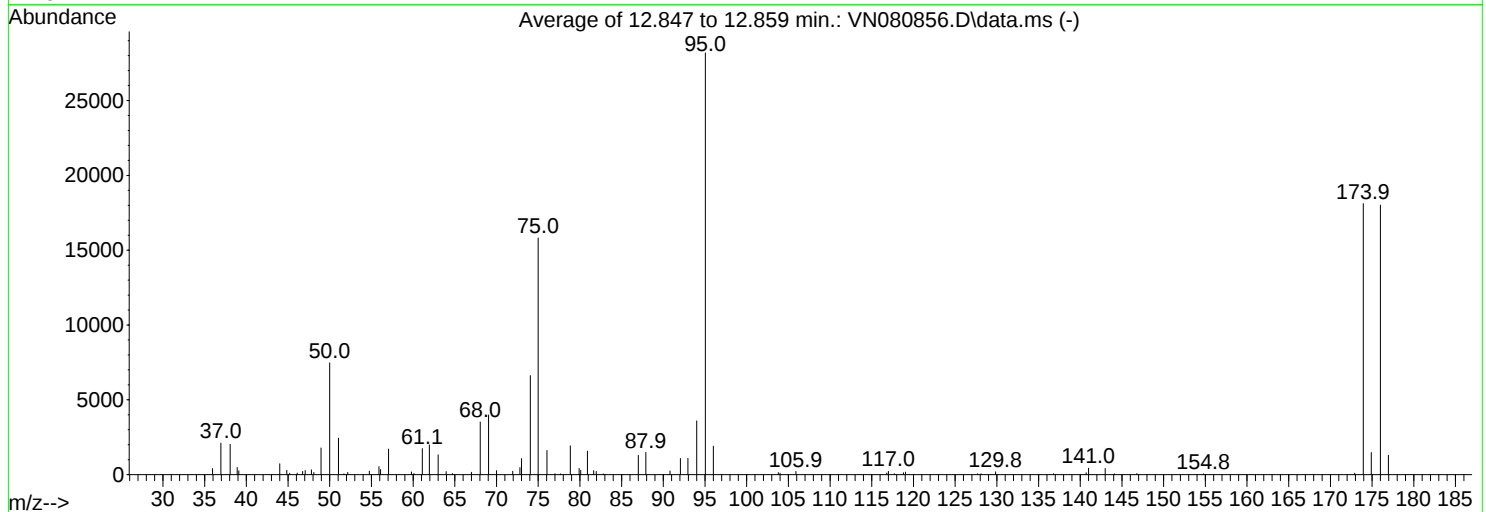


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020124\
Data File : VN080856.D
Acq On : 01 Feb 2024 08:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

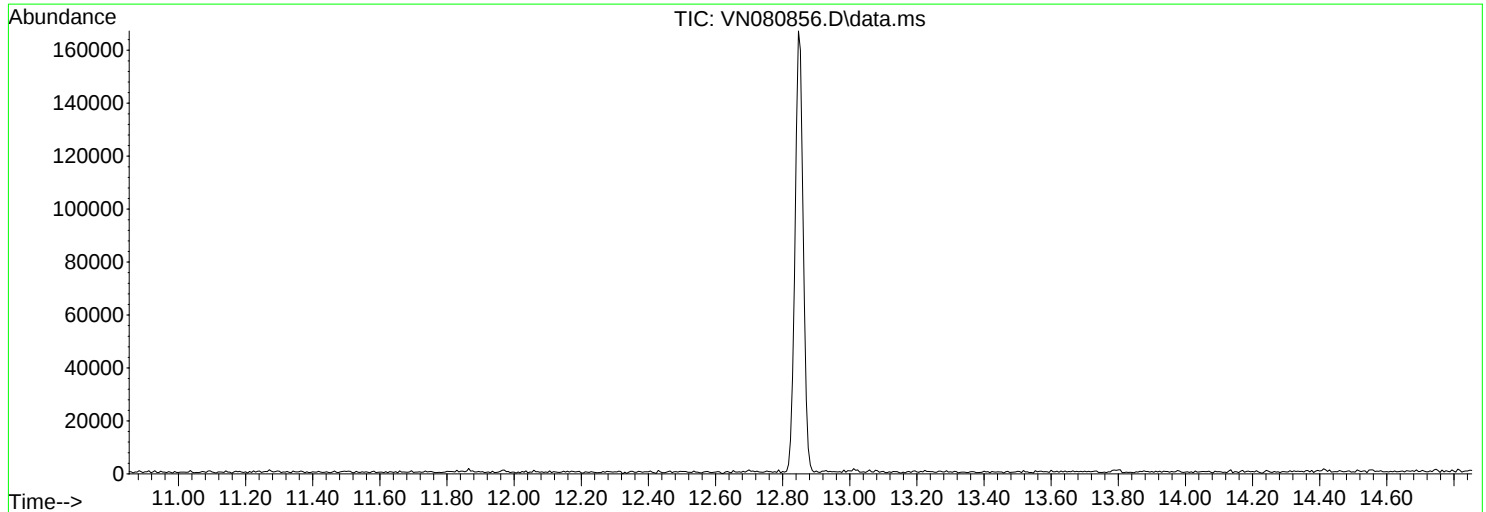

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.5	7475	PASS
75	95	30	60	56.1	15809	PASS
95	95	100	100	100.0	28187	PASS
96	95	5	9	6.8	1907	PASS
173	174	0.00	2	0.5	96	PASS
174	95	50	100	64.3	18116	PASS
175	174	5	9	8.1	1471	PASS
176	174	95	101	99.5	18020	PASS
177	176	5	9	7.2	1290	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	411	47.80	317	59.80	186	71.95	22
36.95	2111	48.10	152	60.10	73	72.80	46
38.05	2018	48.95	1789	61.10	1741	73.00	106
38.90	477	50.00	7475	61.95	1988	74.05	662
39.10	262	51.05	2439	63.00	1330	75.00	15809
44.00	726	51.70	57	63.95	203	76.05	1610
44.85	292	52.15	155	64.70	71	77.00	67
45.20	101	54.75	233	67.00	158	77.70	59
46.10	103	55.90	531	68.05	3518	78.85	1926
46.75	219	56.10	340	69.05	3987	79.90	416
47.05	282	57.05	1709	70.00	272	80.10	291

Average of 12.847 to 12.859 min.: VN080856.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	1569	96.00	1907	129.85	190	176.00	18020
81.65	267	103.80	143	136.80	61	176.95	1290
81.95	209	104.00	95	140.70	127		
82.80	58	105.90	211	141.00	429		
87.00	1293	116.80	109	143.00	415		
87.90	1482	117.00	216	144.10	55		
90.80	250	117.70	60	146.80	74		
92.05	1075	118.80	127	154.80	51		
92.95	1087	119.05	175	172.90	96		
94.00	3595	127.70	67	173.95	18116		
95.05	28187	128.10	64	174.90	1471		

Instrument :

MSVOA_N

ClientSampleId :

BFB