
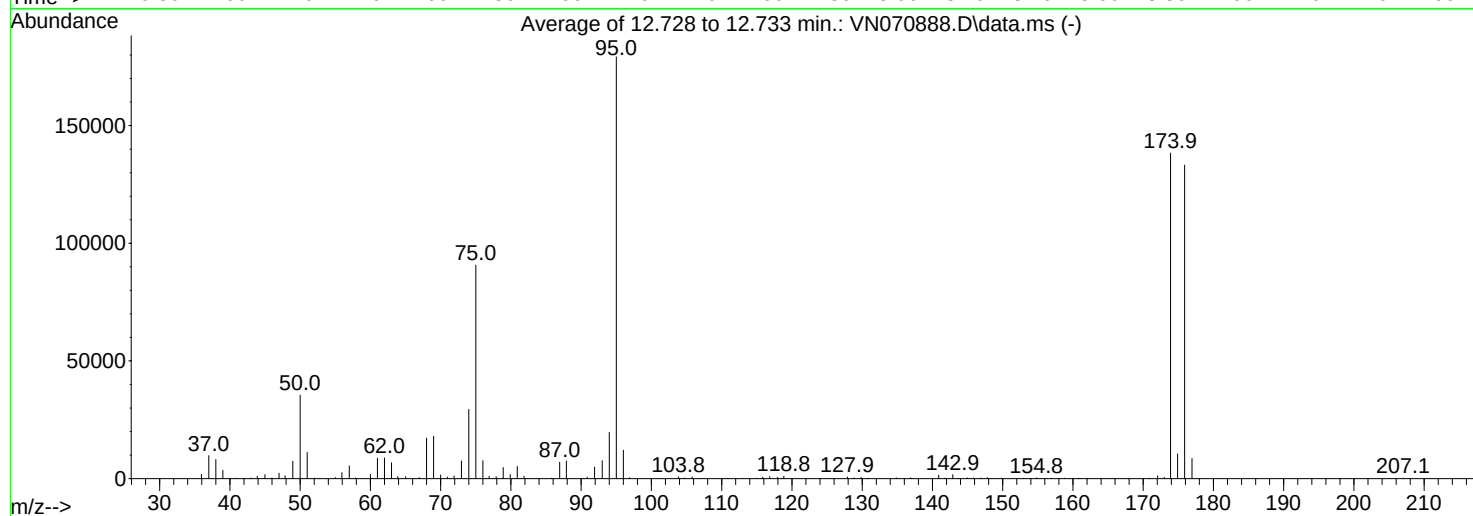


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020222\
Data File : VN070888.D
Acq On : 2 Feb 2022 12:00
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020222W.M
Title : SW846 8260
Last Update : Wed Feb 02 15:30:39 2022

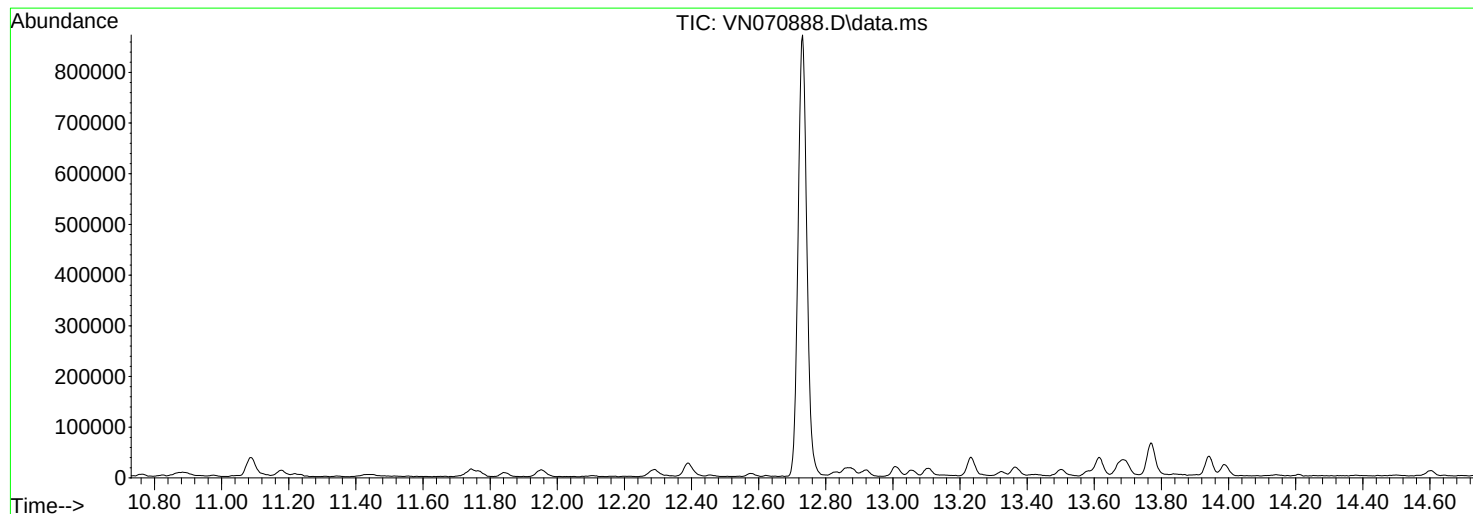

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	35469	PASS
75	95	30	60	50.6	90704	PASS
95	95	100	100	100.0	179200	PASS
96	95	5	9	6.8	12120	PASS
173	174	0.00	2	0.4	515	PASS
174	95	50	100	77.2	138368	PASS
175	174	5	9	7.6	10447	PASS
176	174	95	101	96.3	133269	PASS
177	176	5	9	6.4	8590	PASS