
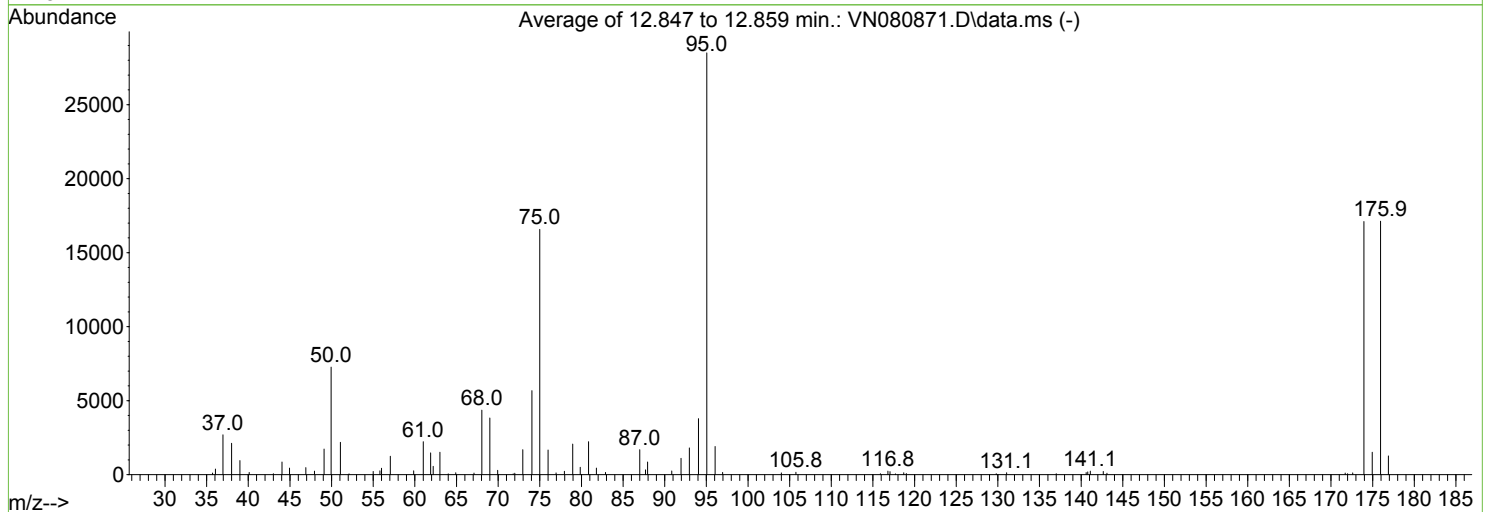


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020224\
Data File : VN080871.D
Acq On : 02 Feb 2024 13:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

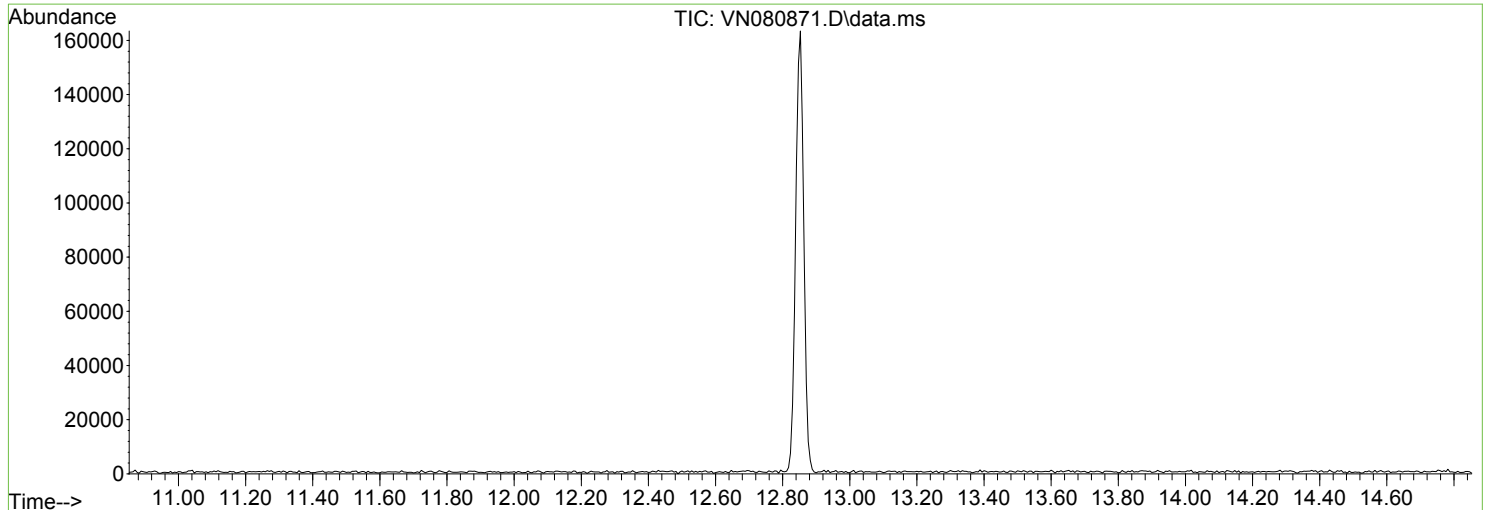

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.5	7269	PASS
75	95	30	60	58.2	16577	PASS
95	95	100	100	100.0	28504	PASS
96	95	5	9	6.7	1904	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	60.0	17104	PASS
175	174	5	9	8.8	1509	PASS
176	174	95	101	100.1	17127	PASS
177	176	5	9	7.4	1266	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	107	49.10	1732	62.20	565	74.05	567
36.05	375	49.95	7269	63.00	1509	75.00	1657
36.95	2695	51.05	2186	64.00	55	76.00	166
38.00	2118	52.10	59	64.90	134	76.95	11
39.00	957	55.00	212	67.10	107	77.95	227
40.10	150	55.80	259	68.05	4360	78.95	2063
43.00	68	56.00	428	69.00	3830	79.85	502
44.05	855	57.05	1246	69.95	292	80.85	2225
44.95	443	59.85	265	71.80	58	81.80	446
46.90	471	61.00	2232	72.00	93	82.90	154
47.95	239	61.90	1466	72.95	1690	87.00	1683

Average of 12.847 to 12.859 min.: VN080871.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.70	322	115.90	66	141.10	239		
87.95	850	116.80	236	142.65	215		
90.85	248	117.05	209	143.10	94		
91.95	1098	117.70	59	171.70	112		
92.95	1804	118.70	125	172.00	62		
94.05	3780	119.00	71	172.60	115		
95.05	28504	129.80	63	173.95	17104		
96.05	1904	131.05	132	174.95	1509		
96.95	151	137.00	60	175.95	17127		
104.00	114	140.60	143	176.90	1266		
105.75	158	140.80	185				

Instrument :

MSVOA_N

ClientSampleId :

BFB