


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020321\
 Data File : VN065692.D
 Acq On : 3 Feb 2021 8:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Feb 03 14:50:04 2021

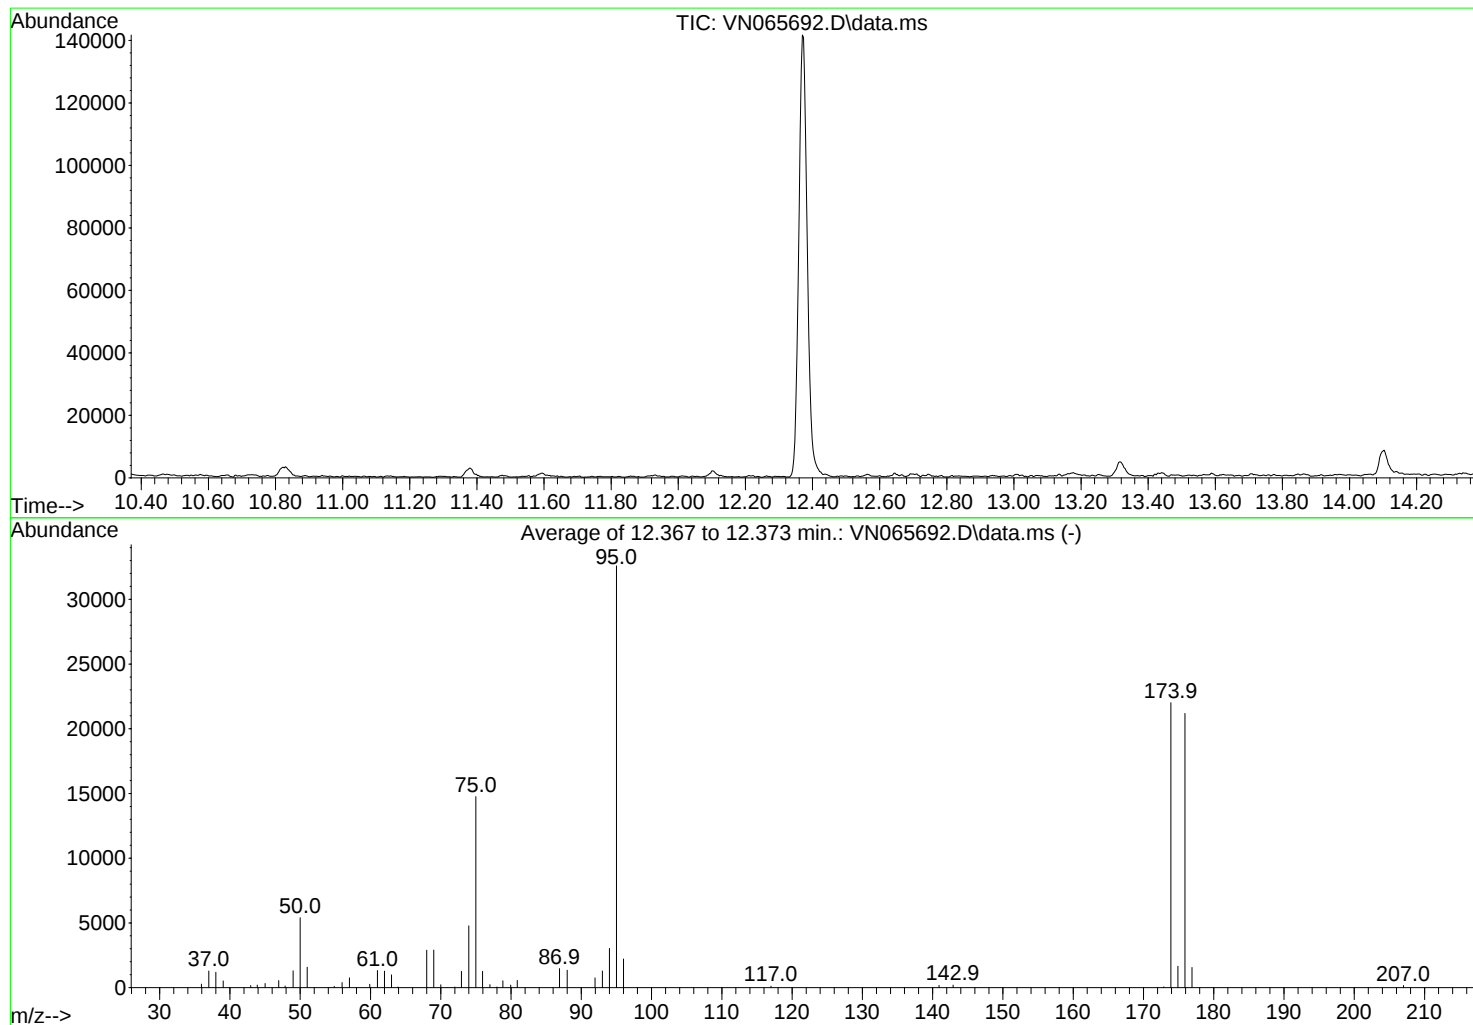

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5400	PASS
75	95	30	60	45.3	14759	PASS
95	95	100	100	100.0	32589	PASS
96	95	5	9	6.8	2216	PASS
173	174	0.00	2	0.3	61	PASS
174	95	50	100	67.6	22019	PASS
175	174	5	9	7.5	1655	PASS
176	174	95	101	96.2	21184	PASS
177	176	5	9	7.3	1552	PASS