

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020322\
 Data File : VN070930.D
 Acq On : 3 Feb 2022 15:17
 Operator : JC/MD
 Sample : N1381-05 10X
 Misc : 6.56g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 04 04:43:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020222W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 02 15:30:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	752182	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1183544	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1216181	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	589970	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	508568	49.950	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.900%		
35) Dibromofluoromethane	8.021	113	352422	49.706	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.420%		
50) Toluene-d8	10.443	98	1504223	51.672	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	103.340%		
62) 4-Bromofluorobenzene	12.731	95	617353	58.855	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	117.720%		
Target Compounds						
					Qvalue	
5) Bromomethane	2.834	94	1370	0.304	ug/l	87
13) Acrolein	4.038	56	575	0.244	ug/l #	82
16) Acetone	4.296	43	4581	0.752	ug/l #	88
18) Methyl Acetate	4.870	43	4801	Below Cal	#	65
31) Cyclohexane	8.083	56	21256	1.229	ug/l #	39
36) 1,1-Dichloropropene	8.083	75	61754	5.361	ug/l #	49
38) Carbon Tetrachloride	8.086	117	75975	7.223	ug/l #	16
39) Methylcyclohexane	9.459	83	41660	2.942	ug/l	91
48) Methyl methacrylate	9.636	41	3140	0.273	ug/l #	74
51) 4-Methyl-2-Pentanone	10.247	43	9179	0.584	ug/l #	37
55) 1,1,2-Trichloroethane	10.880	97	20176	2.369	ug/l #	23
56) Ethyl methacrylate	10.781	69	10514	0.709	ug/l #	1
58) 2-Chloroethyl Vinyl ether	10.202	63	82	19.668	ug/l #	45
59) 2-Hexanone	11.052	43	47599	4.150	ug/l #	29
73) Isopropylbenzene	12.578	105	128219	2.491	ug/l	100
74) N-amyl acetate	12.369	43	92518	4.013	ug/l #	57
75) 1,1,2,2-Tetrachloroethane	12.800	83	7105	0.398	ug/l #	79
76) 1,2,3-Trichloropropane	12.731	75	332641	23.425	ug/l #	1
78) n-propylbenzene	12.918	91	300840	5.125	ug/l	96
79) 2-Chlorotoluene	12.918	91	300840	8.242	ug/l #	38
80) 1,3,5-Trimethylbenzene	13.222	105	8452	0.203	ug/l	74
81) trans-1,4-Dichloro-2-b...	12.731	75	332641	63.496	ug/l #	5
82) 4-Chlorotoluene	12.918	91	300840	8.551	ug/l #	38
83) tert-Butylbenzene	13.321	119	15678	0.431	ug/l	87
84) 1,2,4-Trimethylbenzene	13.222	105	8452	0.207	ug/l	78
85) sec-Butylbenzene	13.500	105	236546	4.646	ug/l	89
86) p-Isopropyltoluene	13.771	119	34938	0.870	ug/l	91
89) n-Butylbenzene	13.943	91	134200	3.793	ug/l	93
90) Hexachloroethane	14.217	117	32057	4.505	ug/l #	6
95) Naphthalene	15.504	128	7029	3.755	ug/l #	80
96) 1,2,3-Trichlorobenzene	15.697	180	502	1.748	ug/l #	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020322\
Data File : VN070930.D
Acq On : 3 Feb 2022 15:17
Operator : JC/MD
Sample : N1381-05 10X
Misc : 6.56g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 04 04:43:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020222W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 02 15:30:39 2022
Response via : Initial Calibration




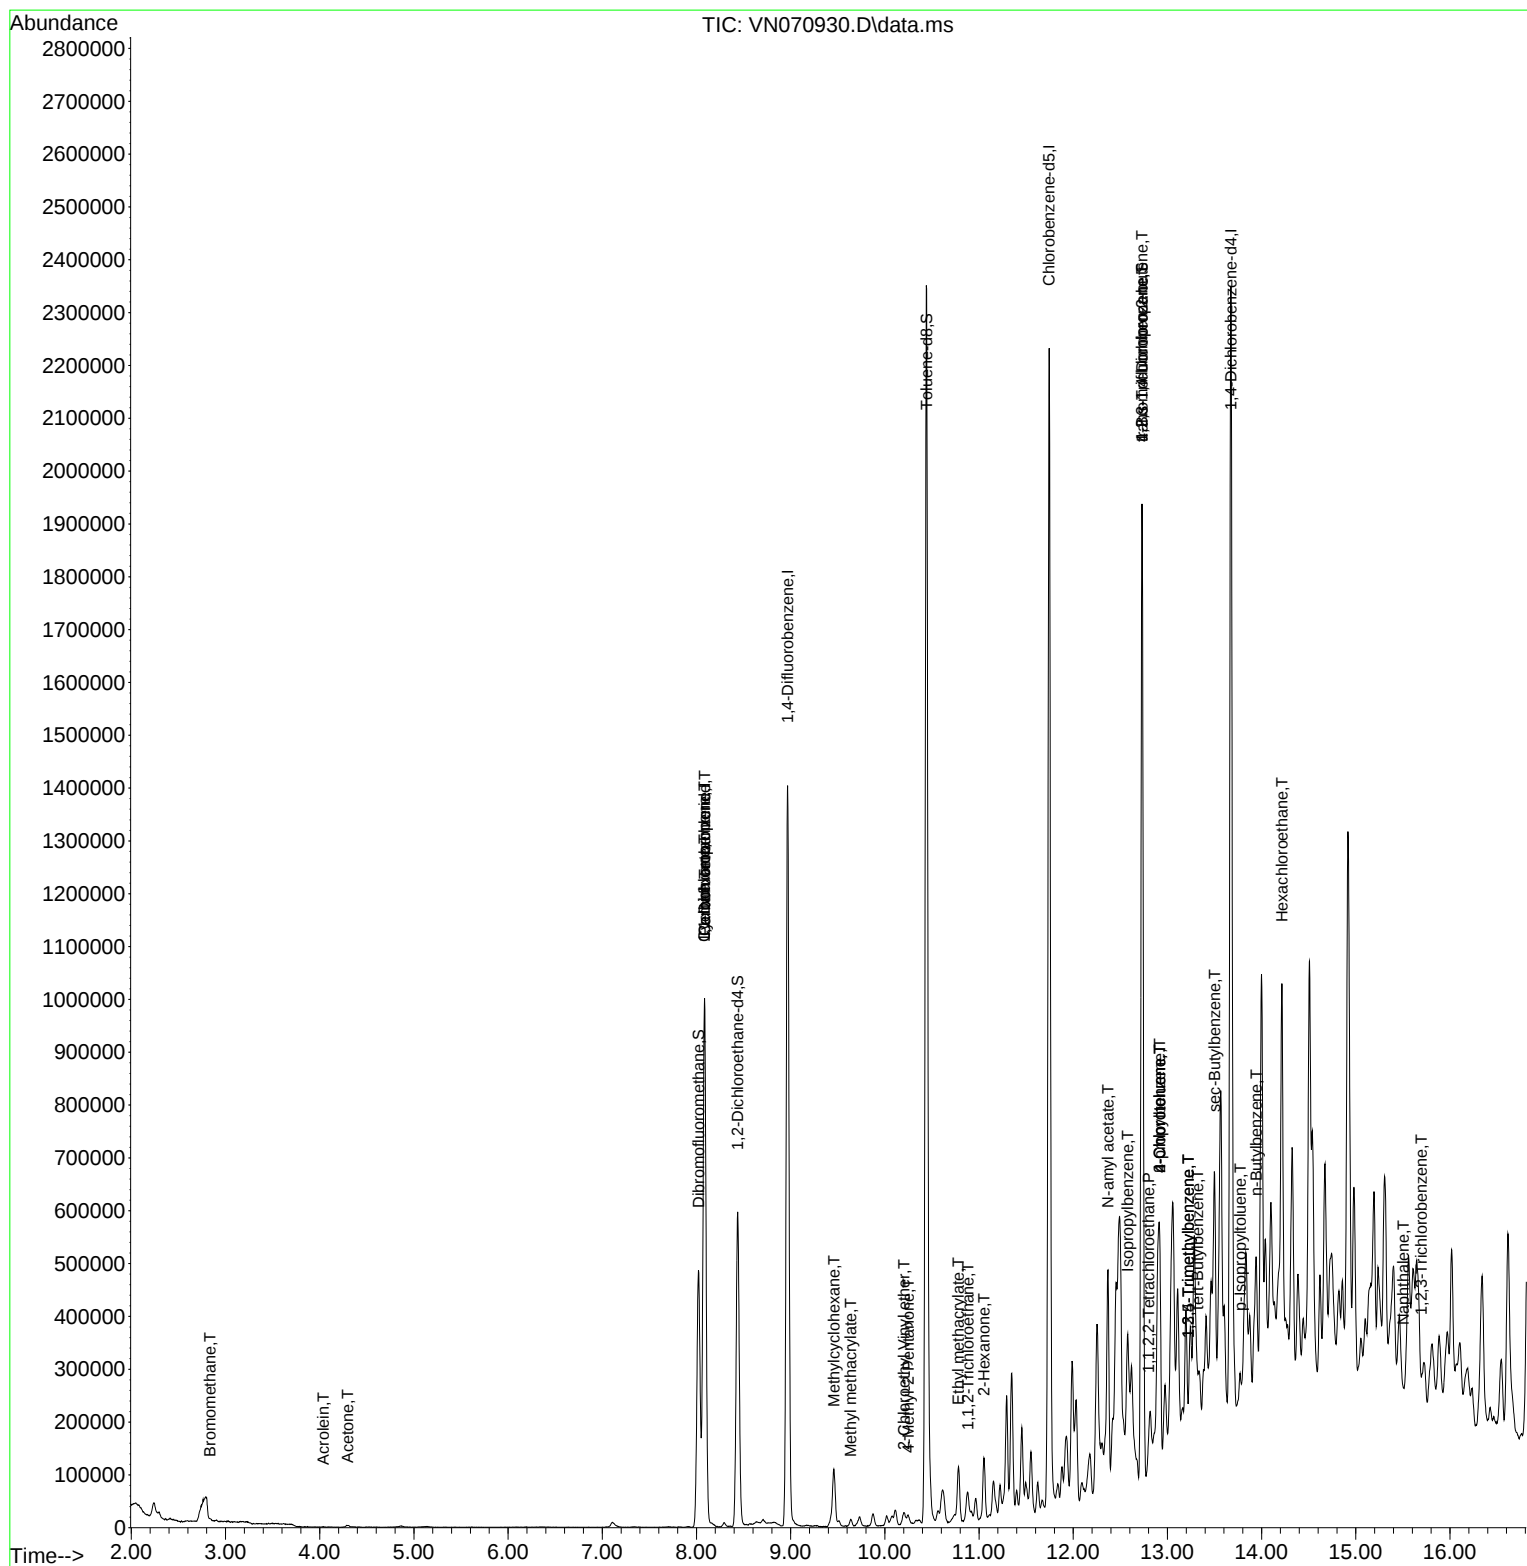




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 752182
Ion Ratio Lower Upper
168 100
99 57.4 41.3 61.9

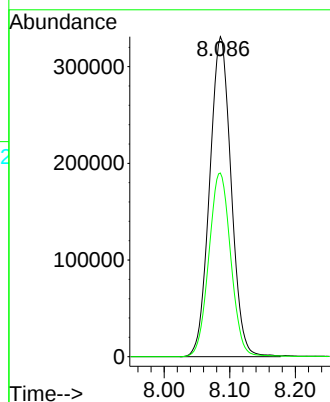

#5
Bromomethane
Concen: 0.304 ug/l
RT: 2.834 min Scan# 315
Delta R.T. 0.002 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 94 Resp: 1370
Ion Ratio Lower Upper
94 100
96 104.4 73.8 110.8



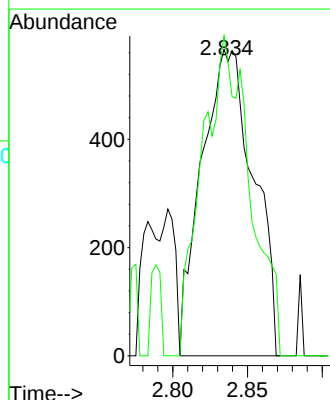
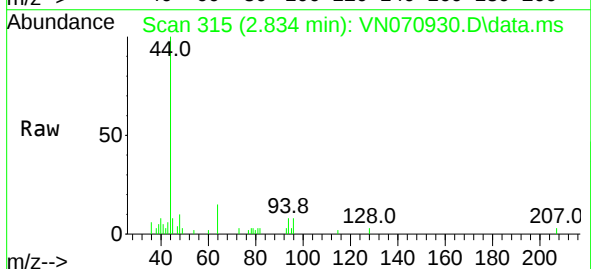




#13
Acrolein
Concen: 0.244 ug/l
RT: 4.038 min Scan# 764
Delta R.T. -0.001 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 575
Ion Ratio Lower Upper
56 100
55 56.3 56.6 85.0#



#16
Acetone
Concen: 0.752 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.011 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17


Tgt Ion: 43 Resp: 4581
Ion Ratio Lower Upper
43 100
58 22.5 23.1 34.7#

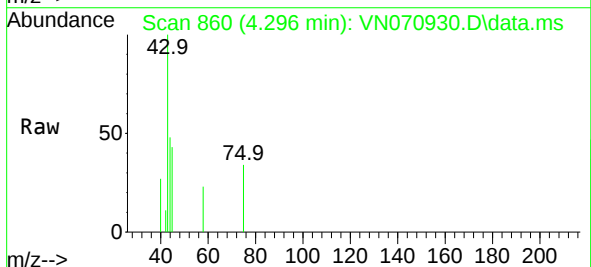






#31
Cyclohexane
Concen: 1.229 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.011 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 21256
Ion Ratio Lower Upper
56 100
69 140.8 27.1 40.7#
84 105.9 73.4 110.0

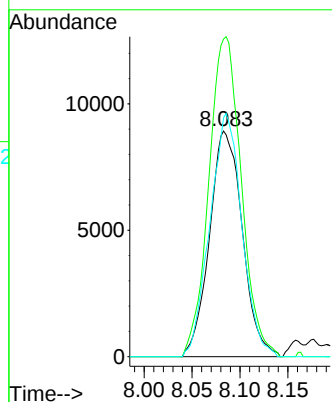

#33
1,2-Dichloroethane-d4
Concen: 49.950 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 65 Resp: 508568
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0

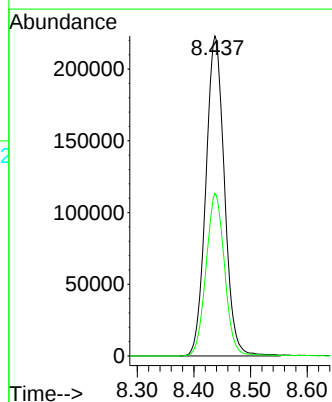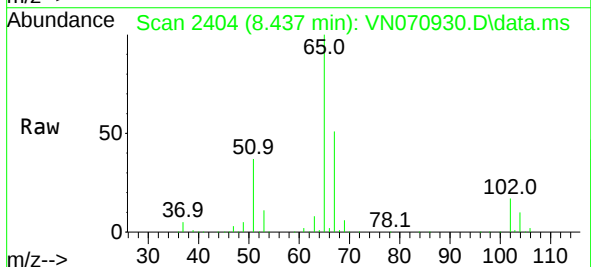



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2

Delta R.T. 0.002 min

Lab File: VN070930.D

Acq: 3 Feb 2022 15:17

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 1183544

Ion Ratio Lower Upper

114 100

63 22.8 0.0 37.8

88 15.9 0.0 27.4

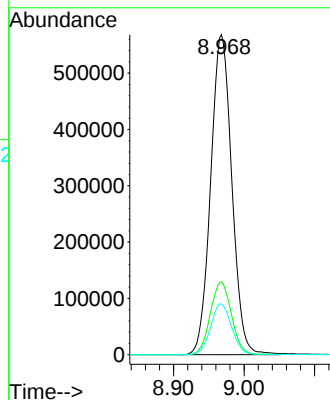

#35

Dibromofluoromethane

Concen: 49.706 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. 0.000 min

Lab File: VN070930.D

Acq: 3 Feb 2022 15:17




Tgt Ion:113 Resp: 352422


Ion Ratio Lower Upper

113 100

111 102.2 82.2 123.2


192 19.4 16.9 25.3

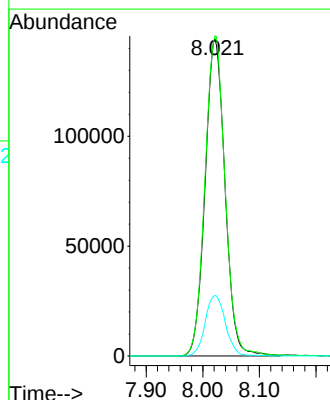






#36
1,1-Dichloropropene
Concen: 5.361 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.137 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 75 Resp: 61754
Ion Ratio Lower Upper
75 100
110 8.6 18.4 55.2#
77 0.0 24.4 36.6#

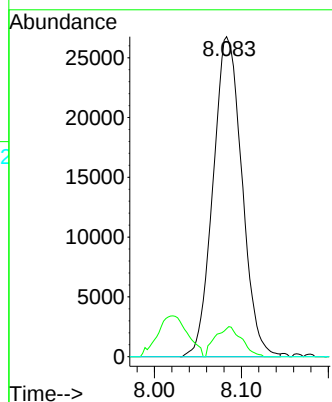


#38
Carbon Tetrachloride
Concen: 7.223 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17



Tgt Ion: 117 Resp: 75975
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 24.2 36.2#









#39
Methylcyclohexane
Concen: 2.942 ug/l
RT: 9.459 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 41660
Ion Ratio Lower Upper
83 100
55 82.4 58.1 87.1
98 44.0 38.4 57.6

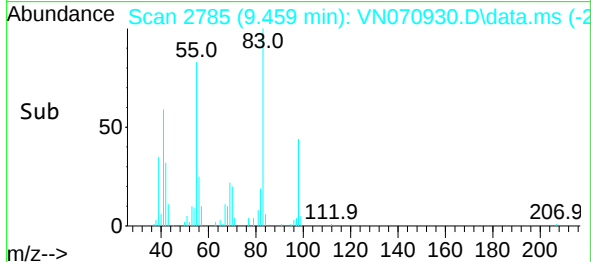

#48
Methyl methacrylate
Concen: 0.273 ug/l
RT: 9.636 min Scan# 2851
Delta R.T. 0.078 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 41 Resp: 3140
Ion Ratio Lower Upper
41 100
69 133.3 72.4 108.6#
39 72.2 58.4 87.6

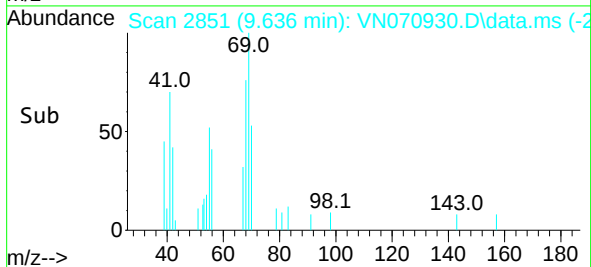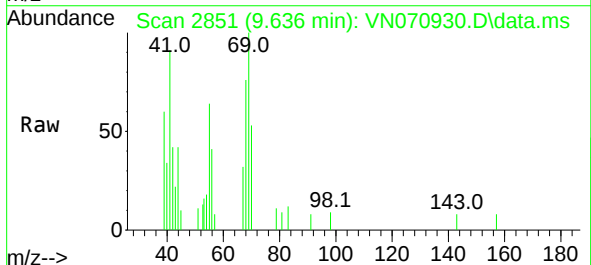

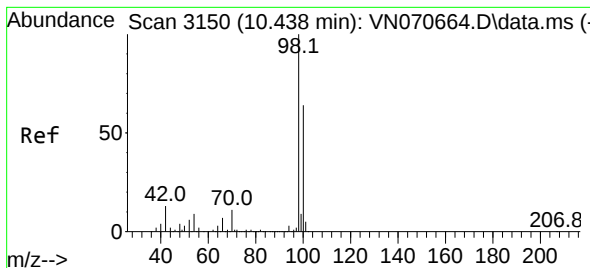

#50

Toluene-d8

Concen: 51.672 ug/l

RT: 10.443 min Scan# 3150

Delta R.T. 0.002 min

Lab File: VN070930.D

Acq: 3 Feb 2022 15:17

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 98 Resp: 1504223

Ion Ratio Lower Upper

98 100

100 63.8 50.4 75.6

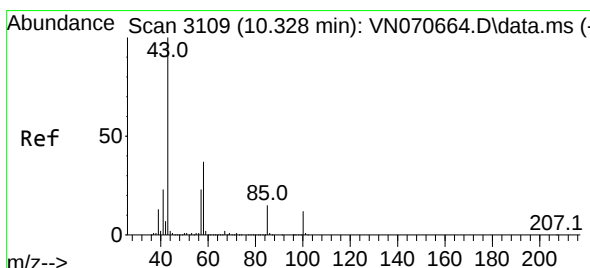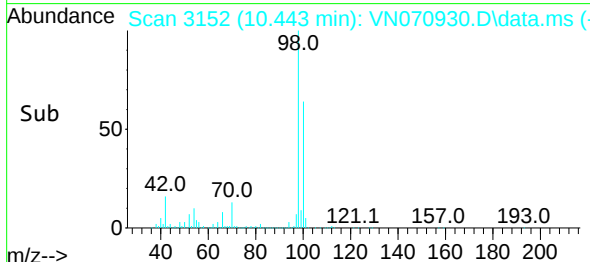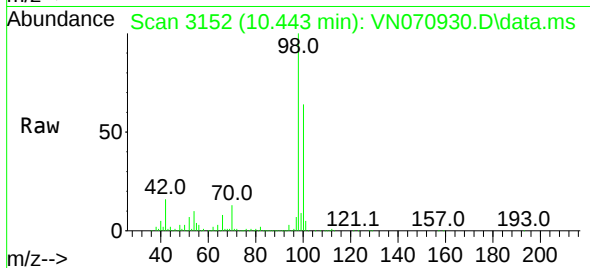

#51

4-Methyl-2-Pentanone

Concen: 0.584 ug/l

RT: 10.247 min Scan# 3079

Delta R.T. -0.084 min

Lab File: VN070930.D




Acq: 3 Feb 2022 15:17


Tgt Ion: 43 Resp: 9179

Ion Ratio Lower Upper

43 100

58 0.0 30.4 45.6#


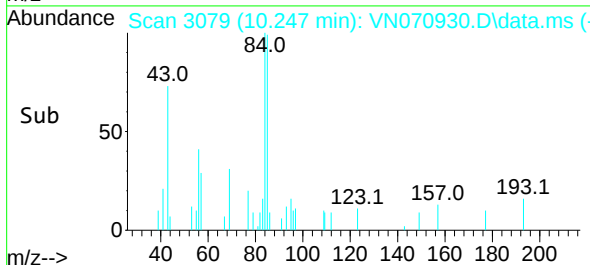

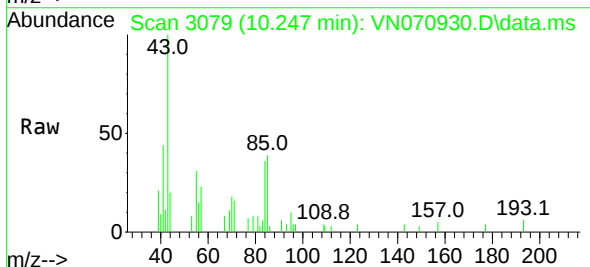




#55
1,1,2-Trichloroethane
Concen: 2.369 ug/l
RT: 10.880 min Scan# 31
Delta R.T. -0.016 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 97 Resp: 20176
Ion Ratio Lower Upper
97 100
83 10.1 67.8 101.6#
85 7.4 45.4 68.2#
99 0.0 49.4 74.0#

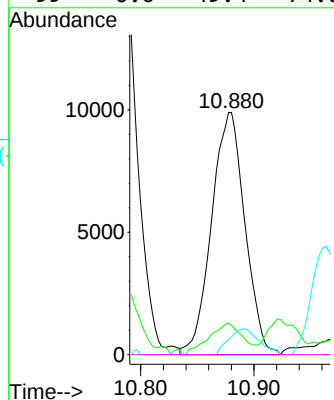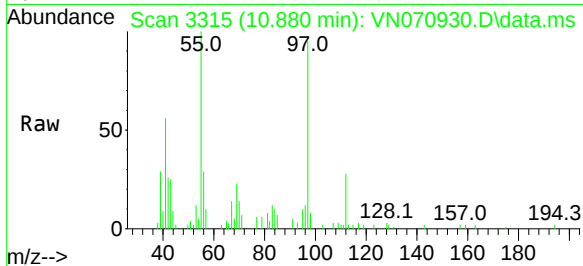

#56
Ethyl methacrylate
Concen: 0.709 ug/l
RT: 10.781 min Scan# 3278
Delta R.T. 0.021 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 69 Resp: 10514
Ion Ratio Lower Upper
69 100
41 174.3 51.4 77.0#
39 91.3 34.6 52.0#


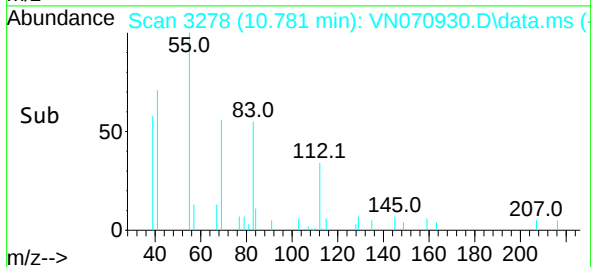
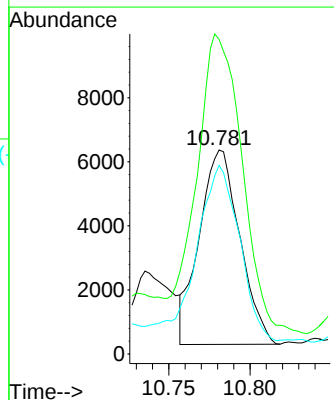
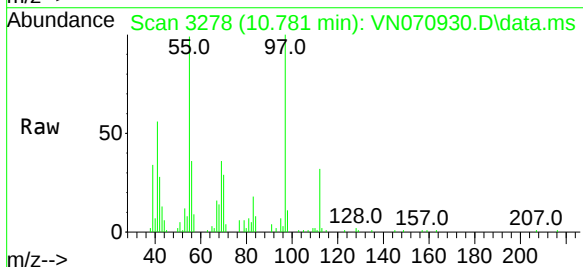




#58
2-Chloroethyl Vinyl ether
Concen: 19.668 ug/l
RT: 10.202 min Scan# 3001
Delta R.T. 0.161 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 82
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

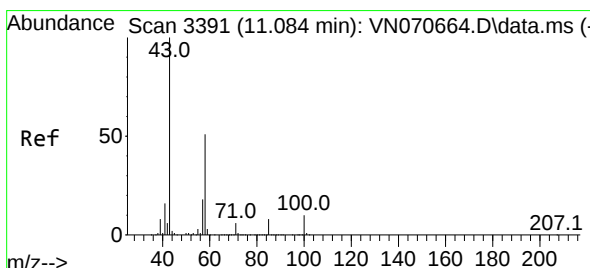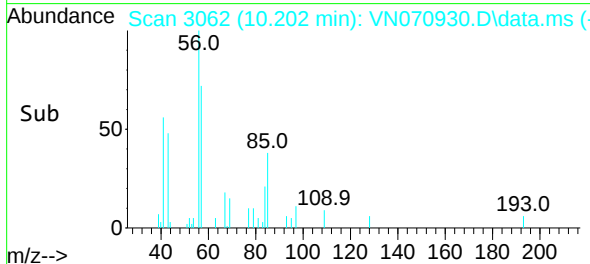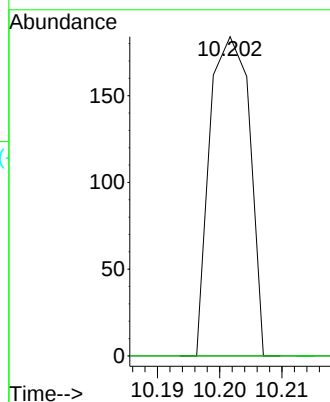

#59
2-Hexanone
Concen: 4.150 ug/l
RT: 11.052 min Scan# 3379
Delta R.T. -0.032 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 43 Resp: 47599
Ion Ratio Lower Upper
43 100
58 3.1 26.9 80.7#


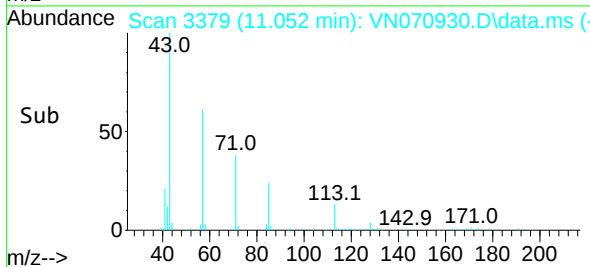
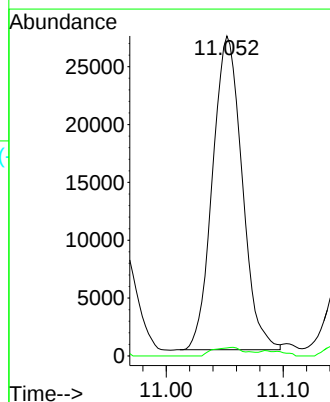
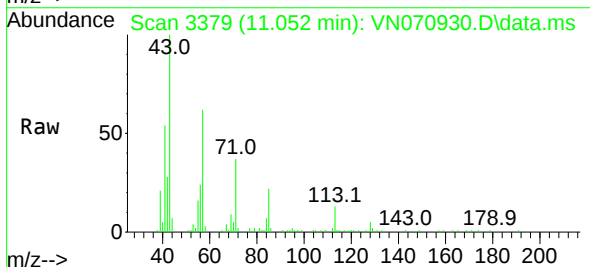




#62
4-Bromofluorobenzene
Concen: 58.855 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 617353
Ion Ratio Lower Upper
95 100
174 77.0 0.0 187.2
176 74.9 0.0 181.4

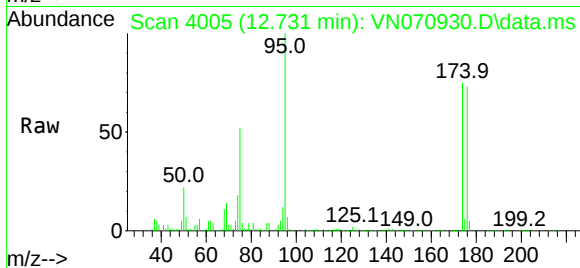

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17


Tgt Ion: 117 Resp: 1216181
Ion Ratio Lower Upper
117 100
82 59.6 42.4 63.6
119 32.5 25.4 38.2

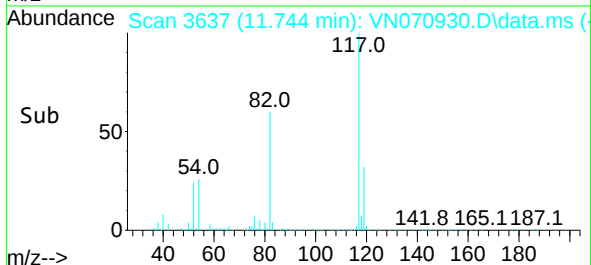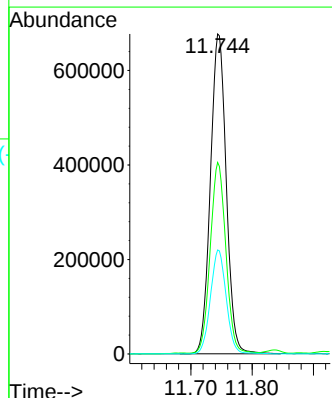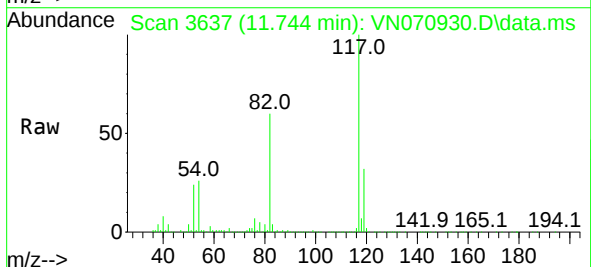






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17


Instrument :
MSVOA_N
ClientSampleId :

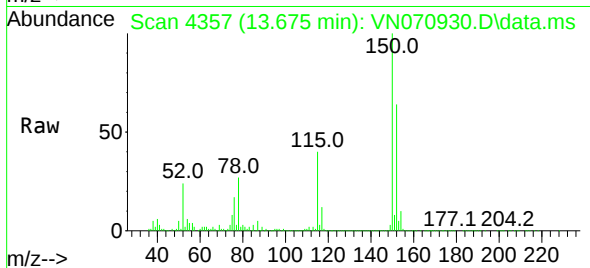



Tgt Ion:152 Resp: 589970
Ion Ratio Lower Upper
152 100
115 60.6 27.5 82.5
150 156.4 0.0 344.4

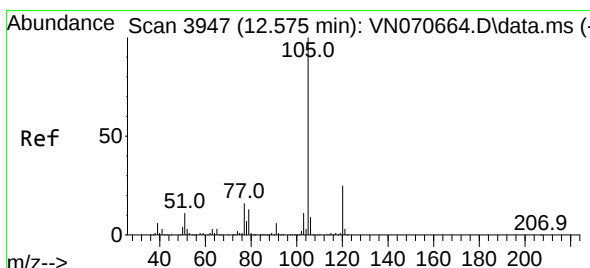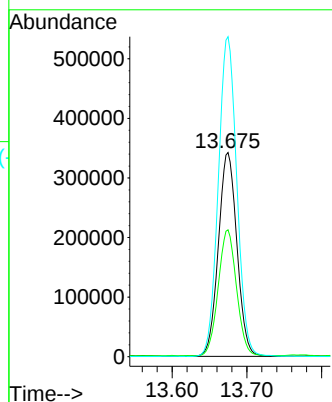


#73
Isopropylbenzene
Concen: 2.491 ug/l
RT: 12.578 min Scan# 3948
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17



Tgt Ion:105 Resp: 128219
Ion Ratio Lower Upper
105 100
120 26.9 13.4 40.1

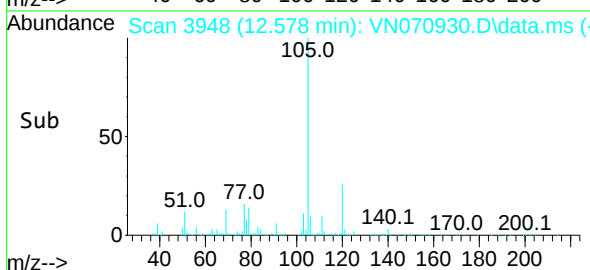







#74
N-amy1 acetate
Concen: 4.013 ug/l
RT: 12.369 min Scan# 31
Delta R.T. -0.019 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion: 43 Resp: 92518




Ion	Ratio	Lower	Upper
43	100		
70	17.8	33.4	50.0#
55	0.0	19.3	28.9#
61	0.0	18.5	27.7#

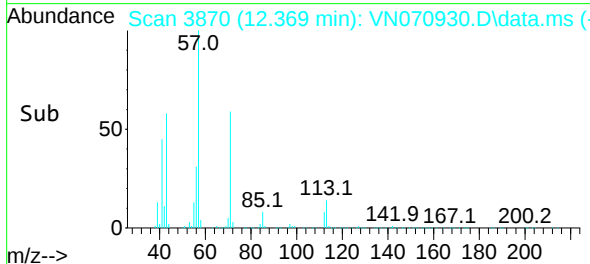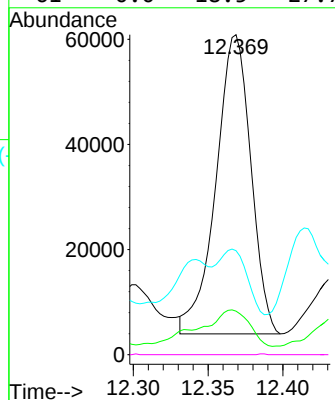


#75
1,1,2,2-Tetrachloroethane
Concen: 0.398 ug/l
RT: 12.800 min Scan# 4031
Delta R.T. -0.025 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 83 Resp: 7105

Ion	Ratio	Lower	Upper
83	100		
131	3.6	5.5	16.5#
85	81.9	32.4	97.2


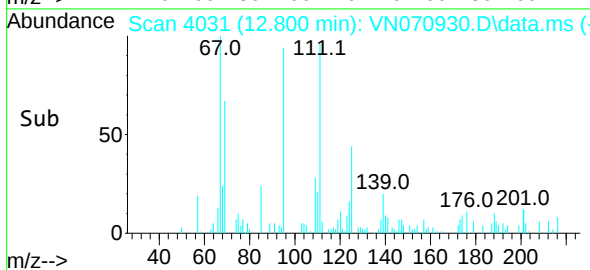
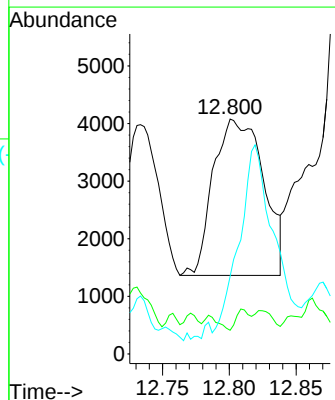
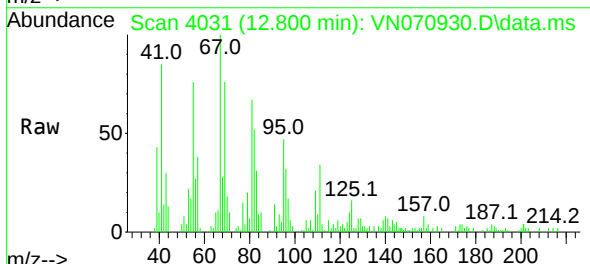




#76
1,2,3-Trichloropropane
Concen: 23.425 ug/l
RT: 12.731 min Scan# 4060
Delta R.T. -0.147 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 332641
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#

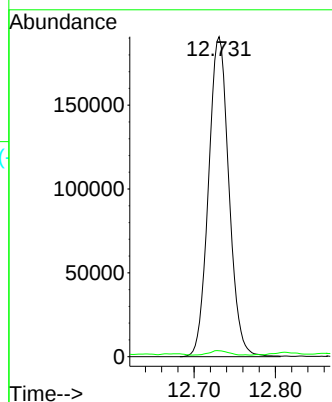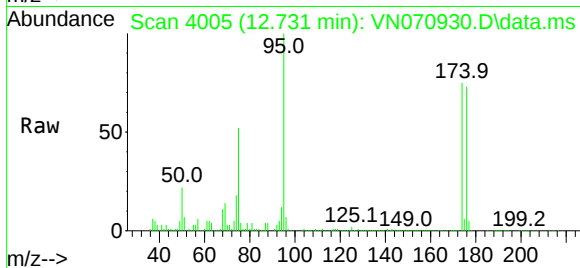

#78
n-propylbenzene
Concen: 5.125 ug/l
RT: 12.918 min Scan# 4075
Delta R.T. -0.001 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 91 Resp: 300840
Ion Ratio Lower Upper
91 100
120 21.9 11.9 35.9

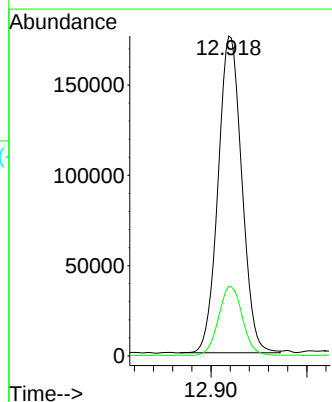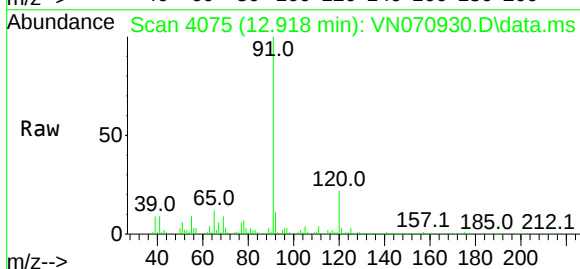



#79

2-Chlorotoluene

Concen: 8.242 ug/l

RT: 12.918 min Scan# 40

Delta R.T. -0.089 min

Lab File: VN070930.D

Acq: 3 Feb 2022 15:17

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 91 Resp: 300840

Ion Ratio Lower Upper

91 100

126 0.0 18.3 54.8#



#80

1,3,5-Trimethylbenzene

Concen: 0.203 ug/l

RT: 13.222 min Scan# 4188

Delta R.T. 0.164 min

Lab File: VN070930.D




Acq: 3 Feb 2022 15:17


Tgt Ion:105 Resp: 8452

Ion Ratio Lower Upper

105 100

120 31.4 24.6 73.6









#81
trans-1,4-Dichloro-2-butene
Concen: 63.496 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 332641
Ion Ratio Lower Upper
75 100
53 0.8 90.5 135.7#
89 0.0 38.2 57.4#

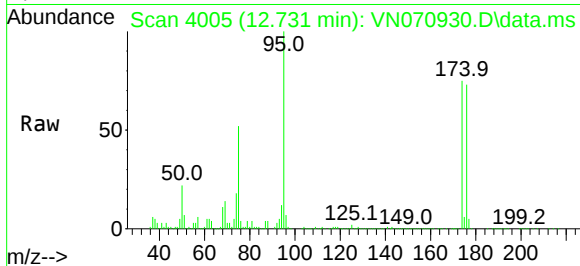

#82
4-Chlorotoluene
Concen: 8.551 ug/l
RT: 12.918 min Scan# 4075
Delta R.T. -0.186 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 91 Resp: 300840
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#



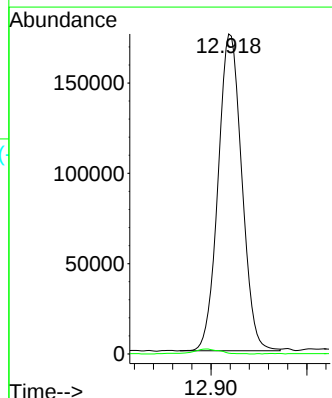
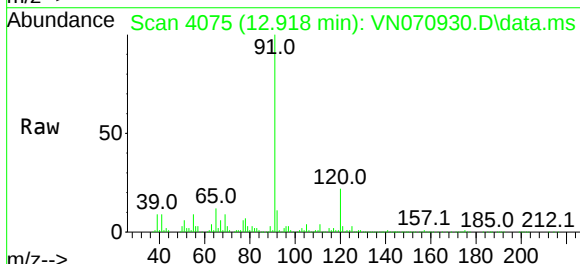




#83
tert-Butylbenzene
Concen: 0.431 ug/l
RT: 13.321 min Scan# 4187
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:119 Resp: 15678
Ion Ratio Lower Upper
119 100
91 76.6 31.5 94.5
134 23.5 12.4 37.4

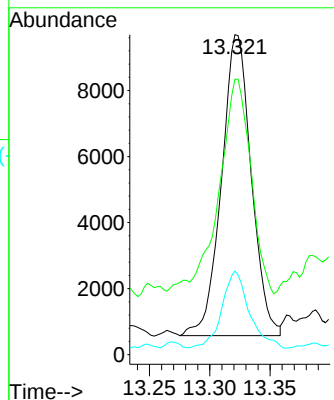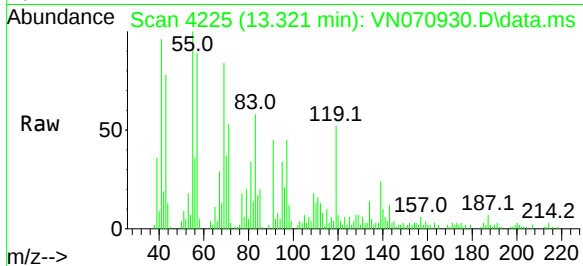

#84
1,2,4-Trimethylbenzene
Concen: 0.207 ug/l
RT: 13.222 min Scan# 4188
Delta R.T. -0.145 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion:105 Resp: 8452
Ion Ratio Lower Upper
105 100
120 31.4 22.8 68.4


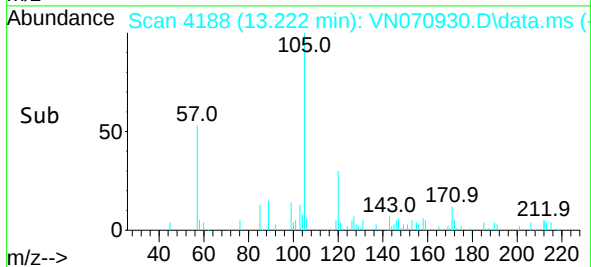
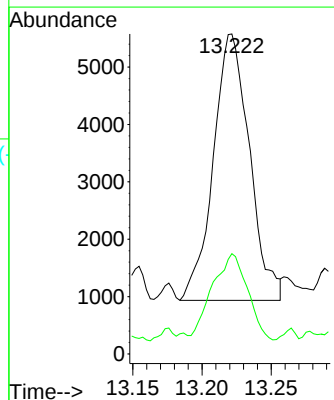
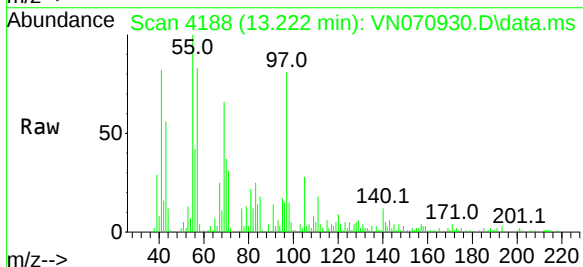




#85
 sec-Butylbenzene
 Concen: 4.646 ug/l
 RT: 13.500 min Scan# 41
 Delta R.T. -0.001 min
 Lab File: VN070930.D
 Acq: 3 Feb 2022 15:17




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 236546
 Ion Ratio Lower Upper
 105 100
 134 25.8 10.4 31.1



#86
 p-Isopropyltoluene
 Concen: 0.870 ug/l
 RT: 13.771 min Scan# 4393
 Delta R.T. 0.158 min
 Lab File: VN070930.D
 Acq: 3 Feb 2022 15:17


Tgt Ion:119 Resp: 34938
 Ion Ratio Lower Upper
 119 100
 134 26.4 13.6 40.7
 91 31.6 11.4 34.1








#89
n-Butylbenzene
Concen: 3.793 ug/l
RT: 13.943 min Scan# 4456
Delta R.T. 0.002 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Instrument :
MSVOA_N
ClientSampleId :



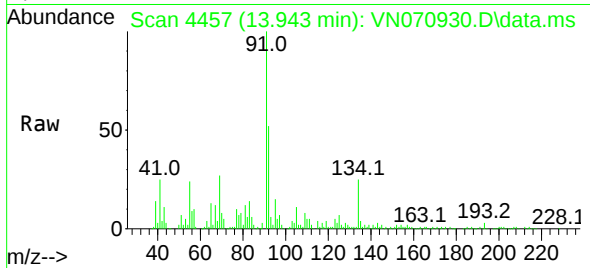



Tgt Ion: 91 Resp: 134200
Ion Ratio Lower Upper
91 100
92 48.3 25.4 76.0
134 34.3 13.6 40.8

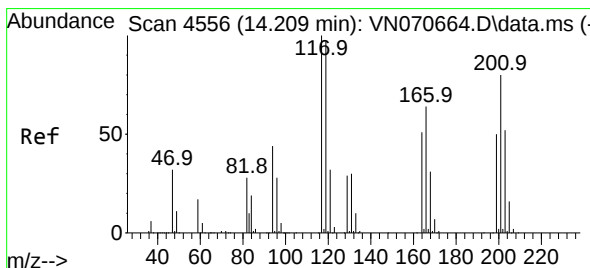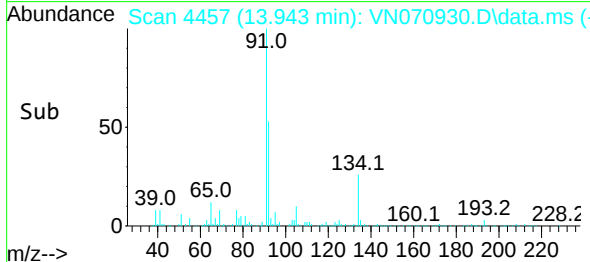

#90
Hexachloroethane
Concen: 4.505 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.008 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion: 117 Resp: 32057
Ion Ratio Lower Upper
117 100
201 0.3 43.9 131.6#


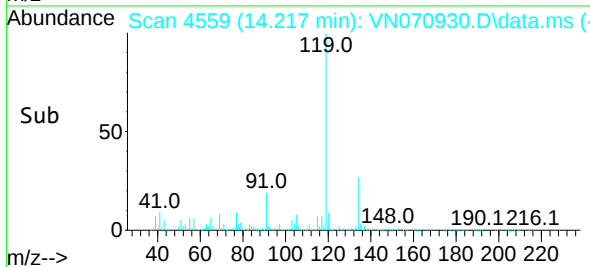

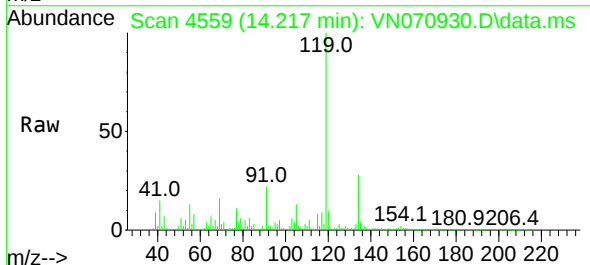




#95
Naphthalene
Concen: 3.755 ug/l
RT: 15.504 min Scan# 5039
Delta R.T. -0.000 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 7029
Ion Ratio Lower Upper
128 100
127 8.3 10.5 15.7#
129 0.0 8.7 13.1#

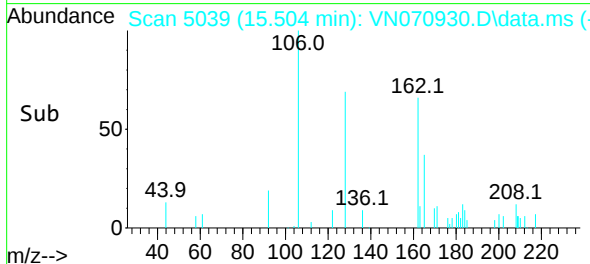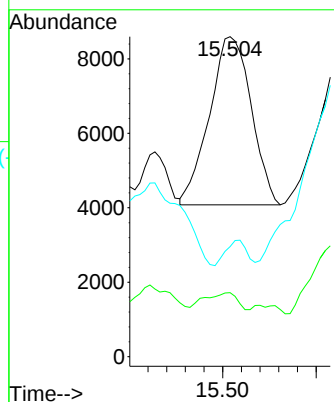

#96
1,2,3-Trichlorobenzene
Concen: 1.748 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.003 min
Lab File: VN070930.D
Acq: 3 Feb 2022 15:17

Tgt Ion:180 Resp: 502
Ion Ratio Lower Upper
180 100
182 168.1 47.4 142.2#
145 0.0 15.0 45.1#

