


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020322\
 Data File : VN070920.D
 Acq On : 3 Feb 2022 9:29
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020222W.M
 Title : SW846 8260
 Last Update : Wed Feb 02 15:30:39 2022

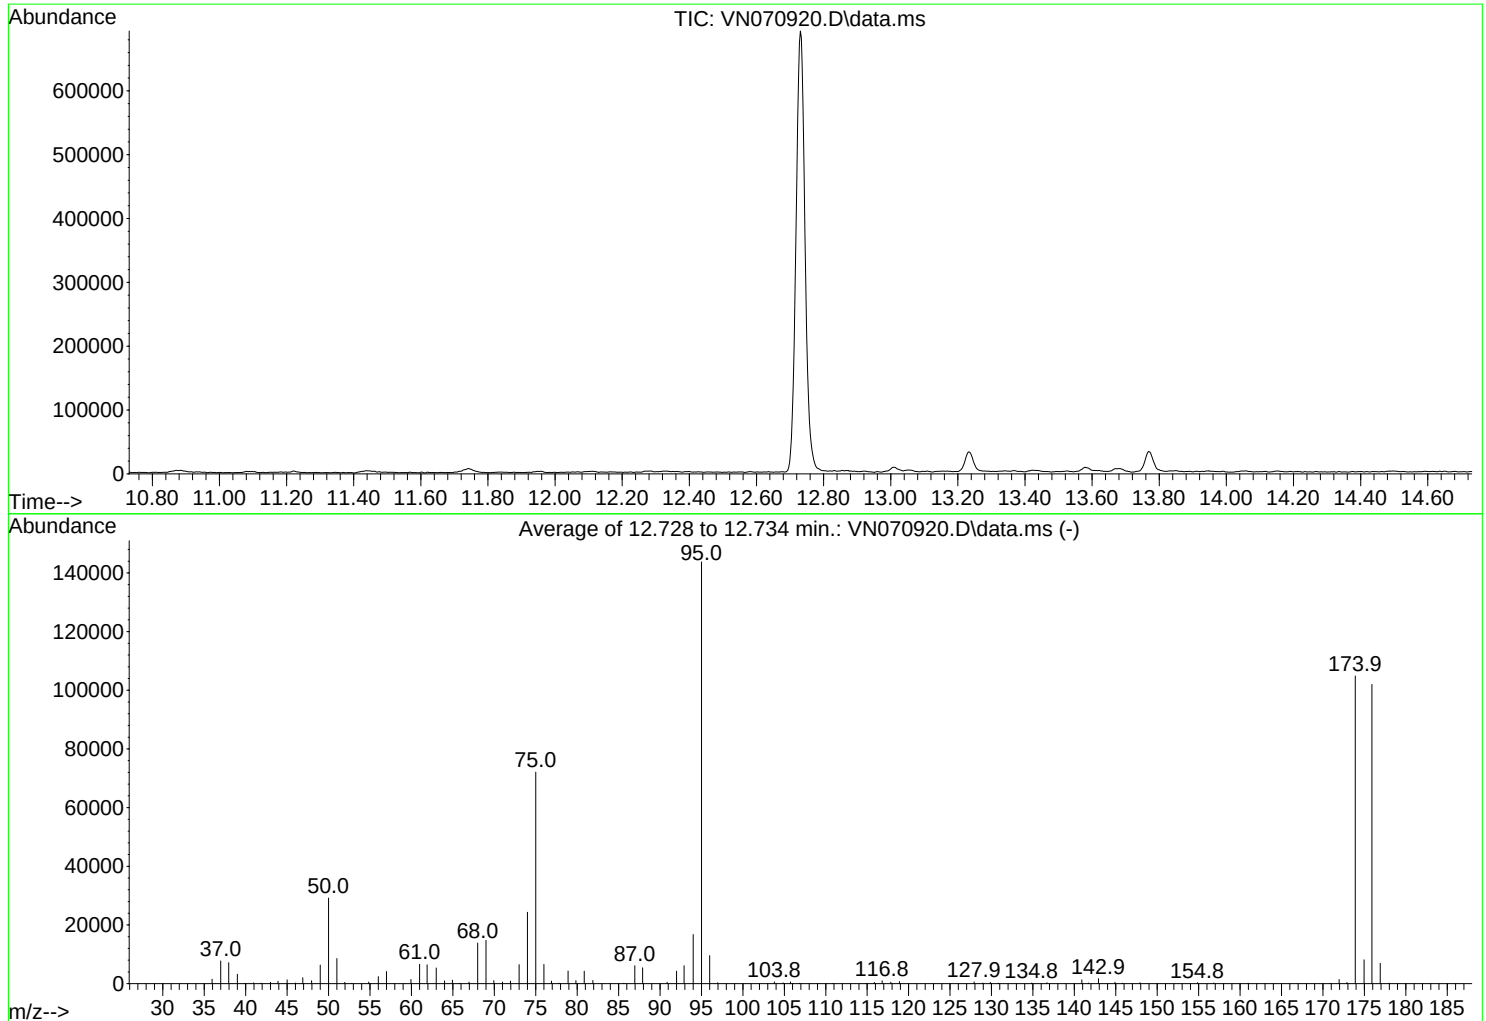

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	29171	PASS
75	95	30	60	50.2	72109	PASS
95	95	100	100	100.0	143765	PASS
96	95	5	9	6.7	9574	PASS
173	174	0.00	2	0.4	454	PASS
174	95	50	100	72.9	104853	PASS
175	174	5	9	7.8	8136	PASS
176	174	95	101	97.2	101960	PASS
177	176	5	9	6.8	6944	PASS