

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020323\
 Data File : VN076530.D
 Acq On : 03 Feb 2023 14:11
 Operator : JC\MD
 Sample : 01415-03 40X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-13-0202

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M

Title : SW846 8260

Signal : TIC: VN076530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.812	623	639	659	rBV	448673	1585568	51.99%	9.069%
2	7.436	904	915	926	rBV	15718	47042	1.54%	0.269%
3	8.171	1030	1040	1045	rBV	430580	1033637	33.89%	5.912%
4	8.230	1045	1050	1063	rVB	848434	1848957	60.63%	10.576%
5	8.583	1101	1110	1123	rBV	419397	952651	31.24%	5.449%
6	8.777	1134	1143	1152	rBV3	19738	60729	1.99%	0.347%
7	9.106	1189	1199	1218	rVB	1138703	2304462	75.57%	13.182%
8	10.571	1437	1448	1465	rBV	1655345	3049620	100.00%	17.444%
9	11.865	1661	1668	1681	rBV	1437028	2605902	85.45%	14.906%
10	12.853	1828	1836	1848	rBV	1105449	1875044	61.48%	10.725%
11	13.794	1989	1996	2006	rVB	1269534	2118917	69.48%	12.120%




Sum of corrected areas: 17482529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020323\
Data File : VN076530.D
Acq On : 03 Feb 2023 14:11
Operator : JC\MD
Sample : 01415-03 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-13-0202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

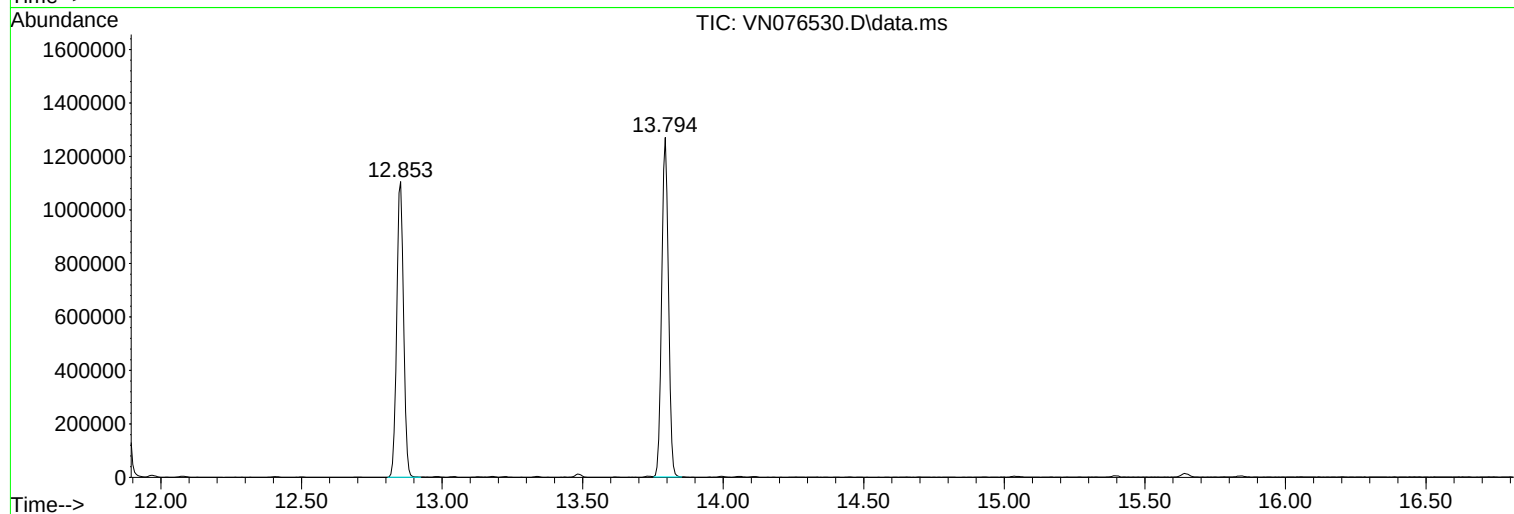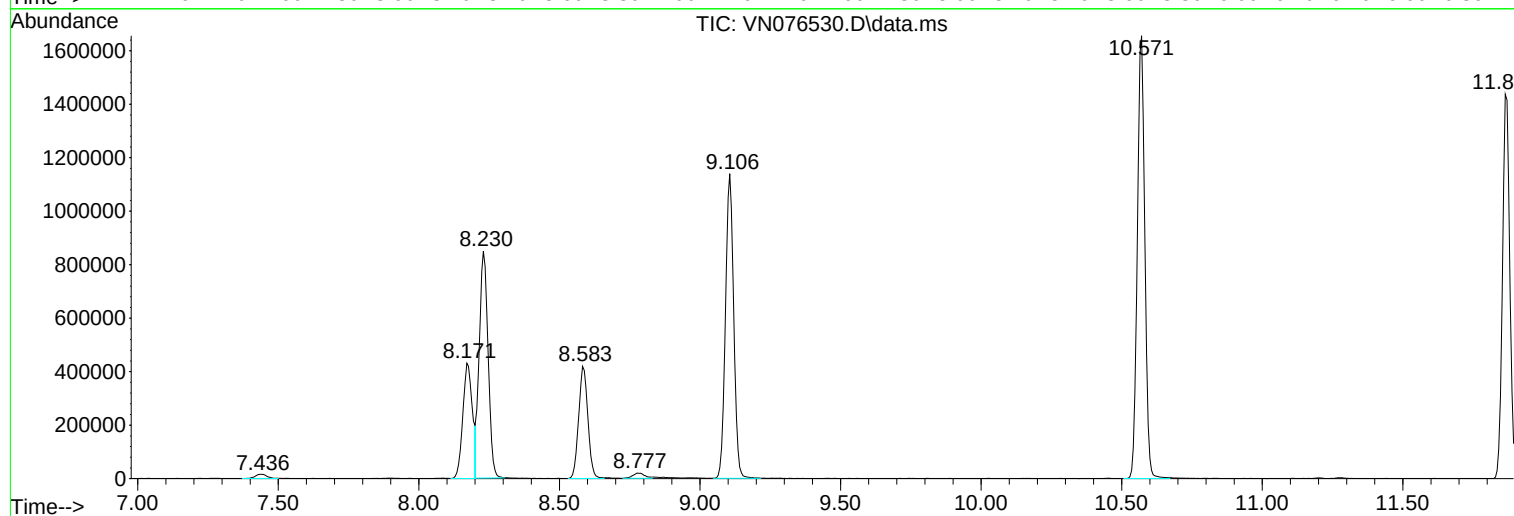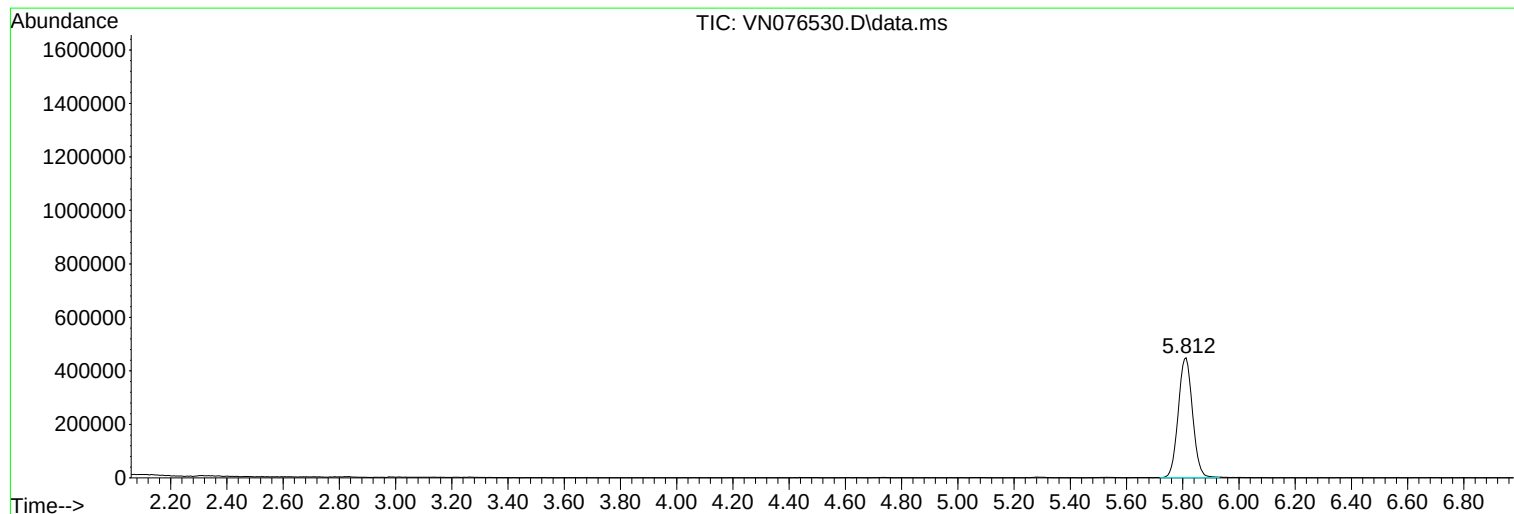

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020323\
Data File : VN076530.D
Acq On : 03 Feb 2023 14:11
Operator : JC\MD
Sample : 01415-03 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-13-0202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020323\
Data File : VN076530.D
Acq On : 03 Feb 2023 14:11
Operator : JC\MD
Sample : 01415-03 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-13-0202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc