
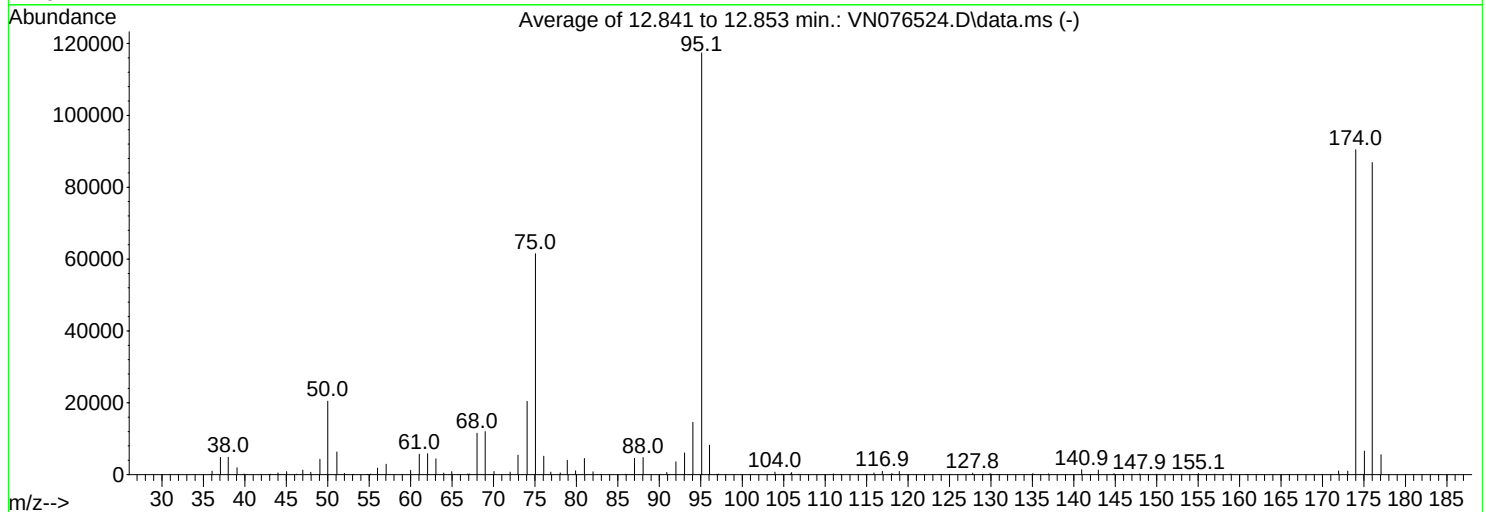


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020323\
Data File : VN076524.D
Acq On : 03 Feb 2023 08:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

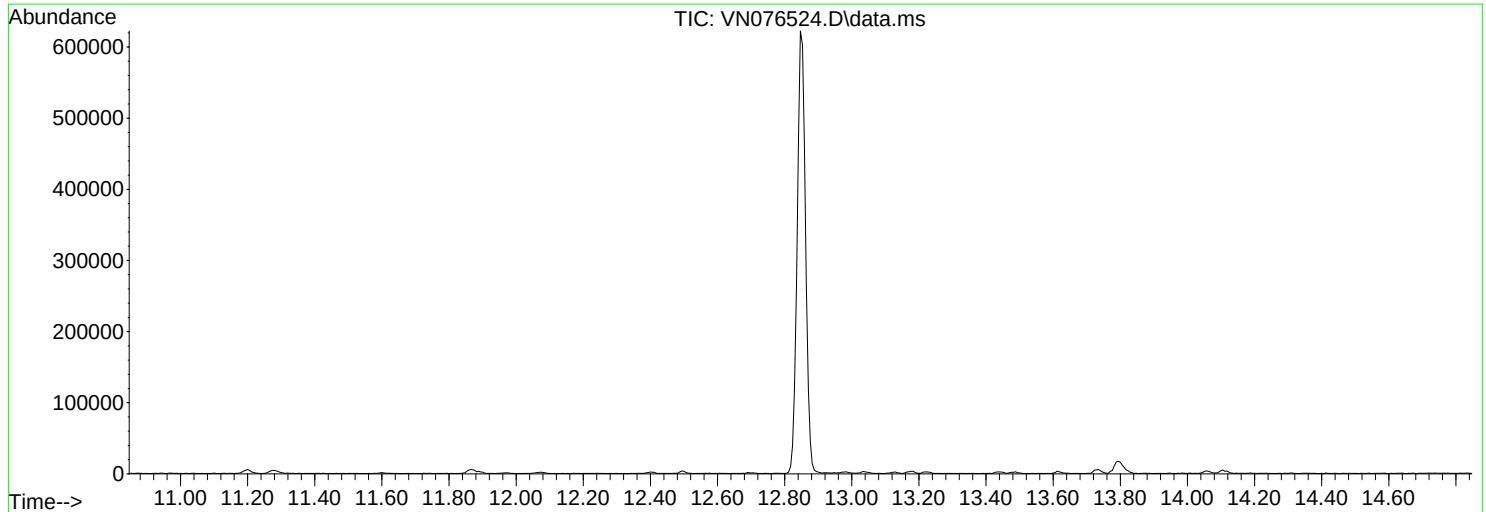

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	20456	PASS
75	95	30	60	52.4	61523	PASS
95	95	100	100	100.0	117400	PASS
96	95	5	9	7.0	8186	PASS
173	174	0.00	2	1.1	976	PASS
174	95	50	100	77.0	90440	PASS
175	174	5	9	7.3	6569	PASS
176	174	95	101	96.1	86888	PASS
177	176	5	9	6.4	5588	PASS

Average of 12.841 to 12.853 min.: VN076524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	986	47.95	654	61.05	5680	72.00	721
37.05	4796	49.05	4292	62.05	5840	72.95	544
38.00	4858	50.00	20456	63.05	4426	74.05	2038
39.05	1907	51.10	6339	64.00	446	75.05	6152
39.90	188	52.00	361	64.95	871	76.05	5130
43.10	153	53.10	74	65.80	52	76.90	733
44.00	496	54.80	101	66.90	241	78.05	505
45.05	834	55.15	169	67.10	162	78.90	4027
46.00	66	56.00	1840	68.00	11540	79.90	1075
46.25	124	57.05	2891	69.00	11973	80.95	4480
47.00	1240	60.00	1204	70.05	887	82.00	820

Average of 12.841 to 12.853 min.: VN076524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.90	57	96.90	72	115.90	503	131.10	57
85.90	117	97.00	74	116.90	940	135.05	300
86.10	74	97.15	185	117.80	98	136.95	244
87.00	4524	103.95	696	118.05	372	140.95	1379
88.05	4753	104.80	159	118.95	878	141.90	54
90.90	604	105.80	212	123.80	65	142.95	1311
92.00	3546	105.95	582	127.80	461	144.85	316
93.05	6060	106.85	121	129.10	65	145.85	145
94.05	14551	111.00	216	129.90	326	147.00	156
95.10	117400	111.90	73	130.10	155	147.95	216
96.05	8186	114.90	67	130.80	64	150.00	154

Average of 12.841 to 12.853 min.: VN076524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.05	125	177.05	5588				
155.05	292	178.00	63				
157.00	201						
158.95	183						
160.80	68						
171.10	70						
171.95	1041						
173.05	976						
174.00	90440						
175.05	6569						
176.00	86888						

Instrument :

MSVOA_N

ClientSampleId :

BFB