


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020325\
Data File : VN085616.D
Acq On : 03 Feb 2025 12:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

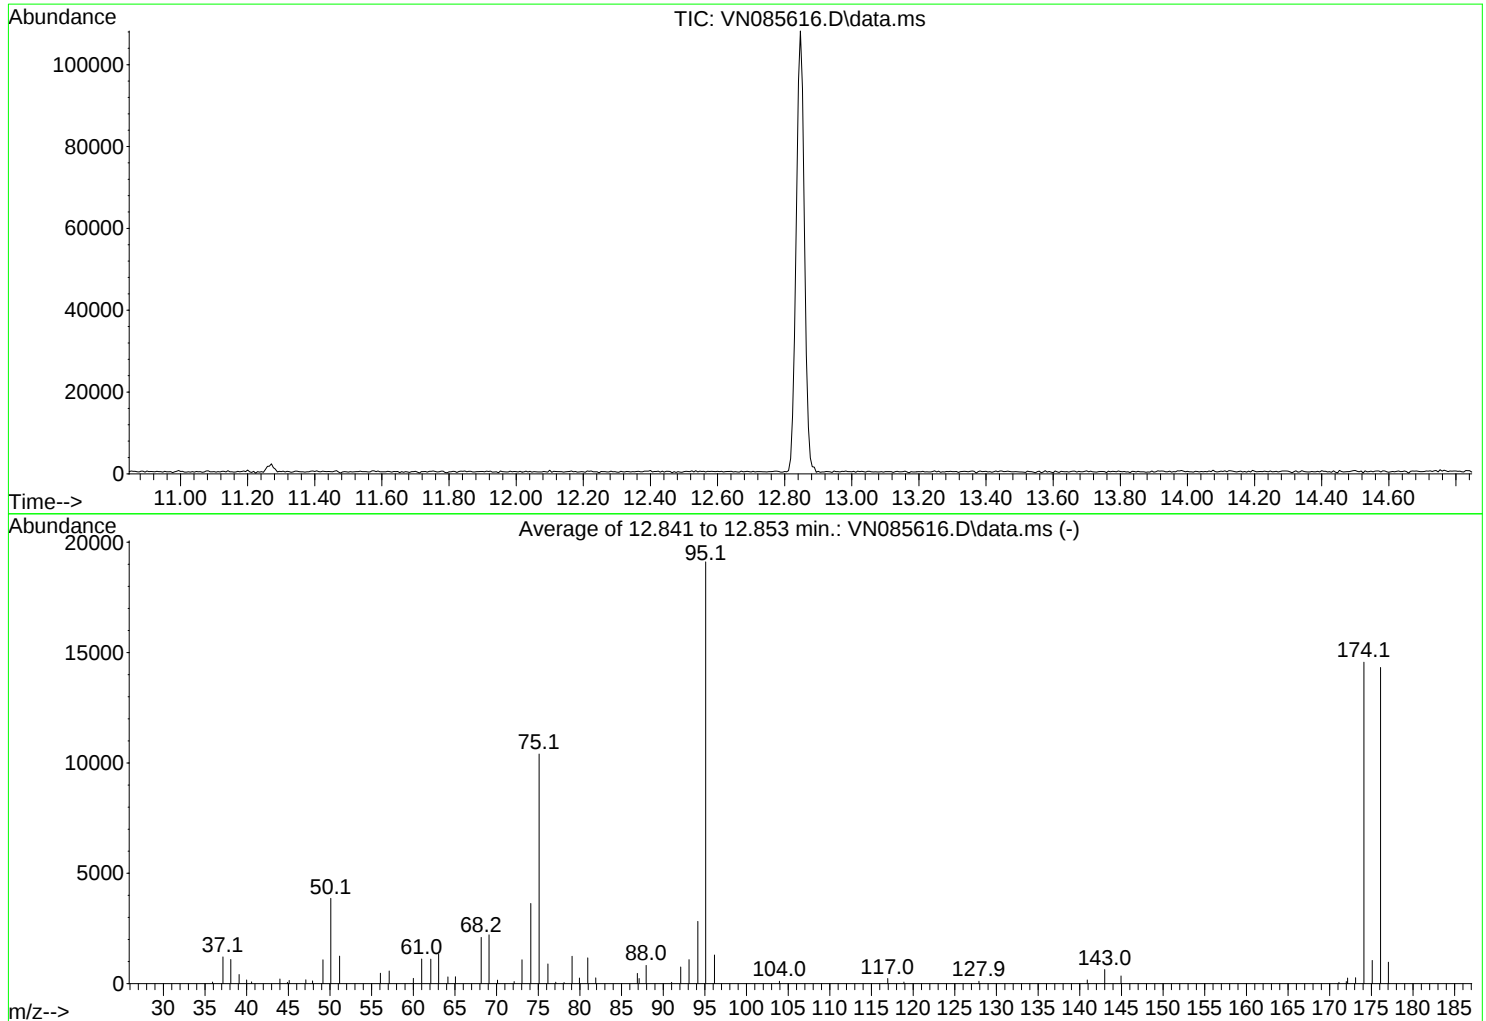

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	3864	PASS
75	95	30	60	54.4	10405	PASS
95	95	100	100	100.0	19112	PASS
96	95	5	9	6.8	1297	PASS
173	174	0.00	2	1.9	270	PASS
174	95	50	100	76.2	14567	PASS
175	174	5	9	7.2	1052	PASS
176	174	95	101	98.4	14328	PASS
177	176	5	9	6.8	972	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	74	49.15	1081	68.15	2097	79.95	254
37.15	1211	50.10	3864	69.10	2213	80.95	116
38.10	1095	51.15	1245	70.10	160	81.90	26
39.10	414	56.05	469	72.10	95	86.90	46
40.00	169	57.10	576	73.05	1077	87.10	230
40.60	80	60.00	237	74.10	3635	87.95	829
44.00	214	61.00	1118	75.10	10405	91.00	56
44.90	60	62.10	1112	76.15	891	92.10	756
45.10	147	63.05	1332	77.10	67	93.10	1091
47.10	175	64.15	308	78.10	54	94.15	2822
47.90	122	65.05	309	79.05	1243	95.10	19112

Average of 12.841 to 12.853 min.: VN085616.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.15	1297	173.10	270				
103.95	109	174.10	14567				
116.95	235	175.10	1052				
118.90	74	176.10	14328				
127.90	109	177.05	972				
140.90	170						
143.00	641						
144.95	346						
171.10	58						
172.00	94						
172.15	255						

Instrument :

MSVOA_N

ClientSampleId :

BFB