


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN020419\
Data File : VN053585.D
Acq On : 4 Feb 2019 9:31
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

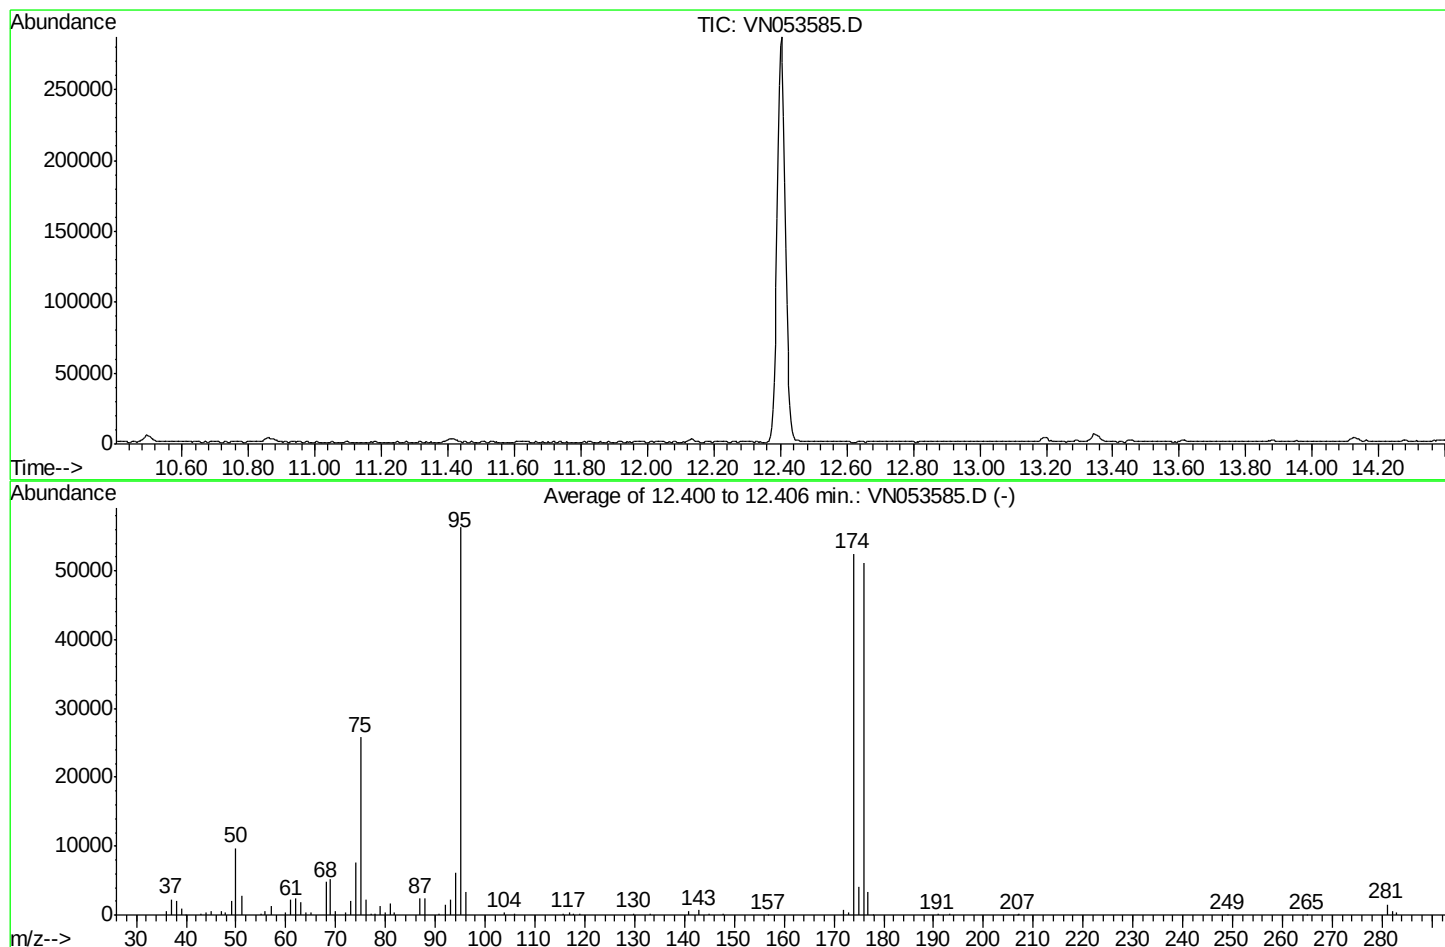

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	9694	PASS
75	95	30	60	45.8	25781	PASS
95	95	100	100	100.0	56322	PASS
96	95	5	9	6.0	3353	PASS
173	174	0.00	2	0.8	434	PASS
174	95	50	100	93.3	52530	PASS
175	174	5	9	7.7	4025	PASS
176	174	95	101	97.3	51130	PASS
177	176	5	9	6.4	3281	PASS