

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020425\
 Data File : VN085656.D
 Acq On : 04 Feb 2025 17:01
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Feb 05 01:08:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 15 02:16:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	210879	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	392094	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	336506	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	139457	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	147962	43.467	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.940%
35) Dibromofluoromethane	8.165	113	127876	47.010	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.020%
50) Toluene-d8	10.565	98	472710	48.911	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.820%
62) 4-Bromofluorobenzene	12.847	95	149817	45.316	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	90.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020425\
Data File : VN085656.D
Acq On : 04 Feb 2025 17:01
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK


Quant Time: Feb 05 01:08:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 02:16:08 2025
Response via : Initial Calibration

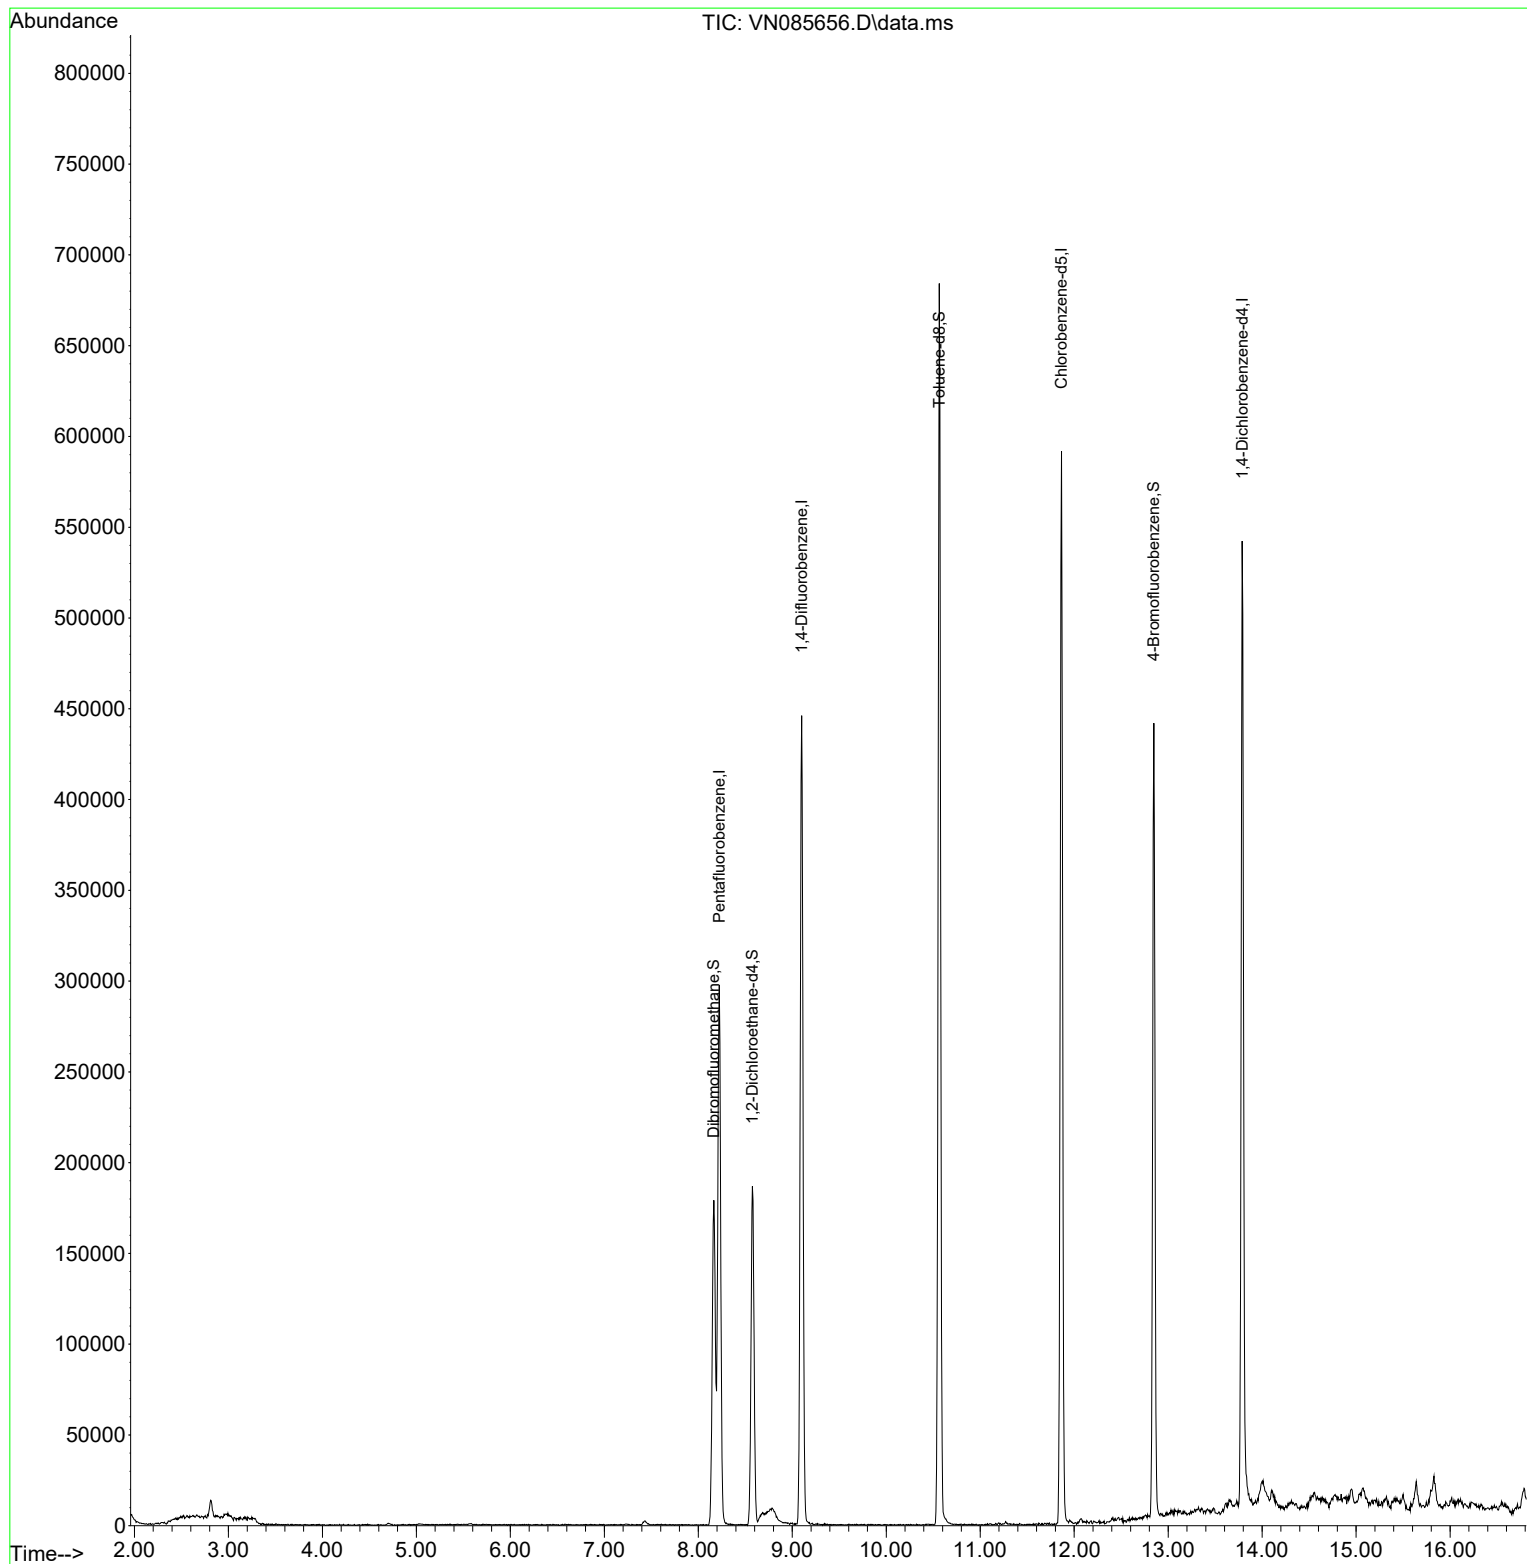



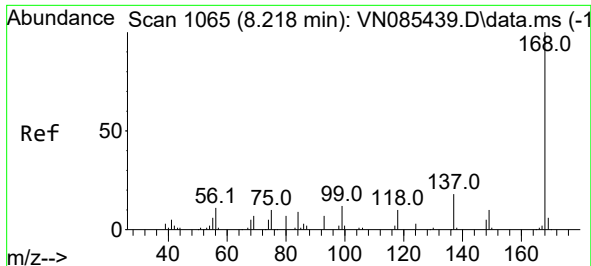


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01

Instrument :
MSVOA_N
ClientSampleId :
IBLK



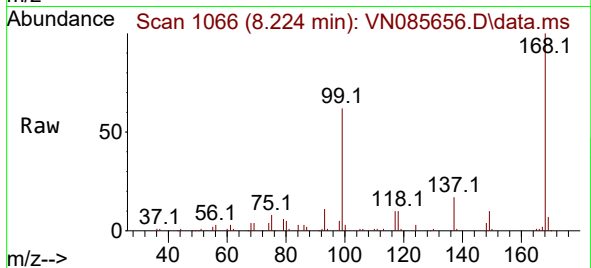



Tgt Ion:168 Resp: 210879
Ion Ratio Lower Upper
168 100
99 62.2 53.6 80.4

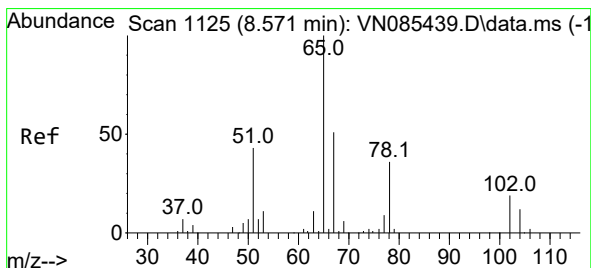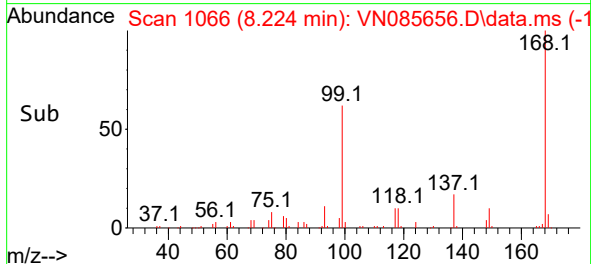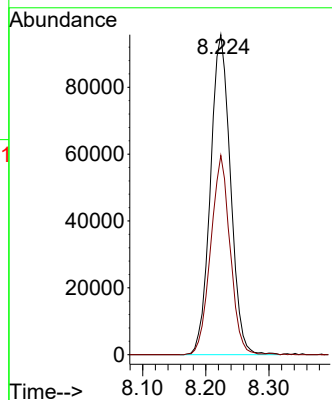

#33
1,2-Dichloroethane-d4
Concen: 43.467 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01

Tgt Ion: 65 Resp: 147962
Ion Ratio Lower Upper
65 100
67 53.1 0.0 101.6

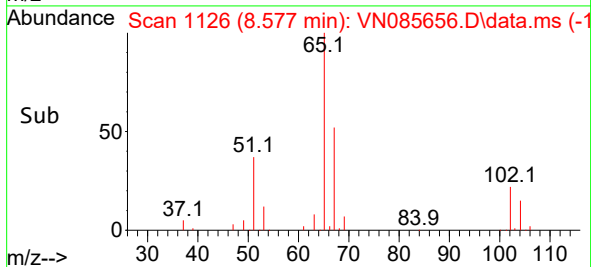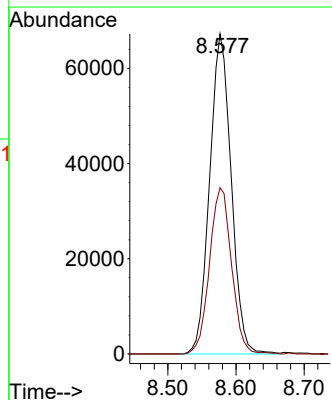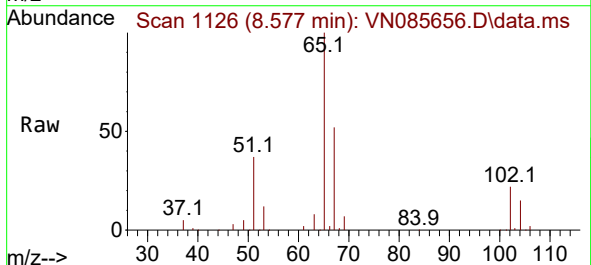

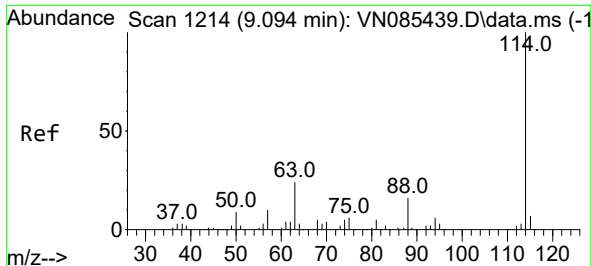

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085656.D

Acq: 04 Feb 2025 17:01

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 392094

Ion Ratio Lower Upper

114 100

63 19.9 0.0 47.6

88 15.0 0.0 32.6

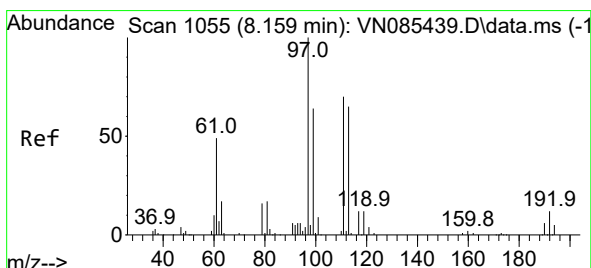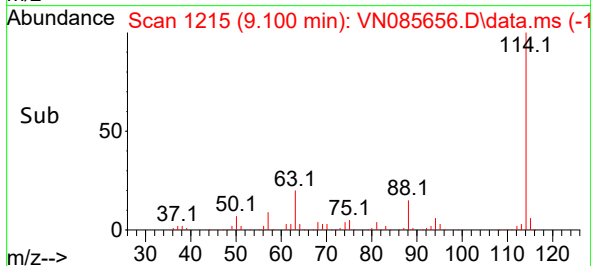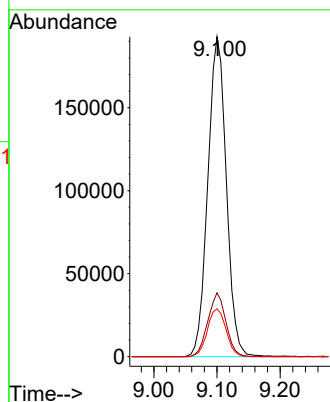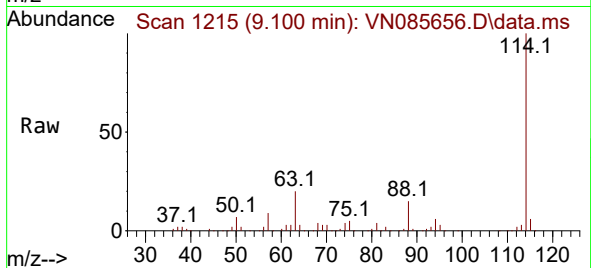

#35

Dibromofluoromethane

Concen: 47.010 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085656.D

Acq: 04 Feb 2025 17:01




Tgt Ion:113 Resp: 127876


Ion Ratio Lower Upper

113 100

111 103.6 82.7 124.1

192 17.4 14.3 21.5


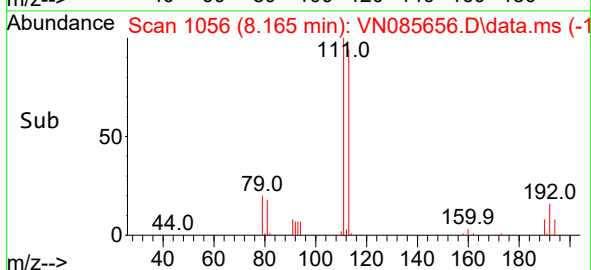
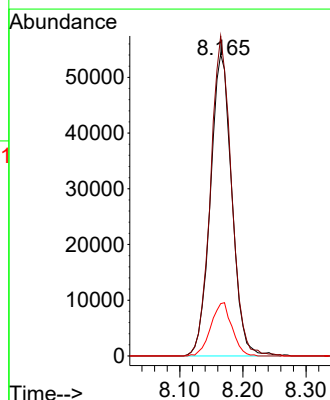
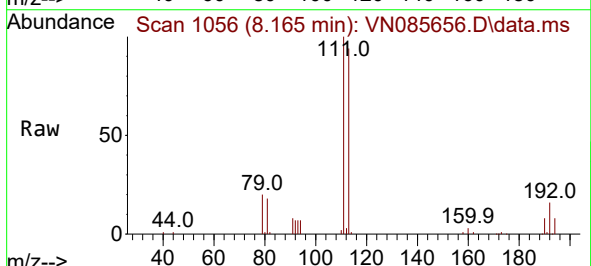


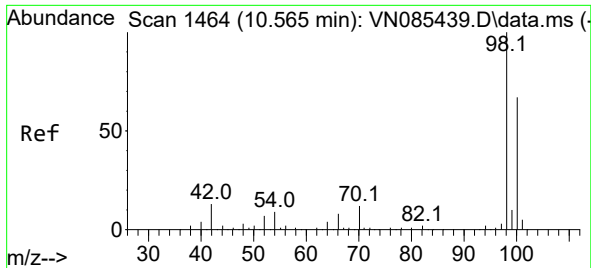

#50
Toluene-d8
Concen: 48.911 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 472710
Ion Ratio Lower Upper
98 100
100 63.1 52.2 78.4

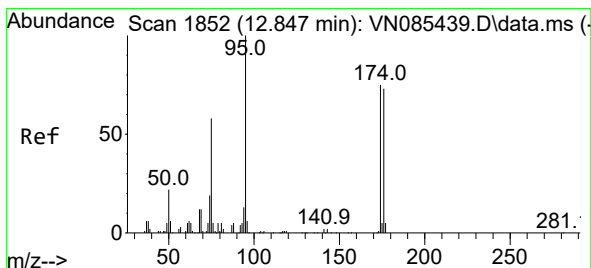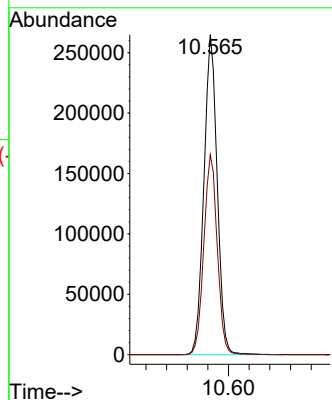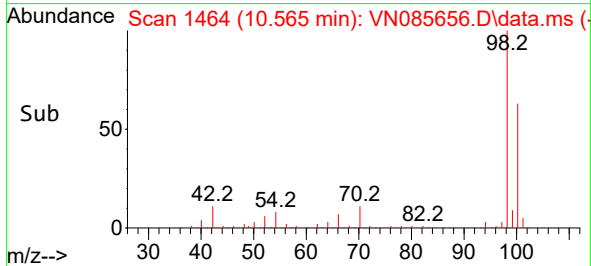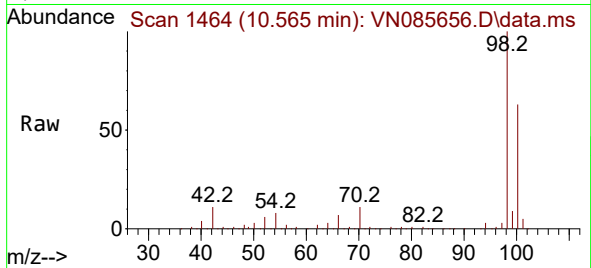

#62
4-Bromofluorobenzene
Concen: 45.316 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01

Tgt Ion: 95 Resp: 149817
Ion Ratio Lower Upper
95 100
174 76.7 0.0 145.0
176 73.0 0.0 142.4


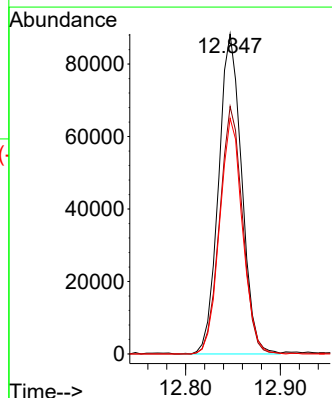
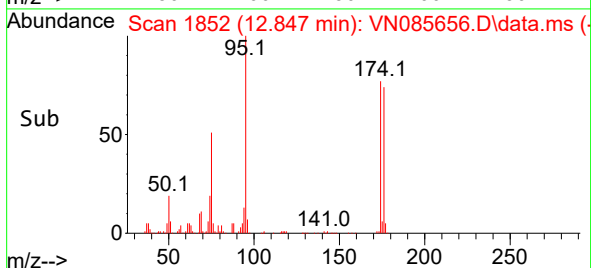
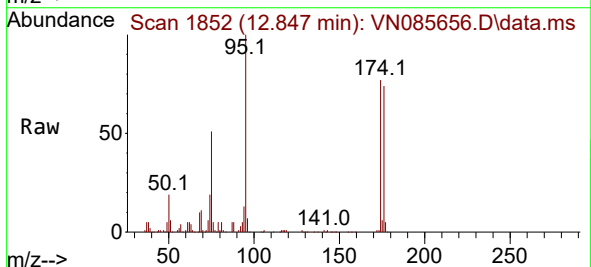


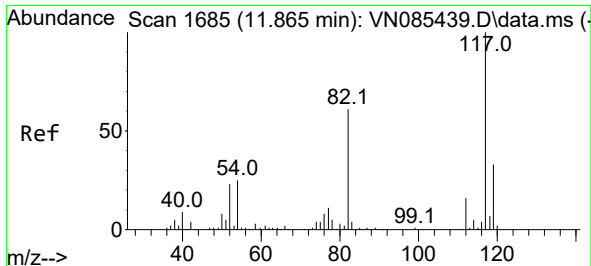

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 336506
Ion Ratio Lower Upper
117 100
82 54.1 48.6 72.8
119 32.5 26.6 39.8

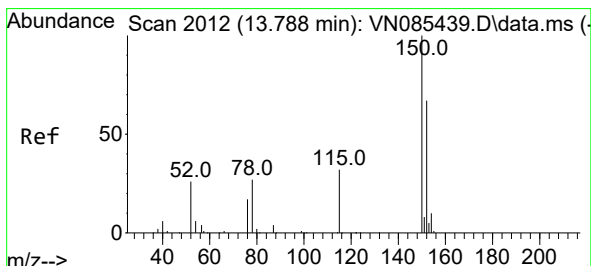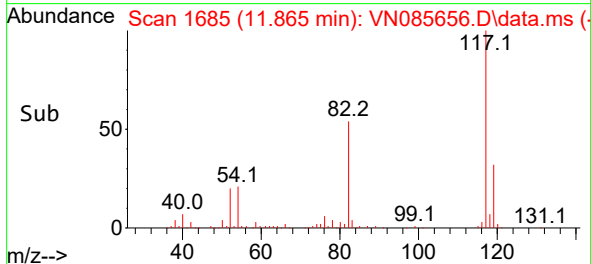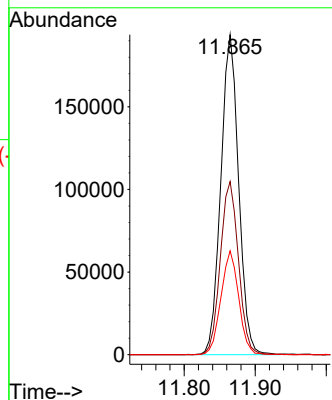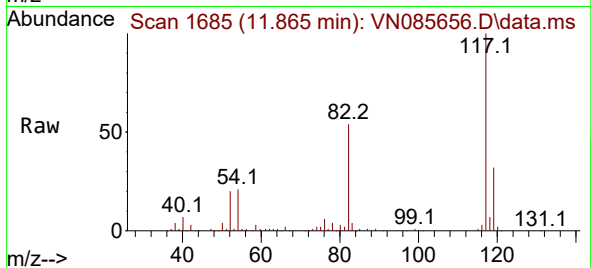

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN085656.D
Acq: 04 Feb 2025 17:01

Tgt Ion:152 Resp: 139457
Ion Ratio Lower Upper
152 100
115 61.9 31.1 93.3
150 158.3 0.0 343.6

