


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020425\
Data File : VN085644.D
Acq On : 04 Feb 2025 09:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

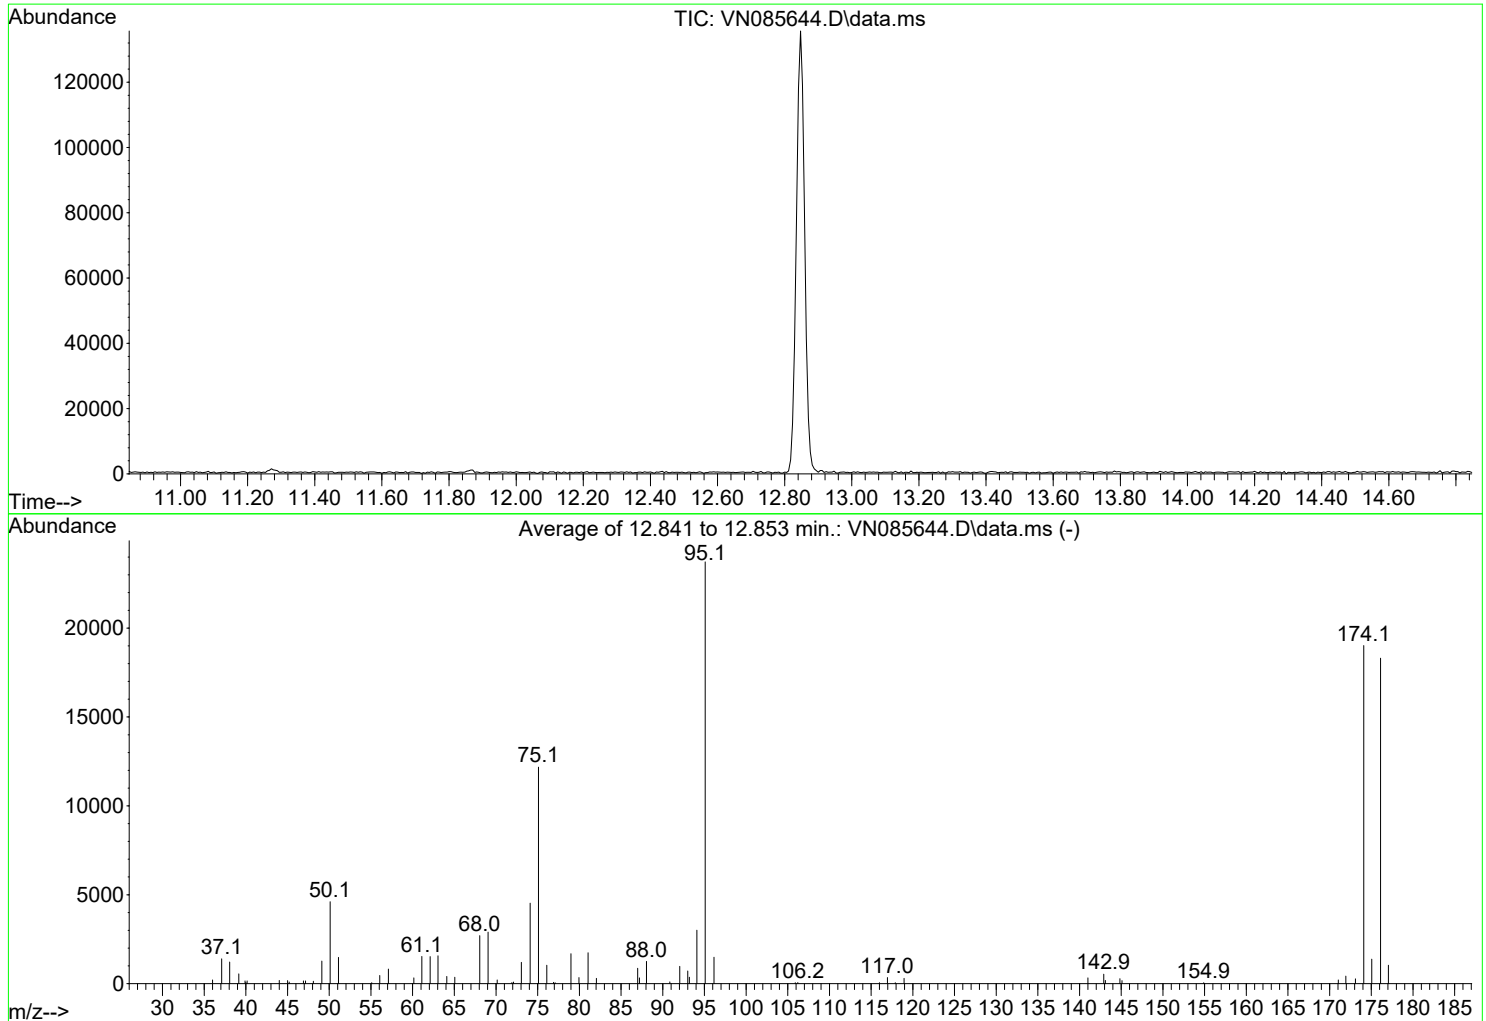

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	4605	PASS
75	95	30	60	51.3	12174	PASS
95	95	100	100	100.0	23728	PASS
96	95	5	9	6.3	1483	PASS
173	174	0.00	2	1.4	274	PASS
174	95	50	100	80.1	19016	PASS
175	174	5	9	7.2	1374	PASS
176	174	95	101	96.3	18307	PASS
177	176	5	9	5.7	1035	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	203	47.15	152	63.05	1569	76.10	1031
37.10	1397	48.10	133	64.10	406	76.90	71
38.05	1215	49.10	1273	65.05	361	77.10	5
39.15	549	50.10	4605	68.05	2699	79.00	168
39.90	155	51.10	1478	69.05	2899	79.95	343
40.00	71	55.10	51	70.15	210	81.05	1741
40.15	151	56.05	461	71.90	59	82.05	293
44.00	181	57.10	816	72.10	91	87.00	867
45.00	171	60.15	321	73.05	1198	87.20	320
45.20	92	61.10	1529	74.10	4528	88.05	1251
46.90	157	62.10	1522	75.10	12174	90.85	102

Average of 12.841 to 12.853 min.: VN085644.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	972	118.95	300	175.05	1374		
93.00	714	141.00	324	176.10	18307		
93.20	356	142.90	533	177.05	1035		
94.10	3005	143.10	179				
95.10	23728	144.85	279				
96.15	1483	145.10	170				
105.90	53	154.90	57				
106.20	61	171.05	211				
116.00	54	171.95	423				
116.95	344	173.10	274				
117.90	53	174.10	19016				

Instrument :

MSVOA_N

ClientSampleId :

BFB