


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN020519\
 Data File : VN053609.D
 Acq On : 5 Feb 2019 9:08
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
 Title : SW846 8260
 Last Update : Fri Feb 01 09:11:52 2019

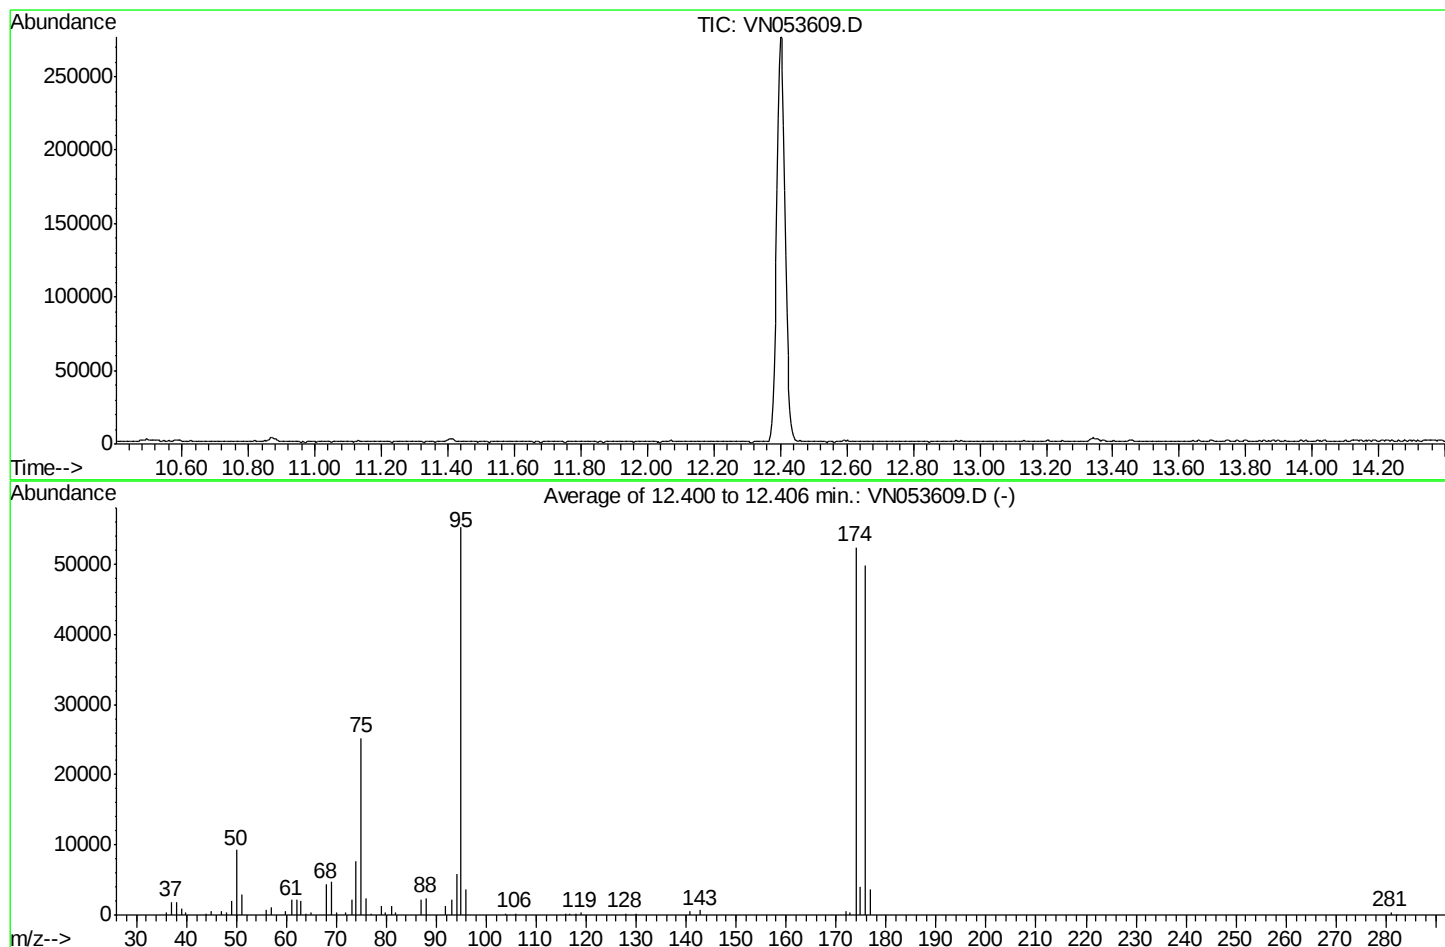

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	9227	PASS
75	95	30	60	45.6	25189	PASS
95	95	100	100	100.0	55256	PASS
96	95	5	9	6.6	3660	PASS
173	174	0.00	2	0.7	341	PASS
174	95	50	100	94.9	52424	PASS
175	174	5	9	7.5	3938	PASS
176	174	95	101	95.0	49802	PASS
177	176	5	9	7.2	3572	PASS