

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020521\
 Data File : VN065737.D
 Acq On : 5 Feb 2021 14:52
 Operator : JC/MD
 Sample : M1288-22
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 152140-FD-01

Quant Time: Feb 05 22:48:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.624	168	189709	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	319845	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	279120	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	98754	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	113682	45.55	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	91.10%		
35) Dibromofluoromethane	7.550	113	91495	48.27	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	96.54%		
50) Toluene-d8	10.058	98	397709	53.38	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	106.76%		
62) 4-Bromofluorobenzene	12.373	95	125090	46.63	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	93.26%		
Target Compounds						
64) Tetrachloroethene	10.601	164	2058	0.88	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020521\
Data File : VN065737.D
Acq On : 5 Feb 2021 14:52
Operator : JC/MD
Sample : M1288-22
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
152140-FD-01

Quant Time: Feb 05 22:48:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration




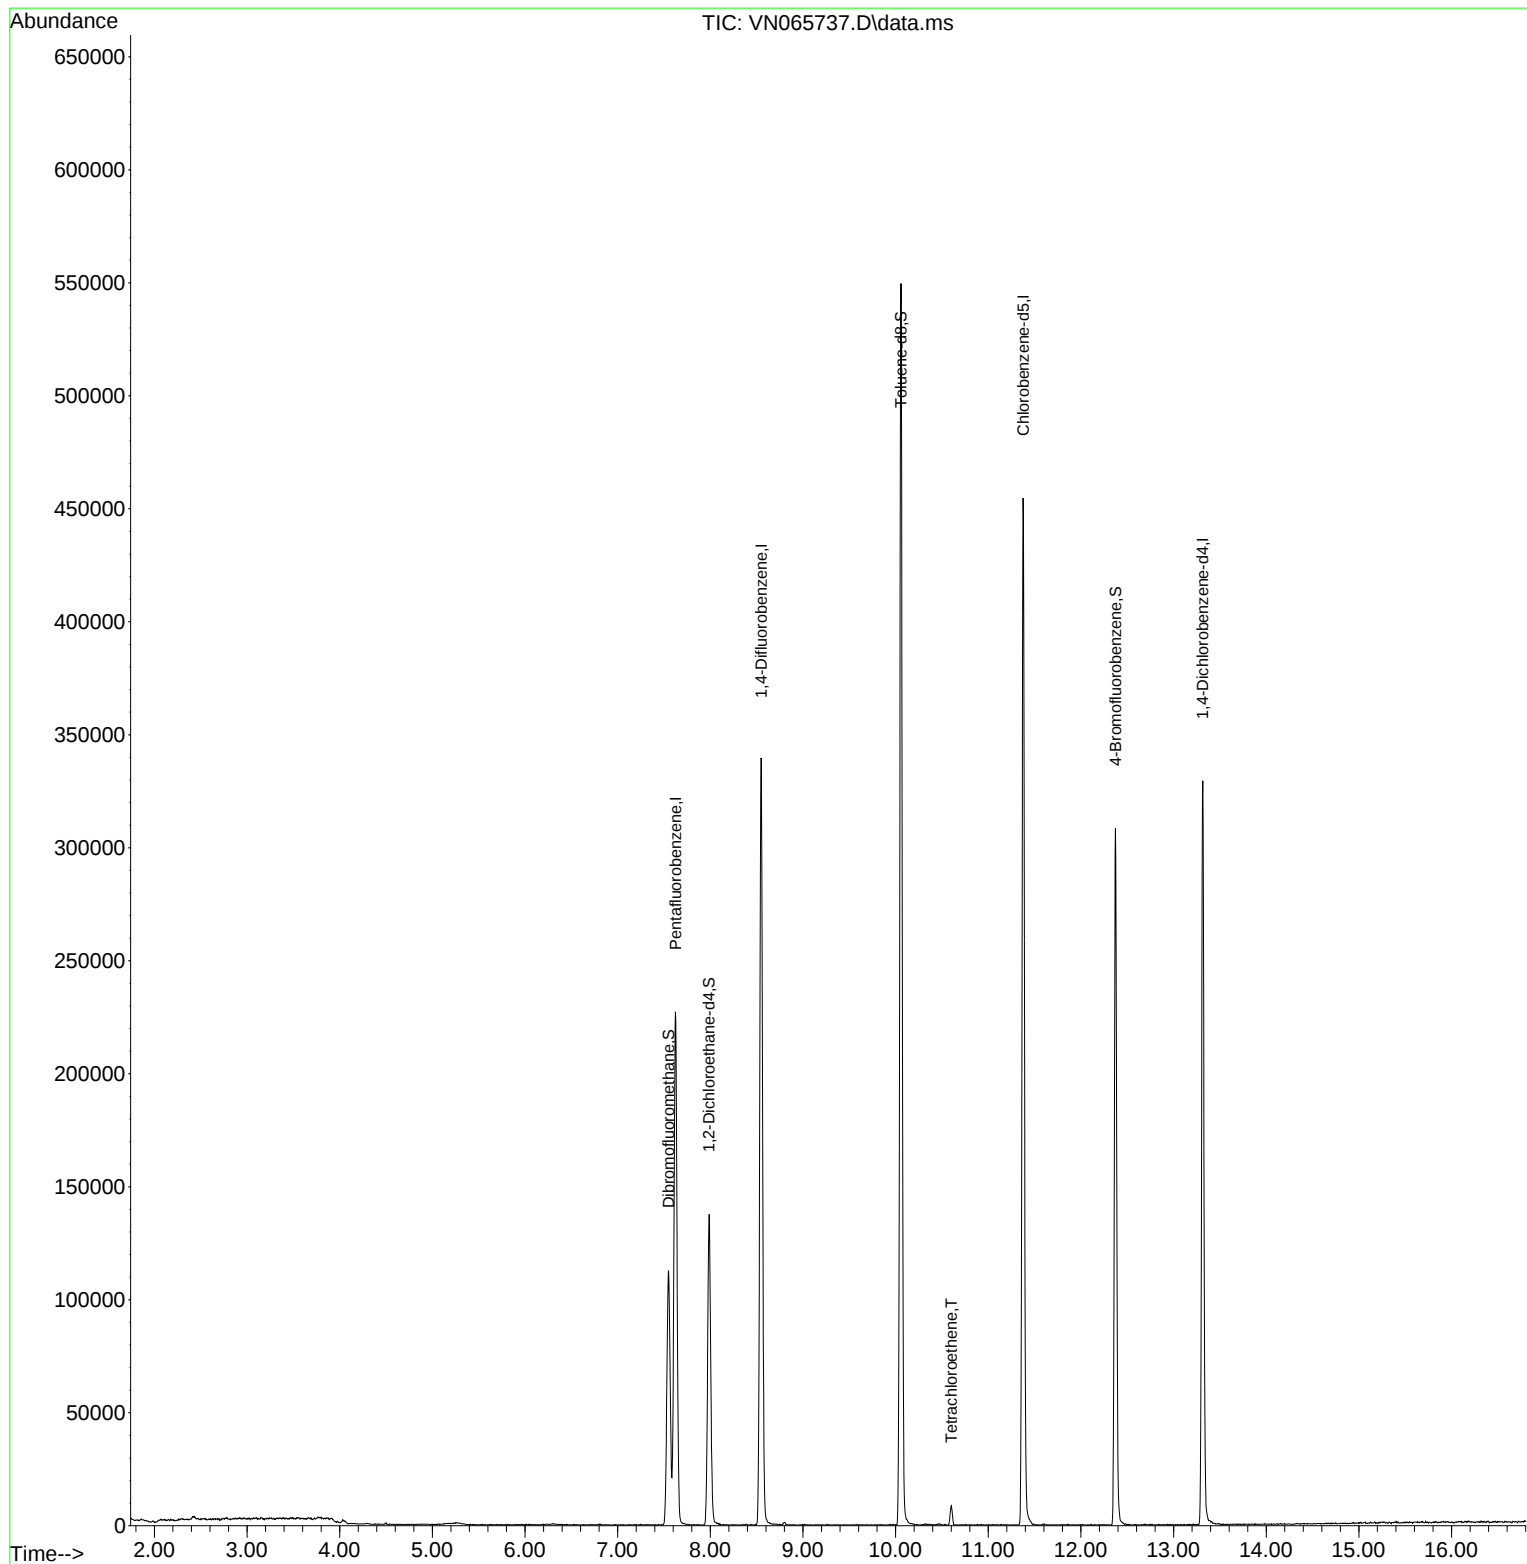


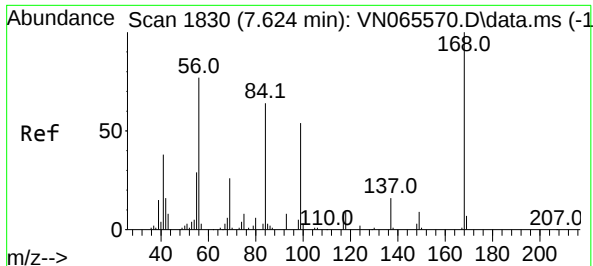

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52




Instrument :
MSVOA_N
ClientSampleId :
152140-FD-01


Tgt Ion:168 Resp: 189709
Ion Ratio Lower Upper
168 100
99 55.1 42.6 63.8

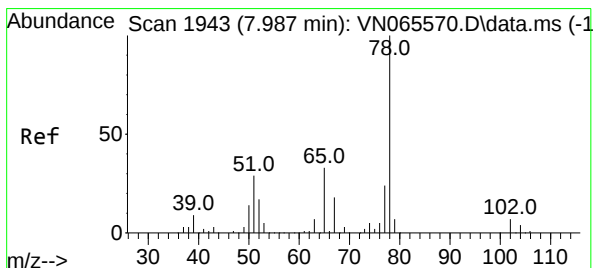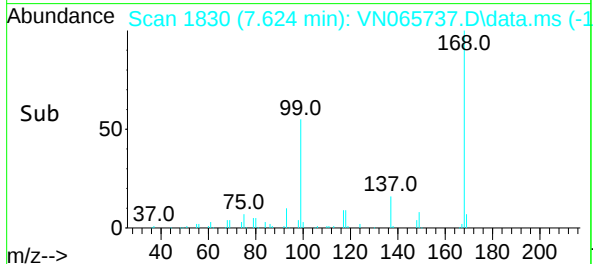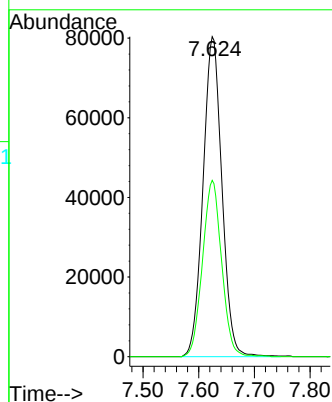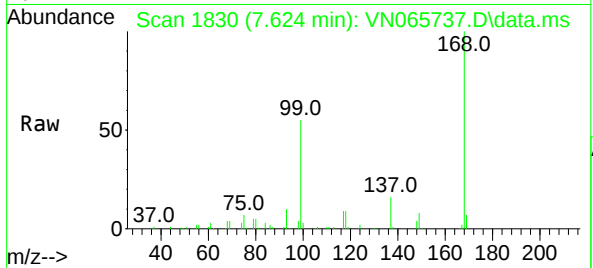

#33
1,2-Dichloroethane-d4
Concen: 45.55 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52


Tgt Ion: 65 Resp: 113682
Ion Ratio Lower Upper
65 100
67 55.6 0.0 107.2

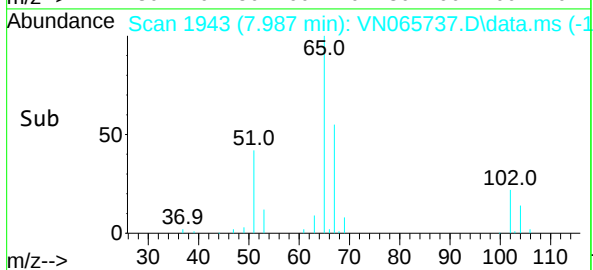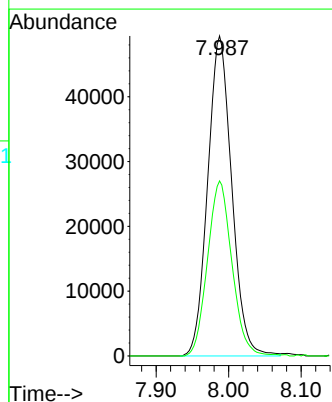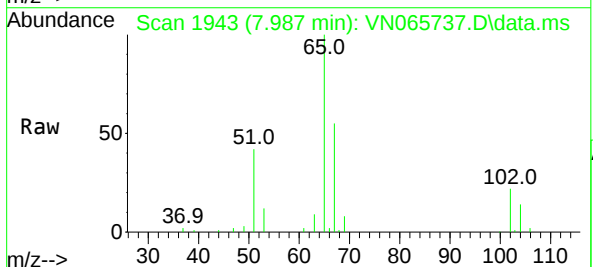



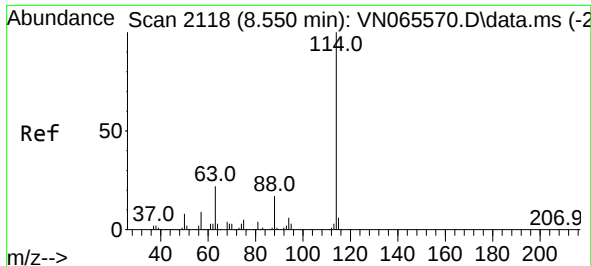


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52

Instrument :
MSVOA_N
ClientSampleId :
152140-FD-01



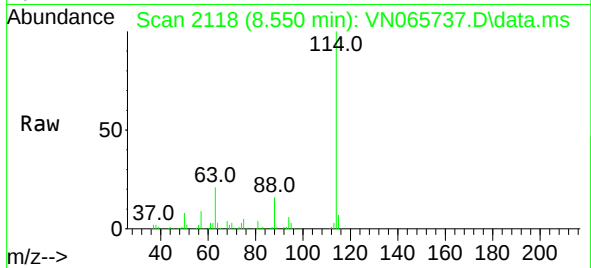



Tgt Ion	Ratio	Lower	Upper
114	100		
63	20.6	0.0	38.6
88	16.0	0.0	30.6

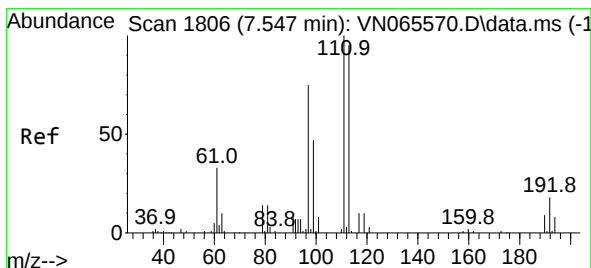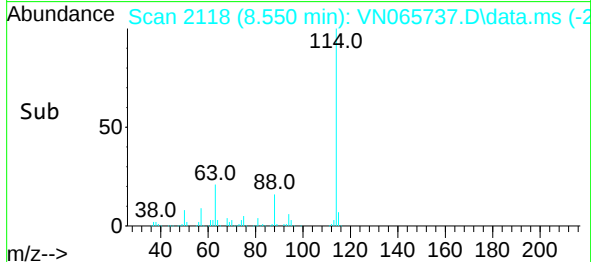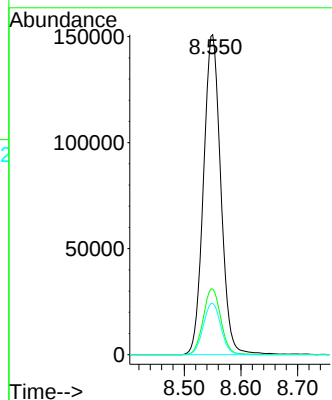

#35
Dibromofluoromethane
Concen: 48.27 ug/l
RT: 7.550 min Scan# 1807
Delta R.T. 0.003 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.6	82.2	123.2
192	18.9	15.4	23.0


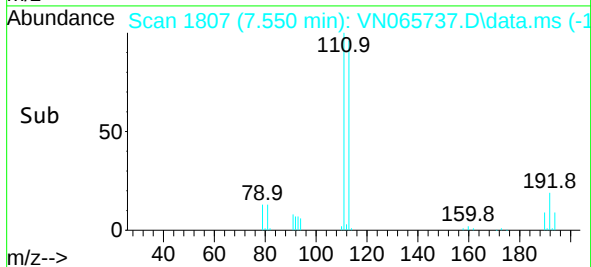
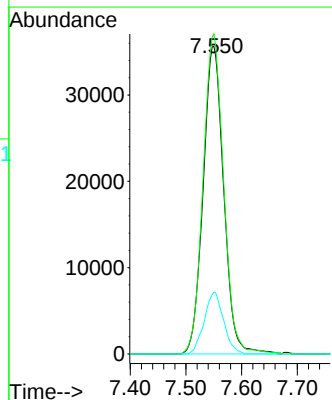
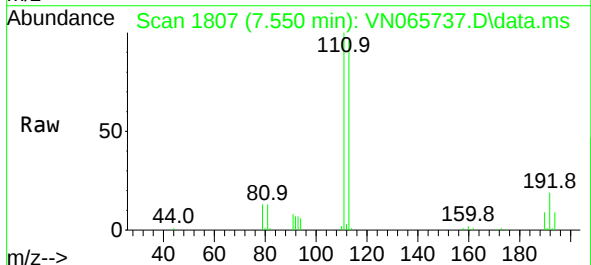


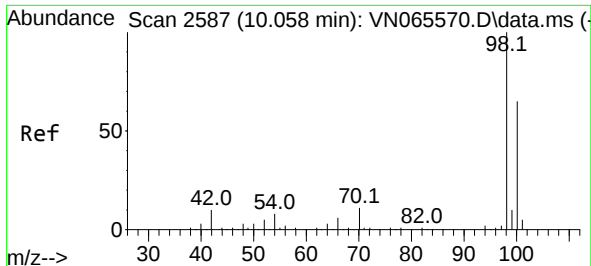

#50
Toluene-d8
Concen: 53.38 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52




Instrument :
MSVOA_N
ClientSampleId :
152140-FD-01


Tgt Ion: 98 Resp: 397709
Ion Ratio Lower Upper
98 100
100 64.8 50.5 75.7

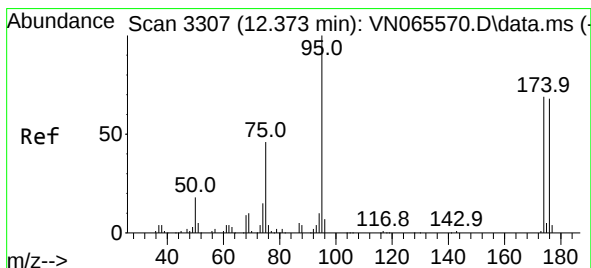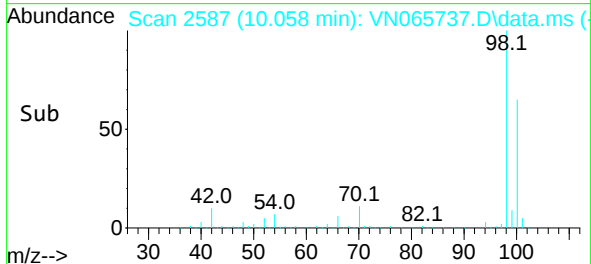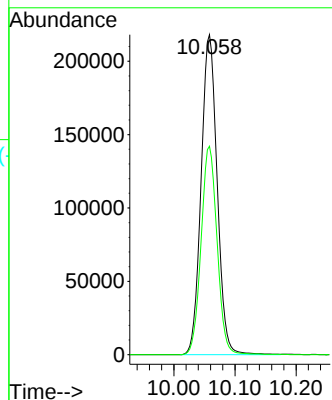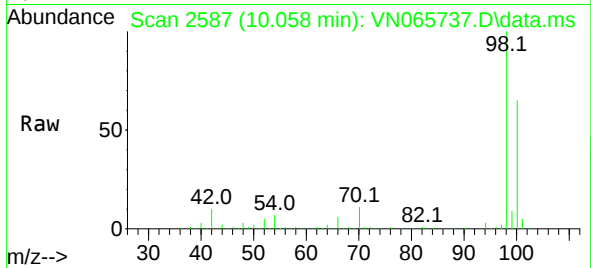

#62
4-Bromofluorobenzene
Concen: 46.63 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52


Tgt Ion: 95 Resp: 125090
Ion Ratio Lower Upper
95 100
174 71.4 0.0 169.0
176 68.4 0.0 162.4

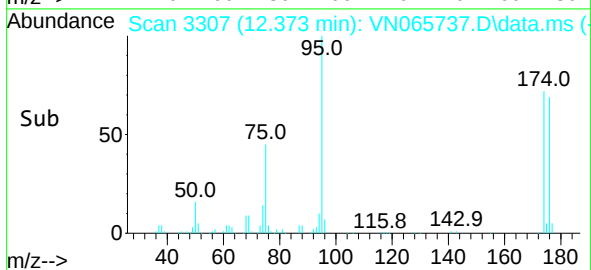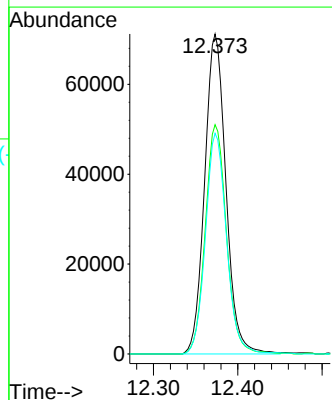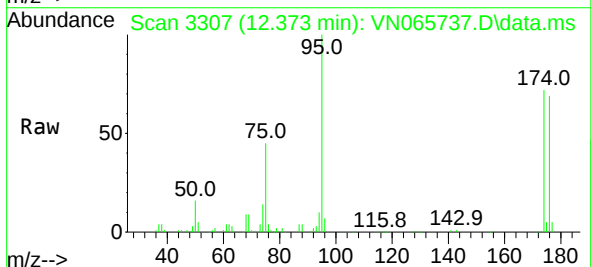



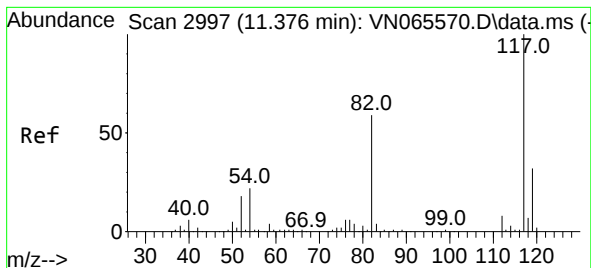


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52


Instrument :
MSVOA_N
ClientSampleId :
152140-FD-01

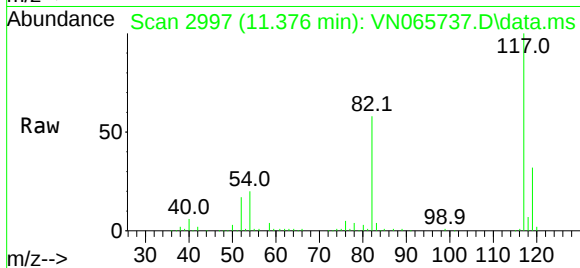



Tgt Ion:117 Resp: 279120
Ion Ratio Lower Upper
117 100
82 57.8 43.7 65.5
119 32.1 26.1 39.1

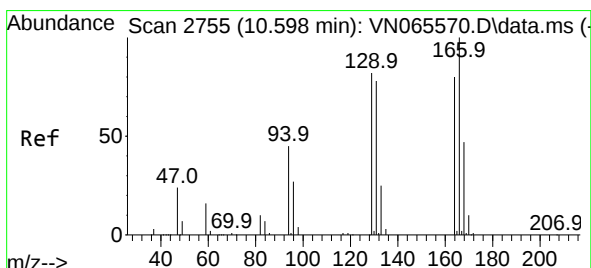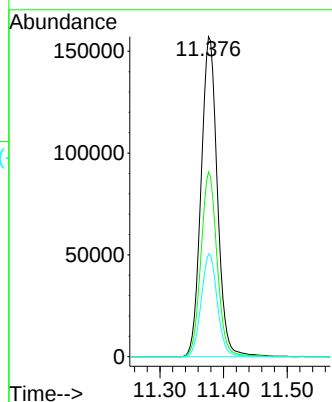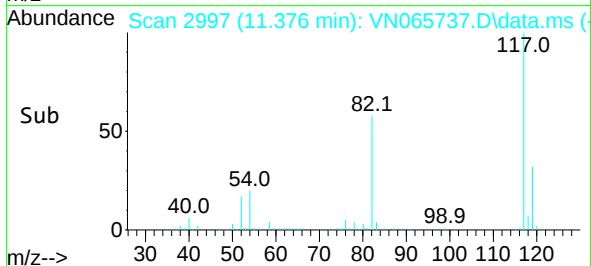


#64
Tetrachloroethene
Concen: 0.88 ug/l
RT: 10.601 min Scan# 2756
Delta R.T. 0.003 min
Lab File: VN065737.D
Acq: 5 Feb 2021 14:52

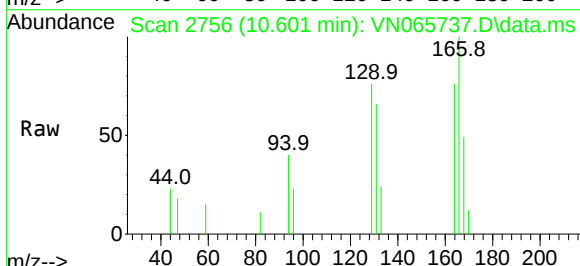


Tgt Ion:164 Resp: 2058
Ion Ratio Lower Upper
164 100
166 131.7 102.6 154.0
129 100.2 76.2 114.4
131 86.9 73.4 110.2

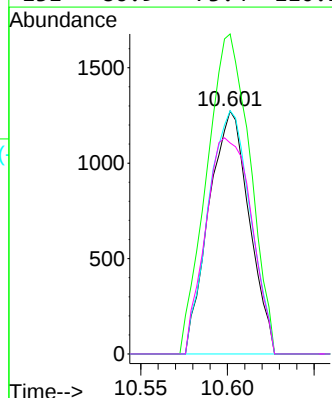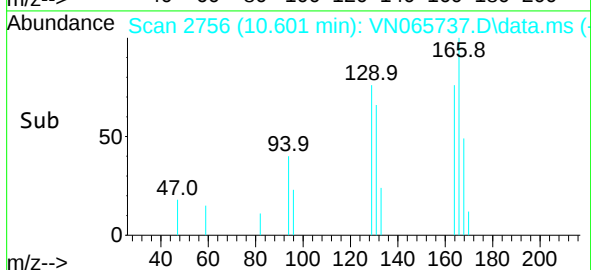

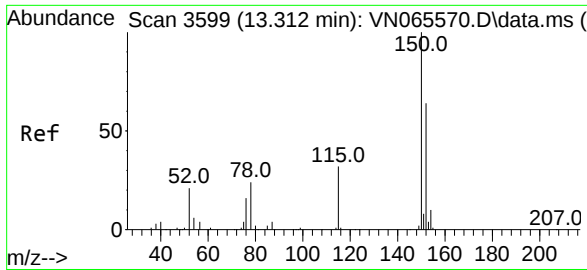

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.315 min Scan# 3600
 Delta R.T. 0.003 min
 Lab File: VN065737.D
 Acq: 5 Feb 2021 14:52

Instrument :
 MSVOA_N
 ClientSampleId :
 152140-FD-01

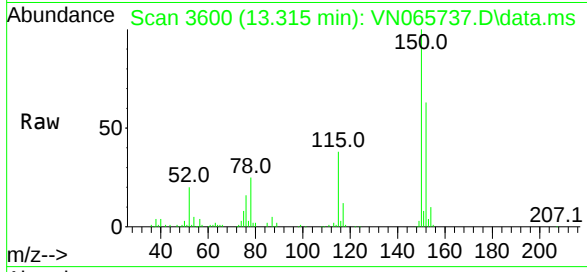

Tgt Ion:152 Resp: 98754
 Ion Ratio Lower Upper
 152 100
 115 59.6 28.5 85.6
 150 155.6 0.0 347.6

