


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020524\
Data File : VN080891.D
Acq On : 05 Feb 2024 11:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

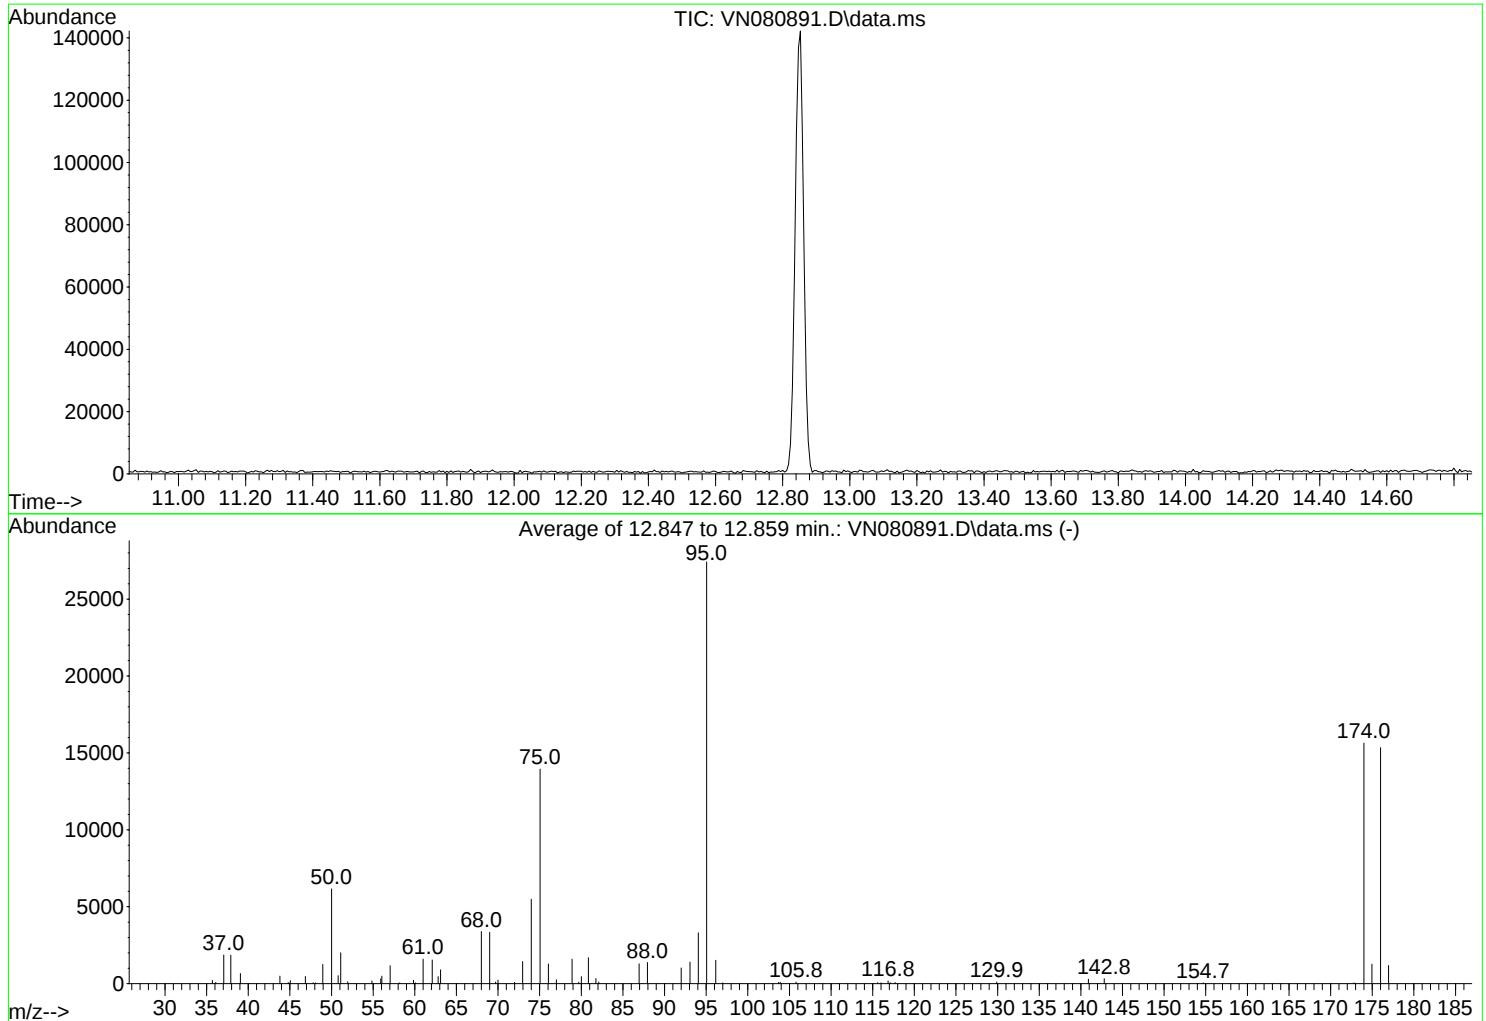

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	6158	PASS
75	95	30	60	50.9	13950	PASS
95	95	100	100	100.0	27424	PASS
96	95	5	9	5.5	1514	PASS
173	174	0.00	2	0.3	54	PASS
174	95	50	100	57.0	15633	PASS
175	174	5	9	8.1	1271	PASS
176	174	95	101	98.1	15341	PASS
177	176	5	9	7.7	1177	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	208	48.95	1250	60.10	55	74.00	549
36.10	86	50.00	6158	61.00	1592	75.05	1395
37.05	1862	50.80	523	62.10	1542	76.05	127
37.90	1848	51.10	2005	62.80	458	77.00	25
39.05	652	51.95	127	63.10	892	78.90	1589
43.80	487	54.85	174	68.00	3389	79.70	91
44.80	75	55.90	308	69.00	3341	80.00	453
45.05	203	56.05	487	69.70	101	80.85	1683
46.85	471	57.05	1166	70.00	230	81.75	336
47.80	60	58.20	55	72.00	82	82.10	106
48.10	51	59.85	217	72.95	1441	86.95	1286

Average of 12.847 to 12.859 min.: VN080891.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	1375	116.00	52	176.00	15341		
92.00	1022	116.85	180	176.95	1177		
93.05	1403	117.10	60				
94.05	3305	117.70	69				
95.05	27424	129.90	102				
96.15	1514	140.90	287				
97.00	56	142.80	318				
103.70	83	154.70	53				
103.90	94	172.80	54				
105.80	109	174.00	15633				
115.60	59	174.95	1271				

Instrument :

MSVOA_N

ClientSampleId :

BFB