

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020525\
 Data File : VN085685.D
 Acq On : 05 Feb 2025 18:23
 Operator : JC\MD
 Sample : Q1287-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 06 00:45:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 15 02:16:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	194090	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	379019	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	348070	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	136813	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	152183	48.574	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.140%		
35) Dibromofluoromethane	8.165	113	124901	47.501	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.000%		
50) Toluene-d8	10.565	98	481747	51.566	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	103.140%		
62) 4-Bromofluorobenzene	12.847	95	142837	44.695	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	89.400%		
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.518	59	92	0.256	ug/l #	71
13) Acrolein	4.183	56	139	0.284	ug/l #	14
16) Acetone	4.424	43	52148	51.514	ug/l	97
17) Carbon Disulfide	4.712	76	4180	0.652	ug/l #	76
18) Methyl Acetate	5.030	43	2925	0.950	ug/l #	66
20) Methylene Chloride	5.283	84	1396	0.557	ug/l #	82
25) 2-Butanone	7.488	43	5642	3.787	ug/l #	87
29) Tetrahydrofuran	7.841	42	583	0.617	ug/l #	49
30) Chloroform	7.971	83	1172	0.248	ug/l	85
31) Cyclohexane	8.218	56	4726	1.189	ug/l #	6
36) 1,1-Dichloropropene	8.224	75	16853	4.567	ug/l #	51
37) Ethyl Acetate	7.559	43	3973	1.067	ug/l #	88
38) Carbon Tetrachloride	8.224	117	20559	4.866	ug/l #	17
41) Methacrylonitrile	7.853	41	679	0.350	ug/l #	31
42) 1,2-Dichloroethane	8.688	62	1035	0.248	ug/l #	76
43) Isopropyl Acetate	8.688	43	164070	27.489	ug/l #	88
45) 1,2-Dichloropropane	9.741	63	1672	0.590	ug/l #	43
48) Methyl methacrylate	9.741	41	127808	47.583	ug/l #	45
49) 1,4-Dioxane	9.741	88	172	3.803	ug/l #	1
51) 4-Methyl-2-Pentanone	10.441	43	10894	3.145	ug/l #	78
53) t-1,3-Dichloropropene	10.724	75	970	0.247	ug/l	98
54) cis-1,3-Dichloropropene	10.353	75	48041	11.430	ug/l #	60
56) Ethyl methacrylate	10.982	69	1528	2.274	ug/l #	1
57) 1,3-Dichloropropane	11.194	76	6948	1.572	ug/l #	43
59) 2-Hexanone	11.200	43	71009	29.137	ug/l #	63
74) N-amyl acetate	12.459	43	1409	0.339	ug/l #	42
76) 1,2,3-Trichloropropane	12.847	75	76747	27.599	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	76747	74.672	ug/l #	3
86) p-Isopropyltoluene	13.729	119	9171	1.326	ug/l	90
95) Naphthalene	15.635	128	28580	4.650	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020525\
Data File : VN085685.D
Acq On : 05 Feb 2025 18:23
Operator : JC\MD
Sample : Q1287-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Feb 06 00:45:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 02:16:08 2025
Response via : Initial Calibration

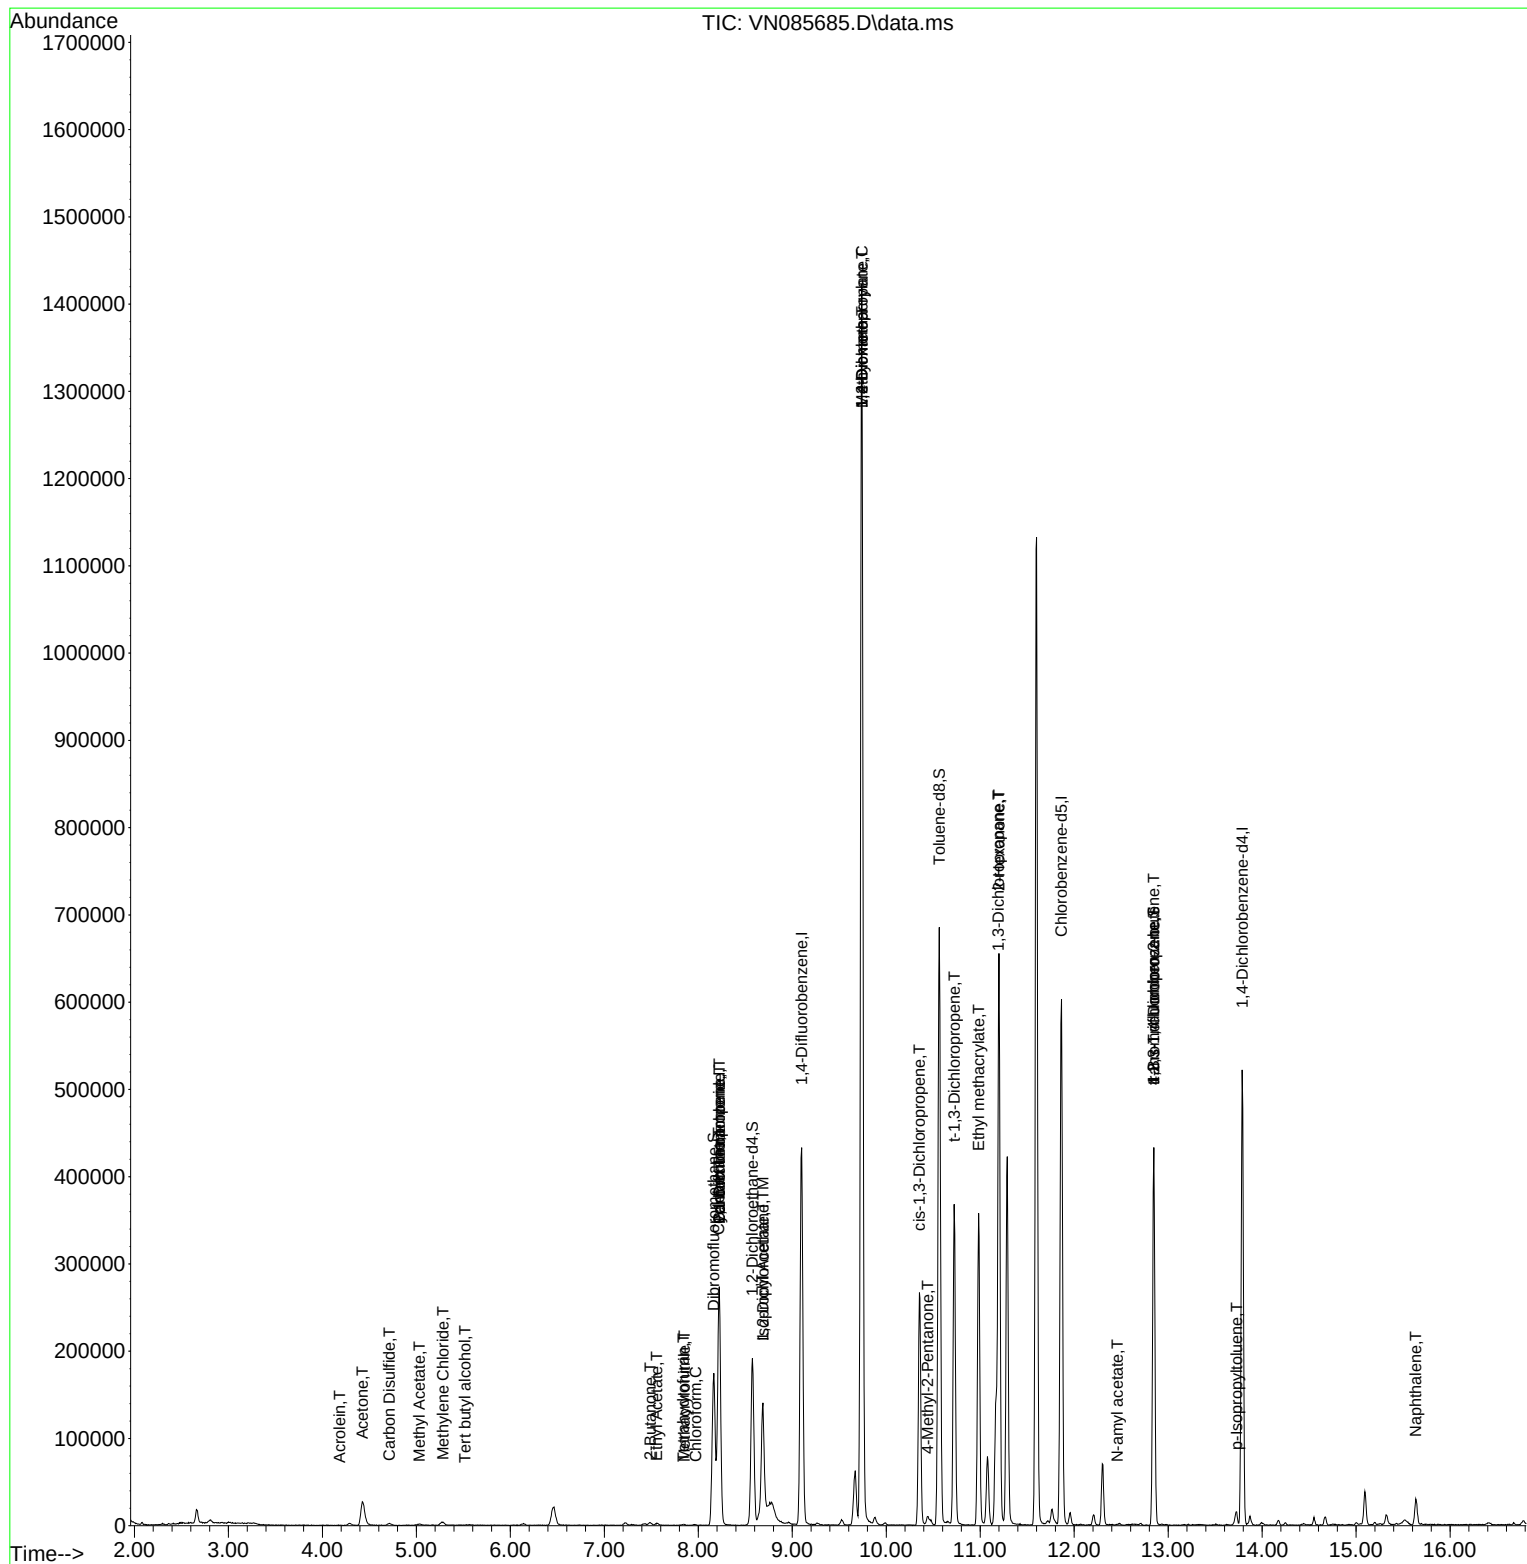



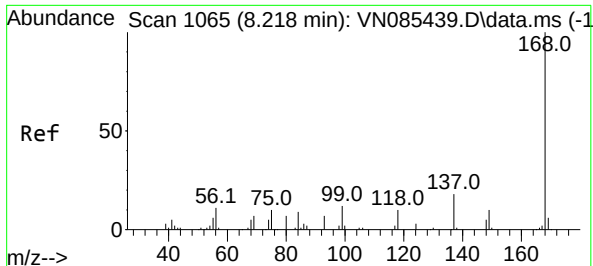


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 194090
Ion Ratio Lower Upper
168 100
99 56.5 53.6 80.4

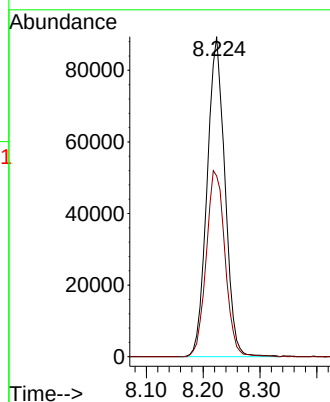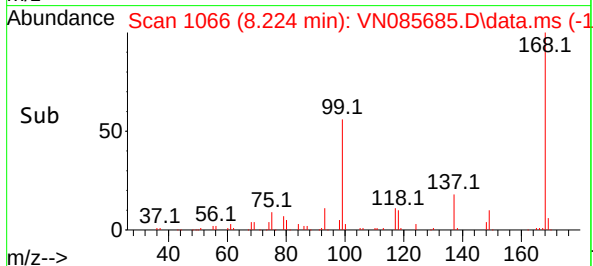

#11
Tert butyl alcohol
Concen: 0.256 ug/l
RT: 5.518 min Scan# 606
Delta R.T. 0.006 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 59 Resp: 92
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0#

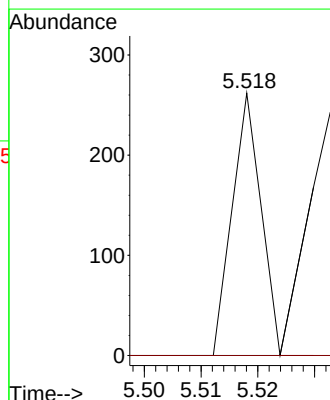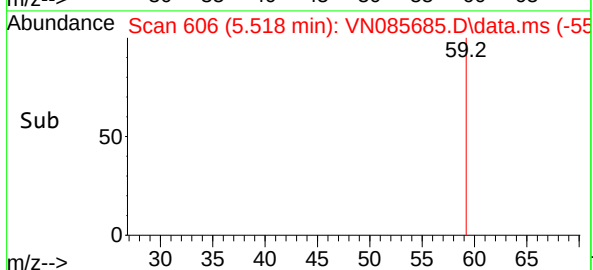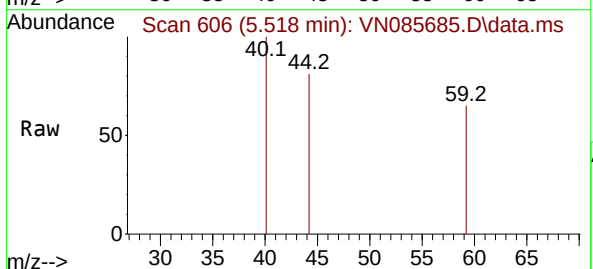



#13

Acrolein

Concen: 0.284 ug/l

RT: 4.183 min Scan# 31

Delta R.T. 0.012 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 56 Resp: 139

Ion Ratio Lower Upper

56 100

55 0.0 56.3 84.5#

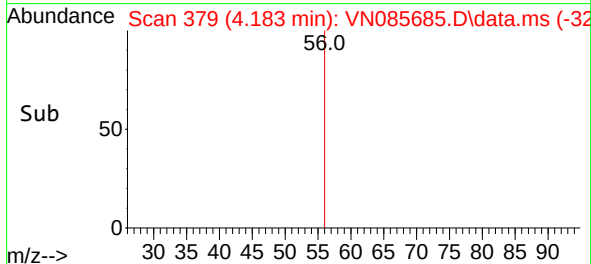

#16

Acetone

Concen: 51.514 ug/l

RT: 4.424 min Scan# 420

Delta R.T. 0.006 min

Lab File: VN085685.D




Acq: 05 Feb 2025 18:23


Tgt Ion: 43 Resp: 52148

Ion Ratio Lower Upper

43 100

58 31.6 23.8 35.6


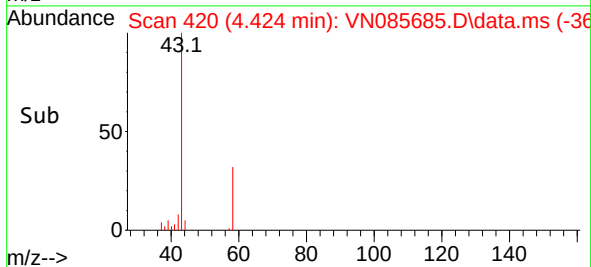

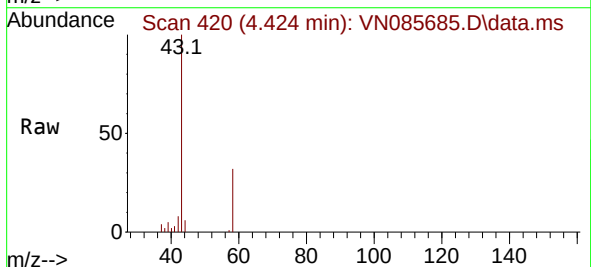




#17
Carbon Disulfide
Concen: 0.652 ug/l
RT: 4.712 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 76 Resp: 4180
Ion Ratio Lower Upper
76 100
78 0.0 6.9 10.3#

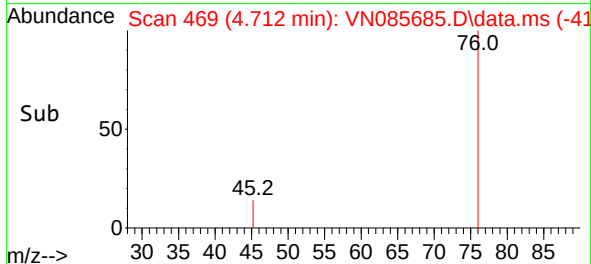

#18
Methyl Acetate
Concen: 0.950 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.012 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23


Tgt Ion: 43 Resp: 2925
Ion Ratio Lower Upper
43 100
74 6.8 18.6 28.0#

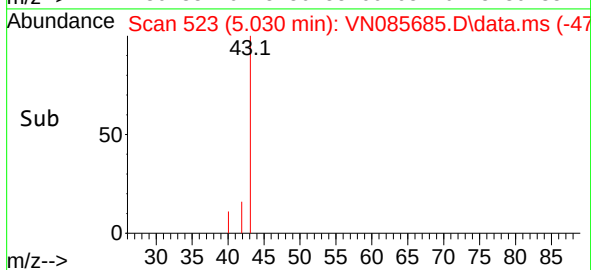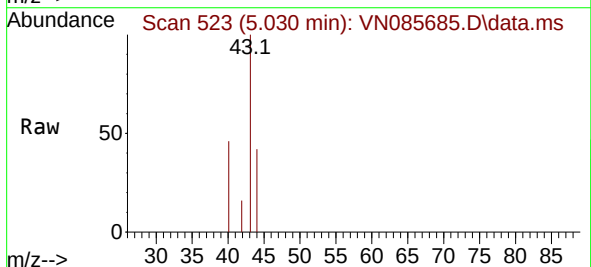






#20
Methylene Chloride
Concen: 0.557 ug/l
RT: 5.283 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	84	Resp:	1396
Ion	Ratio	Lower	Upper
84	100		
49	106.2	104.1	156.1
51	34.6	31.0	46.4
86	49.6	51.9	77.9

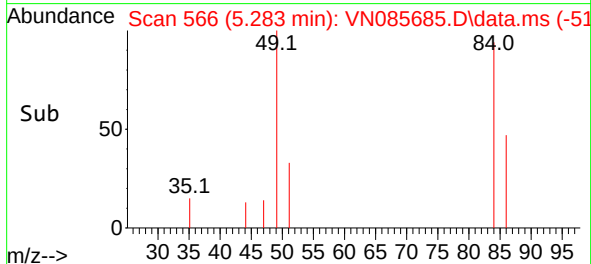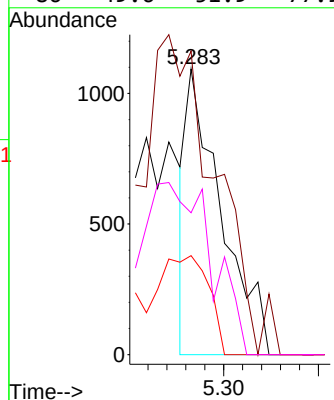

#25
2-Butanone
Concen: 3.787 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.012 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion:	43	Resp:	5642
Ion	Ratio	Lower	Upper
43	100		
72	18.9	20.2	30.4

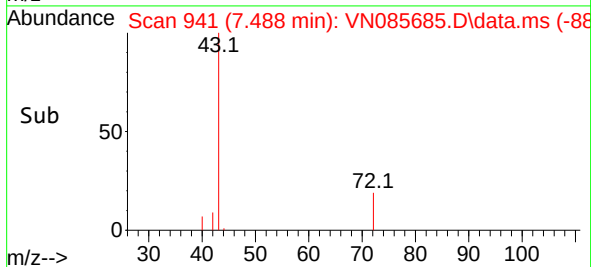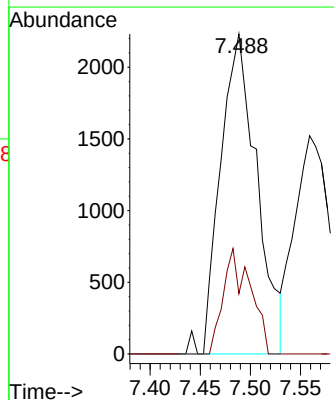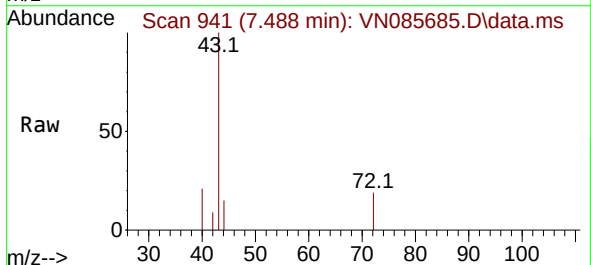



#29

Tetrahydrofuran

Concen: 0.617 ug/l

RT: 7.841 min Scan# 1001

Delta R.T. 0.012 min


Lab File: VN085685.D

Acq: 05 Feb 2025 18:23




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	583
Ion Ratio	Lower	Upper	
42	100		
72	9.1	34.2	51.2#
71	9.4	32.5	48.7#

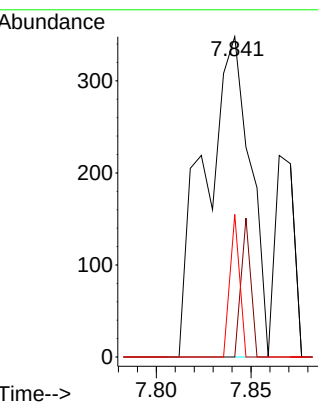

#30

Chloroform

Concen: 0.248 ug/l




RT: 7.971 min Scan# 1023


Delta R.T. 0.012 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23


Tgt Ion:	83	Resp:	1172
Ion Ratio	Lower	Upper	
83	100		
85	52.9	51.8	77.6

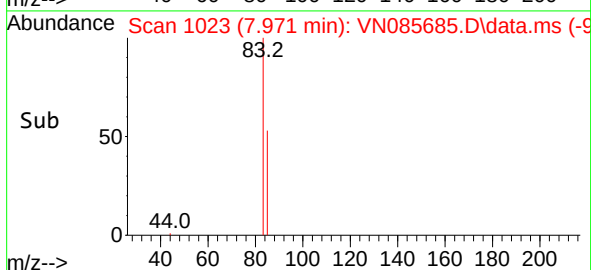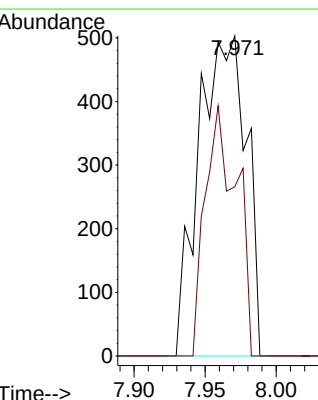






#31
Cyclohexane
Concen: 1.189 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.035 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Instrument :
MSVOA_N
ClientSampleId :



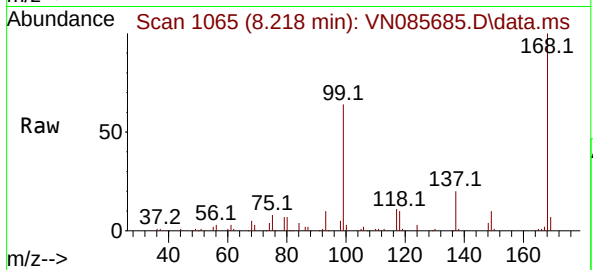



Tgt Ion: 56 Resp: 4726
Ion Ratio Lower Upper
56 100
69 129.0 22.2 33.4#
84 138.2 66.4 99.6#

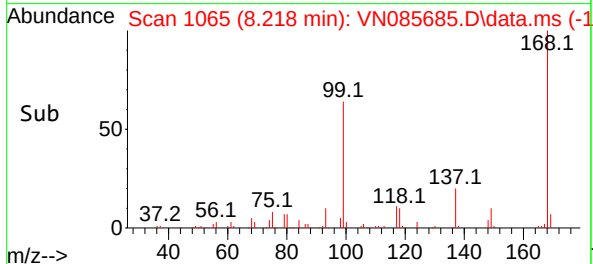

#33
1,2-Dichloroethane-d4
Concen: 48.574 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 65 Resp: 152183
Ion Ratio Lower Upper
65 100
67 51.5 0.0 101.6

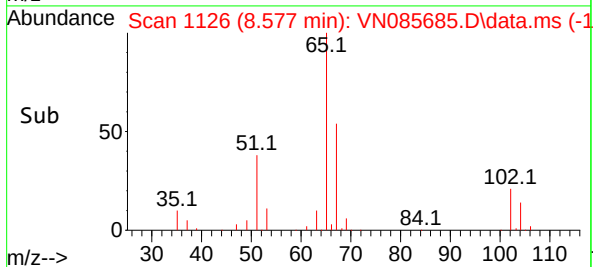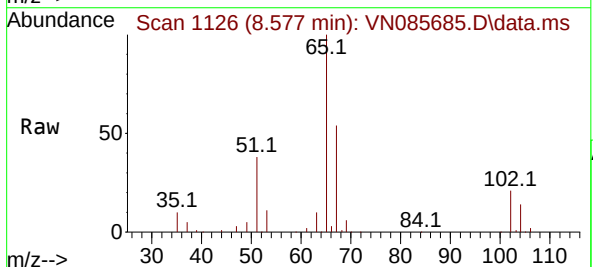

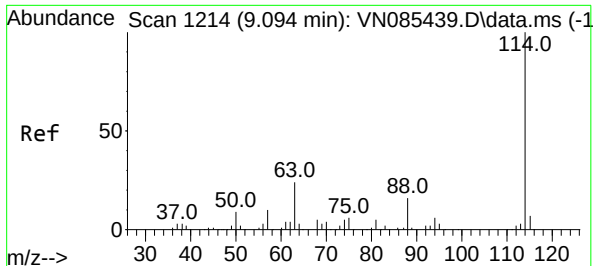

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 379019

Ion Ratio Lower Upper

114 100

63 19.8 0.0 47.6

88 15.9 0.0 32.6

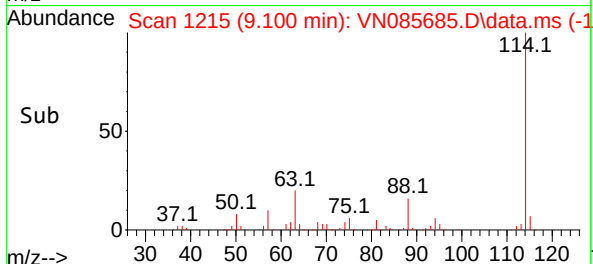

#35

Dibromofluoromethane

Concen: 47.501 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23




Tgt Ion:113 Resp: 124901


Ion Ratio Lower Upper

113 100

111 102.7 82.7 124.1

192 17.3 14.3 21.5

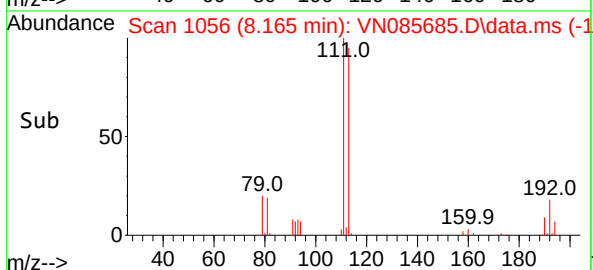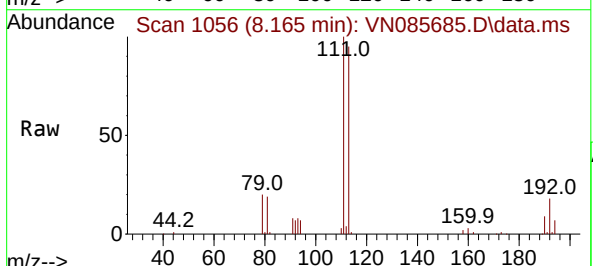



#36

1,1-Dichloropropene

Concen: 4.567 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.141 min


Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 16853

Ion Ratio Lower Upper

75 100

110 9.2 16.5 49.5#

77 0.0 24.4 36.6#



#37

Ethyl Acetate

Concen: 1.067 ug/l

RT: 7.559 min Scan# 953

Delta R.T. 0.006 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23




Tgt Ion: 43 Resp: 3973


Ion Ratio Lower Upper

43 100

61 8.7 10.9 16.3#


70 4.8 7.5 11.3#

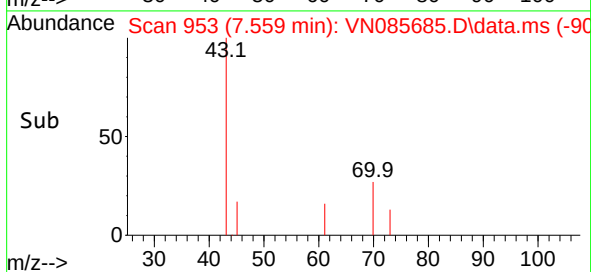






#38
Carbon Tetrachloride
Concen: 4.866 ug/l
RT: 8.224 min Scan# 1003
Delta R.T. -0.135 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Instrument :
MSVOA_N
ClientSampleId :



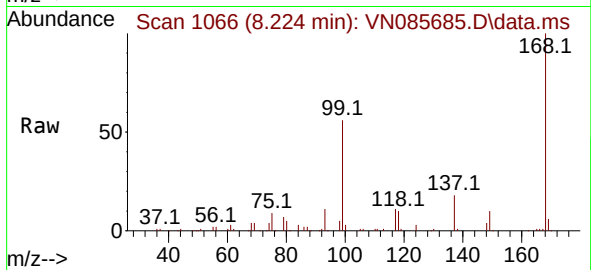



Tgt Ion:117 Resp: 20559
Ion Ratio Lower Upper
117 100
119 5.1 75.4 113.2#
121 0.0 24.6 37.0#

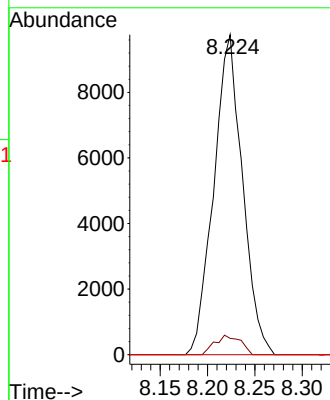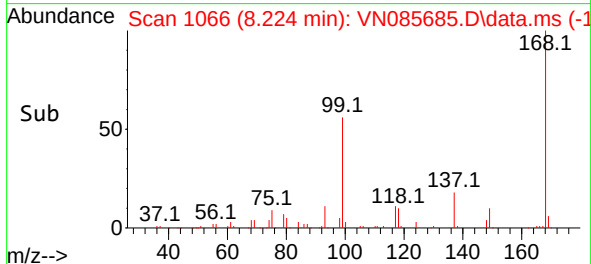

#41
Methacrylonitrile
Concen: 0.350 ug/l
RT: 7.853 min Scan# 1003
Delta R.T. 0.082 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 41 Resp: 679
Ion Ratio Lower Upper
41 100
39 17.5 46.0 69.0#
67 0.0 57.4 86.2#
52 0.0 25.5 38.3#

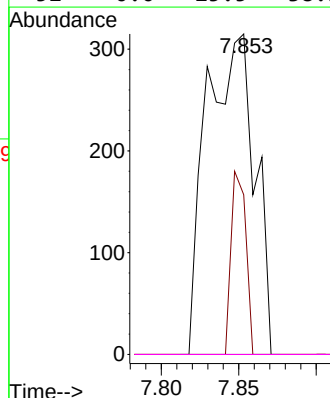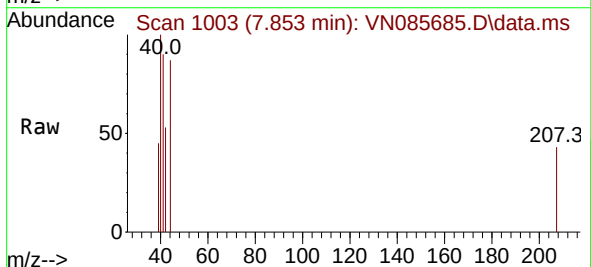

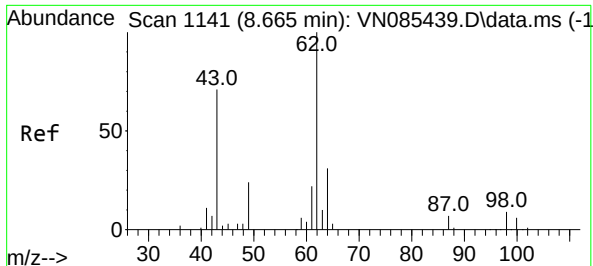

#42

1,2-Dichloroethane

Concen: 0.248 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.024 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 1035

Ion Ratio Lower Upper

62 100

98 0.0 0.0 17.0

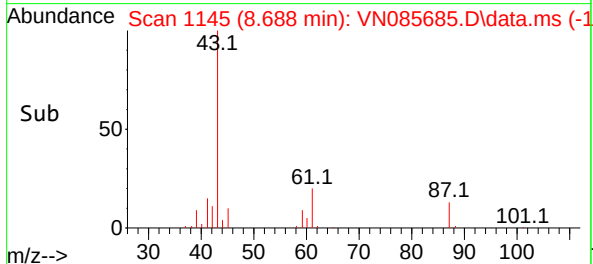

#43

Isopropyl Acetate

Concen: 27.489 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.006 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23




Tgt Ion: 43 Resp: 164070


Ion Ratio Lower Upper

43 100

61 17.2 20.7 31.1#

87 11.6 9.8 14.8

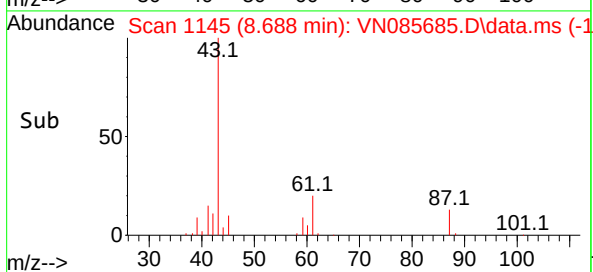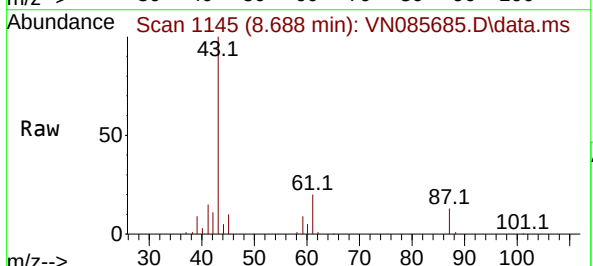

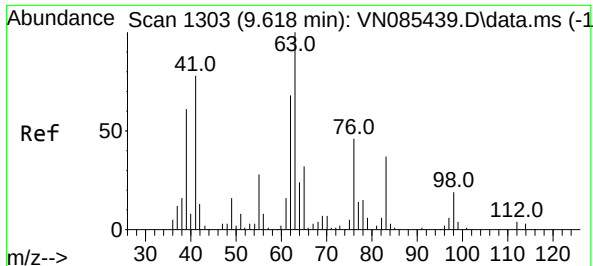

#45

1,2-Dichloropropane

Concen: 0.590 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.124 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 63 Resp: 1672

Ion Ratio Lower Upper

63 100

65 0.0 25.6 38.4#

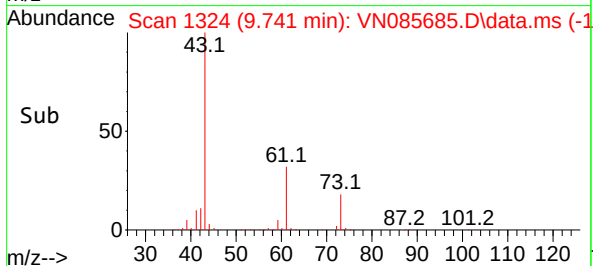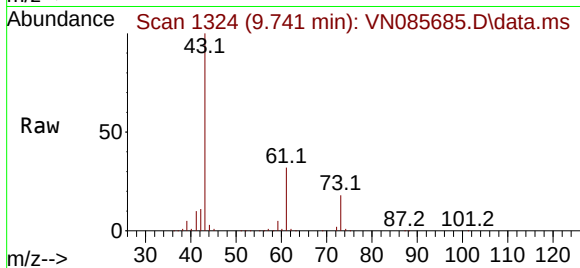

#48

Methyl methacrylate

Concen: 47.583 ug/l

RT: 9.741 min Scan# 1324

Delta R.T. 0.064 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23




Tgt Ion: 41 Resp: 127808


Ion Ratio Lower Upper

41 100

69 0.1 64.7 97.1#

39 55.3 49.0 73.6

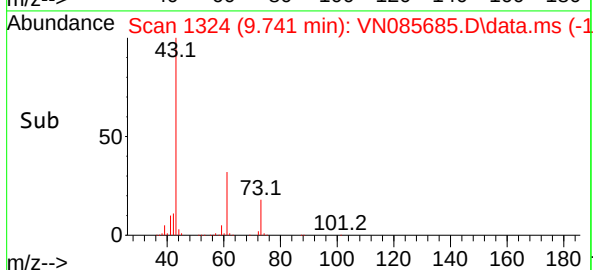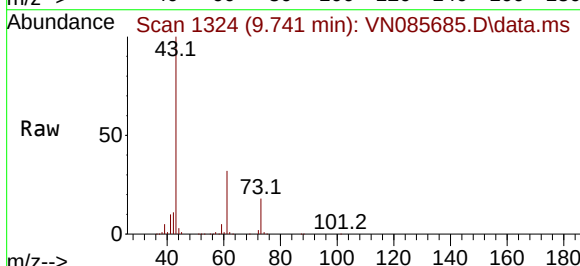

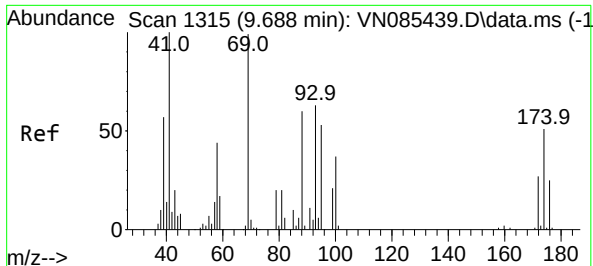

#49

1,4-Dioxane

Concen: 3.803 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.053 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 88 Resp: 172

Ion Ratio Lower Upper

88 100

43 757102.3 26.6 39.8#

58 4314.0 59.5 89.3#

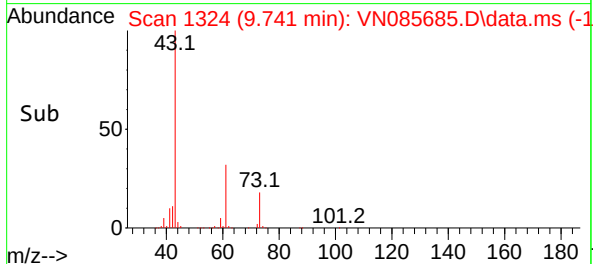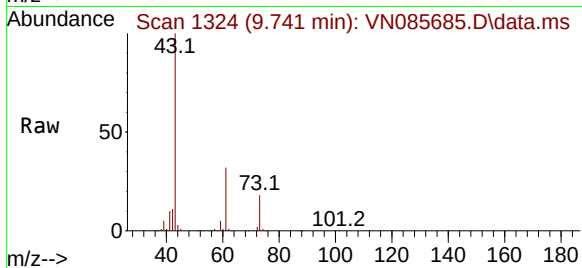

#50

Toluene-d8

Concen: 51.566 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.000 min

Lab File: VN085685.D




Acq: 05 Feb 2025 18:23


Tgt Ion: 98 Resp: 481747

Ion Ratio Lower Upper

98 100

100 64.2 52.2 78.4




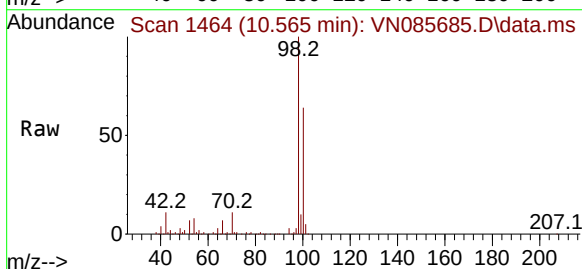




#51
4-Methyl-2-Pentanone
Concen: 3.145 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 10894
Ion Ratio Lower Upper
43 100
58 24.9 30.5 45.7#

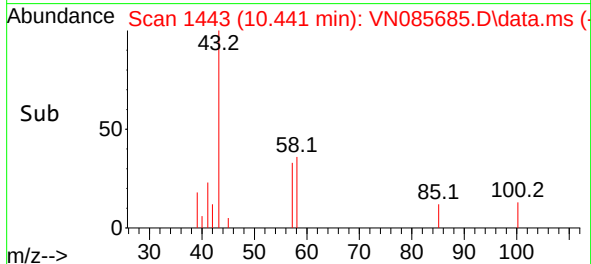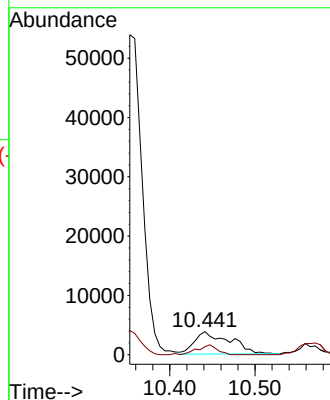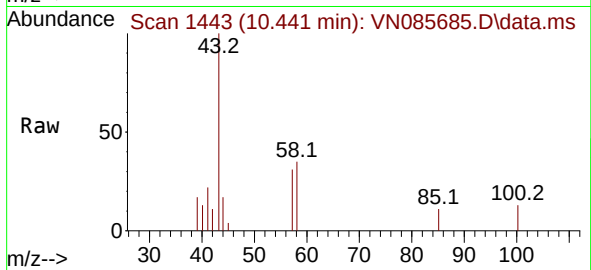

#53
t-1,3-Dichloropropene
Concen: 0.247 ug/l
RT: 10.724 min Scan# 1491
Delta R.T. -0.112 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 75 Resp: 970
Ion Ratio Lower Upper
75 100
77 30.4 23.5 35.3


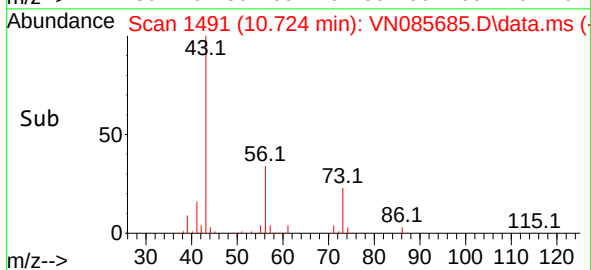
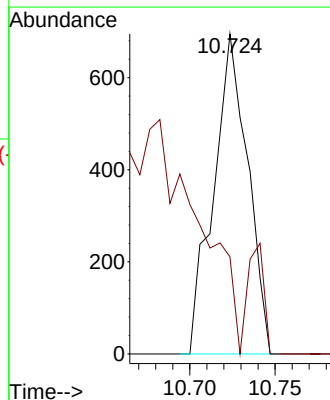
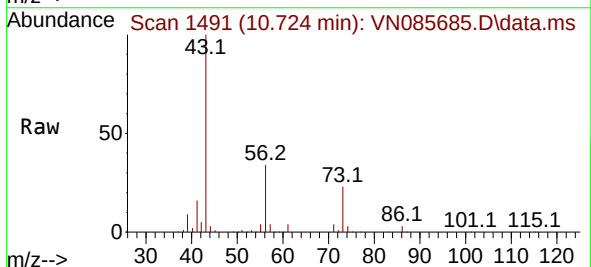




#54
cis-1,3-Dichloropropene
Concen: 11.430 ug/l
RT: 10.353 min Scan# 1428
Delta R.T. 0.047 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 48041
Ion Ratio Lower Upper
75 100
77 0.0 25.0 37.4#
39 31.7 43.1 64.7#

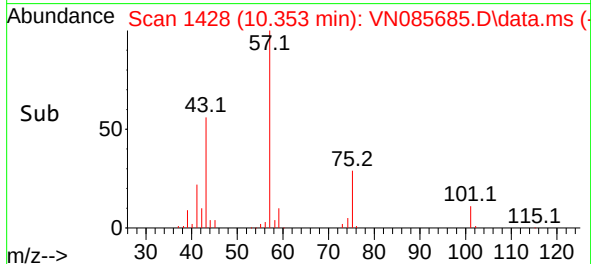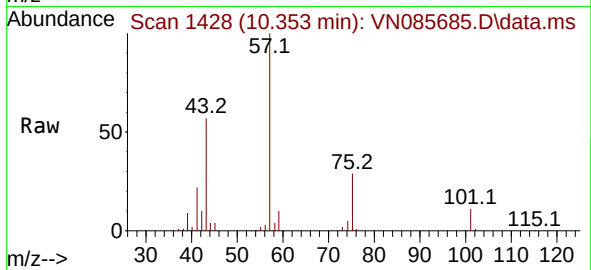

#56
Ethyl methacrylate
Concen: 2.274 ug/l
RT: 10.982 min Scan# 1535
Delta R.T. 0.111 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 69 Resp: 1528
Ion Ratio Lower Upper
69 100
41 4394.5 54.6 82.0#
39 2064.9 32.4 48.6#

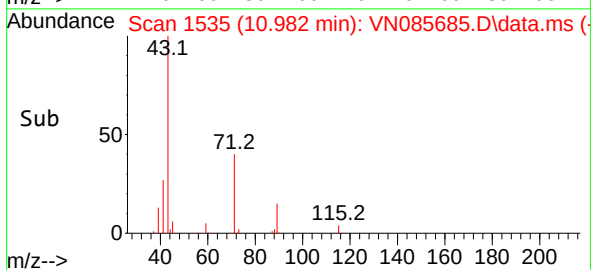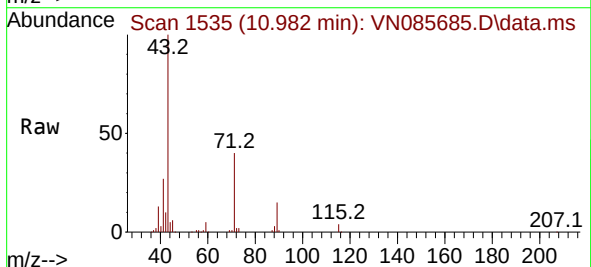



#57

1,3-Dichloropropane

Concen: 1.572 ug/l

RT: 11.194 min Scan# 1571

Delta R.T. 0.035 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 6948

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

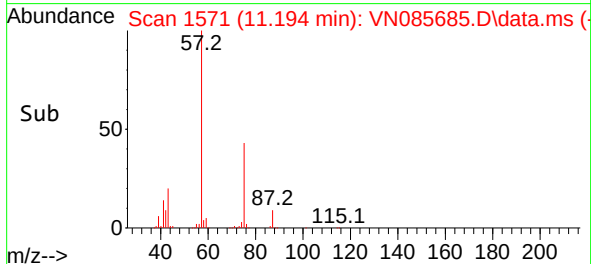

#59

2-Hexanone

Concen: 29.137 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.012 min

Lab File: VN085685.D




Acq: 05 Feb 2025 18:23


Tgt Ion: 43 Resp: 71009

Ion Ratio Lower Upper

43 100

58 26.2 26.2 78.6#


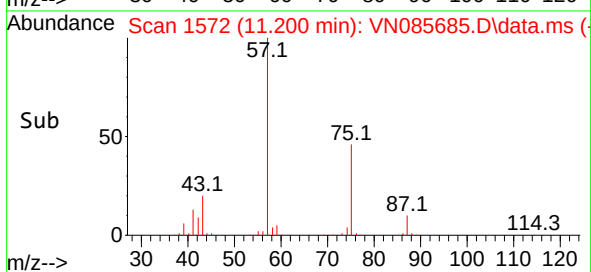






#62
4-Bromofluorobenzene
Concen: 44.695 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 142837
Ion Ratio Lower Upper
95 100
174 77.7 0.0 145.0
176 73.4 0.0 142.4

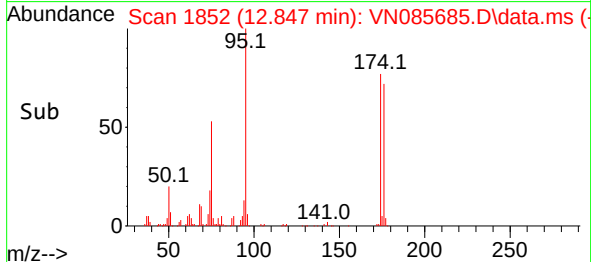

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 117 Resp: 348070
Ion Ratio Lower Upper
117 100
82 58.9 48.6 72.8
119 30.9 26.6 39.8

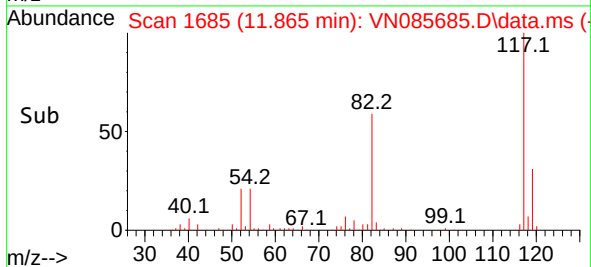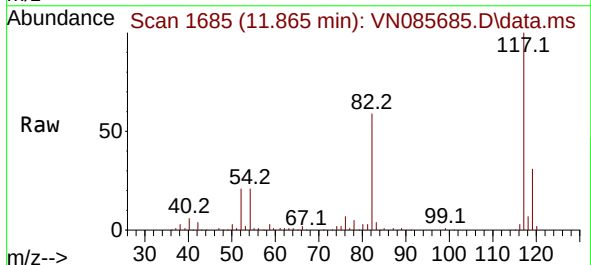



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 20

Delta R.T. 0.000 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:152 Resp: 136813

Ion Ratio Lower Upper

152 100

115 61.0 31.1 93.3

150 158.7 0.0 343.6



#74

N-ethyl acetate

Concen: 0.339 ug/l

RT: 12.459 min Scan# 1786

Delta R.T. -0.029 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Tgt Ion: 43 Resp: 1409




Ion Ratio Lower Upper


43 100

70 0.0 34.0 51.0#

55 0.0 21.4 32.2#

61 0.0 19.0 28.4#


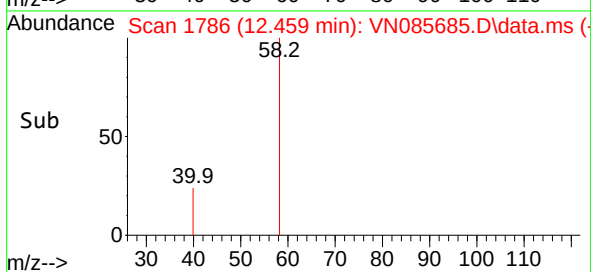






#76
1,2,3-Trichloropropane
Concen: 27.599 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 76747
Ion Ratio Lower Upper
75 100
77 1.6 109.7 329.2#

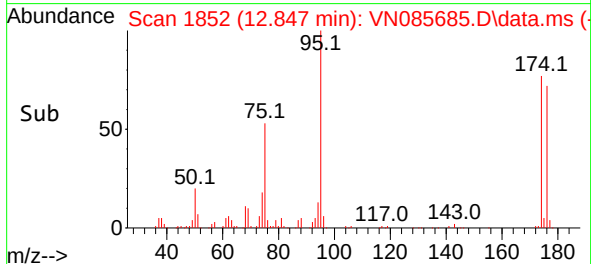

#81
trans-1,4-Dichloro-2-butene
Concen: 74.672 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN085685.D
Acq: 05 Feb 2025 18:23

Tgt Ion: 75 Resp: 76747
Ion Ratio Lower Upper
75 100
53 0.1 95.6 143.4#
89 0.0 37.0 55.6#

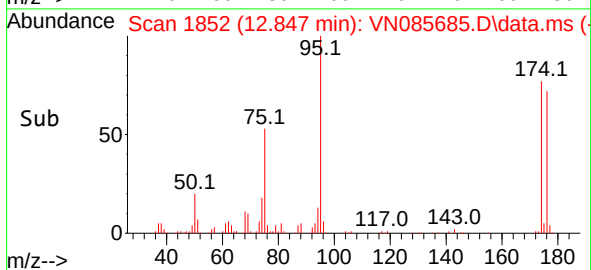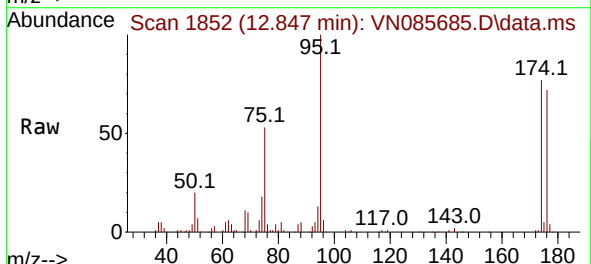



#86

p-Isopropyltoluene

Concen: 1.326 ug/l

RT: 13.729 min Scan# 2001

Delta R.T. 0.006 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:119 Resp: 9171

Ion Ratio Lower Upper

119 100

134 18.8 12.7 38.0

91 28.7 12.7 38.1

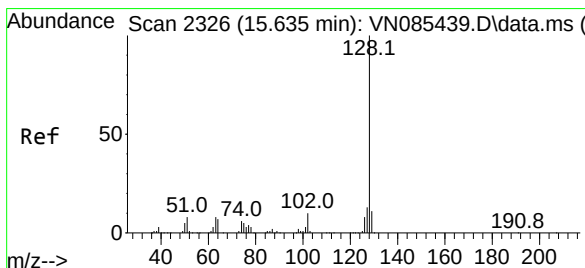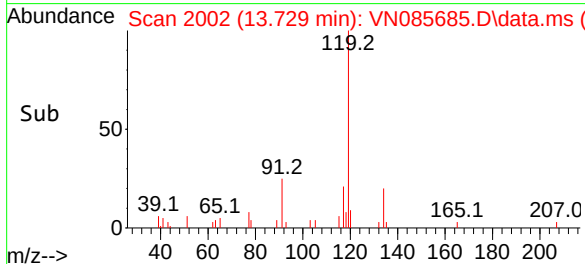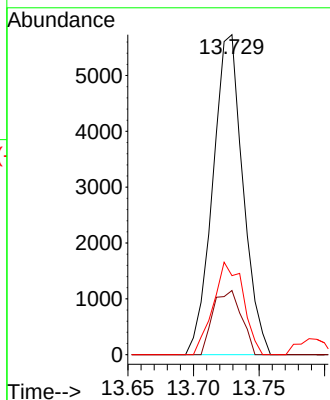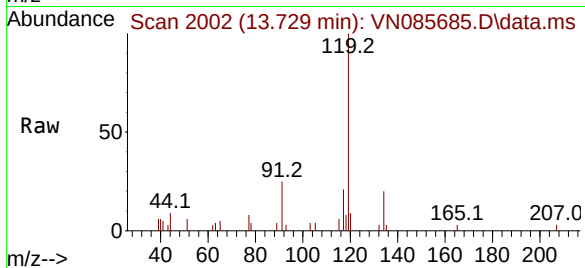

#95

Naphthalene

Concen: 4.650 ug/l

RT: 15.635 min Scan# 2326

Delta R.T. 0.000 min

Lab File: VN085685.D

Acq: 05 Feb 2025 18:23

Tgt Ion:128 Resp: 28580

Ion Ratio Lower Upper

128 100

127 14.4 10.6 16.0

129 11.3 8.8 13.2

