


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020525\
Data File : VN085665.D
Acq On : 05 Feb 2025 08:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

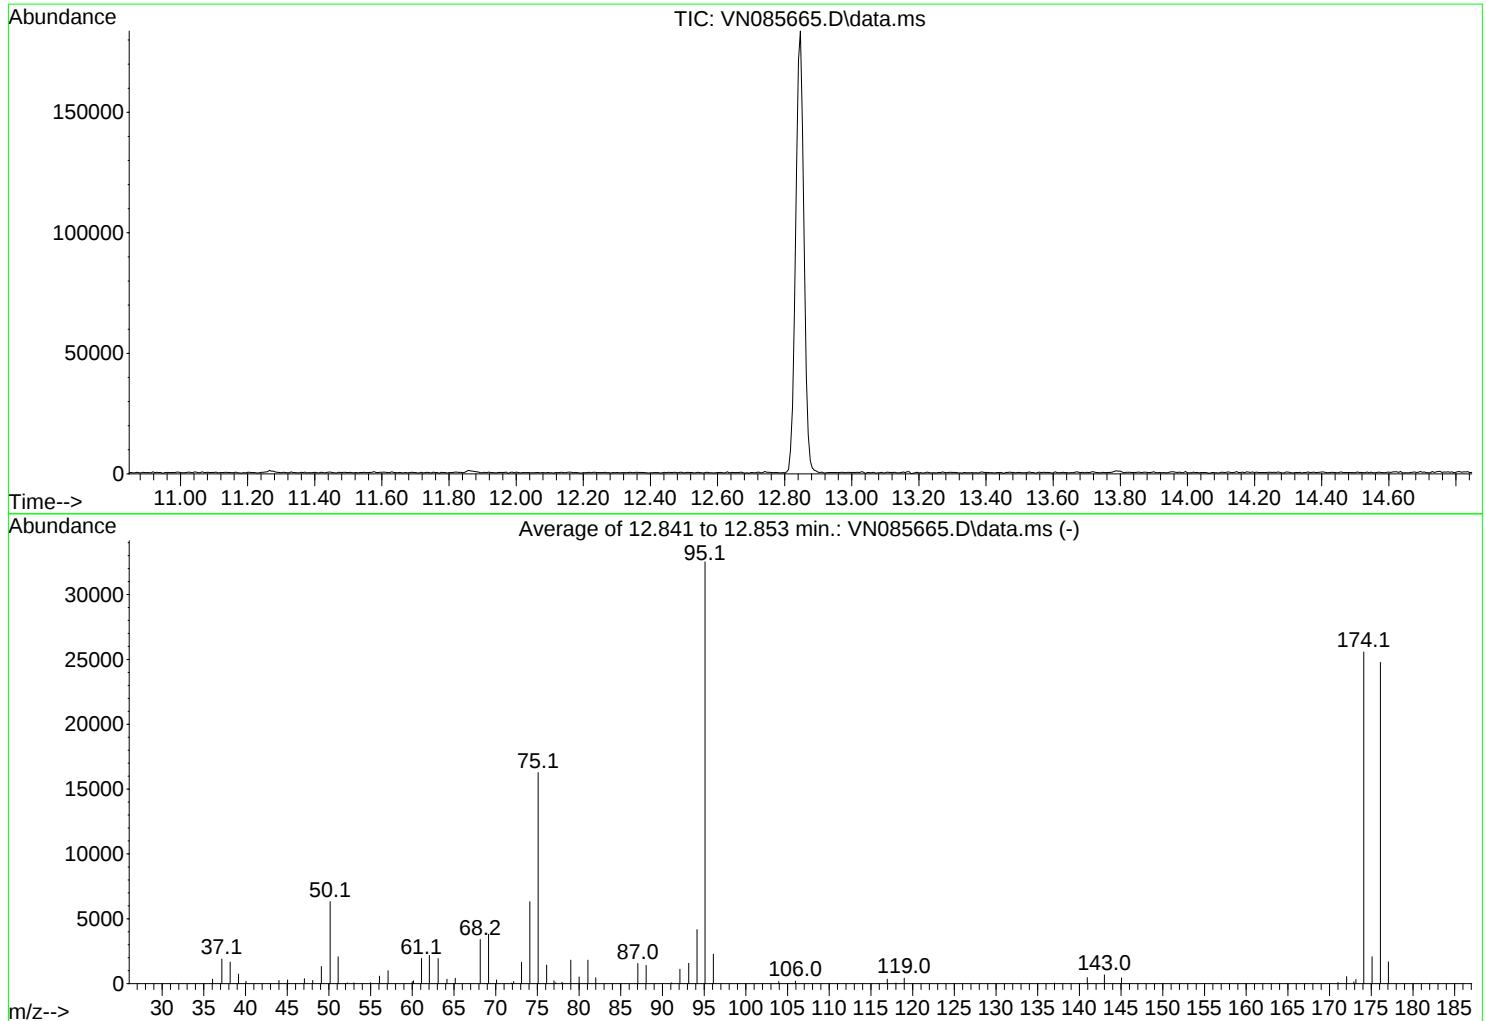

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	6325	PASS
75	95	30	60	50.0	16277	PASS
95	95	100	100	100.0	32523	PASS
96	95	5	9	7.0	2287	PASS
173	174	0.00	2	1.3	325	PASS
174	95	50	100	78.6	25571	PASS
175	174	5	9	8.1	2073	PASS
176	174	95	101	96.9	24768	PASS
177	176	5	9	6.8	1684	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	341	51.10	2069	64.15	351	77.00	221
37.15	1896	52.20	58	65.15	422	77.20	81
38.15	1662	53.00	68	68.15	3410	77.95	111
39.15	747	55.00	78	69.15	3809	79.00	181
40.05	186	56.05	578	70.10	279	80.00	524
44.00	243	57.10	1002	71.90	53	81.05	1809
45.05	289	60.00	158	72.15	169	82.00	462
47.05	389	60.15	224	73.10	1639	87.05	1552
48.05	245	61.10	1940	74.10	6315	88.05	1403
49.10	1321	62.05	2184	75.10	16277	91.10	57
50.15	6325	63.10	1942	76.10	1433	92.10	1116

Average of 12.841 to 12.853 min.: VN085665.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.15	1562	143.00	678				
94.15	4177	145.05	444				
95.10	32523	171.00	84				
96.10	2287	172.05	542				
103.95	162	172.90	138				
105.95	196	173.15	325				
116.95	340	174.10	25571				
118.00	52	175.10	2073				
119.00	416	176.10	24768				
137.00	50	177.05	1684				
140.95	464						

Instrument :

MSVOA_N

ClientSampleId :

BFB