


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN020619\
Data File : VN053623.D
Acq On : 6 Feb 2019 9:22
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

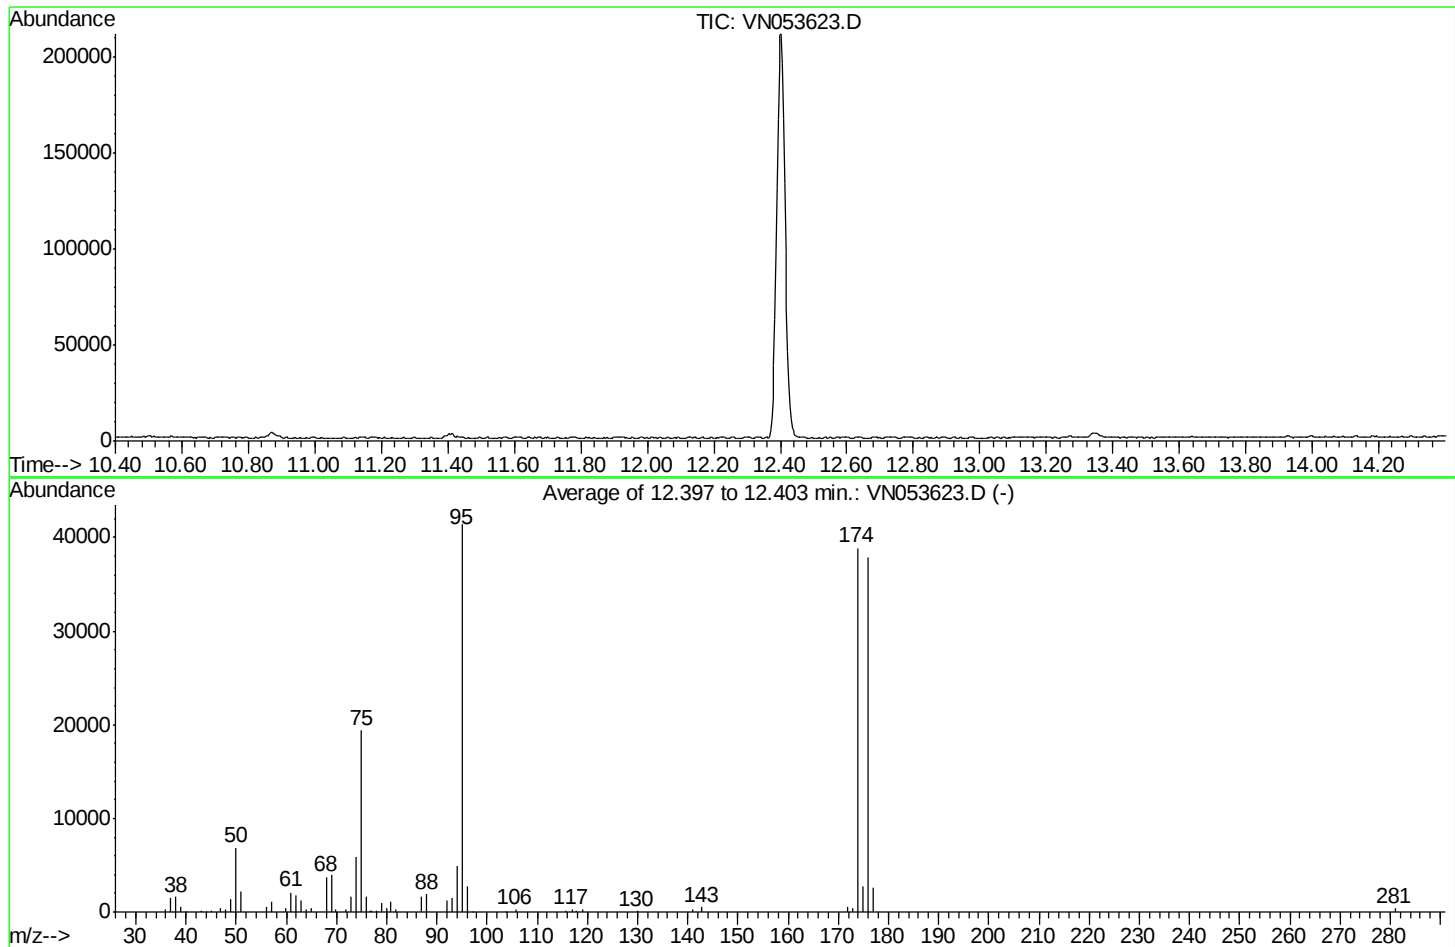

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	6904	PASS
75	95	30	60	46.9	19405	PASS
95	95	100	100	100.0	41410	PASS
96	95	5	9	6.5	2702	PASS
173	174	0.00	2	1.2	466	PASS
174	95	50	100	93.9	38877	PASS
175	174	5	9	7.2	2787	PASS
176	174	95	101	97.4	37858	PASS
177	176	5	9	6.7	2535	PASS