
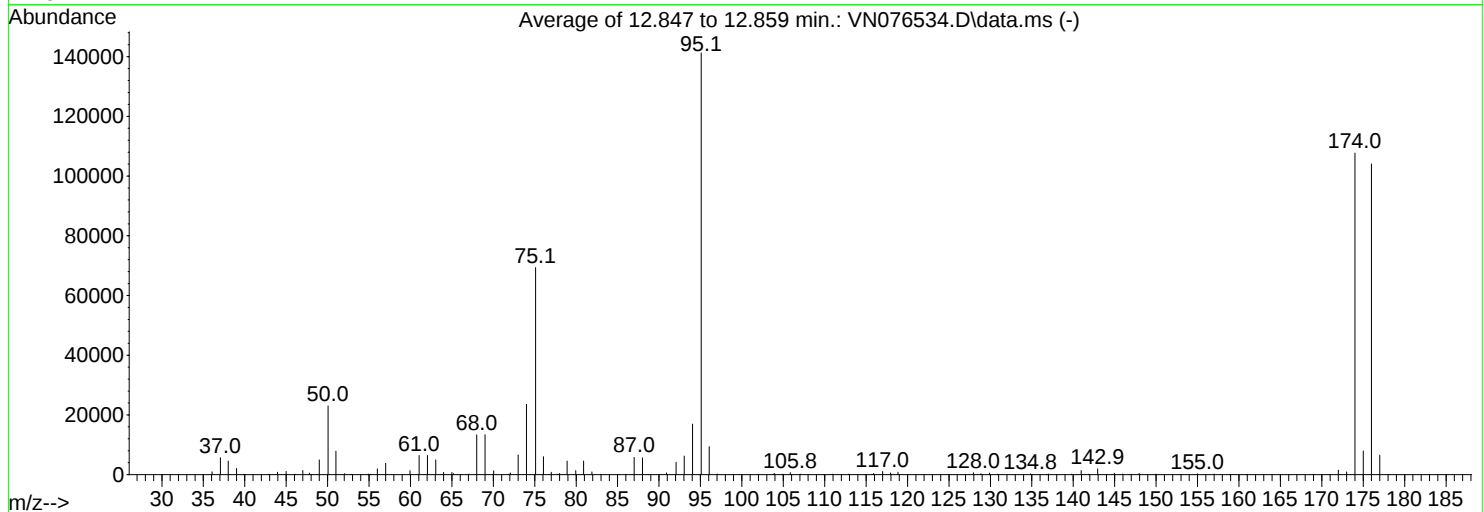


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020623\
Data File : VN076534.D
Acq On : 06 Feb 2023 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020623W.M
Title : SW846 8260
Last Update : Tue Feb 07 01:44:01 2023

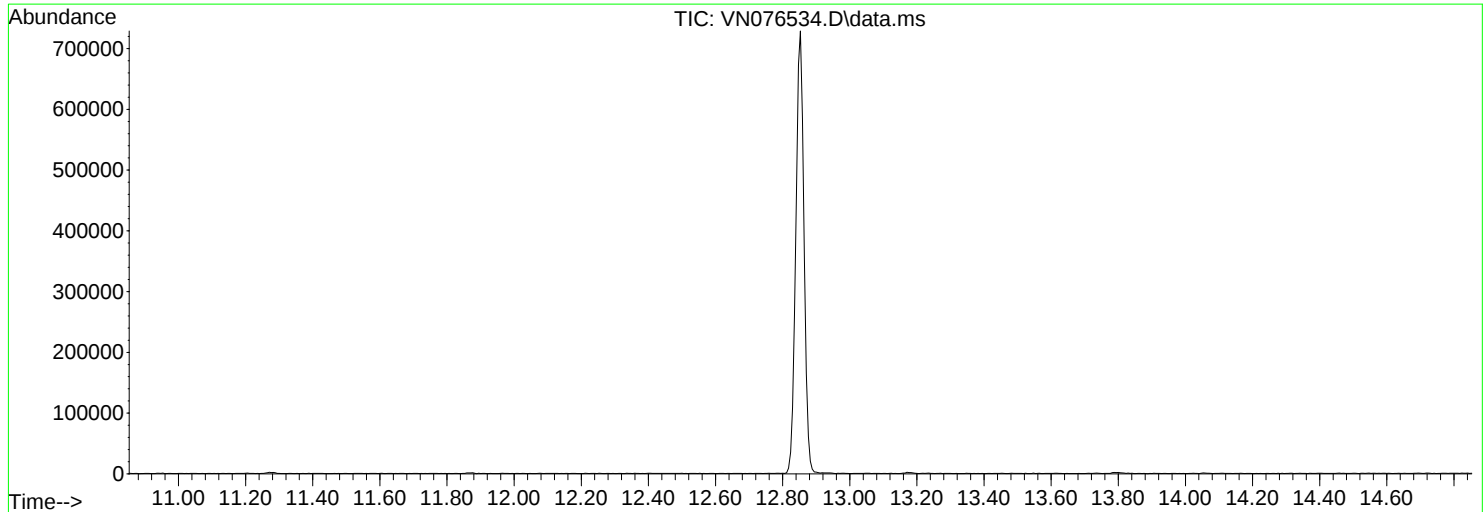

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	23040	PASS
75	95	30	60	49.1	69331	PASS
95	95	100	100	100.0	141277	PASS
96	95	5	9	6.6	9387	PASS
173	174	0.00	2	0.8	901	PASS
174	95	50	100	76.2	107723	PASS
175	174	5	9	7.4	7926	PASS
176	174	95	101	96.6	104072	PASS
177	176	5	9	6.3	6544	PASS

Average of 12.847 to 12.859 min.: VN076534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	954	48.00	132	59.95	1344	69.00	1342
37.05	5694	49.00	4932	61.05	6430	70.05	1281
38.00	4563	50.05	23040	62.05	6413	71.80	18
39.00	2024	51.00	7901	63.05	4929	72.05	57
39.90	12	52.05	325	64.00	755	73.00	6591
42.85	105	52.90	105	65.00	738	74.00	23595
43.95	794	54.90	195	65.20	338	75.10	69331
45.00	1071	55.20	96	66.10	84	76.05	6016
46.10	96	56.00	1920	66.80	77	77.00	829
47.00	1419	57.00	3838	67.05	196	77.80	190
47.80	544	58.00	78	68.00	13327	78.00	388

Average of 12.847 to 12.859 min.: VN076534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	4561	93.05	6247	110.90	170	129.90	550
79.95	1330	94.05	16960	112.00	52	130.85	185
80.90	4559	95.10	141277	112.85	157	134.85	254
81.90	913	96.05	9387	114.80	51	136.80	90
82.95	119	97.05	196	115.70	134	137.00	238
86.00	169	103.80	195	115.90	365	139.80	150
87.00	5814	103.95	371	117.00	1055	140.95	1398
88.00	5647	104.95	141	117.95	583	141.85	143
88.80	69	105.85	721	118.85	818	142.95	1916
90.90	622	107.05	207	127.95	639	144.00	59
92.05	4151	109.90	50	128.85	332	144.95	471

Average of 12.847 to 12.859 min.: VN076534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
145.95	194	172.00	1527				
146.80	60	173.00	901				
147.05	153	174.00	107723				
147.95	410	175.00	7926				
149.90	142	176.00	104072				
152.95	126	177.00	6544				
155.00	295	178.10	64				
157.00	247						
158.90	61						
160.95	132						
170.90	55						

Instrument :

MSVOA_N

ClientSampleId :

BFB