


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN020719\
Data File : VN053645.D
Acq On : 7 Feb 2019 9:58
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

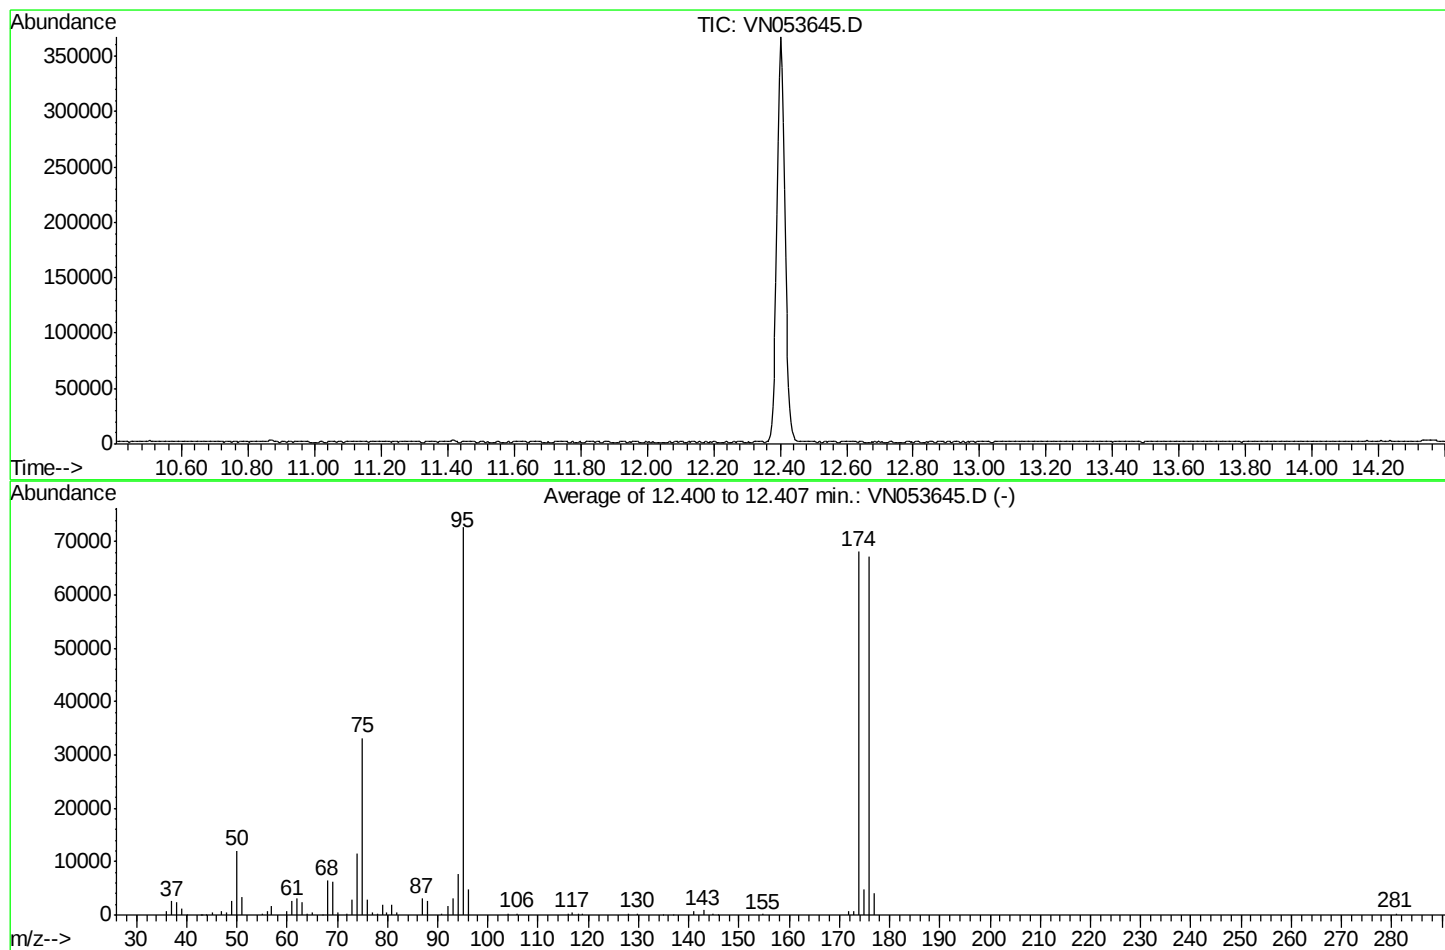

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12069	PASS
75	95	30	60	45.7	33224	PASS
95	95	100	100	100.0	72666	PASS
96	95	5	9	6.8	4916	PASS
173	174	0.00	2	0.9	639	PASS
174	95	50	100	93.7	68114	PASS
175	174	5	9	7.1	4859	PASS
176	174	95	101	98.5	67069	PASS
177	176	5	9	6.2	4158	PASS