

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN020720\
 Data File : VN060023.D
 Acq On : 7 Feb 2020 11:58
 Operator : JC/MD
 Sample : L1431-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 07 23:12:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 18 03:09:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	197297	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	306287	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	291139	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	135795	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	114732	52.36	ug/l	0.00
Spiked Amount			Recovery	=	104.72%	
35) Dibromofluoromethane	7.57	113	94226	51.59	ug/l	0.00
Spiked Amount			Recovery	=	103.18%	
50) Toluene-d8	10.08	98	371961	52.56	ug/l	0.00
Spiked Amount			Recovery	=	105.12%	
62) 4-Bromofluorobenzene	12.40	95	136348	53.44	ug/l	0.00
Spiked Amount			Recovery	=	106.88%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.79	43	6684	Below Cal		95
18) Methyl Acetate	4.30	43	989	0.386	ug/l #	54
20) Methylene Chloride	4.53	84	6213	1.889	ug/l #	78
31) Cyclohexane	7.65	56	3996	1.233	ug/l #	7
36) 1,1-Dichloropropene	7.64	75	13452	5.043	ug/l #	50
38) Carbon Tetrachloride	7.64	117	19014	6.553	ug/l #	15
43) Isopropyl Acetate	8.14	43	44386	10.315	ug/l #	90
45) 1,2-Dichloropropane	9.25	63	948	0.482	ug/l #	44
48) Methyl methacrylate	9.17	41	2385	1.239	ug/l #	13
51) 4-Methyl-2-Pentanone	9.97	43	3424	1.377	ug/l	89
54) cis-1,3-Dichloropropene	9.89	75	20047	6.098	ug/l #	59
57) 1,3-Dichloropropane	10.75	76	3577	1.132	ug/l #	42
59) 2-Hexanone	10.75	43	46211	25.218	ug/l #	54
74) N-amyl acetate	12.03	43	2206	0.571	ug/l #	45
76) 1,2,3-Trichloropropane	12.40	75	69194	30.278	ug/l #	100
78) n-propylbenzene	12.59	91	3929	0.351	ug/l	93
80) 1,3,5-Trimethylbenzene	12.73	105	2636	0.315	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.40	75	69194	65.022	ug/l #	11
83) tert-Butylbenzene	13.04	119	2085	0.288	ug/l #	72
84) 1,2,4-Trimethylbenzene	13.04	105	16382	1.977	ug/l	98
89) n-Butylbenzene	13.61	91	3251	0.433	ug/l #	67
90) Hexachloroethane	13.89	117	1252	0.760	ug/l #	12
92) 1,2-Dibromo-3-Chloropropan	14.23	75	133	Below Cal	#	6
93) 1,2,4-Trichlorobenzene	14.91	180	694	0.267	ug/l #	74
95) Naphthalene	15.13	128	186200	25.154	ug/l	99
96) 1,2,3-Trichlorobenzene	15.32	180	635	0.251	ug/l #	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN020720\
Data File : VN060023.D
Acq On : 7 Feb 2020 11:58
Operator : JC/MD
Sample : L1431-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 07 23:12:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Quant Title : SW846 8260
QLast Update : Sat Jan 18 03:09:32 2020
Response via : Initial Calibration

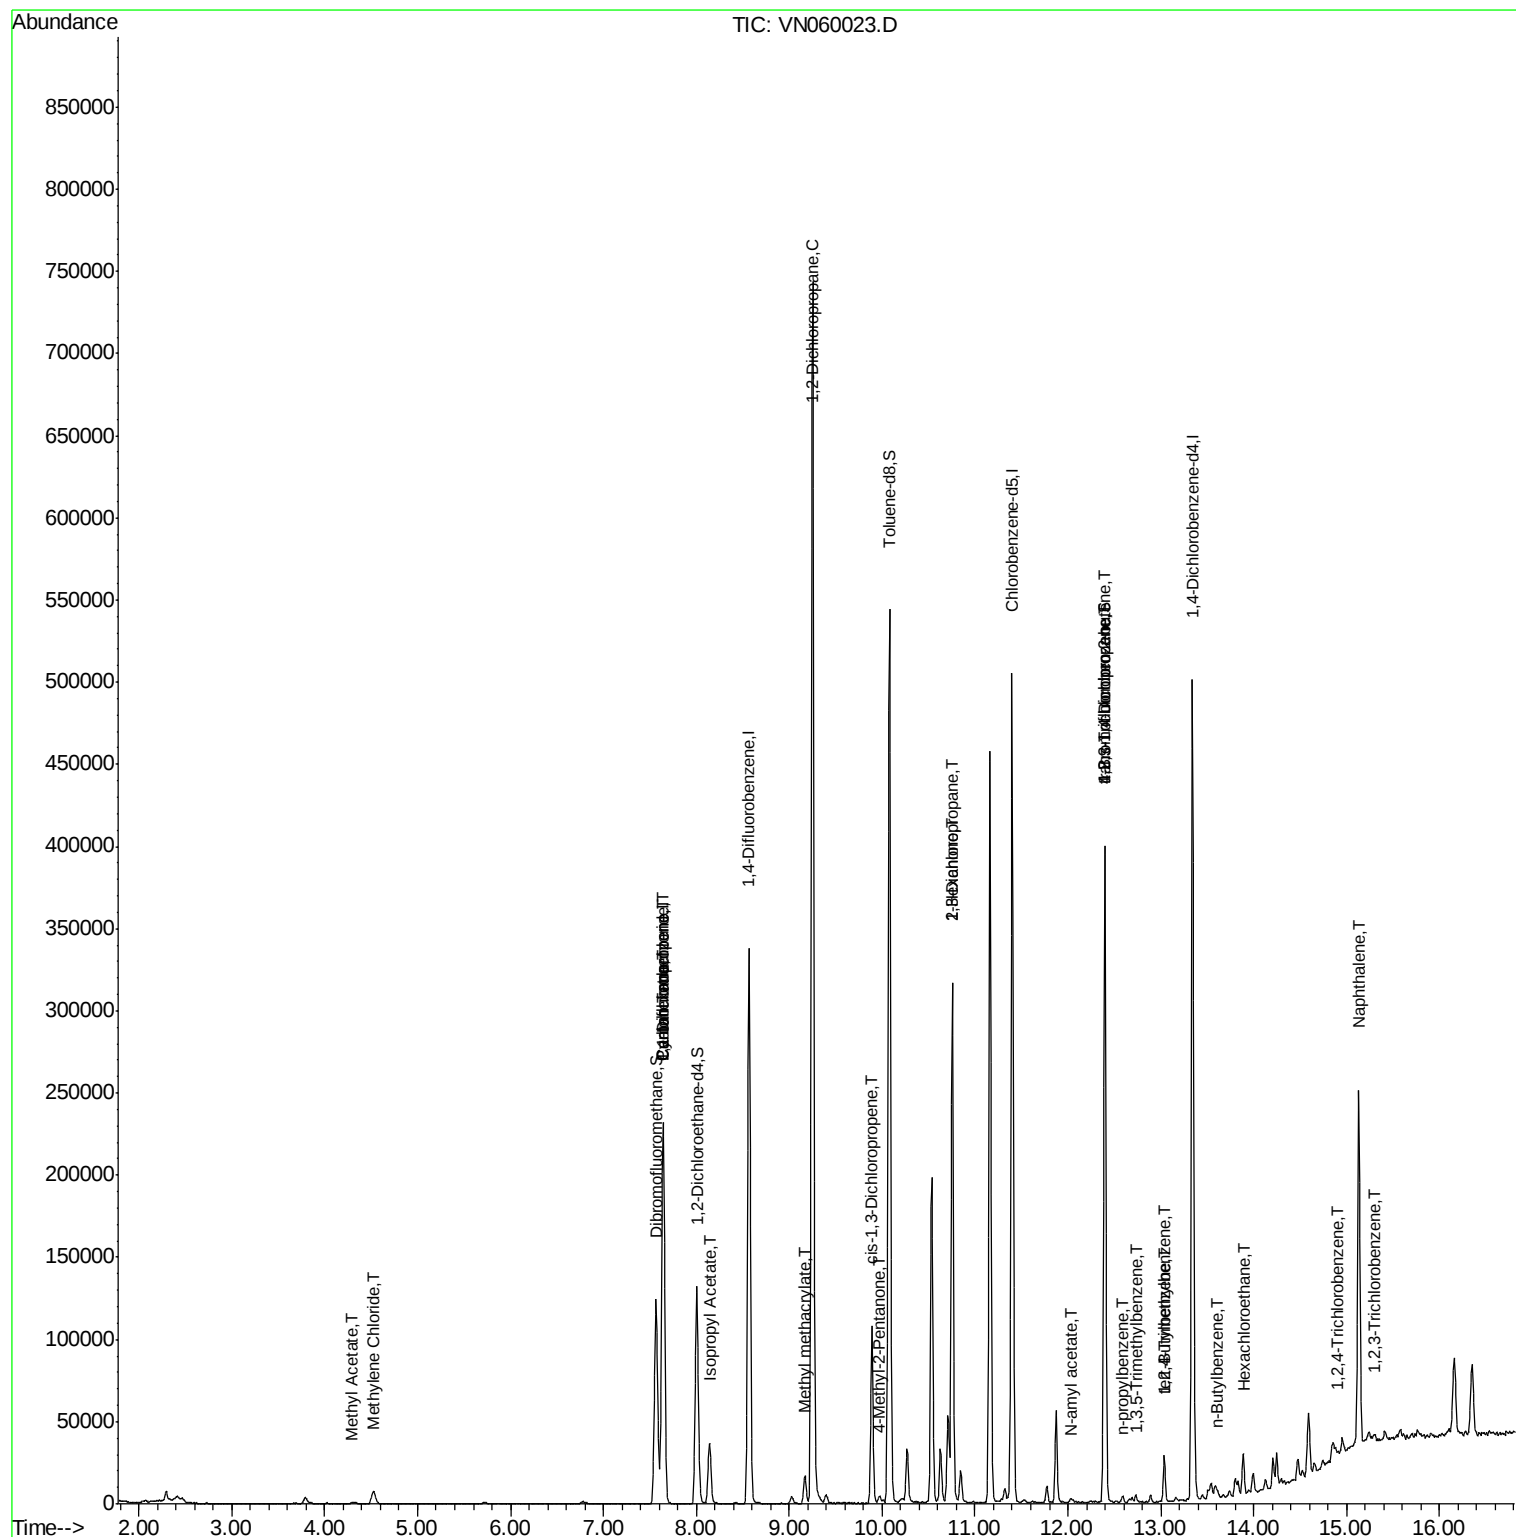



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. 0.00 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58


Instrument :
MSVOA_N
ClientSampled :

Tot Ion:168 Resp: 197297

Ion Ratio Lower Upper




168 100

99 54.7 48.2 72.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

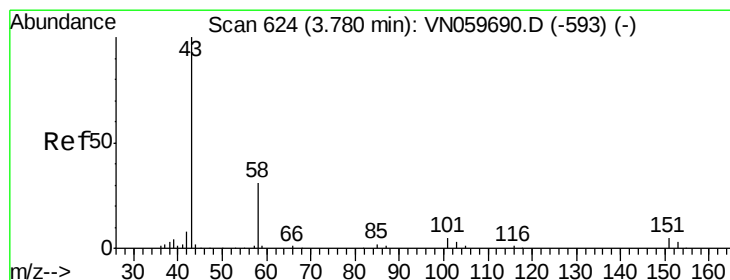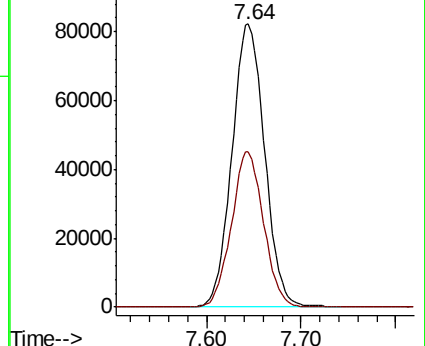

#16

Acetone

Concen: Below Cal

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN060023.D


Acq: 7 Feb 2020 11:58

Tgt Ion: 43 Resp: 6684

Ion Ratio Lower Upper



43 100


58 32.2 23.6 35.4

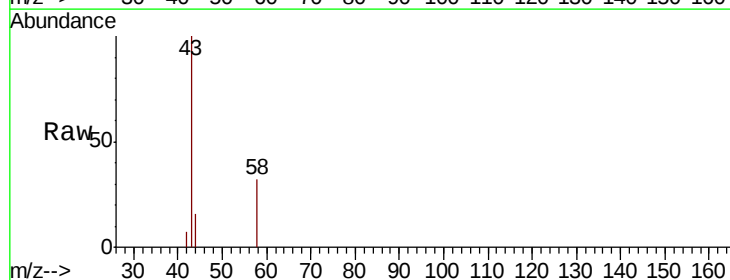

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0


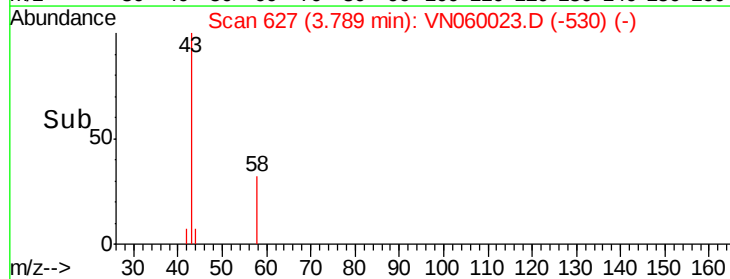
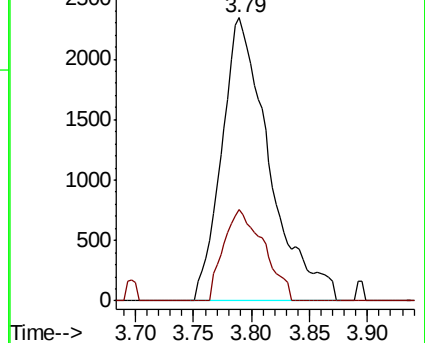


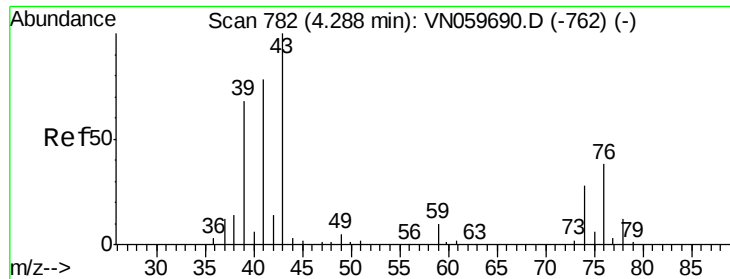

#18
Methyl Acetate
Concen: 0.386 ug/l
RT: 4.30 min Scan# 785
Delta R.T. 0.01 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 43 Resp: 989
Ion Ratio Lower Upper
43 100
74 0.0 17.5 26.3#

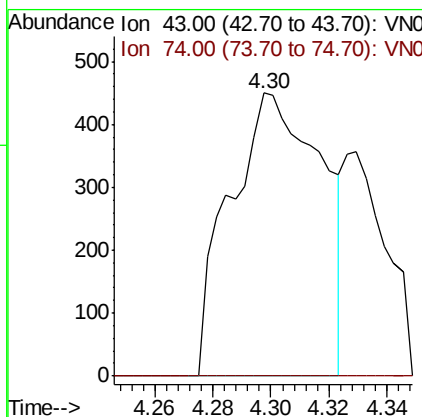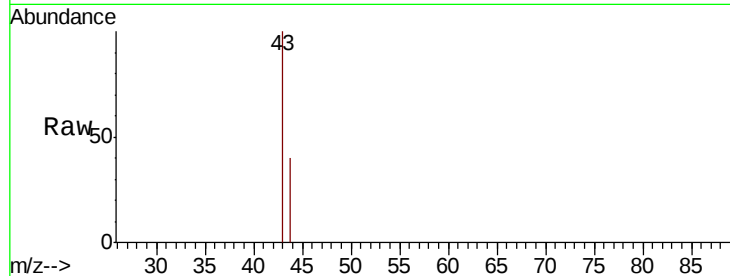

#20
Methylene Chloride
Concen: 1.889 ug/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Tgt Ion: 84 Resp: 6213
Ion Ratio Lower Upper
84 100
49 99.0 106.6 160.0#
51 30.6 31.9 47.9#
86 55.1 50.8 76.2

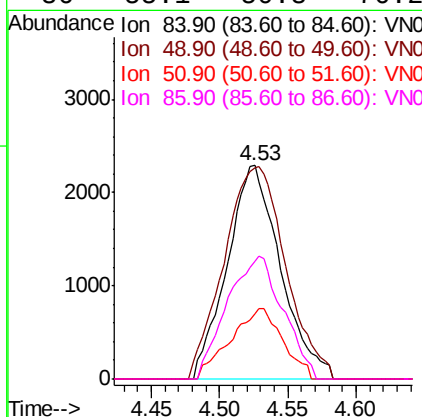


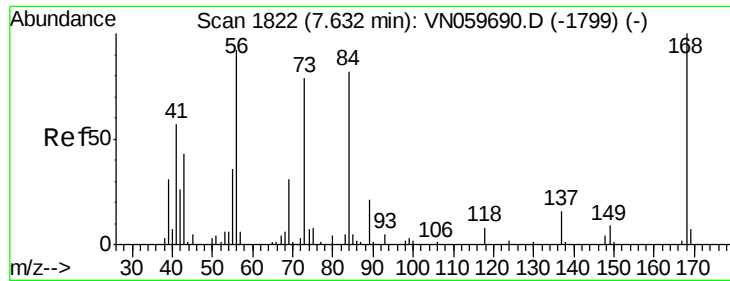




#31
Cyclohexane
Concen: 1.233 ug/l
RT: 7.65 min Scan# 1828
Delta R.T. 0.02 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 56 Resp: 3996
Ion Ratio Lower Upper
56 100
69 145.0 26.5 39.7#
84 127.2 65.3 97.9#

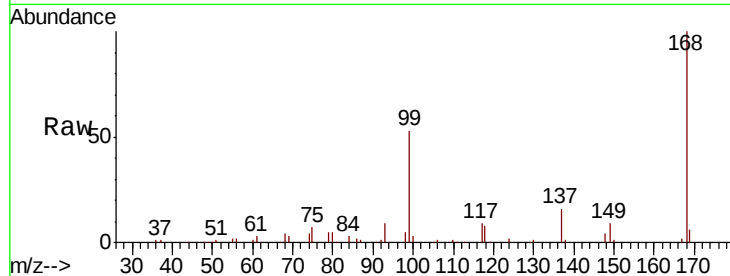


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

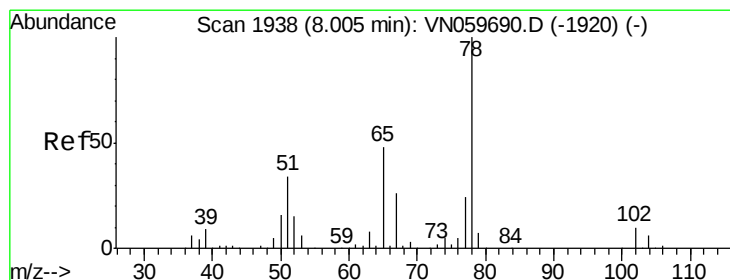
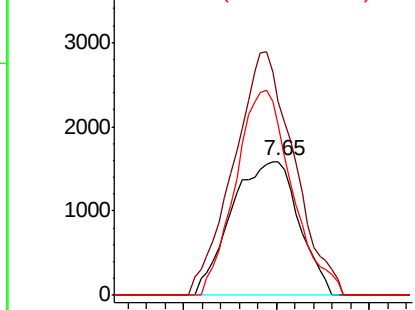



#33
1,2-Dichloroethane-d4
Concen: 52.364 ug/l
RT: 8.00 min Scan# 1938
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Tgt Ion: 65 Resp: 114732
Ion Ratio Lower Upper
65 100
67 51.2 0.0 103.0



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

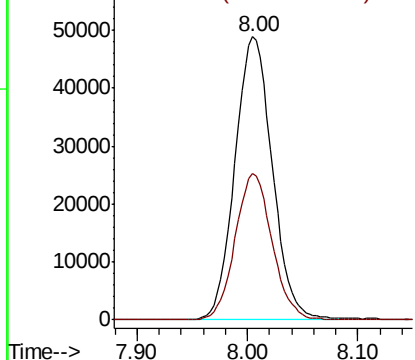


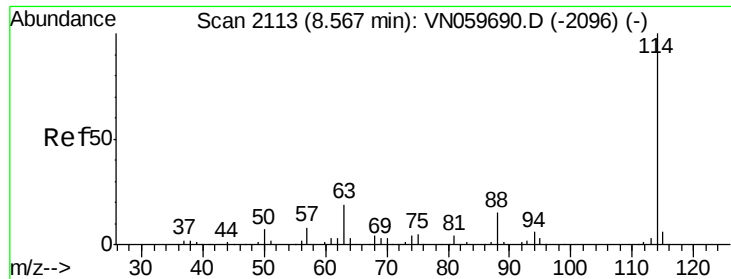




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
114	100		
63	20.1	0.0	43.6
88	15.8	0.0	31.4

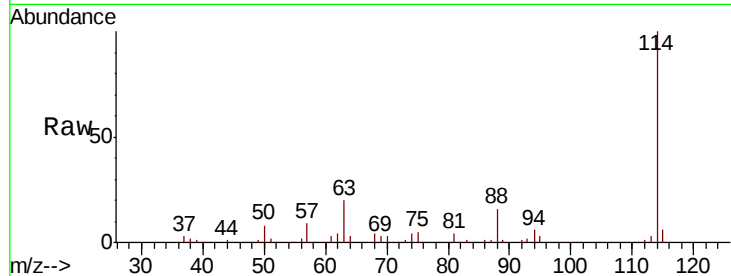


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

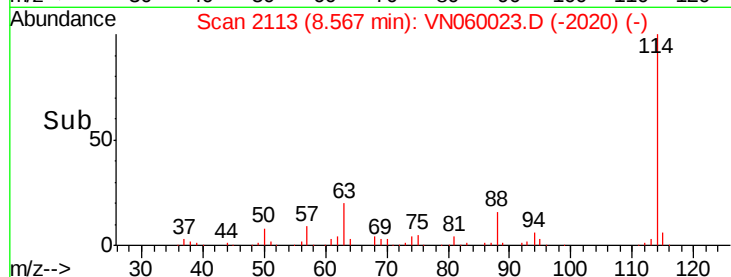
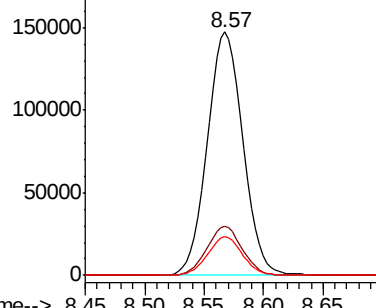



#35
 Dibromofluoromethane
 Concen: 51.588 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.1	83.5	125.3
192	20.3	15.4	23.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

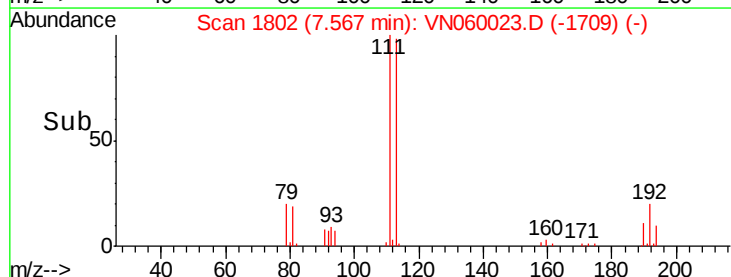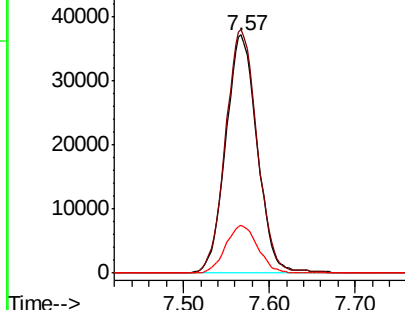


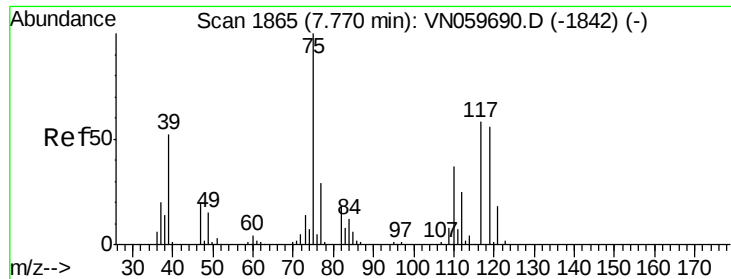




#36
 1,1-Dichloropropene
 Concen: 5.043 ug/l
 RT: 7.64 min Scan# 1826
 Delta R.T. -0.13 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
75	100		
110	8.7	16.6	49.7#
77	0.0	25.1	37.7#

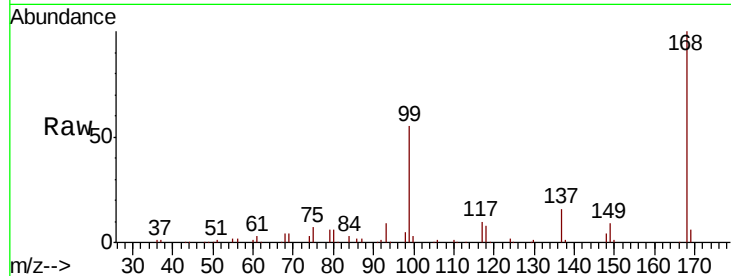


Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VN0

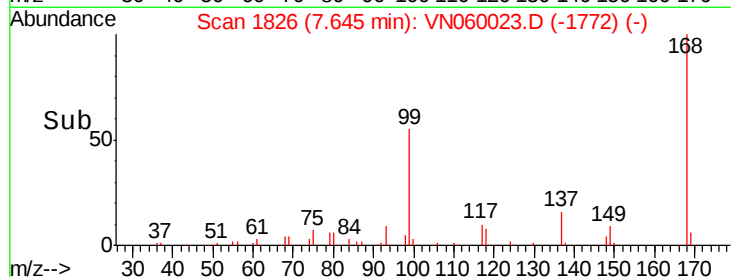
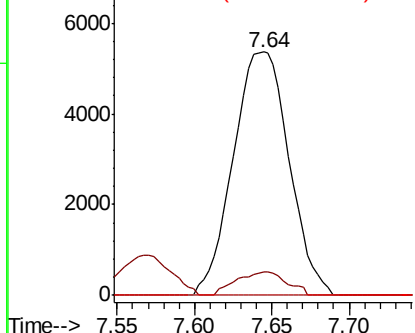



#38
 Carbon Tetrachloride
 Concen: 6.553 ug/l
 RT: 7.64 min Scan# 1826
 Delta R.T. -0.11 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion	Ratio	Lower	Upper
117	100		
119	3.7	76.5	114.7#
121	0.0	25.1	37.7#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

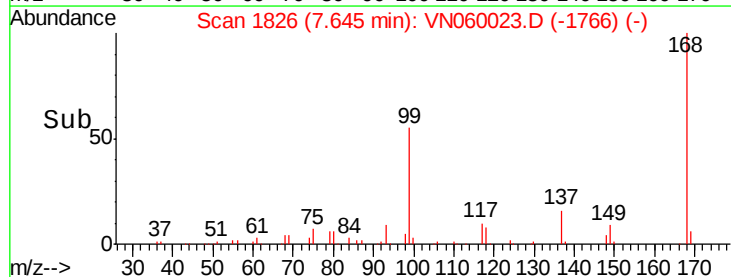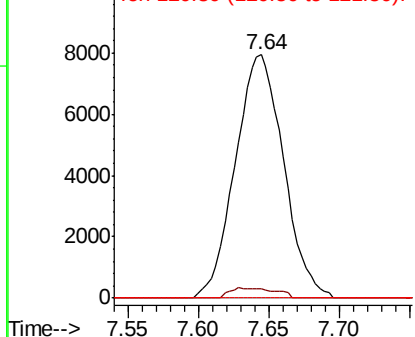

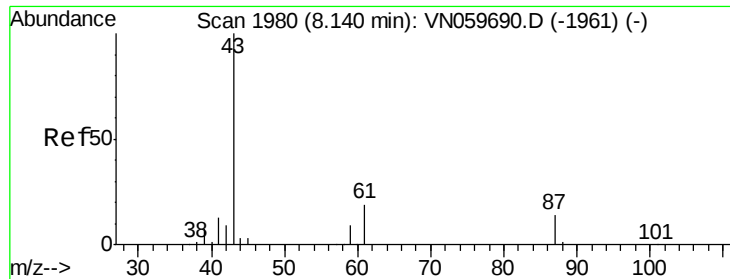

#43

Isopropyl Acetate

Concen: 10.315 ug/l

RT: 8.14 min Scan# 1981

Delta R.T. 0.00 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 43 Resp: 44386

Ion Ratio Lower Upper

43 100

61 19.5 20.2 30.2#




87 14.1 9.5 14.3

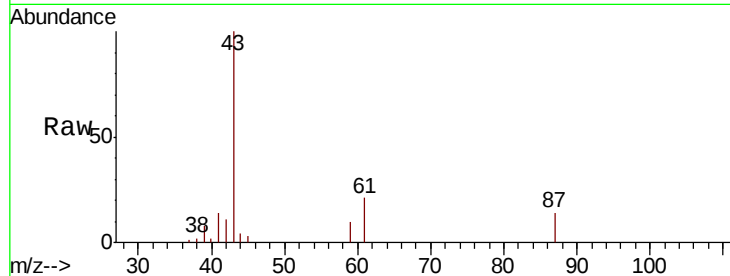

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

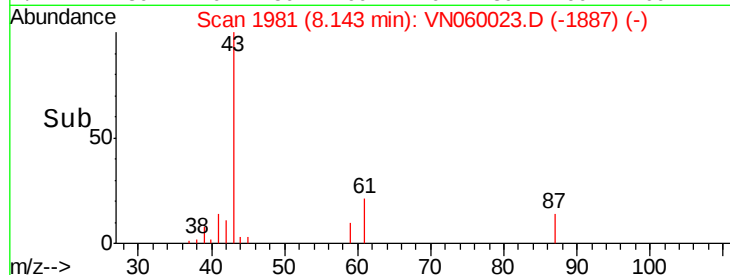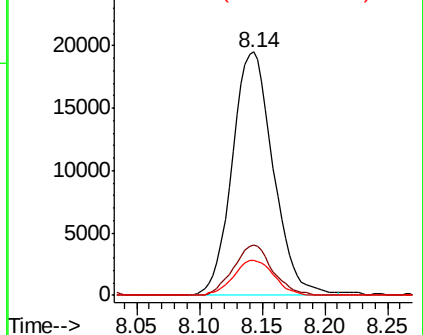

#45

1,2-Dichloropropane

Concen: 0.482 ug/l

RT: 9.25 min Scan# 2324

Delta R.T. 0.14 min

Lab File: VN060023.D


Acq: 7 Feb 2020 11:58

Tgt Ion: 63 Resp: 948

Ion Ratio Lower Upper



63 100


65 0.0 24.9 37.3#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0




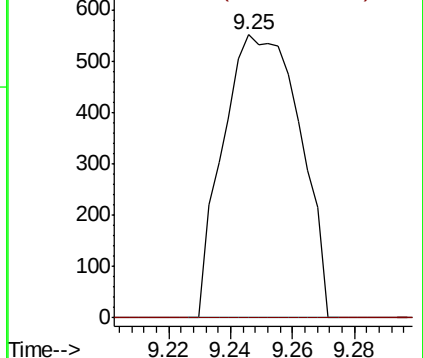


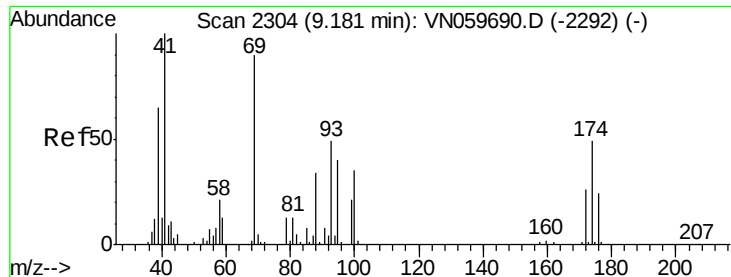

#48
Methvl methacrylate
Concen: 1.239 ug/l
RT: 9.17 min Scan# 2299
Delta R.T. -0.02 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 41 Resp: 2385
Ion Ratio Lower Upper
41 100
69 0.0 64.4 96.6#
39 0.0 51.3 76.9#

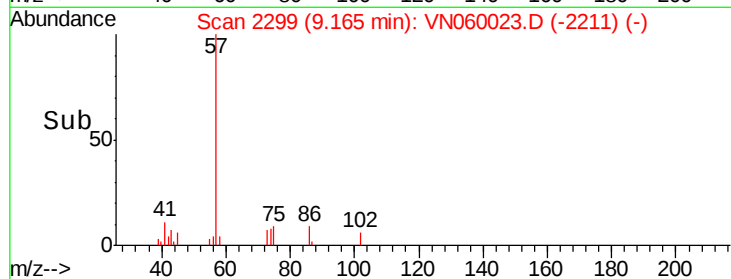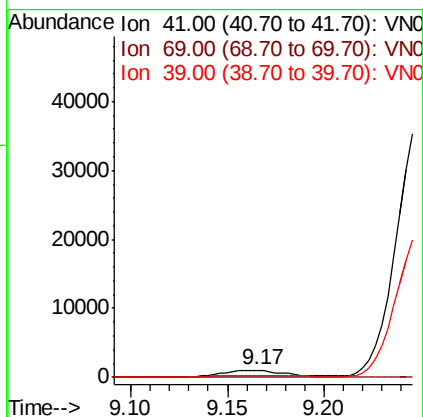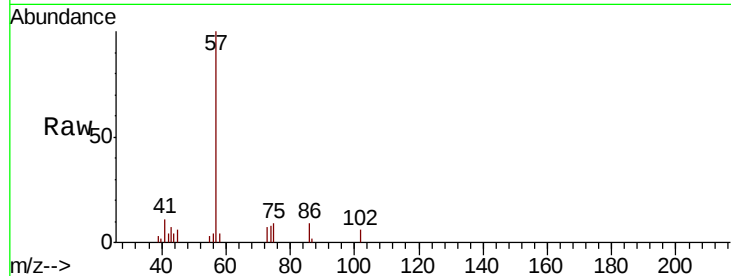

#50
Toluene-d8
Concen: 52.560 ug/l
RT: 10.08 min Scan# 2583
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Tgt Ion: 98 Resp: 371961
Ion Ratio Lower Upper
98 100
100 64.4 51.2 76.8

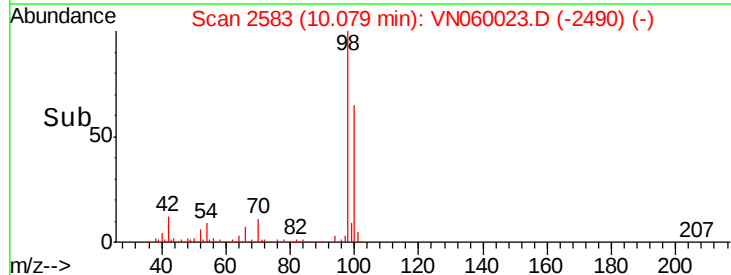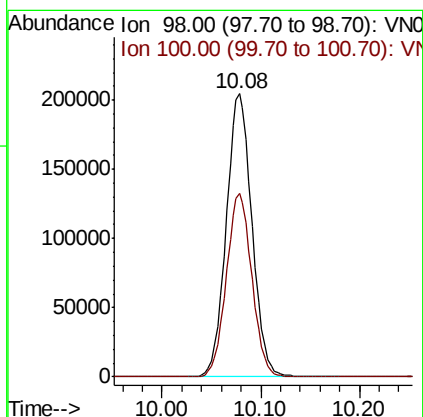

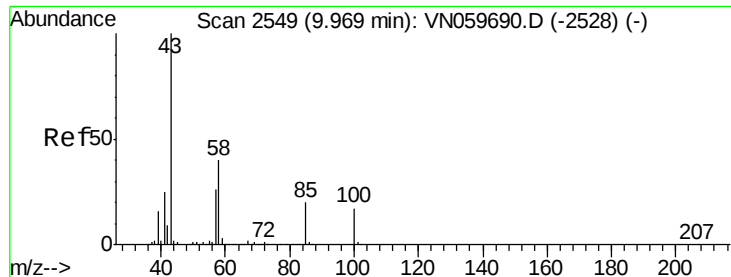

#51

4-Methyl-2-Pentanone

Concen: 1.377 ug/l

RT: 9.97 min Scan# 2549

Delta R.T. 0.00 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 43 Resp: 3424

Ion Ratio Lower Upper




43 100

58 30.8 29.8 44.8

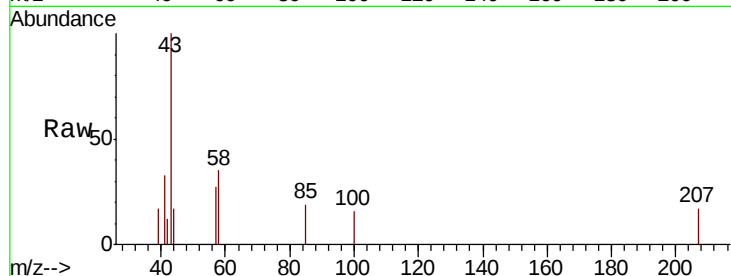

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

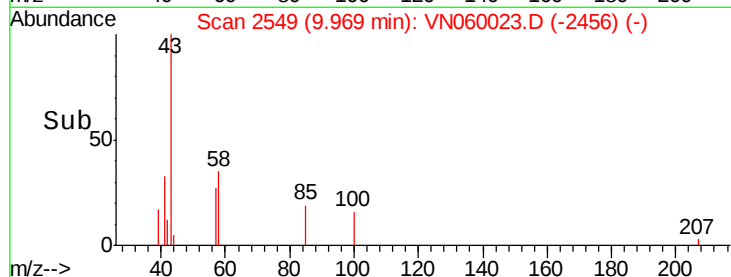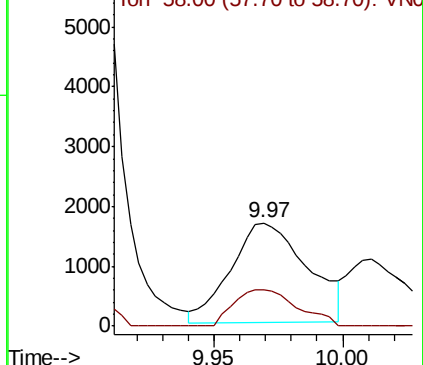

#54

cis-1,3-Dichloropropene

Concen: 6.098 ug/l

RT: 9.89 min Scan# 2525

Delta R.T. 0.07 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58


Tgt Ion: 75 Resp: 20047

Ion Ratio Lower Upper

75 100

77 0.0 25.1 37.7#



39 33.1 46.1 69.1#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0



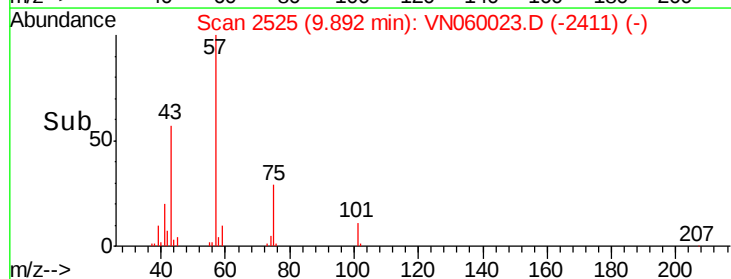
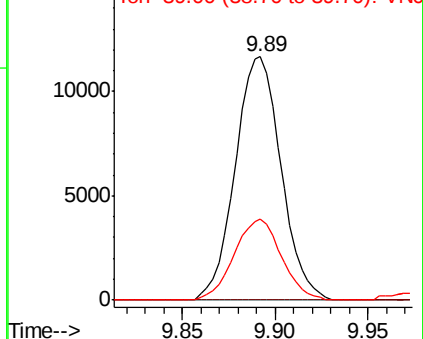




#57
 1,3-Dichloropropane
 Concen: 1.132 ug/l
 RT: 10.75 min Scan# 2793
 Delta R.T. 0.06 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 76 Resp: 3577
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.8#

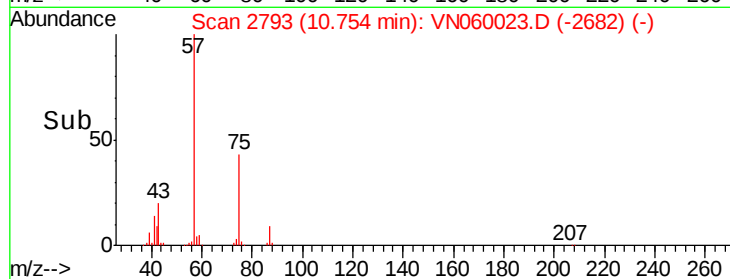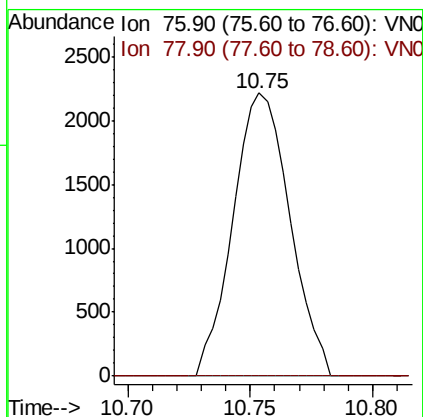

#59
 2-Hexanone
 Concen: 25.218 ug/l
 RT: 10.75 min Scan# 2793
 Delta R.T. 0.01 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion: 43 Resp: 46211
 Ion Ratio Lower Upper
 43 100
 58 19.2 25.8 77.3#



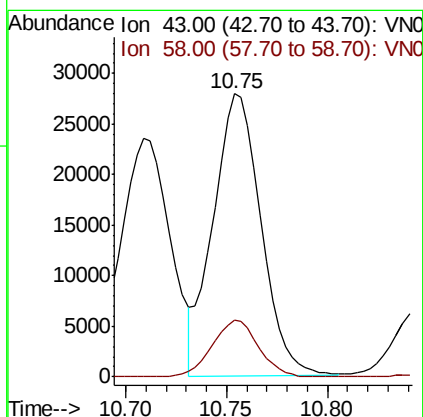



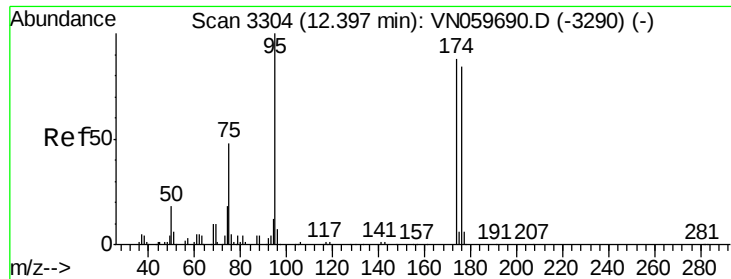

#62
4-Bromofluorobenzene
Concen: 53.445 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 95 Resp: 136348
Ion Ratio Lower Upper
95 100
174 85.3 0.0 151.4
176 82.3 0.0 146.0

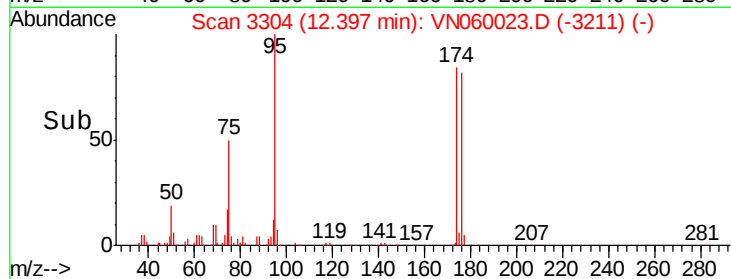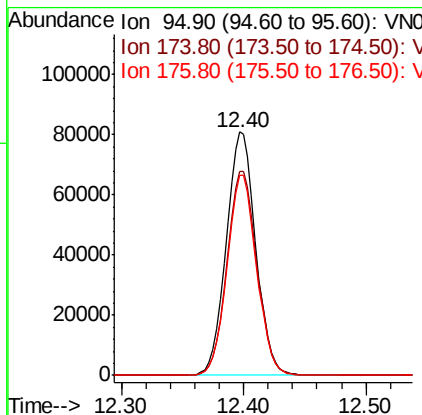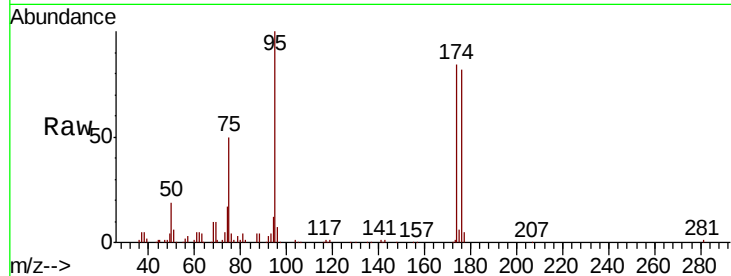

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Tgt Ion: 117 Resp: 291139
Ion Ratio Lower Upper
117 100
82 53.6 45.9 68.9
119 31.6 25.5 38.3

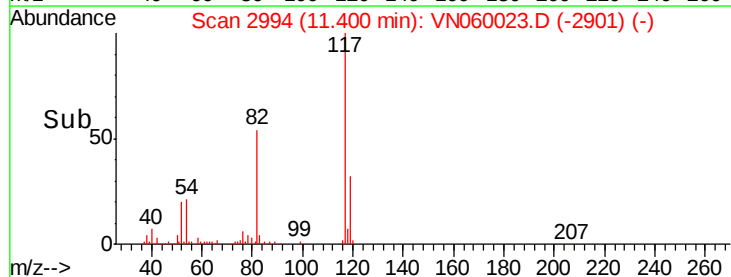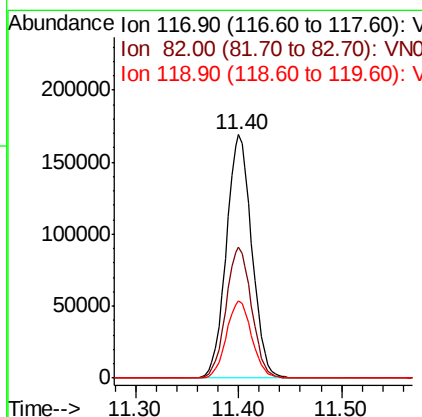



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 135795

Ion Ratio Lower Upper

152 100

115 58.3 30.3 90.9




150 156.2 0.0 345.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

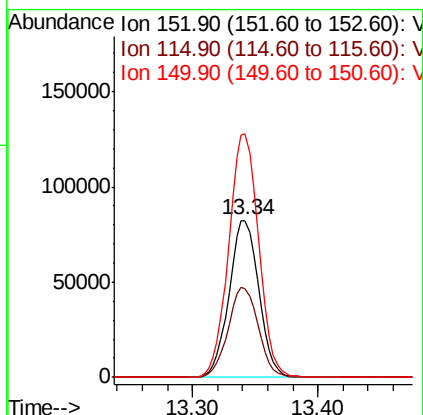

#74

N-ethyl acetate

Concen: 0.571 ug/l

RT: 12.03 min Scan# 3189

Delta R.T. -0.04 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58

Tgt Ion: 43 Resp: 2206


Ion Ratio Lower Upper

43 100

70 0.0 31.3 46.9#

55 0.0 19.8 29.6#

61 0.0 18.3 27.5#






Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

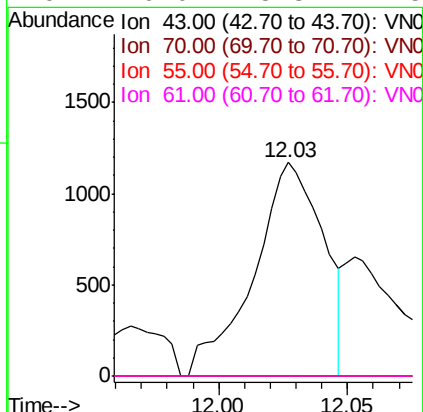



#76

1,2,3-Trichloropropane

Concen: 30.278 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 75 Resp: 69194

Ion Ratio Lower Upper




75 100

77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

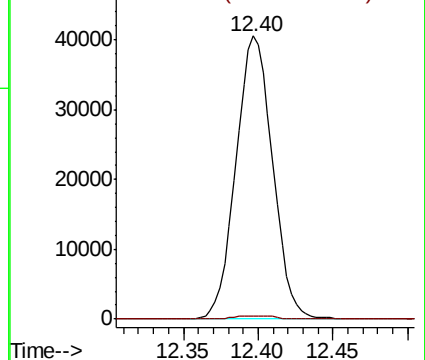

#78

n-propylbenzene

Concen: 0.351 ug/l

RT: 12.59 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN060023.D


Acq: 7 Feb 2020 11:58

Tgt Ion: 91 Resp: 3929

Ion Ratio Lower Upper



91 100


120 19.1 11.1 33.3



Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 120.00 (119.70 to 120.70): V




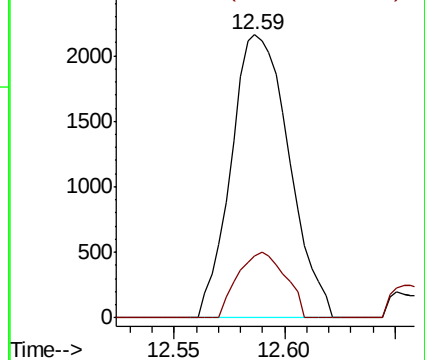




#80
 1,3,5-Trimethylbenzene
 Concen: 0.315 ug/l
 RT: 12.73 min Scan# 3409
 Delta R.T. 0.01 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:105 Resp: 2636
 Ion Ratio Lower Upper
 105 100
 120 47.8 24.1 72.4

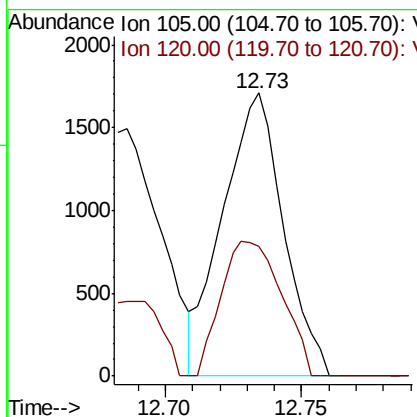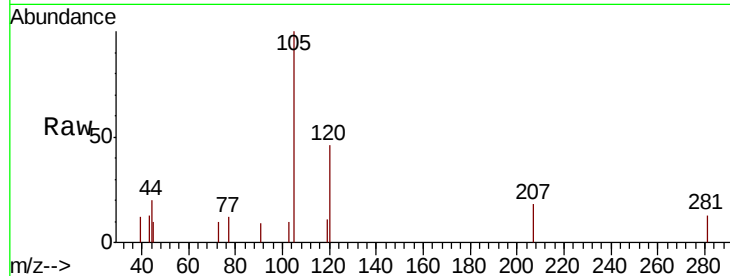

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.022 ug/l
 RT: 12.40 min Scan# 3304
 Delta R.T. 0.10 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion: 75 Resp: 69194
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.1 117.1#
 89 0.0 35.4 53.2#



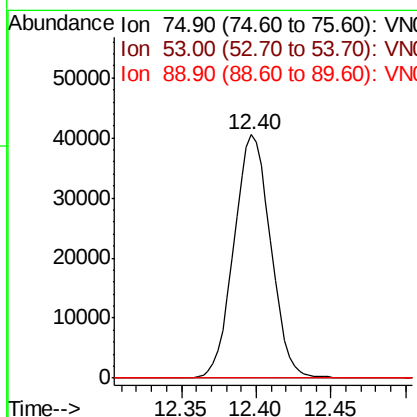
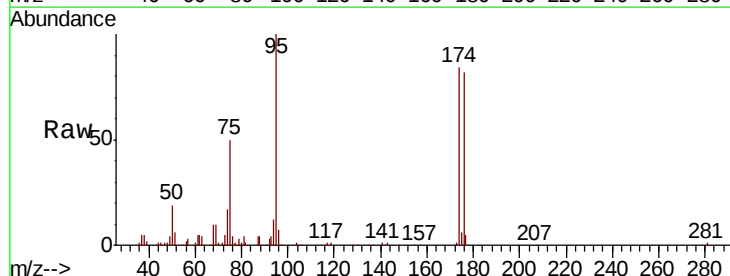




#83
 tert-Butylbenzene
 Concen: 0.288 ug/l
 RT: 13.04 min Scan# 3503
 Delta R.T. 0.05 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:119 Resp: 2085
 Ion Ratio Lower Upper
 119 100
 91 86.3 34.8 104.4
 134 0.0 12.3 36.9#

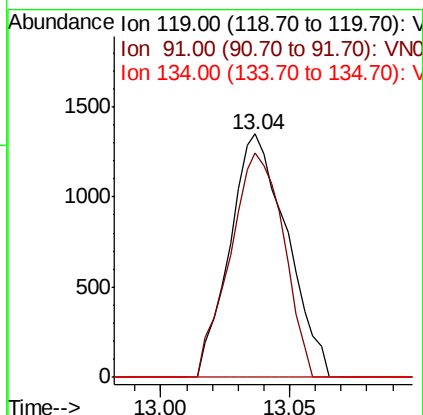

#84
 1,2,4-Trimethylbenzene
 Concen: 1.977 ug/l
 RT: 13.04 min Scan# 3503
 Delta R.T. 0.00 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion:105 Resp: 16382
 Ion Ratio Lower Upper
 105 100
 120 45.6 22.3 66.9

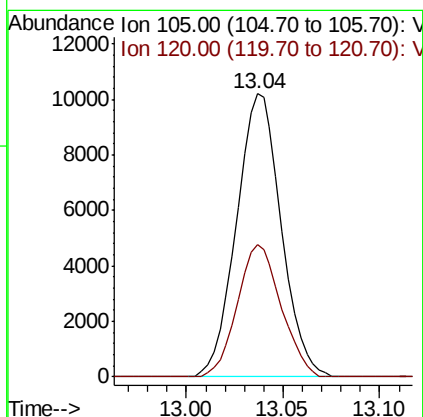



#89

n-Butylbenzene

Concen: 0.433 ug/l

RT: 13.61 min Scan# 3682

Delta R.T. 0.00 min

Lab File: VN060023.D


Acq: 7 Feb 2020 11:58

Instrument :

MSVOA_N

ClientSampled :

Tot Ion:	91	Resp:	3251
Ion	Ratio	Lower	Upper
91	100		
92	34.2	25.9	77.7
134	0.0	12.3	36.8#




Abundance Ion 91.00 (90.70 to 91.70): VN060023.D (-3667) (-)


Ion 92.00 (91.70 to 92.70): VN060023.D (-3667) (-)

Ion 134.00 (133.70 to 134.70): VN060023.D (-3667) (-)

Time-->



Time-->



#90

Hexachloroethane

Concen: 0.760 ug/l


RT: 13.89 min Scan# 3768

Delta R.T. 0.02 min

Lab File: VN060023.D

Acq: 7 Feb 2020 11:58


Tgt Ion:	117	Resp:	1252
Ion	Ratio	Lower	Upper
117	100		
201	0.0	37.8	113.4#




Abundance Ion 116.80 (116.50 to 117.50): VN060023.D (-3669) (-)

Ion 200.70 (200.40 to 201.40): VN060023.D (-3669) (-)

Time-->







Time-->

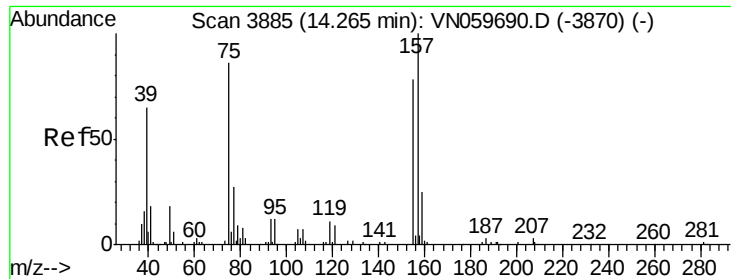

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.23 min Scan# 3875
 Delta R.T. -0.03 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 75 Resp: 133
 Ion Ratio Lower Upper
 75 100
 155 0.0 37.0 110.9#
 157 0.0 48.4 145.2#

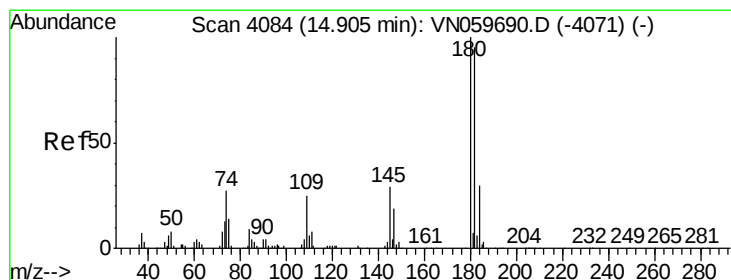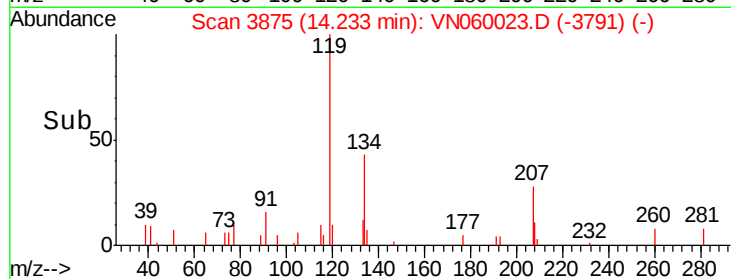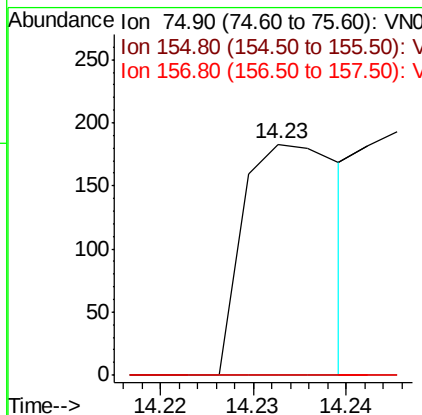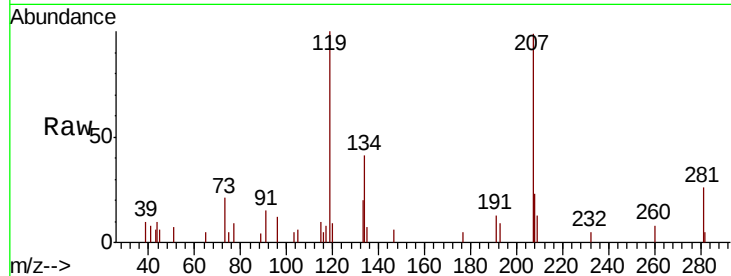

#93
 1,2,4-Trichlorobenzene
 Concen: 0.267 ug/l
 RT: 14.91 min Scan# 4085
 Delta R.T. 0.00 min
 Lab File: VN060023.D
 Acq: 7 Feb 2020 11:58

Tgt Ion: 180 Resp: 694
 Ion Ratio Lower Upper
 180 100
 182 79.1 46.9 140.7
 145 62.4 15.0 45.1#

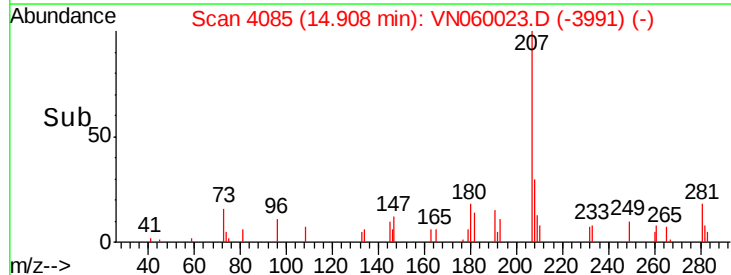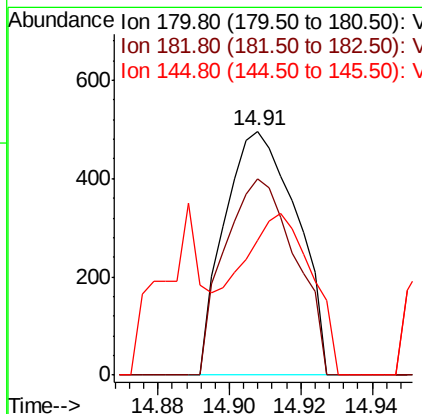


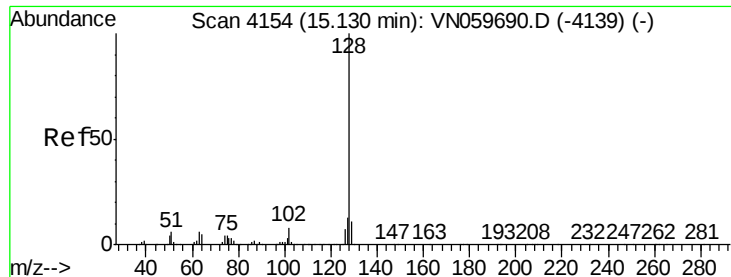




#95
Naphthalene
Concen: 25.154 ug/l
RT: 15.13 min Scan# 4154
Delta R.T. 0.00 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Instrument :
MSVOA_N
ClientSampled :

Tot Ion:128 Resp: 186200
Ion Ratio Lower Upper
128 100
127 13.2 10.4 15.6
129 10.9 8.6 12.8

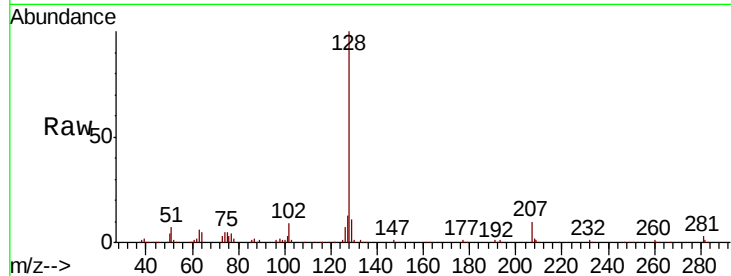


Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

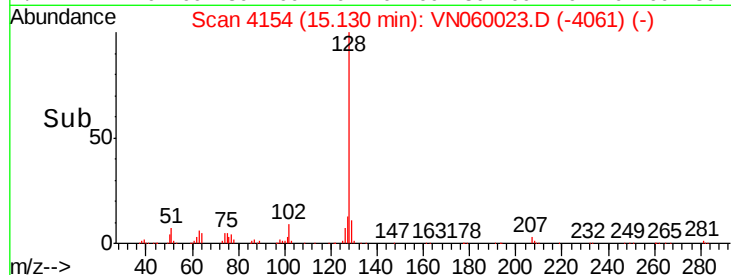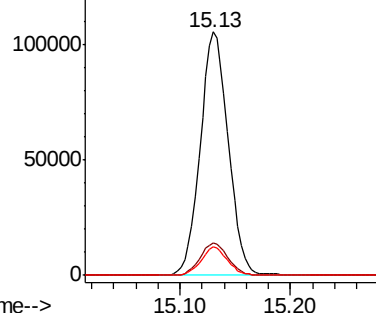

#96
1,2,3-Trichlorobenzene
Concen: 0.251 ug/l
RT: 15.32 min Scan# 4212
Delta R.T. 0.01 min
Lab File: VN060023.D
Acq: 7 Feb 2020 11:58

Tgt Ion:180 Resp: 635
Ion Ratio Lower Upper
180 100
182 89.9 47.4 142.3
145 59.5 16.3 48.9#

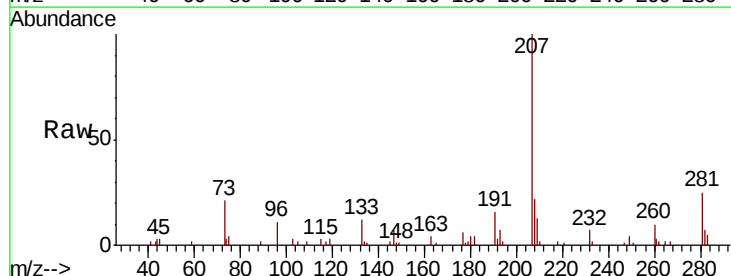

Abundance Ion 179.80 (179.50 to 180.50): V
Ion 181.80 (181.50 to 182.50): V
Ion 144.90 (144.60 to 145.60): V

