
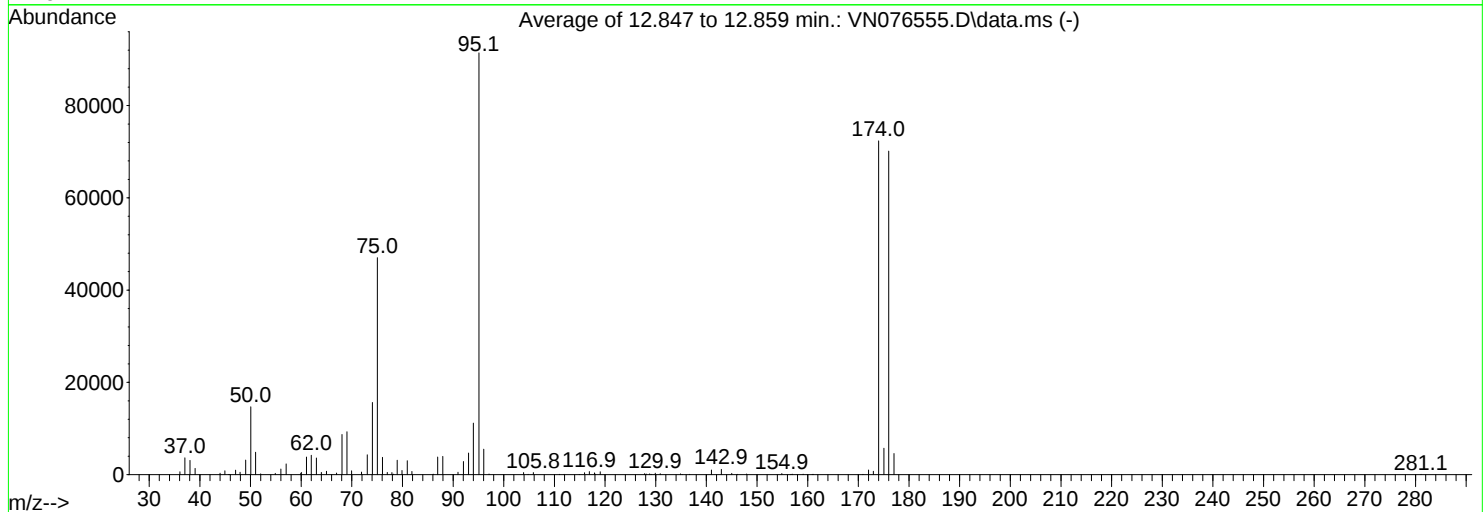


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN0723\
Data File : VN076555.D
Acq On : 07 Feb 2023 09:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020723S.M
Title : SW846 8260
Last Update : Wed Feb 08 04:26:58 2023

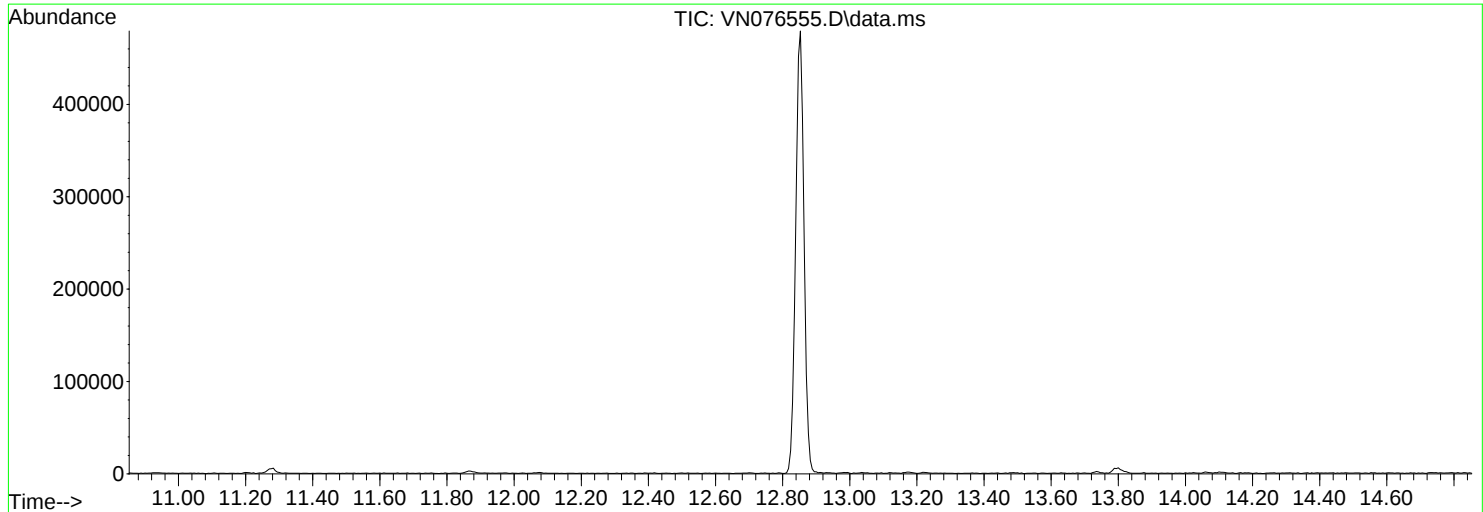

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	14724	PASS
75	95	30	60	51.4	47037	PASS
95	95	100	100	100.0	91435	PASS
96	95	5	9	6.0	5526	PASS
173	174	0.00	2	1.0	734	PASS
174	95	50	100	79.1	72355	PASS
175	174	5	9	7.9	5721	PASS
176	174	95	101	96.9	70117	PASS
177	176	5	9	6.5	4589	PASS