

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
 Data File : VN080929.D
 Acq On : 07 Feb 2024 10:17
 Operator : JC\MD
 Sample : VN0207MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0207MBL01

Quant Time: Feb 08 00:21:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 07 06:22:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	324362	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	672329	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	1010766	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	312093	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	191502	46.801	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.600%		
35) Dibromofluoromethane	8.165	113	182392	50.556	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	101.120%		
50) Toluene-d8	10.565	98	812504	62.263	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	124.520%#		
62) 4-Bromofluorobenzene	12.847	95	273226	57.636	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	115.280%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	3873	Below Cal	#	67
5) Bromomethane	2.971	94	2428	0.786	ug/l #	65
6) Chloroethane	3.136	64	694	0.205	ug/l #	42
10) Methyl Iodide	4.600	142	1290	0.377	ug/l #	64
13) Acrolein	4.183	56	554	0.780	ug/l #	73
15) Acrylonitrile	5.724	53	1056	0.685	ug/l #	59
16) Acetone	4.436	43	659	0.490	ug/l #	44
17) Carbon Disulfide	4.706	76	2653	0.302	ug/l #	78
18) Methyl Acetate	5.036	43	1166	Below Cal	#	79
20) Methylene Chloride	5.277	84	1754	0.430	ug/l #	87
25) 2-Butanone	7.483	43	694	0.321	ug/l #	51
31) Cyclohexane	8.224	56	7612	1.361	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	28363	5.285	ug/l #	51
38) Carbon Tetrachloride	8.224	117	35979	6.539	ug/l #	18
39) Methylcyclohexane	9.594	83	1402	0.234	ug/l #	81
49) 1,4-Dioxane	9.706	88	79	1.017	ug/l #	18
59) 2-Hexanone	11.206	43	1197	0.351	ug/l #	47
76) 1,2,3-Trichloropropane	12.847	75	150060	23.582	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	150060	64.069	ug/l #	14
83) tert-Butylbenzene	13.447	119	3831	0.228	ug/l	93
85) sec-Butylbenzene	13.618	105	7461	0.330	ug/l #	75
86) p-Isopropyltoluene	13.729	119	6220	0.326	ug/l	91
87) 1,3-Dichlorobenzene	13.735	146	2697	0.247	ug/l	85
88) 1,4-Dichlorobenzene	13.735	146	2697	0.244	ug/l	87
89) n-Butylbenzene	14.053	91	8846	0.524	ug/l	93
90) Hexachloroethane	14.335	117	651	0.216	ug/l	99
93) 1,2,4-Trichlorobenzene	15.388	180	3547	0.686	ug/l	96
94) Hexachlorobutadiene	15.500	225	2595	1.158	ug/l	94
95) Naphthalene	15.641	128	11283	0.661	ug/l #	90
96) 1,2,3-Trichlorobenzene	15.847	180	3990	0.784	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
Data File : VN080929.D
Acq On : 07 Feb 2024 10:17
Operator : JC\MD
Sample : VN0207MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01

Quant Time: Feb 08 00:21:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 07 06:22:23 2024
Response via : Initial Calibration

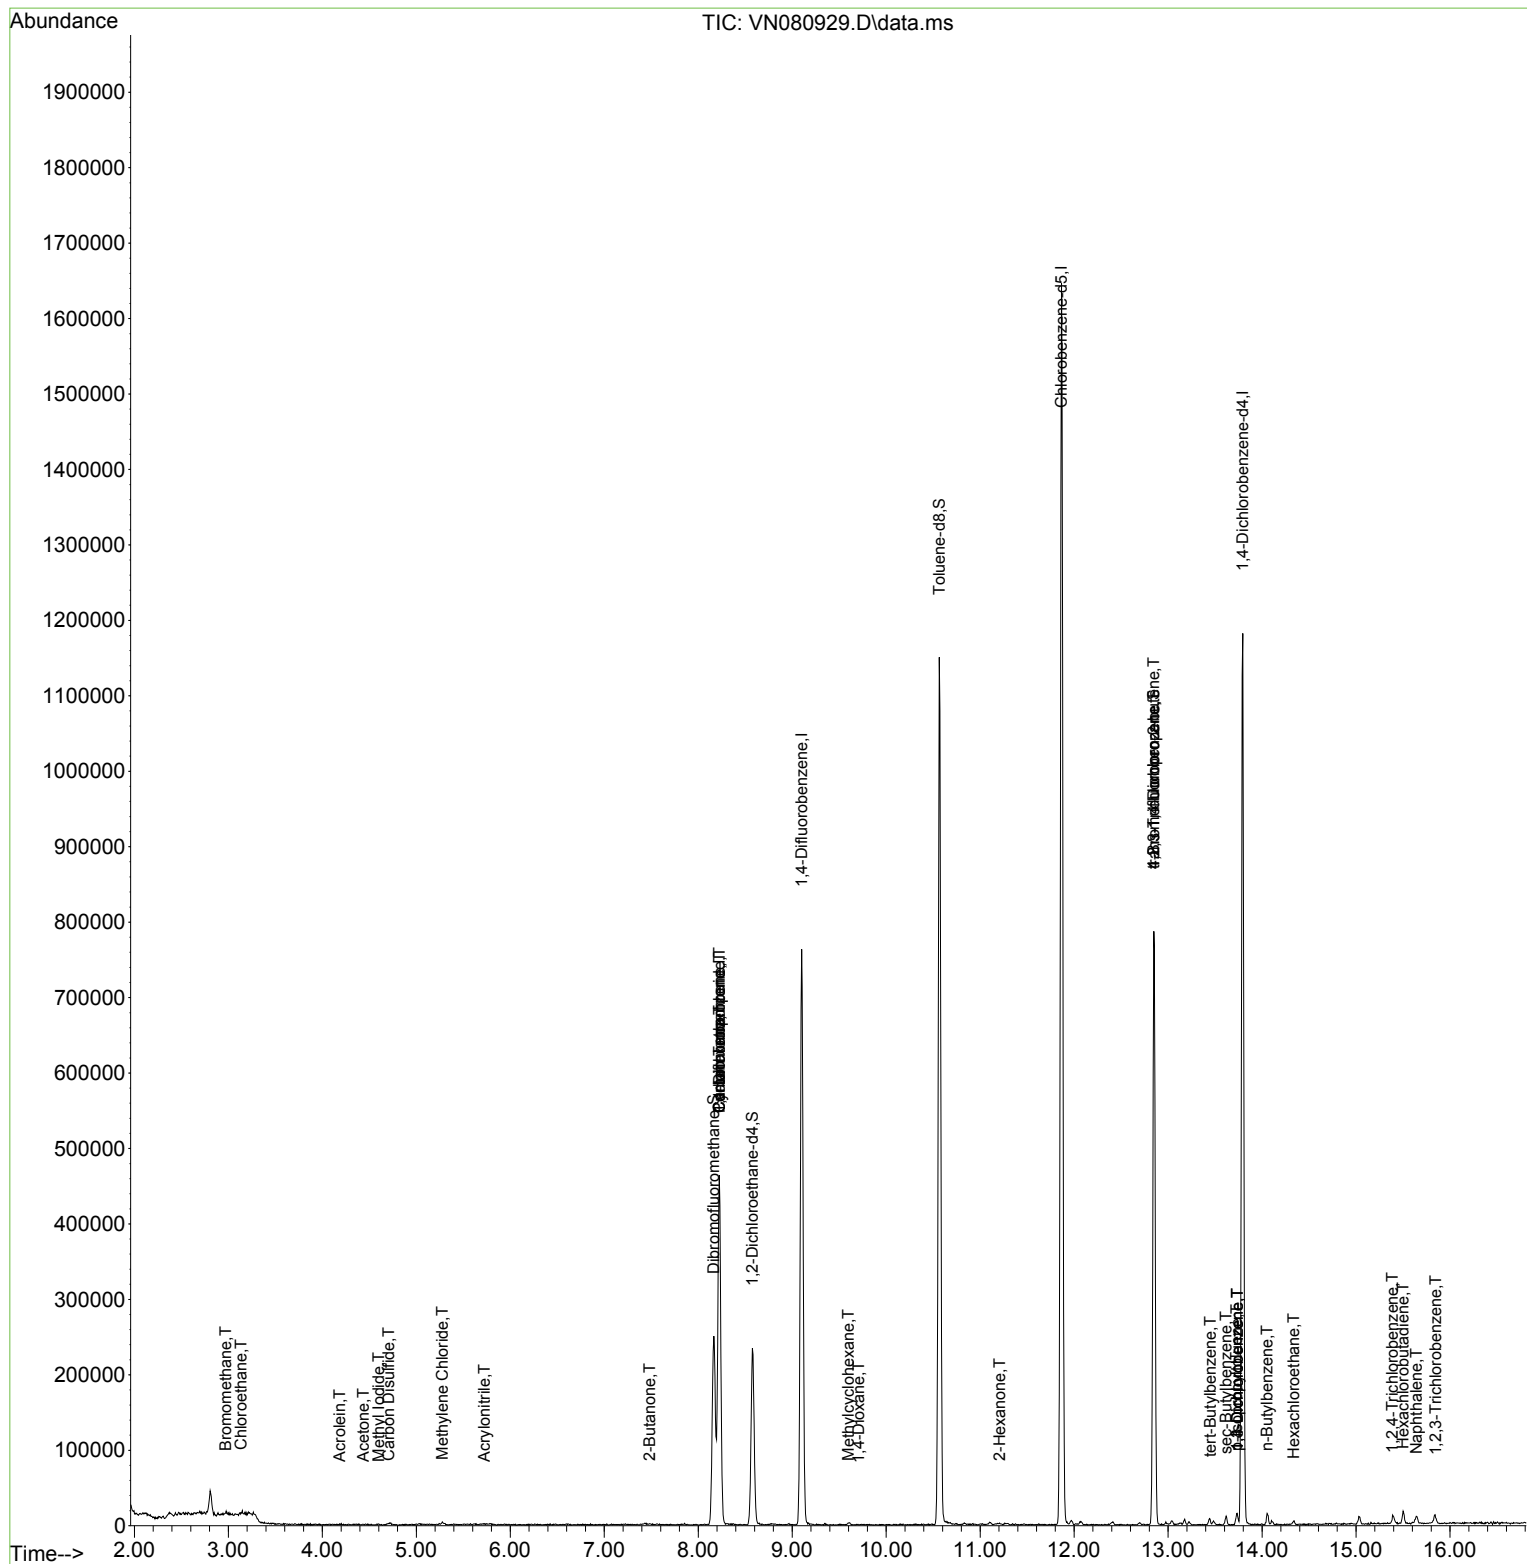



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Instrument :

MSVOA_N

ClientSampleId :





VN0207MBL01

Tgt Ion:168 Resp: 324362

Ion Ratio Lower Upper

168 100

99 66.7 59.9 89.9

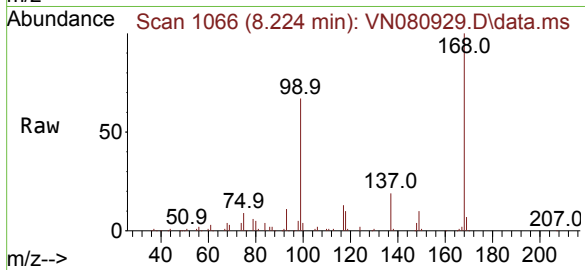

#3

Chloromethane

Concen: Below Cal

RT: 2.365 min Scan# 70

Delta R.T. 0.006 min

Lab File: VN080929.D




Acq: 07 Feb 2024 10:17


Tgt Ion: 50 Resp: 3873

Ion Ratio Lower Upper

50 100

52 49.2 25.0 37.4#




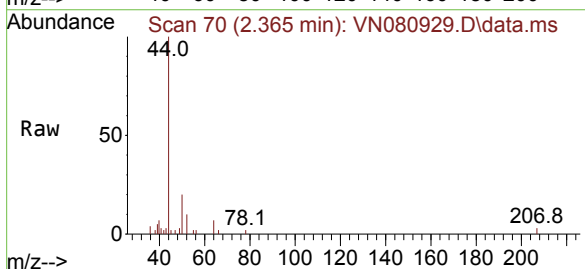




#5
Bromomethane
Concen: 0.786 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 94 Resp: 2428
Ion Ratio Lower Upper
94 100
96 54.1 69.2 103.8#



#6
Chloroethane
Concen: 0.205 ug/l
RT: 3.136 min Scan# 201
Delta R.T. 0.018 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17


Tgt Ion: 64 Resp: 694
Ion Ratio Lower Upper
64 100
66 0.0 26.4 39.6#








#10
Methyl Iodide
Concen: 0.377 ug/l
RT: 4.600 min Scan# 411
Delta R.T. 0.012 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17


Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01





Tgt Ion:142 Resp: 1290
Ion Ratio Lower Upper
142 100
127 22.7 37.0 55.4#
141 0.0 12.5 18.7#

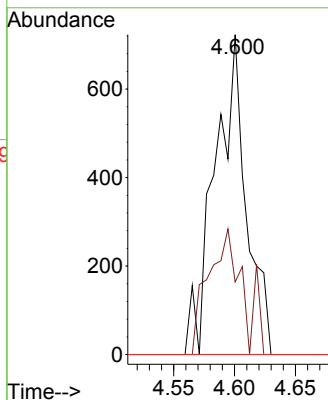


#13
Acrolein
Concen: 0.780 ug/l
RT: 4.183 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

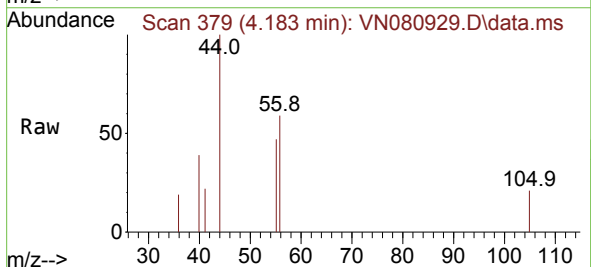

Tgt Ion: 56 Resp: 554
Ion Ratio Lower Upper
56 100
55 91.3 55.3 82.9#



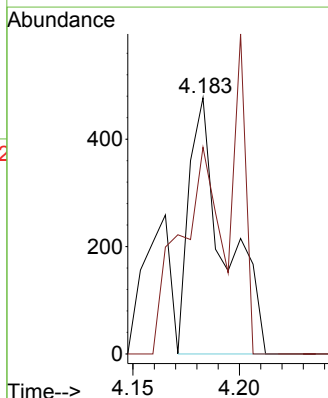
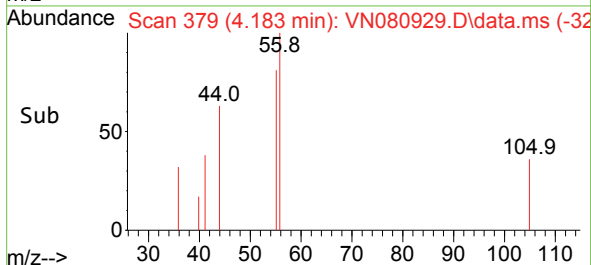




#15
Acrylonitrile
Concen: 0.685 ug/l
RT: 5.724 min Scan# 641
Delta R.T. 0.006 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 53 Resp: 1056
Ion Ratio Lower Upper
53 100
52 41.9 64.8 97.2#
51 15.0 26.9 40.3#



#16
Acetone
Concen: 0.490 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.012 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion: 43 Resp: 659
Ion Ratio Lower Upper
43 100
58 0.0 24.8 37.2#



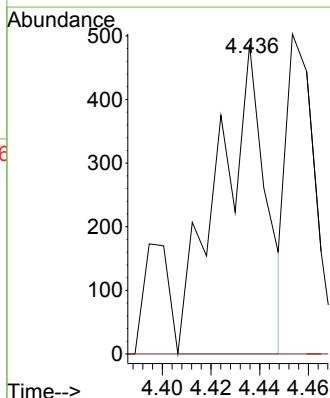





#17
Carbon Disulfide
Concen: 0.302 ug/l
RT: 4.706 min Scan# 41
Delta R.T. -0.012 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 76 Resp: 2653
Ion Ratio Lower Upper
76 100
78 0.0 6.3 9.5#

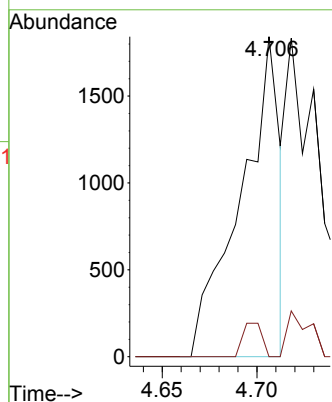

#18
Methyl Acetate
Concen: Below Cal
RT: 5.036 min Scan# 524
Delta R.T. 0.018 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17


Tgt Ion: 43 Resp: 1166
Ion Ratio Lower Upper
43 100
74 11.8 17.3 25.9#

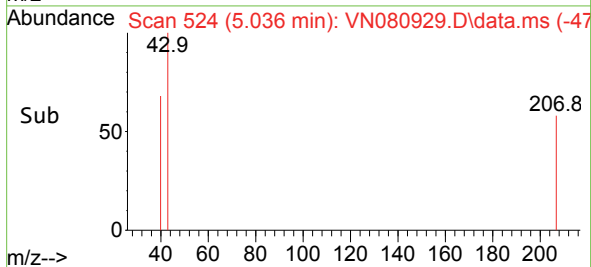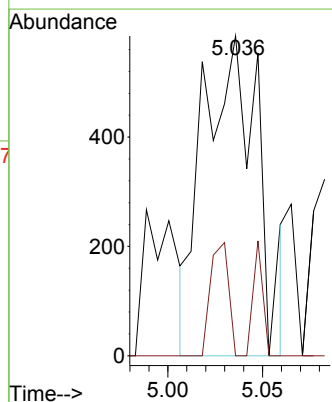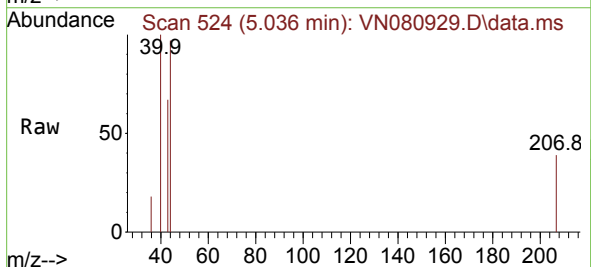






#20
Methylene Chloride
Concen: 0.430 ug/l
RT: 5.277 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01



Tgt Ion: 84 Resp: 1754




Ion	Ratio	Lower	Upper
84	100		
49	128.1	108.1	162.1
51	51.0	32.9	49.3#
86	80.4	48.6	73.0#




#25
2-Butanone
Concen: 0.321 ug/l
RT: 7.483 min Scan# 940
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion: 43 Resp: 694

Ion	Ratio	Lower	Upper
43	100		
72	0.0	19.5	29.3#









#31
Cyclohexane
Concen: 1.361 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 56 Resp: 7612
Ion Ratio Lower Upper
56 100
69 139.8 20.1 30.1#
84 164.7 56.9 85.3#

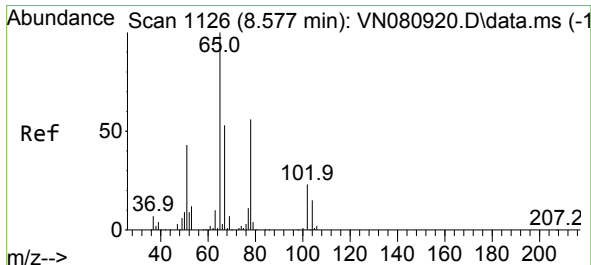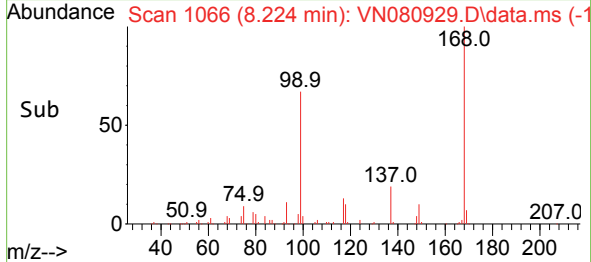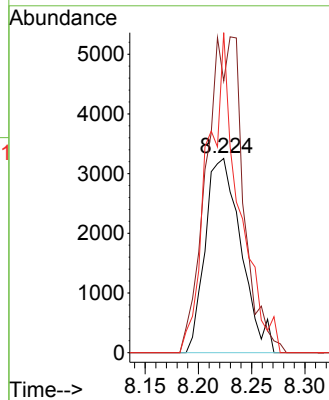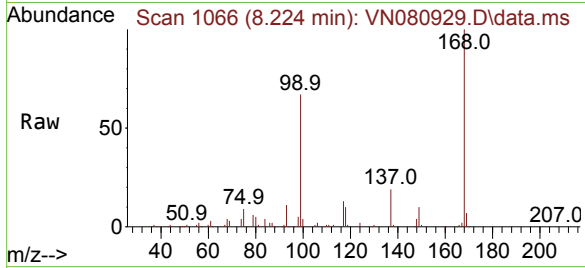

#33
1,2-Dichloroethane-d4
Concen: 46.801 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17


Tgt Ion: 65 Resp: 191502
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.4

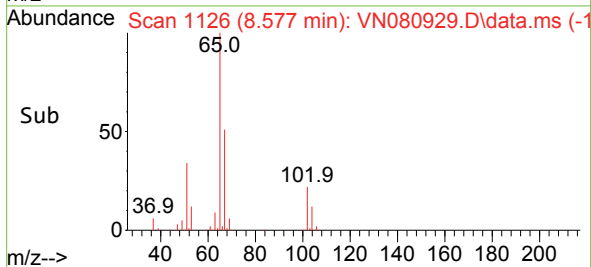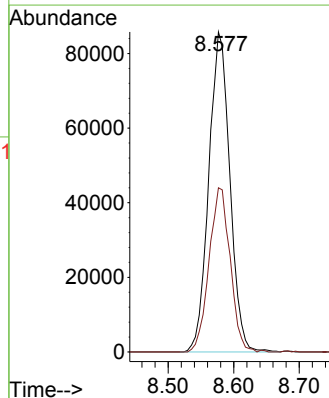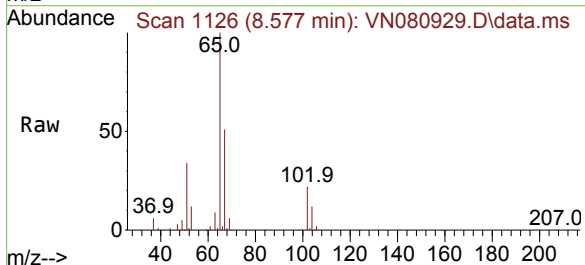






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01







Tgt Ion:114 Resp: 672329
Ion Ratio Lower Upper
114 100
63 19.3 0.0 48.0
88 15.3 0.0 34.8

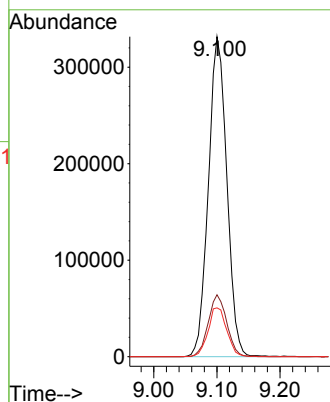

#35
Dibromofluoromethane
Concen: 50.556 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion:113 Resp: 182392
Ion Ratio Lower Upper
113 100
111 102.2 82.2 123.4
192 17.4 12.5 18.7









#36
1,1-Dichloropropene
Concen: 5.285 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 75 Resp: 28363
Ion Ratio Lower Upper
75 100
110 9.3 16.0 48.0#
77 0.0 25.8 38.6#

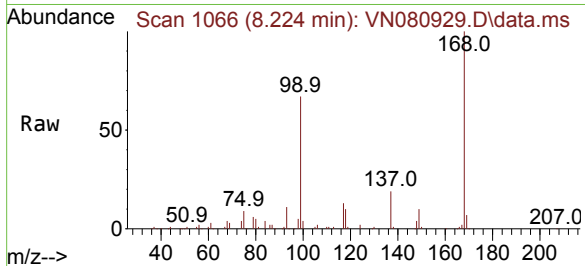

#38
Carbon Tetrachloride
Concen: 6.539 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.135 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion: 117 Resp: 35979
Ion Ratio Lower Upper
117 100
119 5.0 73.4 110.2#
121 0.0 24.4 36.6#

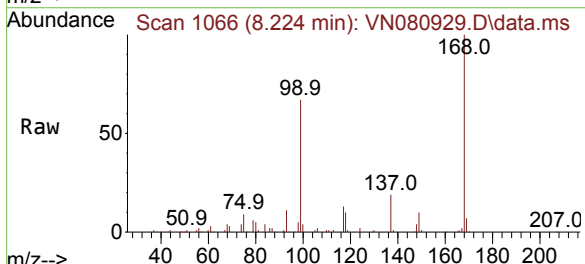



#39

Methylcyclohexane

Concen: 0.234 ug/l

RT: 9.594 min Scan# 1300

Delta R.T. -0.006 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Instrument :

MSVOA_N

ClientSampleId :

VN0207MBL01





Tgt Ion: 83 Resp: 1402

Ion Ratio Lower Upper

83 100

55 75.5 65.7 98.5

98 16.4 33.8 50.6#

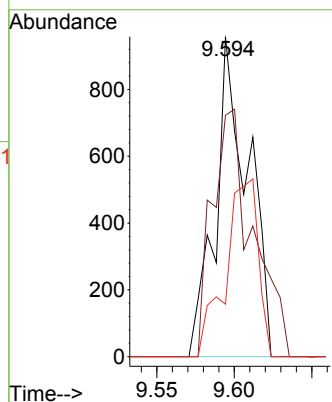

#49

1,4-Dioxane

Concen: 1.017 ug/l

RT: 9.706 min Scan# 1318

Delta R.T. 0.012 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17




Tgt Ion: 88 Resp: 79


Ion Ratio Lower Upper

88 100

43 0.0 30.1 45.1#

58 0.0 63.9 95.9#









#50
Toluene-d8
Concen: 62.263 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 98 Resp: 812504
Ion Ratio Lower Upper
98 100
100 65.3 51.4 77.0

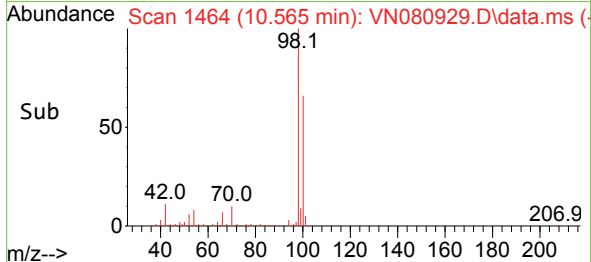

#59
2-Hexanone
Concen: 0.351 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.012 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion: 43 Resp: 1197
Ion Ratio Lower Upper
43 100
58 14.4 25.9 77.8#


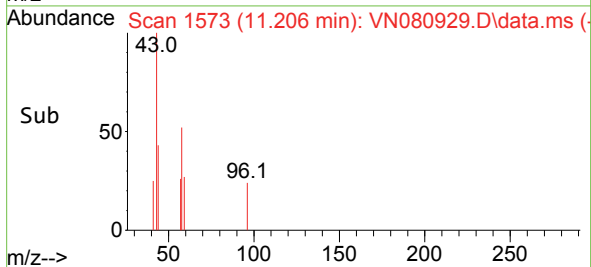

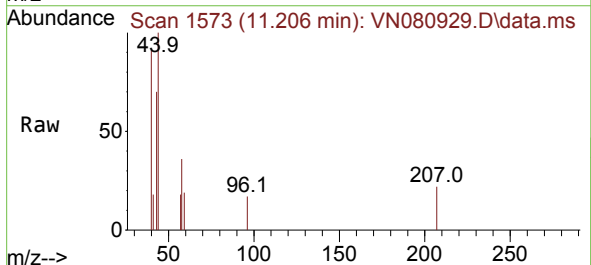


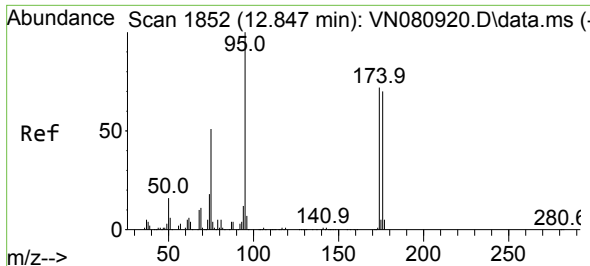

#62
4-Bromofluorobenzene
Concen: 57.636 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion: 95 Resp: 273226
Ion Ratio Lower Upper
95 100
174 73.3 0.0 120.4
176 70.4 0.0 121.0

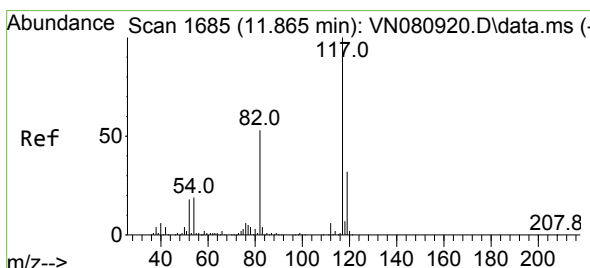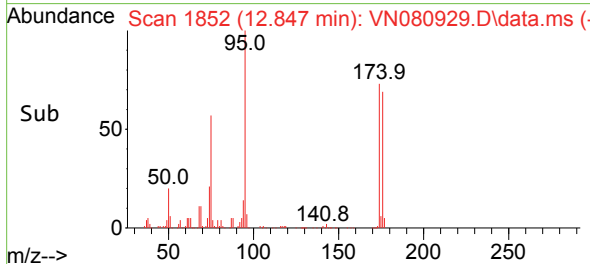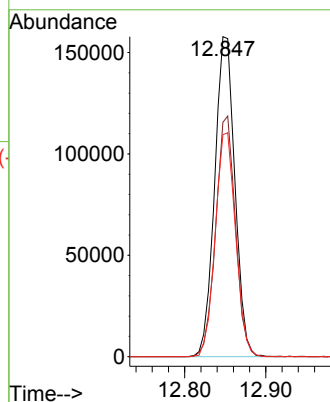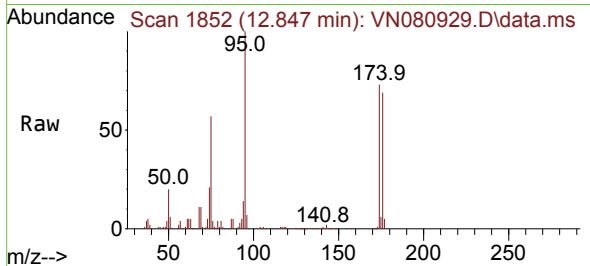

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion: 117 Resp: 1010766
Ion Ratio Lower Upper
117 100
82 53.7 52.7 79.1
119 31.5 25.3 37.9


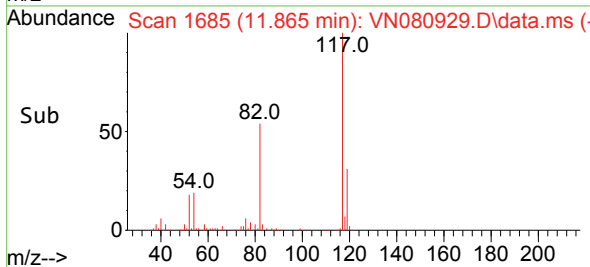
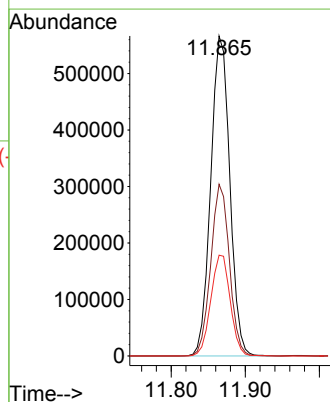
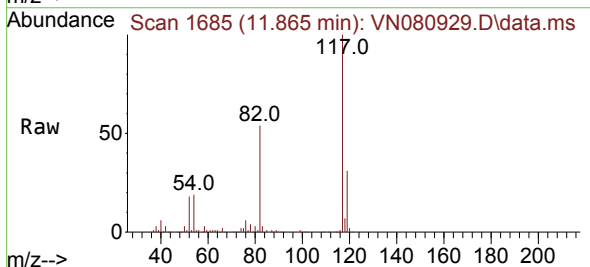


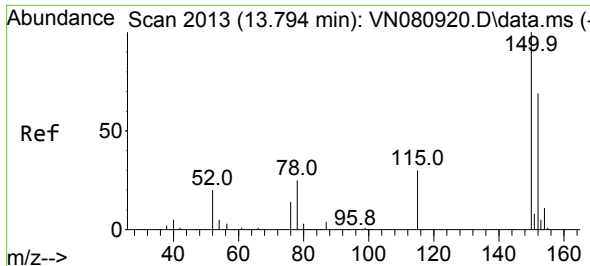

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 2013
 Delta R.T. -0.000 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0207MBL01


Tgt Ion:152 Resp: 312093
 Ion Ratio Lower Upper
 152 100
 115 63.1 32.3 96.8
 150 155.9 0.0 339.8

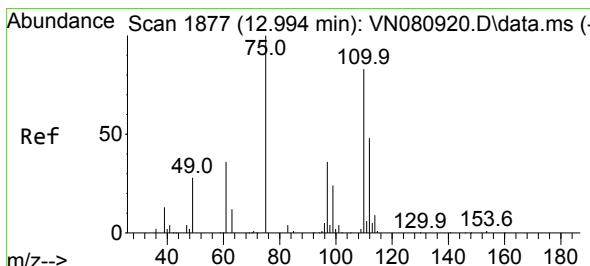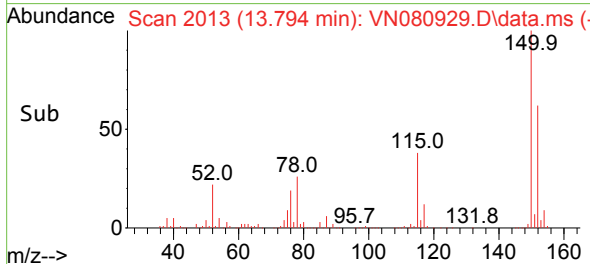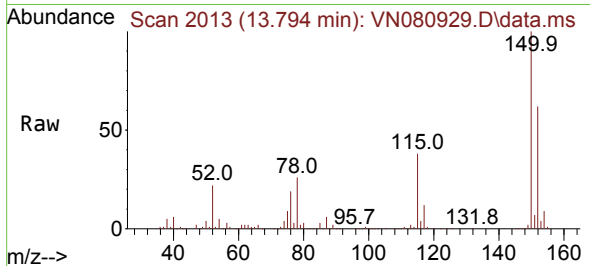

#76
 1,2,3-Trichloropropane
 Concen: 23.582 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.147 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17

Tgt Ion: 75 Resp: 150060
 Ion Ratio Lower Upper
 75 100
 77 1.4 91.0 272.8#


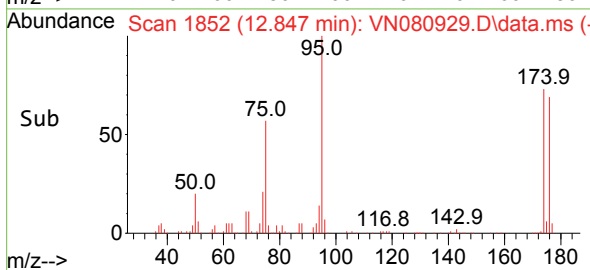

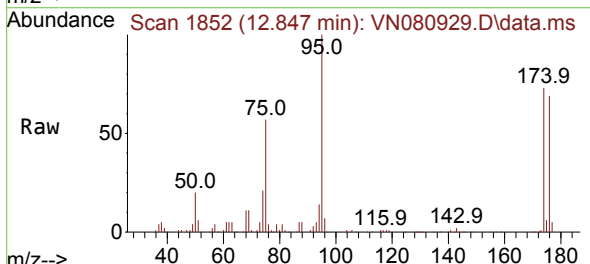




#81
 trans-1,4-Dichloro-2-butene
 Concen: 64.069 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. 0.112 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0207MBL01


Tgt Ion: 75 Resp: 150060
 Ion Ratio Lower Upper
 75 100
 53 0.1 71.4 107.2#
 89 0.0 33.4 50.0#

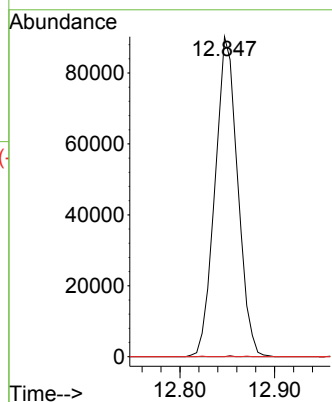

#83
 tert-Butylbenzene
 Concen: 0.228 ug/l
 RT: 13.447 min Scan# 1954
 Delta R.T. 0.006 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17

Tgt Ion: 119 Resp: 3831
 Ion Ratio Lower Upper
 119 100
 91 80.0 36.8 110.4
 134 22.6 12.4 37.4

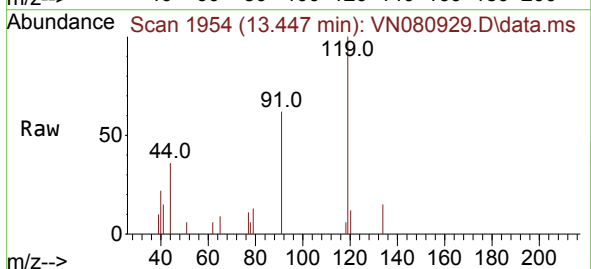

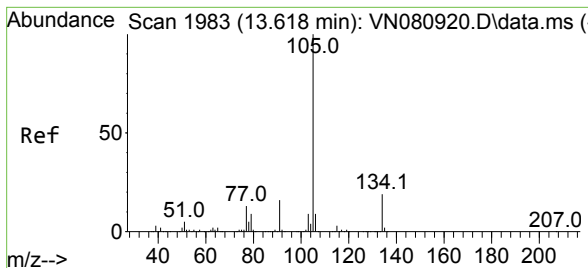

#85

sec-Butylbenzene

Concen: 0.330 ug/l

RT: 13.618 min Scan# 1983

Delta R.T. -0.000 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Instrument :

MSVOA_N

ClientSampleId :





VN0207MBL01

Tgt Ion:105 Resp: 7461

Ion Ratio Lower Upper

105 100

134 28.0 8.6 25.8#

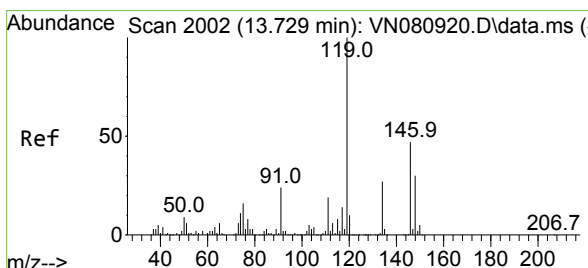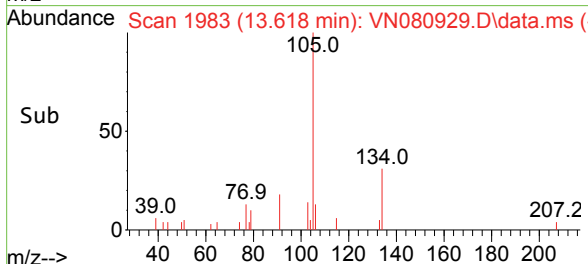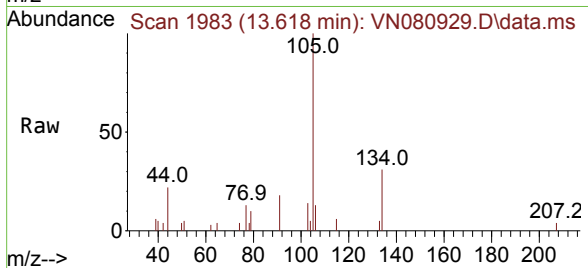

#86

p-Isopropyltoluene

Concen: 0.326 ug/l

RT: 13.729 min Scan# 2002

Delta R.T. -0.000 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17




Tgt Ion:119 Resp: 6220


Ion Ratio Lower Upper

119 100

134 27.8 12.4 37.2

91 21.0 13.5 40.4

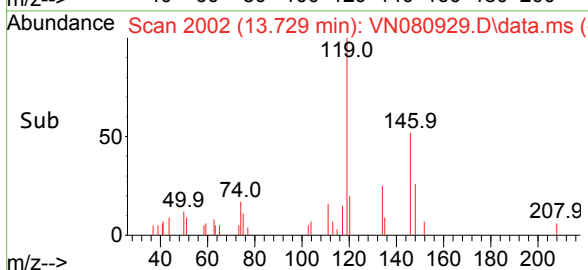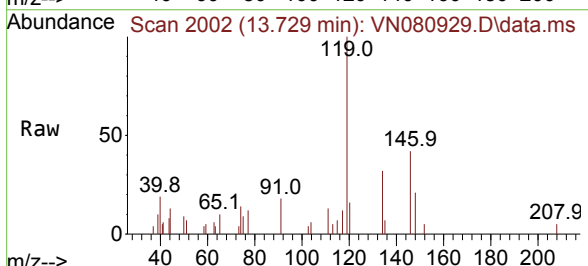



#87

1,3-Dichlorobenzene

Concen: 0.247 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. -0.000 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Instrument :

MSVOA_N

ClientSampleId :

VN0207MBL01





Tgt Ion:146 Resp: 2697

Ion Ratio Lower Upper

146 100

111 33.6 23.9 71.7

148 56.6 32.6 97.7



#88

1,4-Dichlorobenzene

Concen: 0.244 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. -0.076 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17




Tgt Ion:146 Resp: 2697


Ion Ratio Lower Upper

146 100

111 33.6 22.6 67.7

148 56.6 31.9 95.5



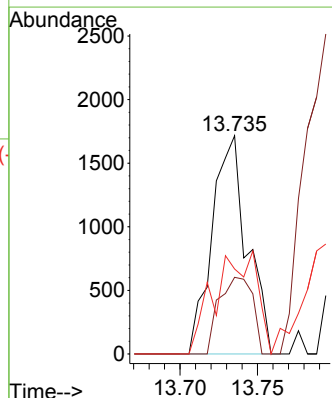



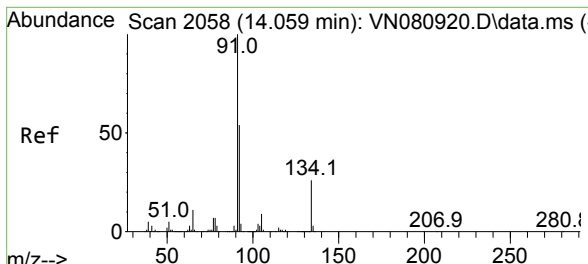

#89
 n-Butylbenzene
 Concen: 0.524 ug/l
 RT: 14.053 min Scan# 2057
 Delta R.T. -0.006 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0207MBL01


Tgt Ion:	91	Resp:	8846
Ion	Ratio	Lower	Upper
91	100		
92	46.3	26.7	80.1
134	22.0	10.8	32.4

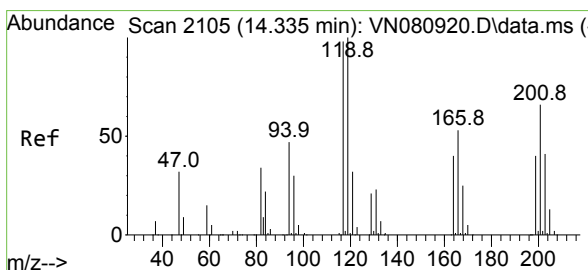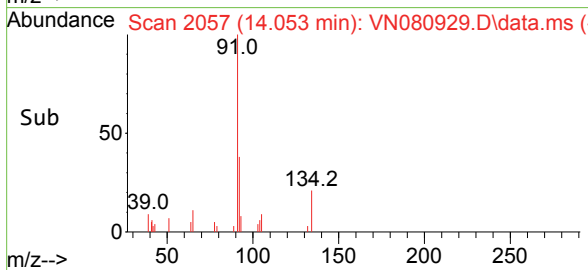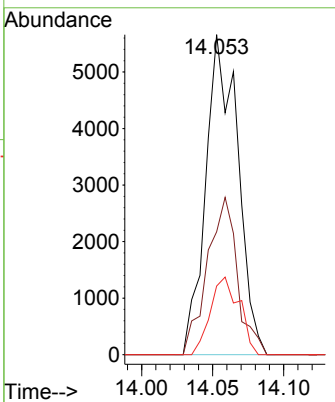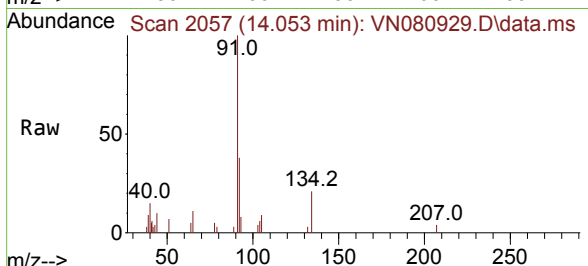

#90
 Hexachloroethane
 Concen: 0.216 ug/l
 RT: 14.335 min Scan# 2105
 Delta R.T. -0.000 min
 Lab File: VN080929.D
 Acq: 07 Feb 2024 10:17

Tgt Ion:	117	Resp:	651
Ion	Ratio	Lower	Upper
117	100		
201	59.1	30.0	90.0


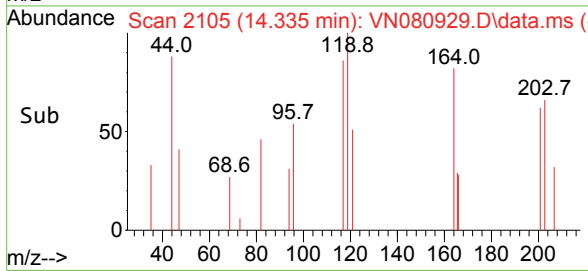
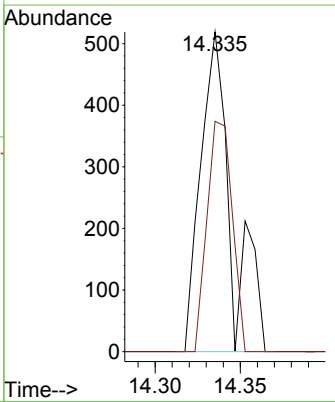
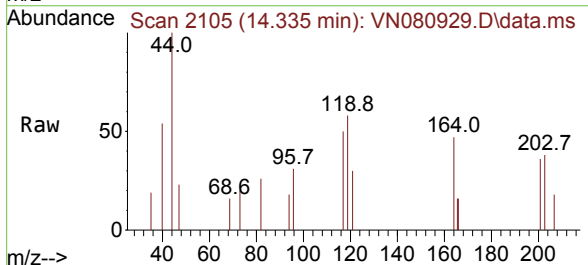




#93
1,2,4-Trichlorobenzene
Concen: 0.686 ug/l
RT: 15.388 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17




Instrument :
MSVOA_N
ClientSampleId :
VN0207MBL01


Tgt Ion:180 Resp: 3547
Ion Ratio Lower Upper
180 100
182 97.4 46.6 139.7
145 31.1 16.8 50.3

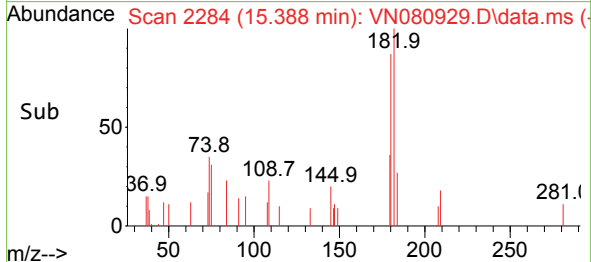

#94
Hexachlorobutadiene
Concen: 1.158 ug/l
RT: 15.500 min Scan# 2303
Delta R.T. -0.006 min
Lab File: VN080929.D
Acq: 07 Feb 2024 10:17

Tgt Ion:225 Resp: 2595
Ion Ratio Lower Upper
225 100
223 62.4 33.3 99.8
227 72.2 33.1 99.2

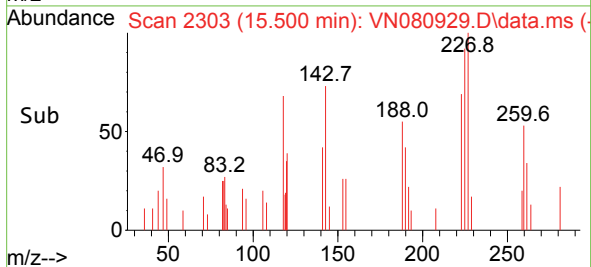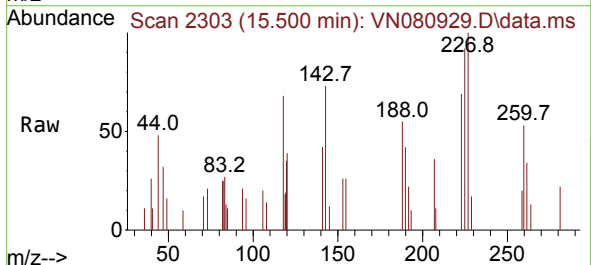



#95

Naphthalene

Concen: 0.661 ug/l

RT: 15.641 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Instrument :

MSVOA_N

ClientSampleId :

VN0207MBL01





Tgt Ion:128 Resp: 11283

Ion Ratio Lower Upper

128 100

127 6.2 10.0 15.0#

129 9.4 8.7 13.1

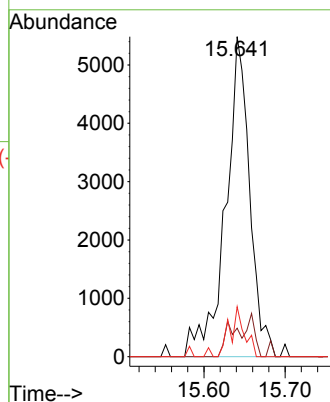

#96

1,2,3-Trichlorobenzene

Concen: 0.784 ug/l

RT: 15.847 min Scan# 2362

Delta R.T. 0.006 min

Lab File: VN080929.D

Acq: 07 Feb 2024 10:17

Tgt Ion:180 Resp: 3990

Ion Ratio Lower Upper

180 100

182 97.2 46.5 139.3

145 34.9 17.8 53.4

