

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
 Data File : VN080936.D
 Acq On : 07 Feb 2024 14:51
 Operator : JC\MD
 Sample : P1367-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EB-5-6-8

Quant Time: Feb 08 00:26:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 07 06:22:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	445400	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	9.100	114	909414	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	1032140	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	469377	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	268636	47.811	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	95.620%		
35) Dibromofluoromethane	8.165	113	262811	53.856	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	107.720%		
50) Toluene-d8	10.571	98	979012	55.465	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	110.920%		
62) 4-Bromofluorobenzene	12.847	95	414171	64.591	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	129.180%#		
Target Compounds						
						Qvalue
3) Chloromethane	2.359	50	4568	Below Cal		95
4) Vinyl Chloride	2.501	62	1343	0.204	ug/l	99
5) Bromomethane	2.977	94	2345	0.553	ug/l #	20
11) Tert butyl alcohol	5.530	59	3408	4.402	ug/l #	76
13) Acrolein	4.200	56	1550	1.589	ug/l	100
16) Acetone	4.430	43	50149	27.129	ug/l	92
18) Methyl Acetate	5.042	43	5885	Below Cal	#	78
20) Methylene Chloride	5.277	84	23876	4.263	ug/l #	77
21) trans-1,2-Dichloroethene	5.777	96	3032	0.566	ug/l #	27
25) 2-Butanone	7.483	43	18960	6.390	ug/l #	80
27) cis-1,2-Dichloroethene	7.477	96	6261	1.005	ug/l	66
29) Tetrahydrofuran	7.841	42	1496	0.825	ug/l #	59
31) Cyclohexane	8.224	56	9119	1.187	ug/l #	1
36) 1,1-Dichloropropene	8.230	75	33313	4.589	ug/l #	52
37) Ethyl Acetate	7.559	43	11204	2.040	ug/l	99
38) Carbon Tetrachloride	8.224	117	45258	6.081	ug/l #	16
42) 1,2-Dichloroethane	8.682	62	2186	0.284	ug/l #	75
43) Isopropyl Acetate	8.688	43	301695	29.867	ug/l #	91
44) Trichloroethene	9.359	130	14488	2.158	ug/l	84
48) Methyl methacrylate	9.665	41	8494	1.492	ug/l #	50
49) 1,4-Dioxane	9.682	88	62	0.590	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	20381	3.348	ug/l #	80
52) Toluene	10.635	92	5793	0.391	ug/l	89
54) cis-1,3-Dichloropropene	10.359	75	117977	12.595	ug/l #	62
56) Ethyl methacrylate	10.988	69	3051	0.446	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	13935	1.501	ug/l #	43
59) 2-Hexanone	11.171	43	231334	50.139	ug/l #	26
74) N-amyl acetate	12.453	43	2737	0.208	ug/l #	46
76) 1,2,3-Trichloropropane	12.853	75	214685	22.432	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	214685	60.946	ug/l #	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
Data File : VN080936.D
Acq On : 07 Feb 2024 14:51
Operator : JC\MD
Sample : P1367-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8

Quant Time: Feb 08 00:26:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 07 06:22:23 2024
Response via : Initial Calibration




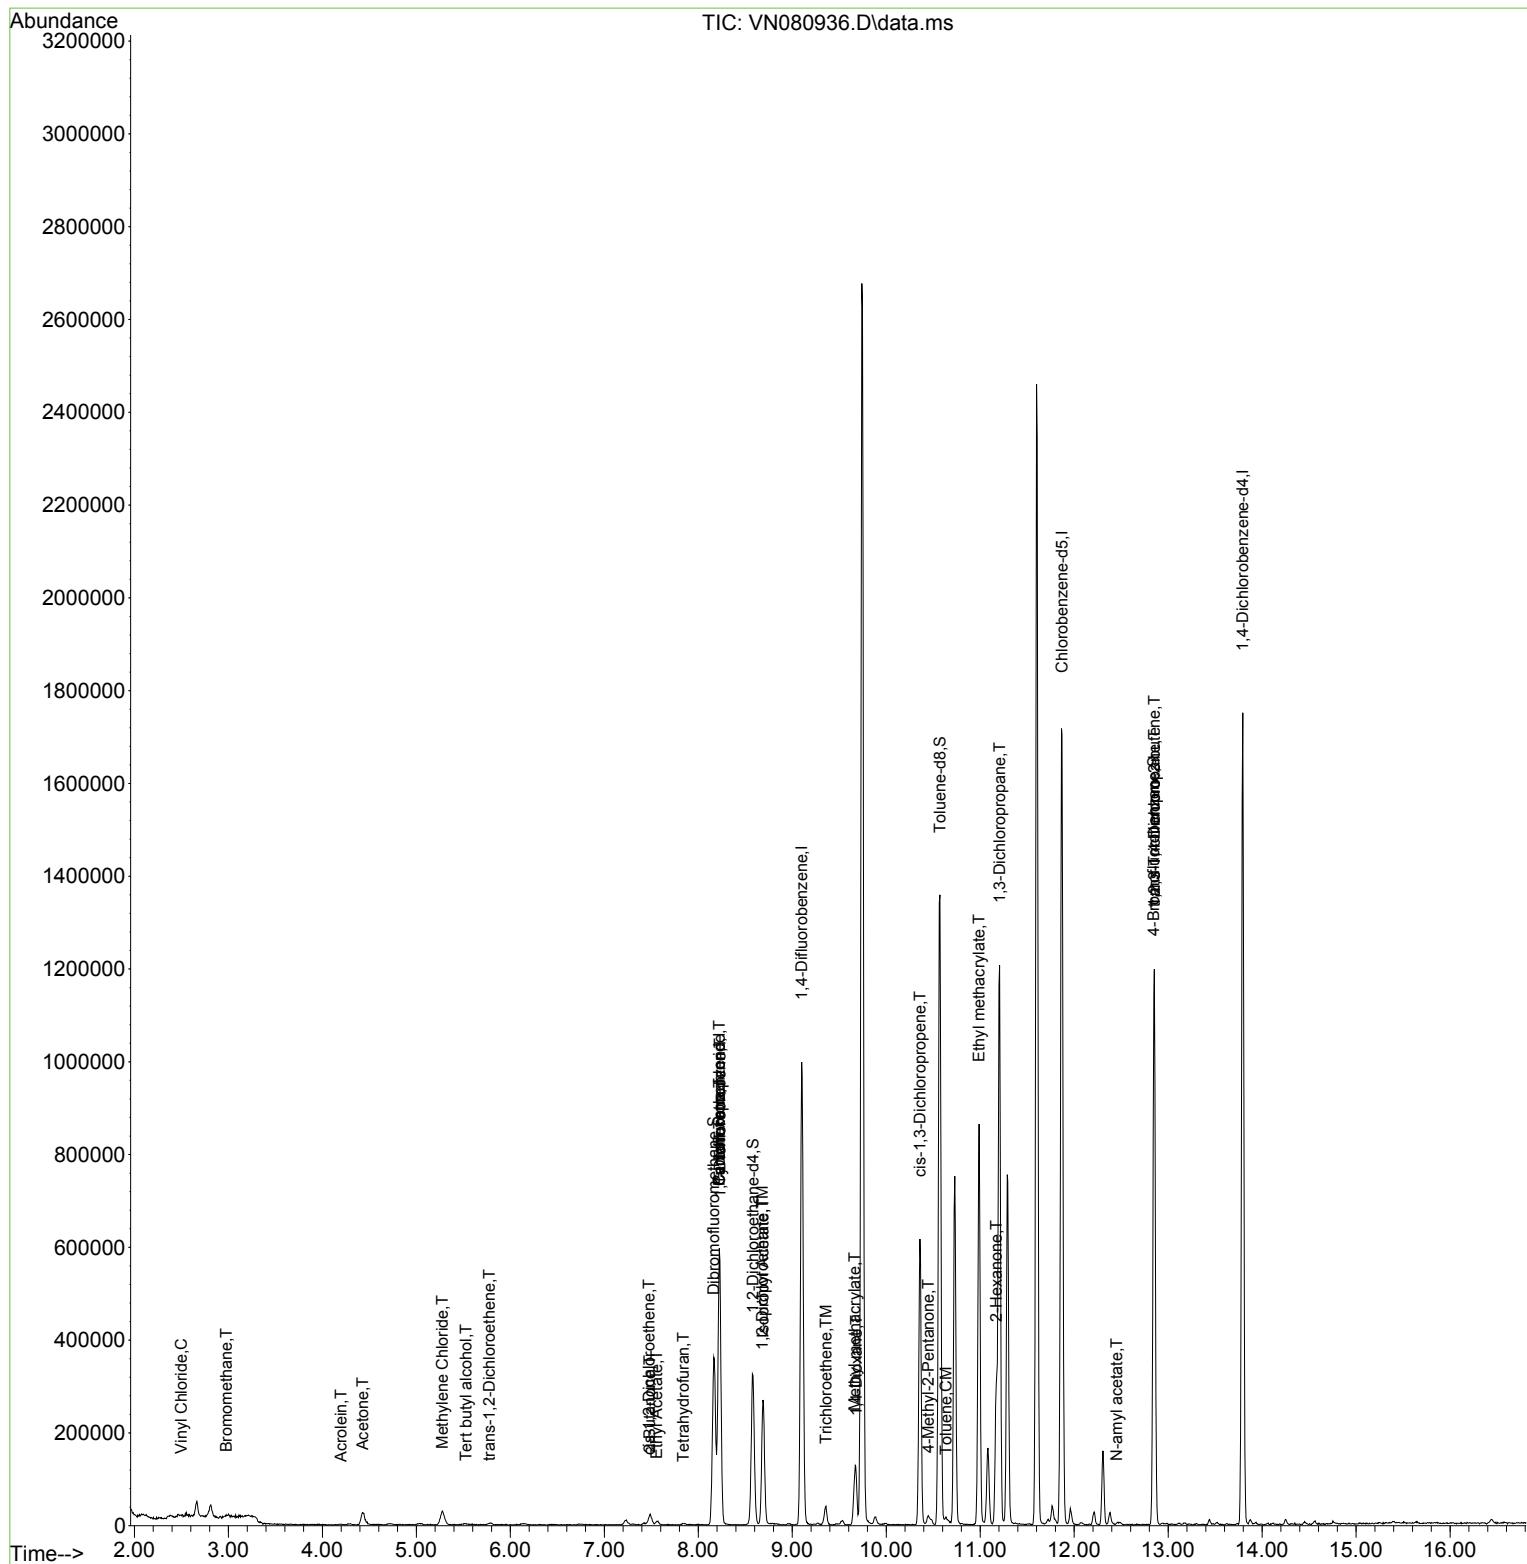




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion:168 Resp: 445400
Ion Ratio Lower Upper
168 100
99 58.8 59.9 89.9#

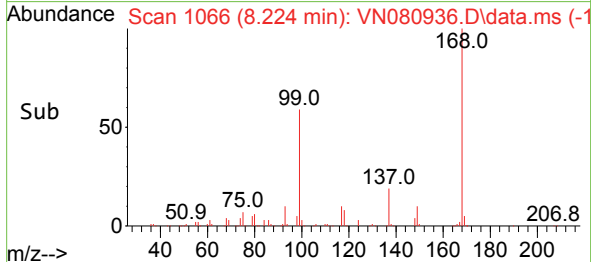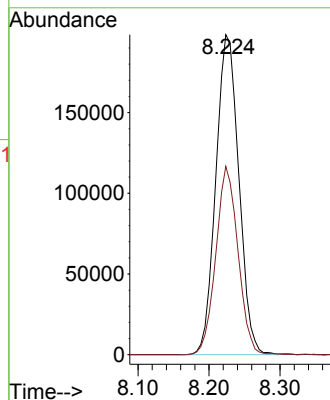

#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 50 Resp: 4568
Ion Ratio Lower Upper
50 100
52 33.7 25.0 37.4


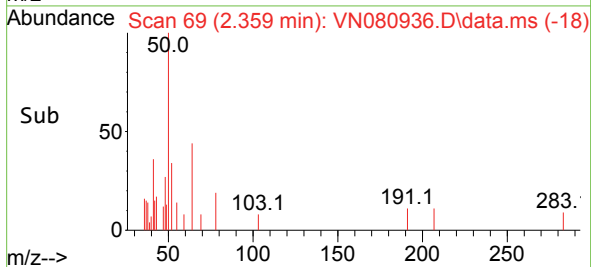
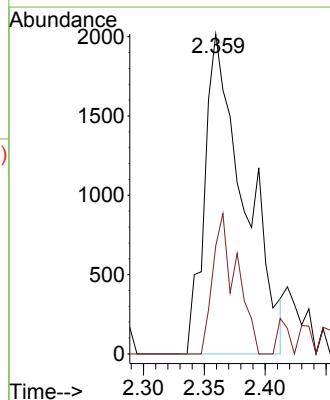
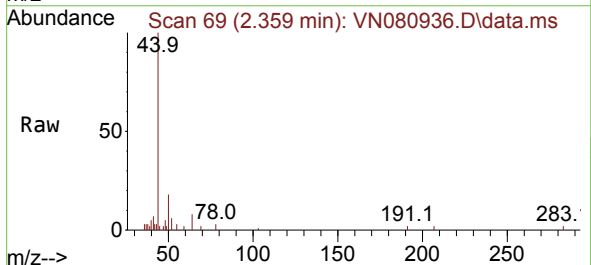




#4
Vinyl Chloride
Concen: 0.204 ug/l
RT: 2.501 min Scan# 91
Delta R.T. -0.012 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 62 Resp: 1343
Ion Ratio Lower Upper
62 100
64 27.9 22.7 34.1

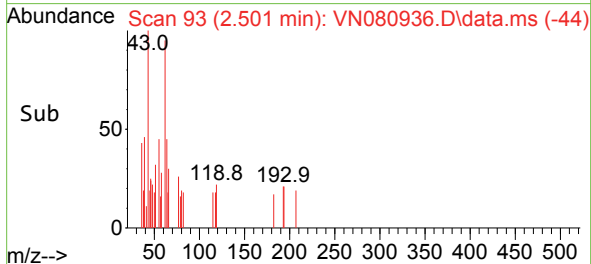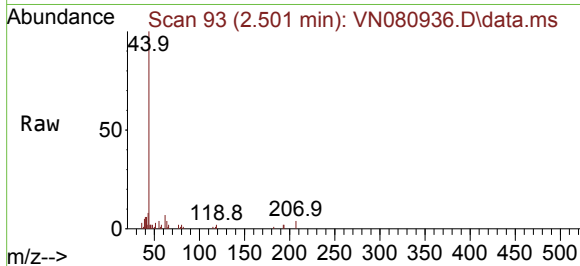

#5
Bromomethane
Concen: 0.553 ug/l
RT: 2.977 min Scan# 174
Delta R.T. 0.029 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 94 Resp: 2345
Ion Ratio Lower Upper
94 100
96 160.5 69.2 103.8#


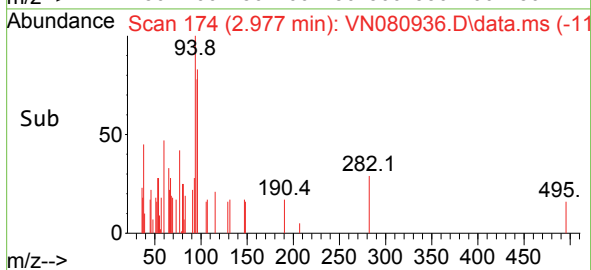

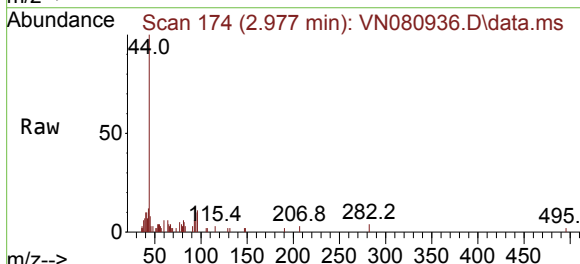




#11
Tert butyl alcohol
Concen: 4.402 ug/l
RT: 5.530 min Scan# 605
Delta R.T. 0.018 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 59 Resp: 3408
Ion Ratio Lower Upper
59 100
57 1.7 8.6 12.8#

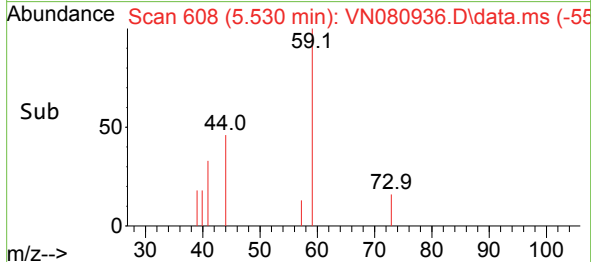

#13
Acrolein
Concen: 1.589 ug/l
RT: 4.200 min Scan# 382
Delta R.T. 0.023 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 56 Resp: 1550
Ion Ratio Lower Upper
56 100
55 69.0 55.3 82.9


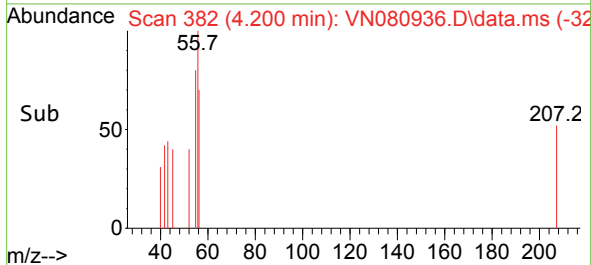

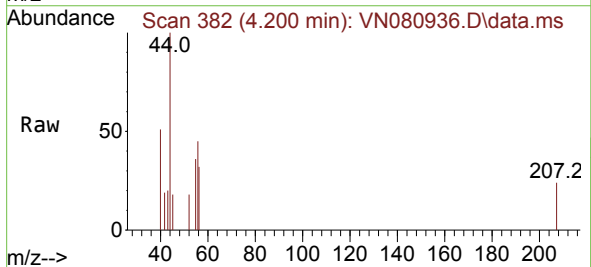




#16
Acetone
Concen: 27.129 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 43 Resp: 50149
Ion Ratio Lower Upper
43 100
58 35.2 24.8 37.2

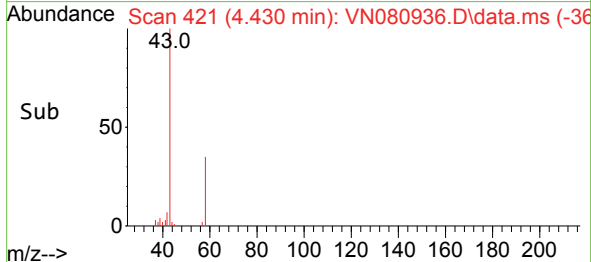

#18
Methyl Acetate
Concen: Below Cal
RT: 5.042 min Scan# 525
Delta R.T. 0.024 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 43 Resp: 5885
Ion Ratio Lower Upper
43 100
74 32.0 17.3 25.9#


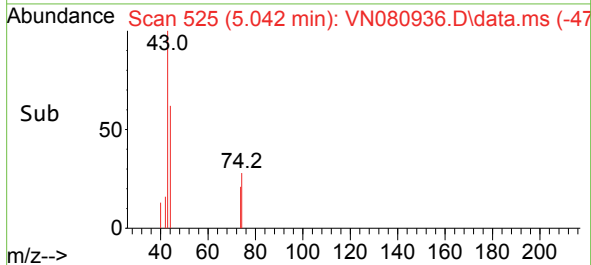

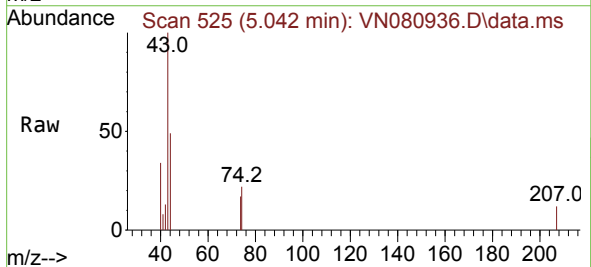




#20
Methylene Chloride
Concen: 4.263 ug/l
RT: 5.277 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion:	84	Resp:	23876
Ion	Ratio	Lower	Upper
84	100		
49	103.4	108.1	162.1#
51	32.0	32.9	49.3#
86	77.6	48.6	73.0#

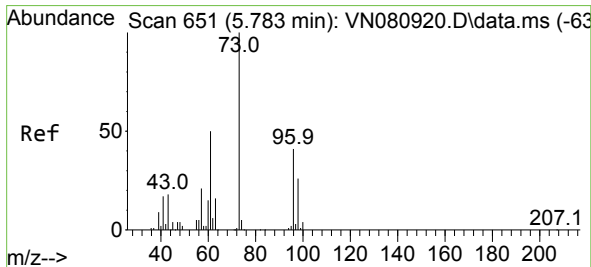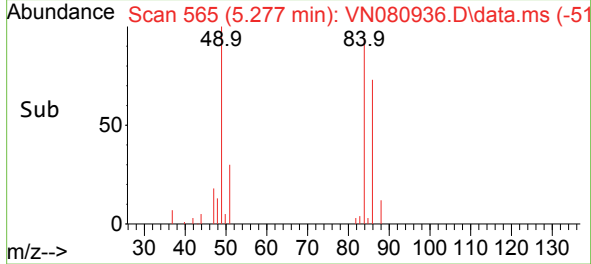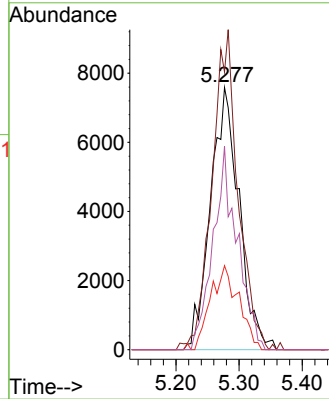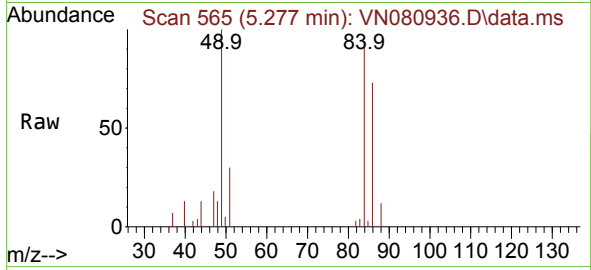

#21
trans-1,2-Dichloroethene
Concen: 0.566 ug/l
RT: 5.777 min Scan# 650
Delta R.T. -0.006 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion:	96	Resp:	3032
Ion	Ratio	Lower	Upper
96	100		
61	47.5	112.8	169.2#
98	13.3	51.0	76.4#


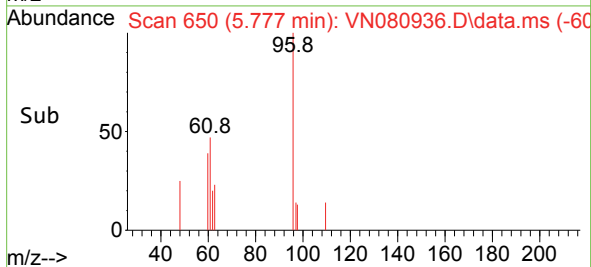
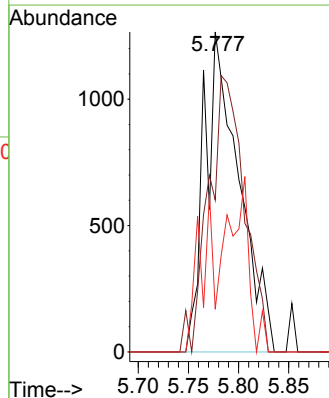
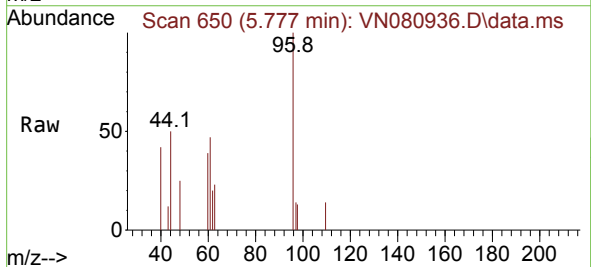




#25
2-Butanone
Concen: 6.390 ug/l
RT: 7.483 min Scan# 940
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 43 Resp: 18960
Ion Ratio Lower Upper
43 100
72 34.4 19.5 29.3#

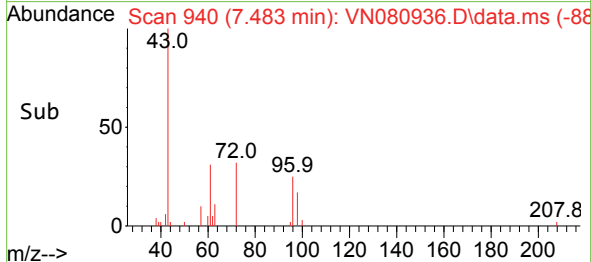

#27
cis-1,2-Dichloroethene
Concen: 1.005 ug/l
RT: 7.477 min Scan# 939
Delta R.T. -0.012 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 96 Resp: 6261
Ion Ratio Lower Upper
96 100
61 103.0 0.0 325.4
98 58.5 0.0 130.4

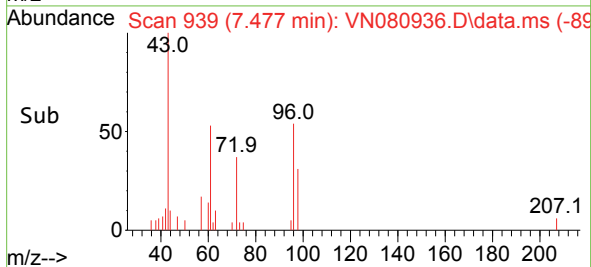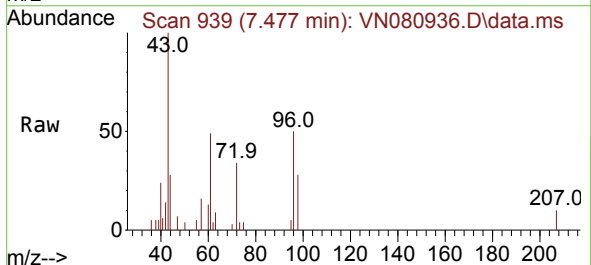



#29

Tetrahydrofuran

Concen: 0.825 ug/l

RT: 7.841 min Scan# 1066

Delta R.T. 0.006 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :

EB-5-6-8





Tgt Ion: 42 Resp: 1496

Ion Ratio Lower Upper

42 100

72 24.8 31.1 46.7#

71 0.0 28.3 42.5#

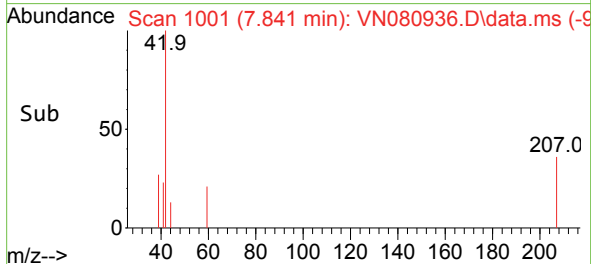

#31

Cyclohexane

Concen: 1.187 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.035 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51




Tgt Ion: 56 Resp: 9119


Ion Ratio Lower Upper

56 100

69 134.3 20.1 30.1#

84 125.3 56.9 85.3#

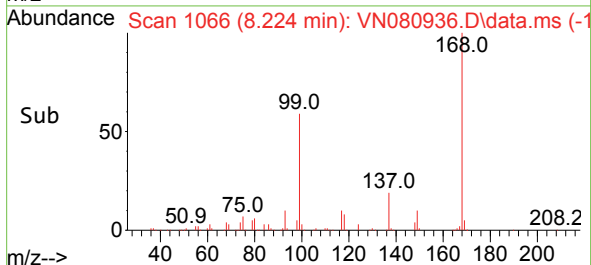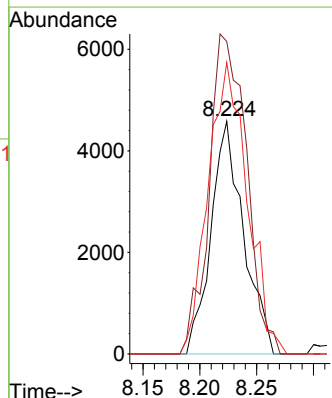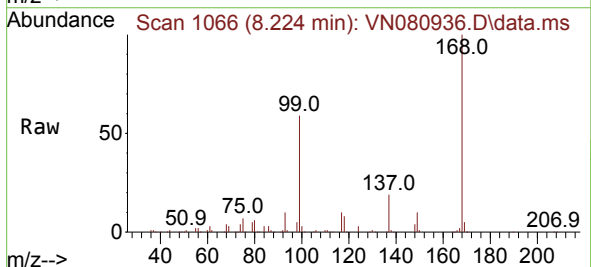



#33

1,2-Dichloroethane-d4

Concen: 47.811 ug/l

RT: 8.582 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :





EB-5-6-8

Tgt Ion: 65 Resp: 268636

Ion Ratio Lower Upper

65 100

67 51.7 0.0 102.4

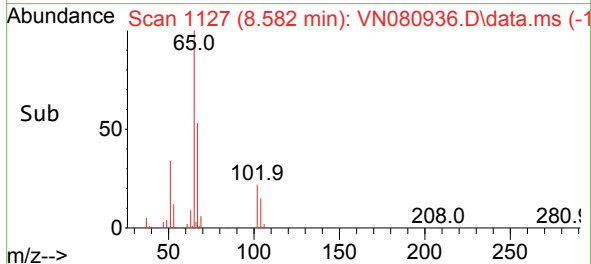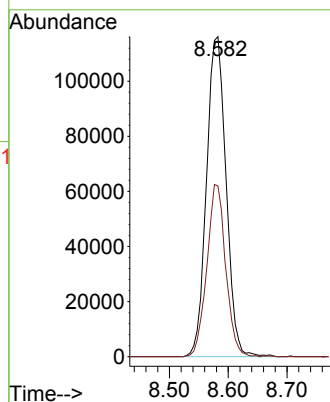

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.000 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51




Tgt Ion: 114 Resp: 909414


Ion Ratio Lower Upper

114 100

63 18.8 0.0 48.0

88 14.2 0.0 34.8


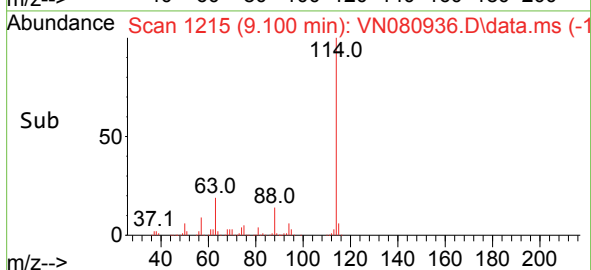
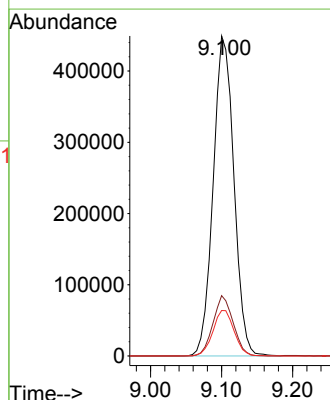





#35
Dibromofluoromethane
Concen: 53.856 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion:113 Resp: 262811
Ion Ratio Lower Upper
113 100
111 102.3 82.2 123.4
192 18.8 12.5 18.7#

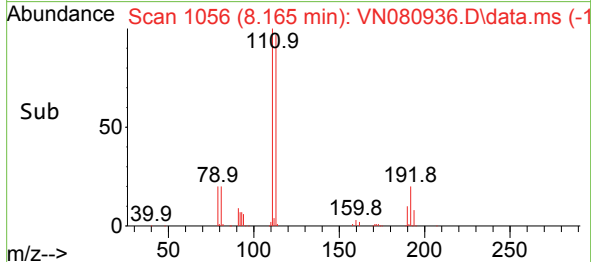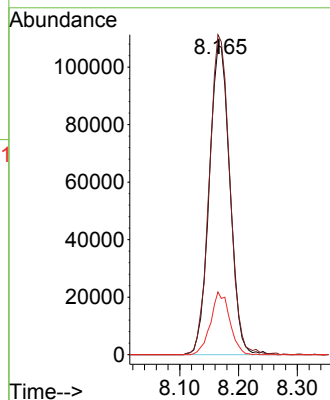

#36
1,1-Dichloropropene
Concen: 4.589 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.141 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 75 Resp: 33313
Ion Ratio Lower Upper
75 100
110 10.4 16.0 48.0#
77 0.2 25.8 38.6#

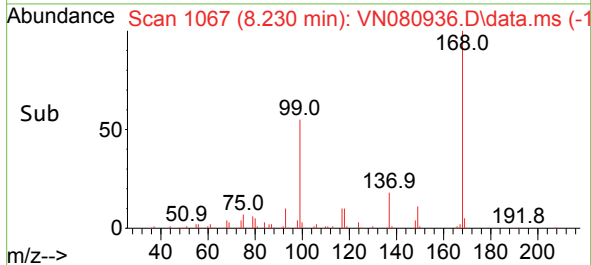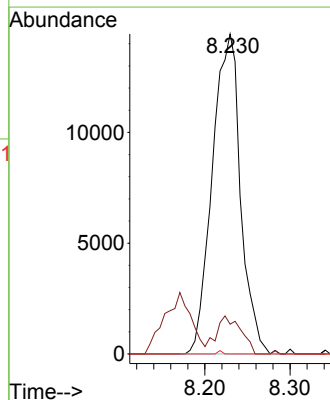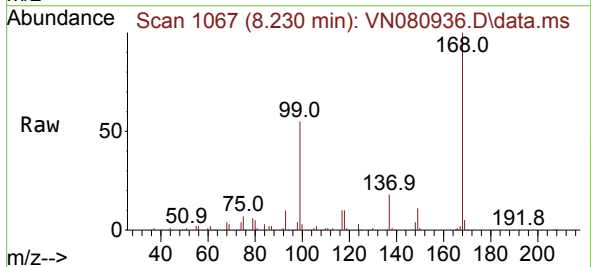



#37

Ethyl Acetate

Concen: 2.040 ug/l

RT: 7.559 min Scan# 91

Delta R.T. -0.000 min

Lab File: VN080936.D


Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :

EB-5-6-8

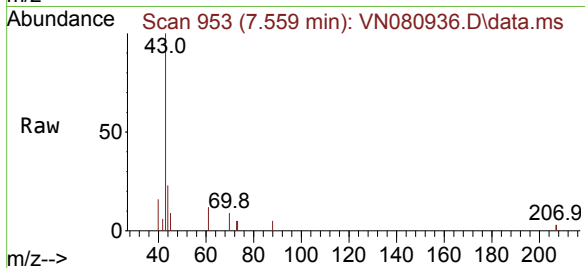




Tgt Ion: 43 Resp: 11204

Ion Ratio Lower Upper

43 100

61 13.5 10.6 15.8

70 10.0 8.0 12.0

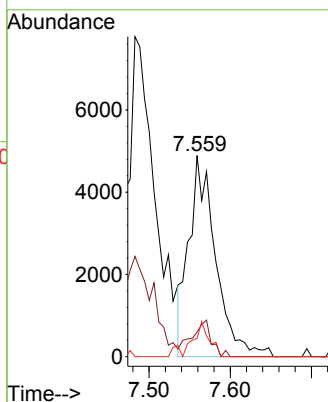

#38

Carbon Tetrachloride

Concen: 6.081 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.135 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51




Tgt Ion: 117 Resp: 45258


Ion Ratio Lower Upper

117 100

119 3.4 73.4 110.2#

121 0.0 24.4 36.6#

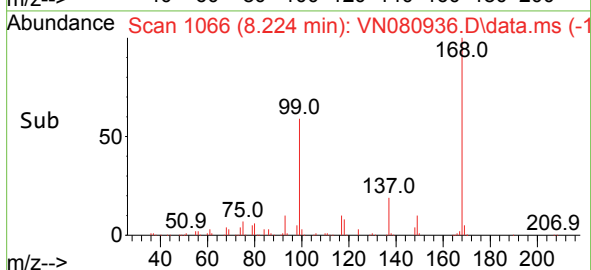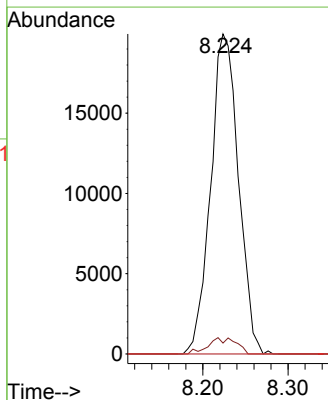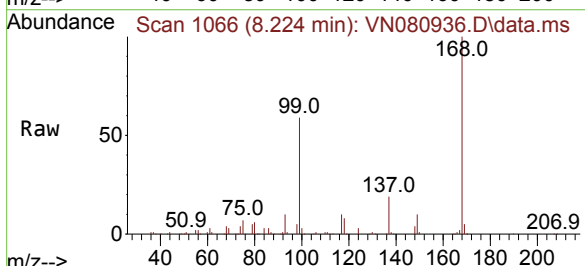



#42

1,2-Dichloroethane

Concen: 0.284 ug/l

RT: 8.682 min Scan# 1144

Delta R.T. 0.012 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :





EB-5-6-8

Tgt Ion: 62 Resp: 2186

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.0

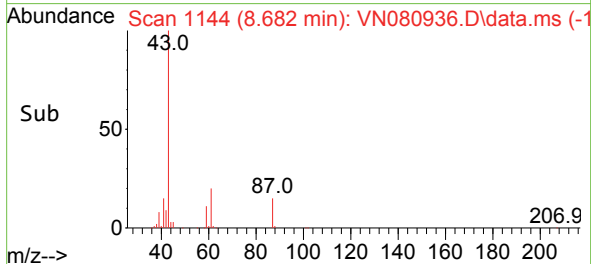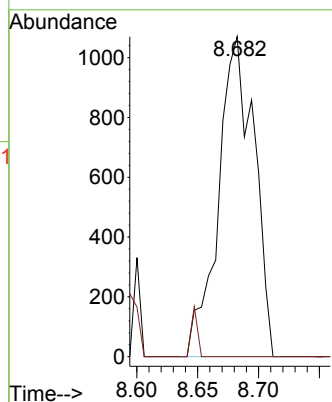

#43

Isopropyl Acetate

Concen: 29.867 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. -0.000 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51




Tgt Ion: 43 Resp: 301695


Ion Ratio Lower Upper

43 100

61 20.9 19.9 29.9

87 15.8 9.0 13.6#



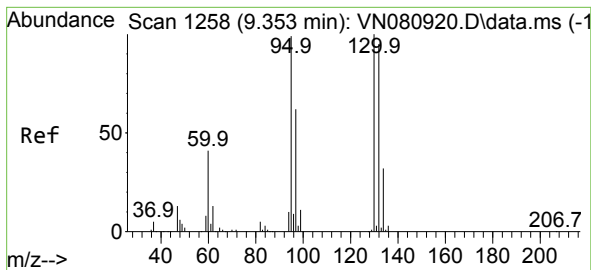

#44

Trichloroethene

Concen: 2.158 ug/l

RT: 9.359 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :





EB-5-6-8

Tgt Ion:130 Resp: 14488

Ion Ratio Lower Upper

130 100

95 88.2 0.0 210.4

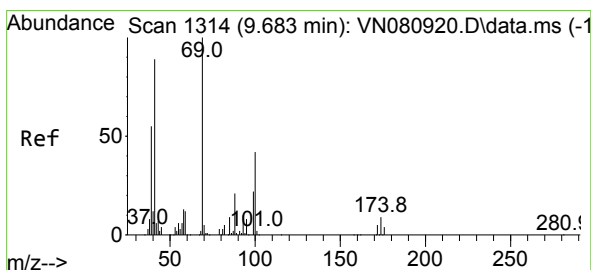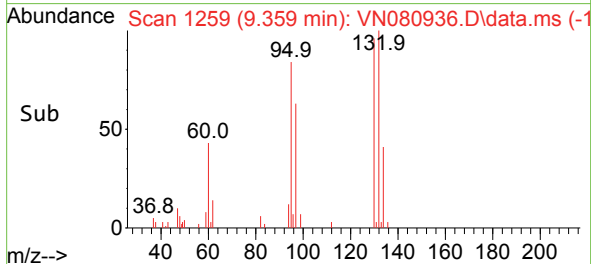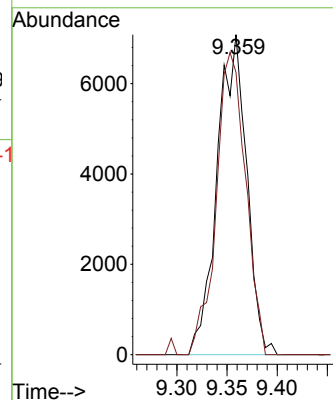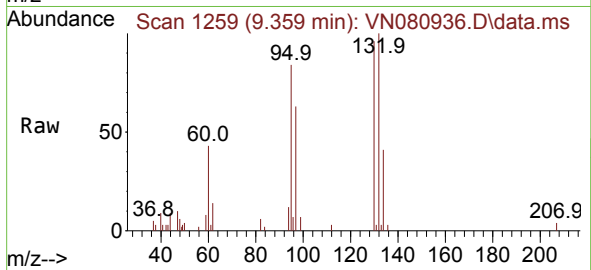

#48

Methyl methacrylate

Concen: 1.492 ug/l

RT: 9.665 min Scan# 1311

Delta R.T. -0.018 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51




Tgt Ion: 41 Resp: 8494


Ion Ratio Lower Upper

41 100

69 1.6 62.2 93.2#

39 59.2 47.6 71.4

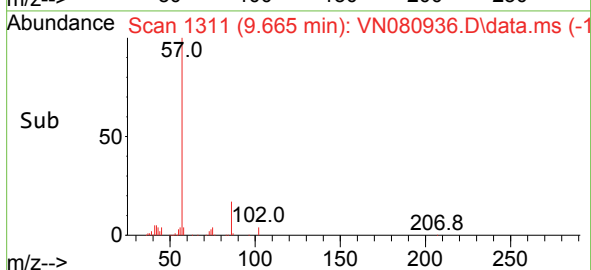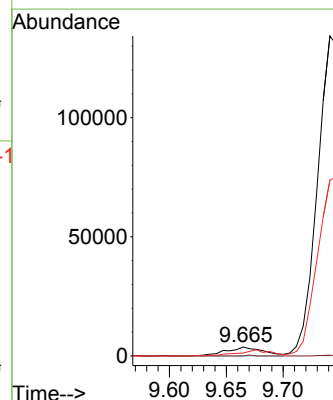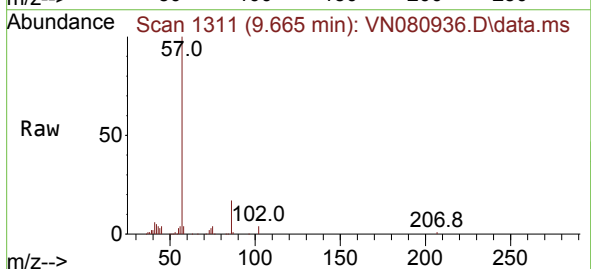



#49

1,4-Dioxane

Concen: 0.590 ug/l

RT: 9.682 min Scan# 11

Delta R.T. -0.012 min

Lab File: VN080936.D


Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :

EB-5-6-8






Tgt Ion: 88 Resp: 62

Ion Ratio Lower Upper

88 100

43 0.0 30.1 45.1#

58 11461.3 63.9 95.9#

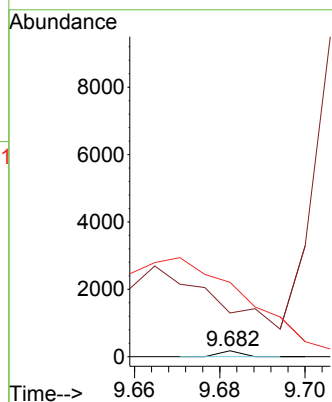

#50

Toluene-d8

Concen: 55.465 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN080936.D




Acq: 07 Feb 2024 14:51


Tgt Ion: 98 Resp: 979012

Ion Ratio Lower Upper

98 100

100 65.3 51.4 77.0


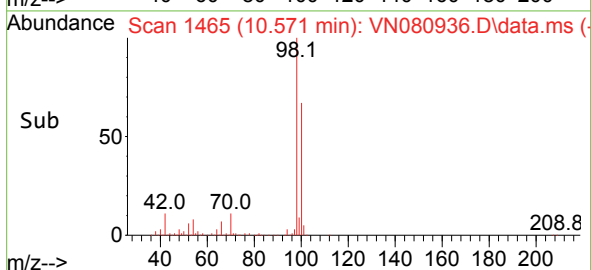




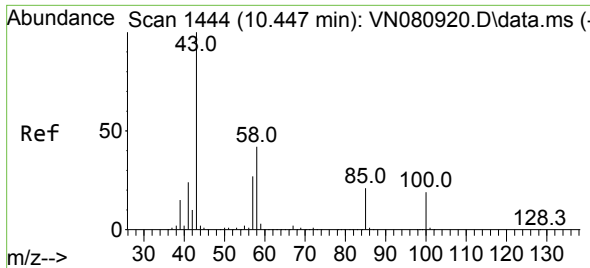

#51
4-Methyl-2-Pentanone
Concen: 3.348 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 43 Resp: 20381
Ion Ratio Lower Upper
43 100
58 25.0 29.4 44.0#

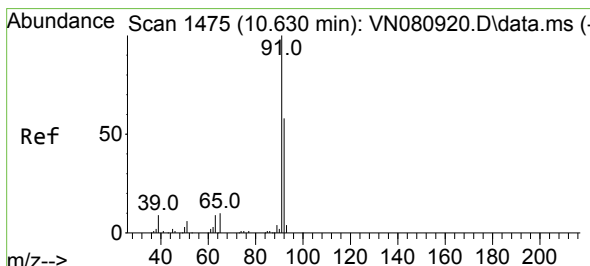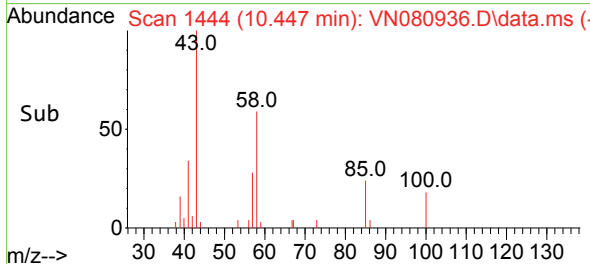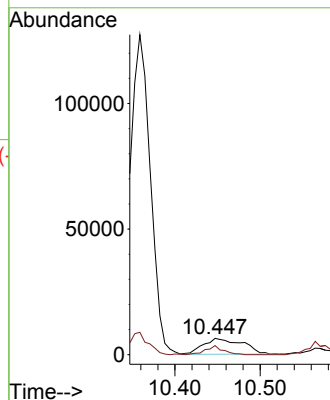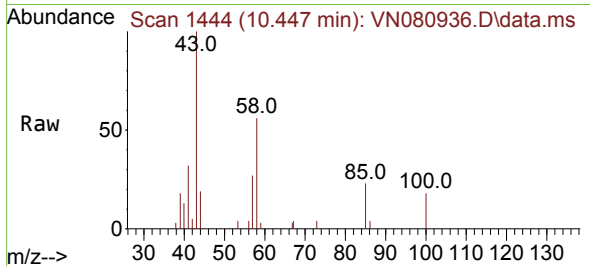

#52
Toluene
Concen: 0.391 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 92 Resp: 5793
Ion Ratio Lower Upper
92 100
91 159.5 139.4 209.0


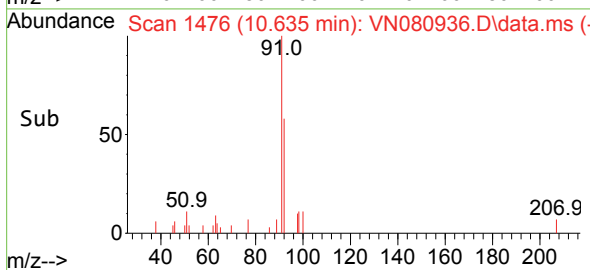
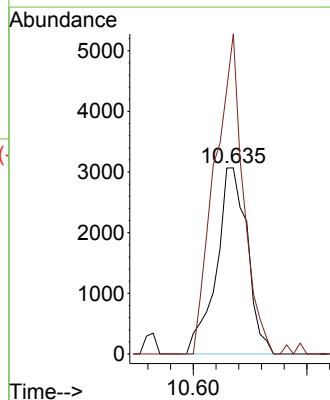
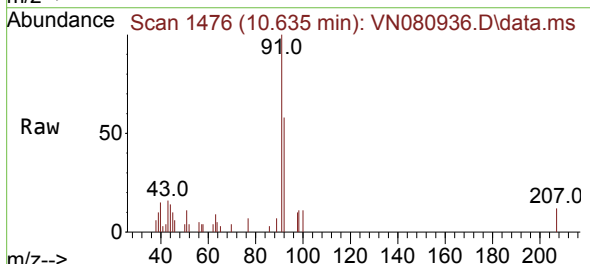


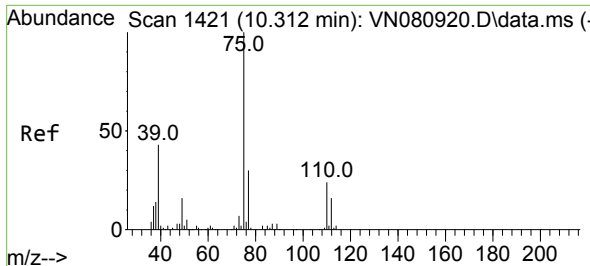

#54
 cis-1,3-Dichloropropene
 Concen: 12.595 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.047 min
 Lab File: VN080936.D
 Acq: 07 Feb 2024 14:51




Instrument :
 MSVOA_N
 ClientSampleId :
 EB-5-6-8


Tgt Ion: 75 Resp: 117977
 Ion Ratio Lower Upper
 75 100
 77 0.4 23.3 34.9#
 39 33.4 44.6 66.8#

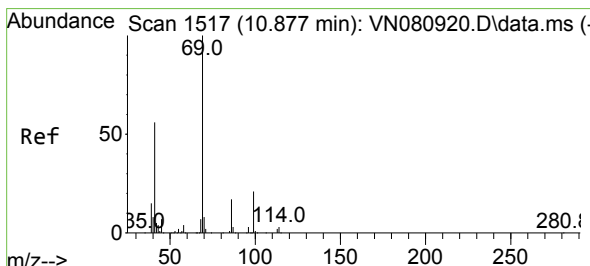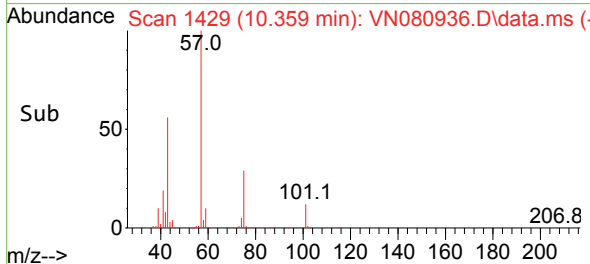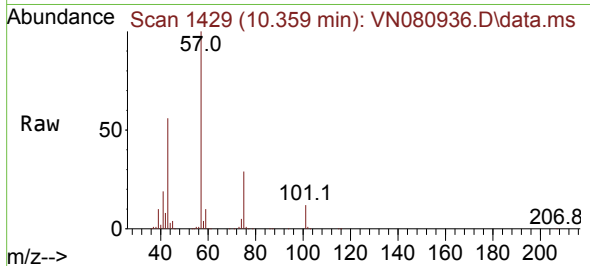

#56
 Ethyl methacrylate
 Concen: 0.446 ug/l
 RT: 10.988 min Scan# 1536
 Delta R.T. 0.111 min
 Lab File: VN080936.D
 Acq: 07 Feb 2024 14:51

Tgt Ion: 69 Resp: 3051
 Ion Ratio Lower Upper
 69 100
 41 5169.2 61.0 91.6#
 39 2421.0 31.8 47.6#

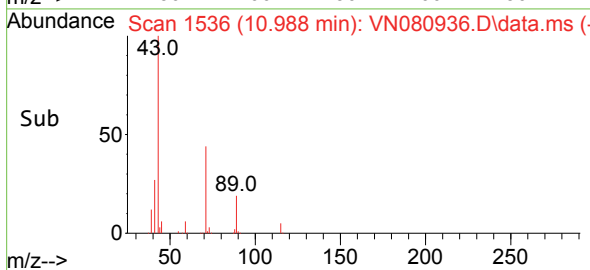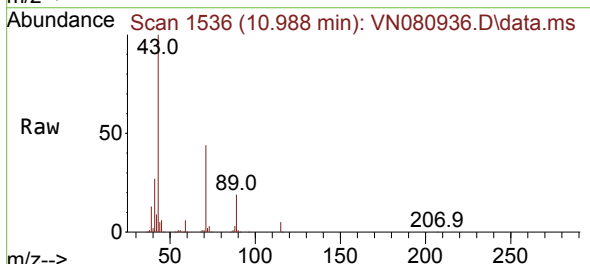



#57

1,3-Dichloropropane

Concen: 1.501 ug/l

RT: 11.206 min Scan# 1

Delta R.T. 0.041 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :





EB-5-6-8

Tgt Ion: 76 Resp: 13935

Ion Ratio Lower Upper

76 100

78 0.0 25.5 38.3#

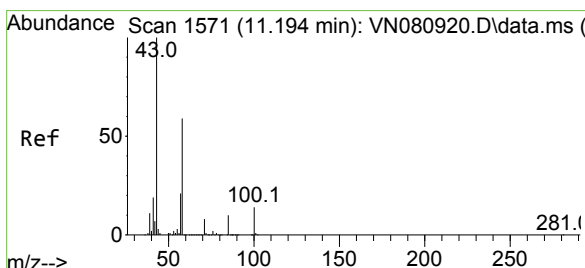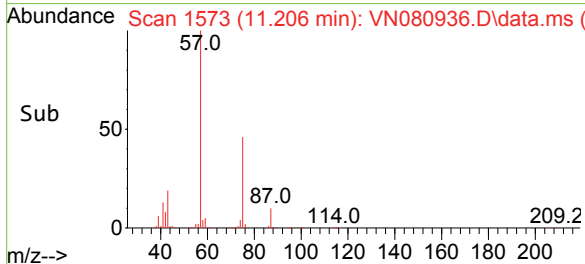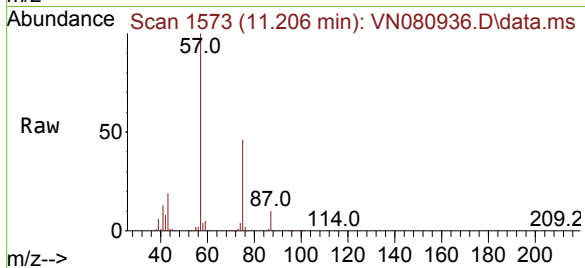

#59

2-Hexanone

Concen: 50.139 ug/l

RT: 11.171 min Scan# 1567

Delta R.T. -0.024 min

Lab File: VN080936.D




Acq: 07 Feb 2024 14:51


Tgt Ion: 43 Resp: 231334

Ion Ratio Lower Upper

43 100

58 0.0 25.9 77.8#


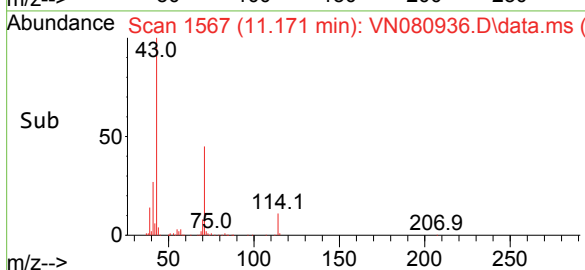

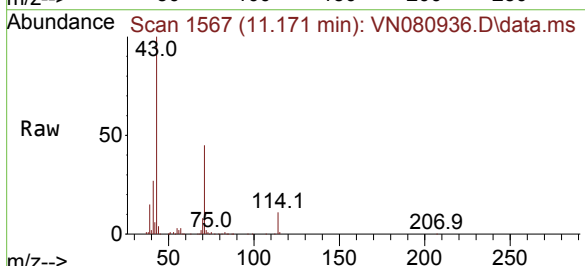


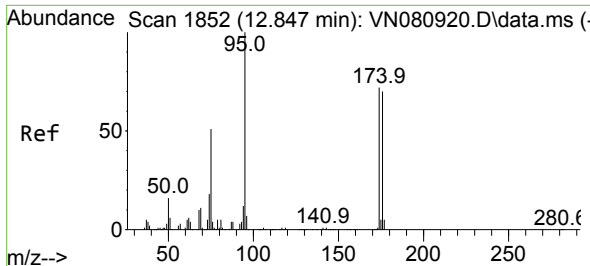

#62
4-Bromofluorobenzene
Concen: 64.591 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
EB-5-6-8


Tgt Ion: 95 Resp: 414171
Ion Ratio Lower Upper
95 100
174 83.0 0.0 120.4
176 77.5 0.0 121.0

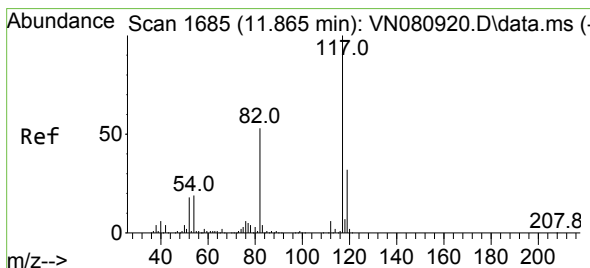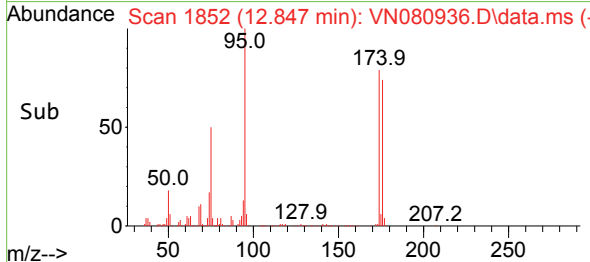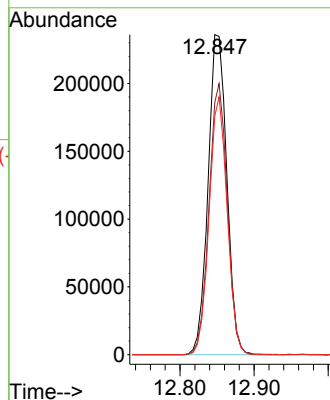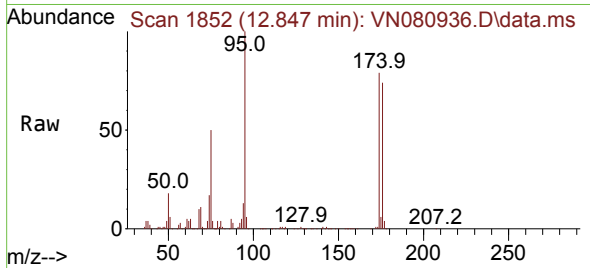

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN080936.D
Acq: 07 Feb 2024 14:51

Tgt Ion: 117 Resp: 1032140
Ion Ratio Lower Upper
117 100
82 51.1 52.7 79.1#
119 33.2 25.3 37.9


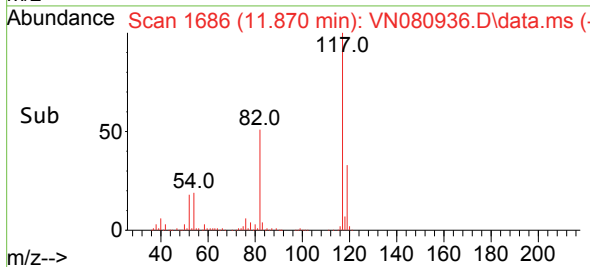
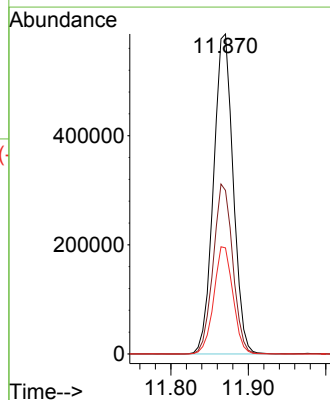
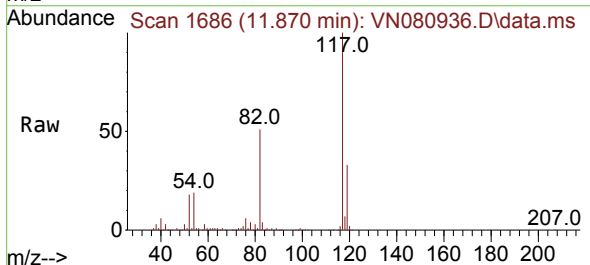


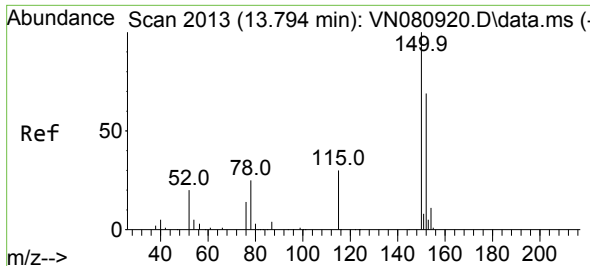

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN080936.D
 Acq: 07 Feb 2024 14:51




Instrument :
 MSVOA_N
 ClientSampleId :
 EB-5-6-8


Tgt Ion:152 Resp: 469377
 Ion Ratio Lower Upper
 152 100
 115 60.7 32.3 96.8
 150 159.5 0.0 339.8

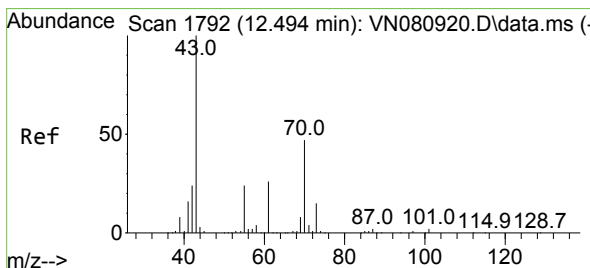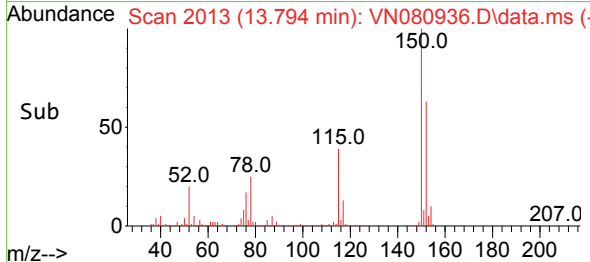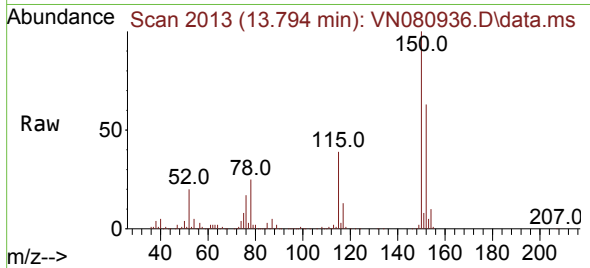

#74
 N-ethyl acetate
 Concen: 0.208 ug/l
 RT: 12.453 min Scan# 1785
 Delta R.T. -0.041 min
 Lab File: VN080936.D
 Acq: 07 Feb 2024 14:51

Tgt Ion: 43 Resp: 2737
 Ion Ratio Lower Upper
 43 100
 70 0.0 30.1 45.1#
 55 0.0 17.0 25.4#
 61 0.0 17.5 26.3#

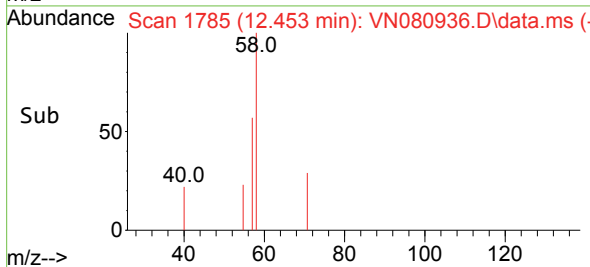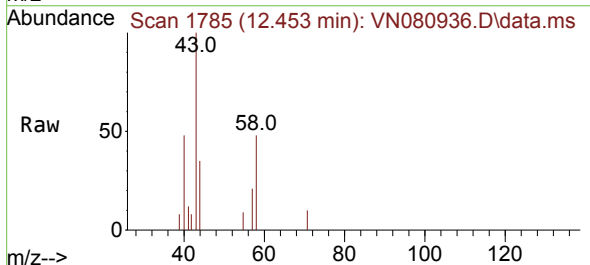



#76

1,2,3-Trichloropropane

Concen: 22.432 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :





EB-5-6-8

Tgt Ion: 75 Resp: 214685

Ion Ratio Lower Upper

75 100

77 1.1 91.0 272.8#

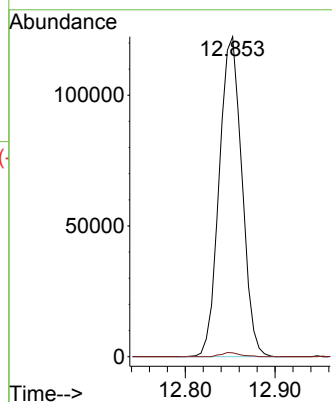

#81

trans-1,4-Dichloro-2-butene

Concen: 60.946 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.117 min

Lab File: VN080936.D

Acq: 07 Feb 2024 14:51

Tgt Ion: 75 Resp: 214685

Ion Ratio Lower Upper

75 100

53 0.0 71.4 107.2#

89 0.0 33.4 50.0#

