

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
 Data File : VN080940.D
 Acq On : 07 Feb 2024 16:51
 Operator : JC\MD
 Sample : PB158850ZHE#04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB158850ZHE#04

Quant Time: Feb 08 00:28:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 07 06:22:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	259437	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	563789	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	712562	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	304100	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	191914	58.639	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 117.280%	
35) Dibromofluoromethane	8.171	113	176804	58.442	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 116.880%	
50) Toluene-d8	10.571	98	705445	64.467	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 128.940%#	
62) 4-Bromofluorobenzene	12.853	95	293620	73.862	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 147.720%#	
Target Compounds						
					Qvalue	
3) Chloromethane	2.359	50	3295	Below Cal	#	74
5) Bromomethane	2.971	94	1502	0.608	ug/l #	21
6) Chloroethane	3.118	64	881	0.325	ug/l #	42
11) Tert butyl alcohol	5.512	59	450	0.998	ug/l #	72
13) Acrolein	4.177	56	296	0.521	ug/l #	46
16) Acetone	4.430	43	43853	40.727	ug/l	95
18) Methyl Acetate	5.042	43	5134	Below Cal	#	69
20) Methylene Chloride	5.289	84	8428	2.584	ug/l	86
25) 2-Butanone	7.506	43	6222	3.600	ug/l #	87
29) Tetrahydrofuran	7.836	42	526	0.498	ug/l #	38
31) Cyclohexane	8.224	56	6854	1.532	ug/l #	1
36) 1,1-Dichloropropene	8.218	75	21797	4.843	ug/l #	52
37) Ethyl Acetate	7.559	43	8504	2.497	ug/l #	89
38) Carbon Tetrachloride	8.230	117	26788	5.806	ug/l #	17
42) 1,2-Dichloroethane	8.688	62	1628	0.341	ug/l	86
43) Isopropyl Acetate	8.688	43	290435	46.379	ug/l #	89
48) Methyl methacrylate	9.741	41	234832	66.558	ug/l #	48
49) 1,4-Dioxane	9.671	88	165	2.533	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	11195	2.966	ug/l #	87
53) t-1,3-Dichloropropene	10.735	75	2531	0.489	ug/l #	43
54) cis-1,3-Dichloropropene	10.359	75	112266	19.333	ug/l #	58
56) Ethyl methacrylate	10.982	69	2732	0.644	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	15177	2.638	ug/l #	43
59) 2-Hexanone	11.171	43	221577	77.466	ug/l #	26
65) Chlorobenzene	11.894	112	3397	0.227	ug/l #	44
74) N-amyl acetate	12.488	43	3157	0.370	ug/l #	46
76) 1,2,3-Trichloropropane	12.853	75	160753	25.926	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	160753	70.438	ug/l #	14
95) Naphthalene	15.647	128	3559	0.214	ug/l #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020724\
Data File : VN080940.D
Acq On : 07 Feb 2024 16:51
Operator : JC\MD
Sample : PB158850ZHE#04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04

Quant Time: Feb 08 00:28:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 07 06:22:23 2024
Response via : Initial Calibration




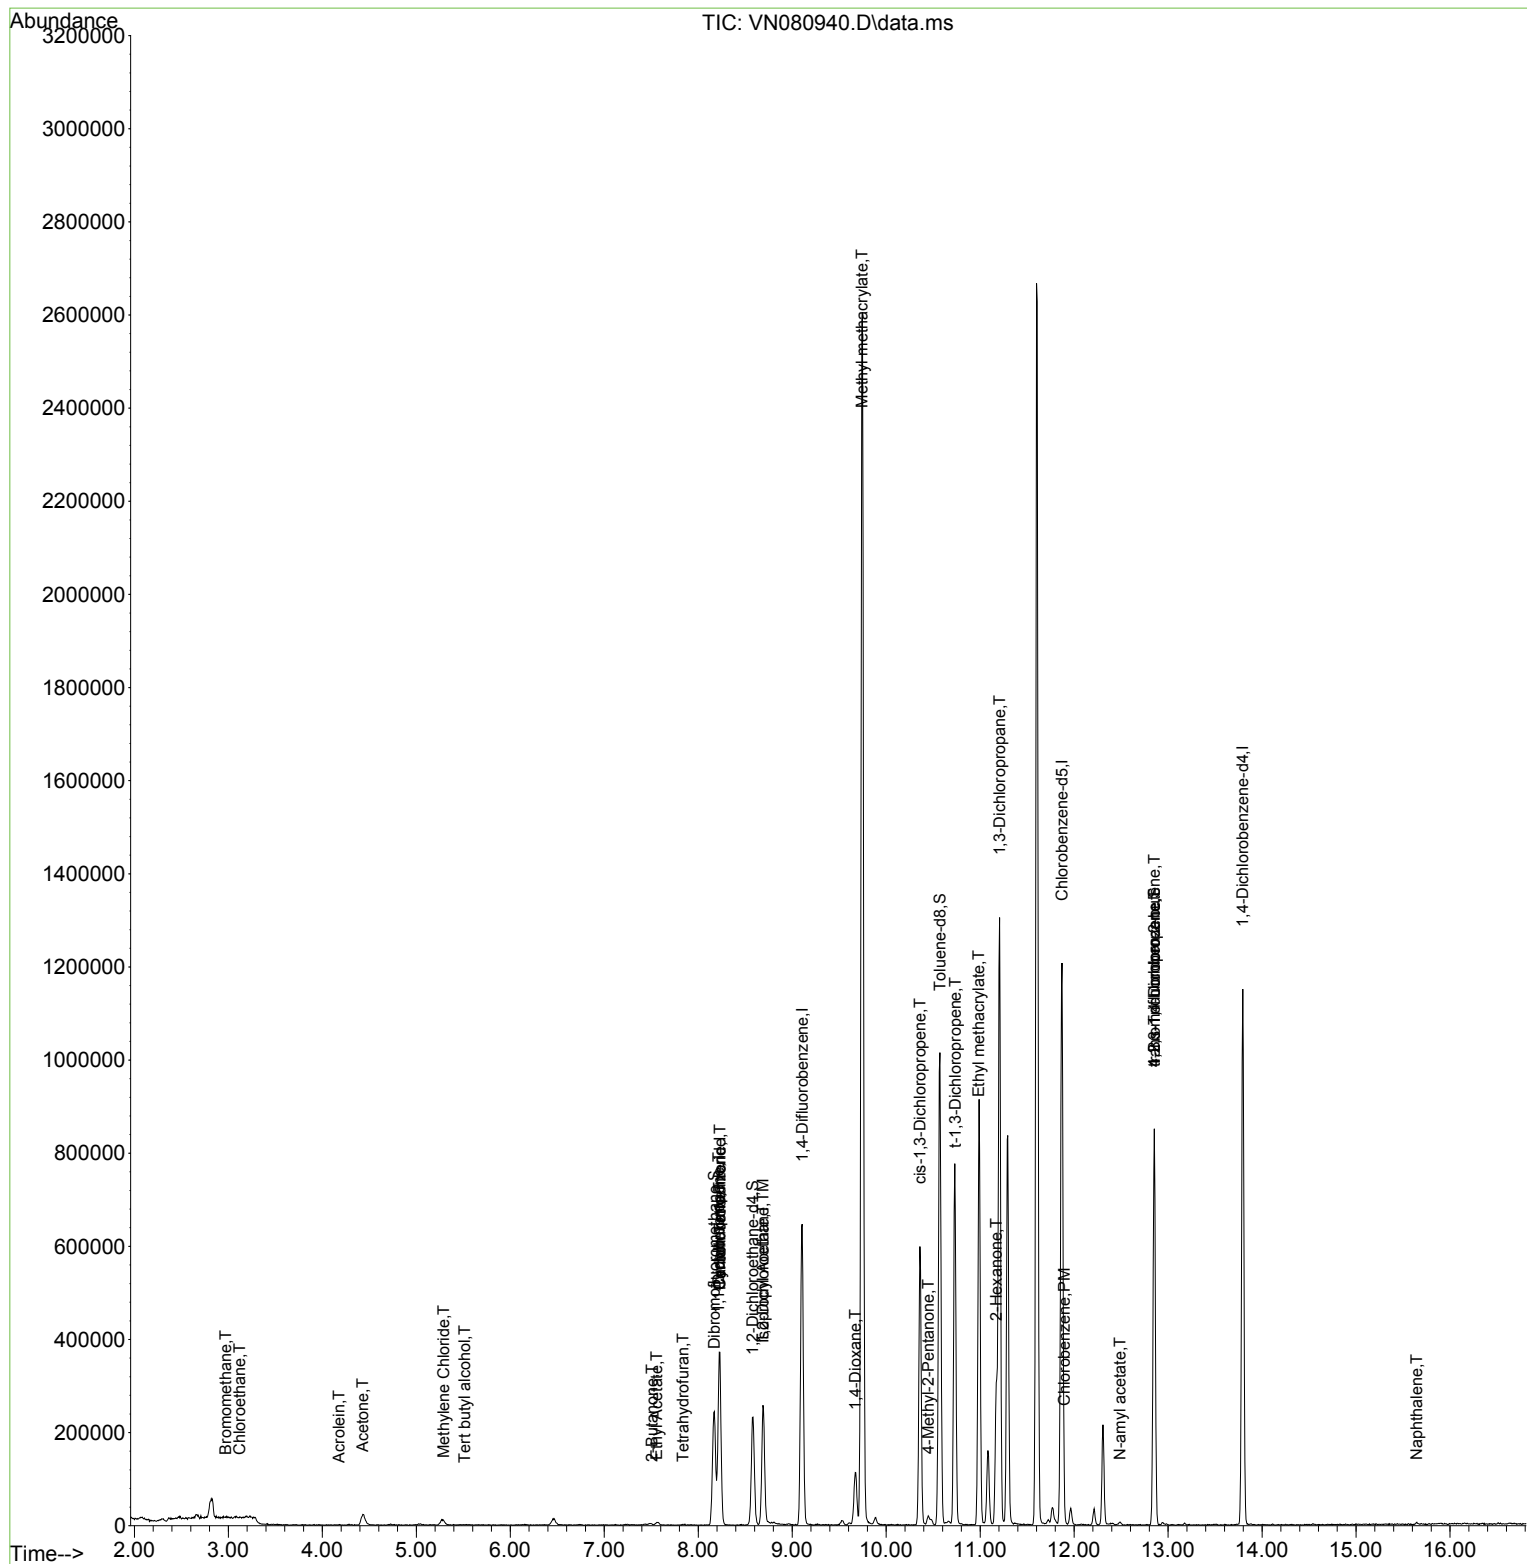




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion:168 Resp: 259437
Ion Ratio Lower Upper
168 100
99 62.4 59.9 89.9

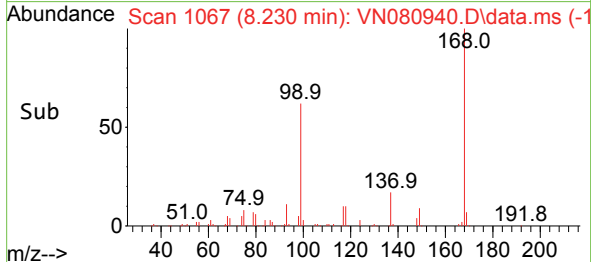

#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 50 Resp: 3295
Ion Ratio Lower Upper
50 100
52 16.9 25.0 37.4#









#5
Bromomethane
Concen: 0.608 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.024 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 94 Resp: 1502
Ion Ratio Lower Upper
94 100
96 13.6 69.2 103.8#

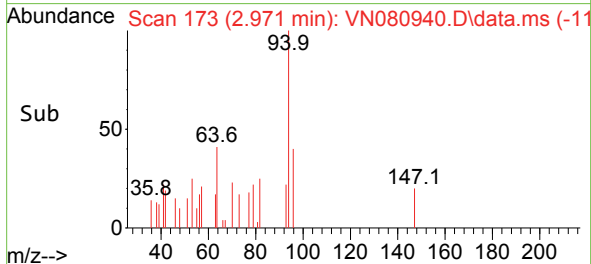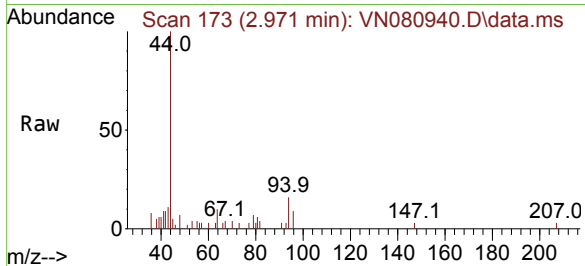

#6
Chloroethane
Concen: 0.325 ug/l
RT: 3.118 min Scan# 198
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 64 Resp: 881
Ion Ratio Lower Upper
64 100
66 0.0 26.4 39.6#




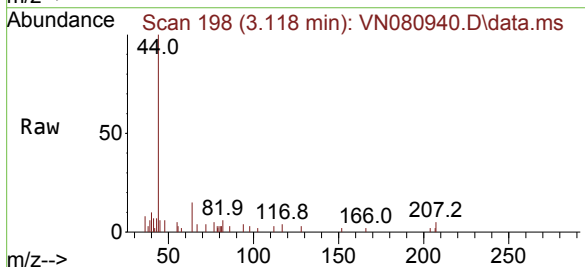




#11
Tert butyl alcohol
Concen: 0.998 ug/l
RT: 5.512 min Scan# 605
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 59 Resp: 450
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

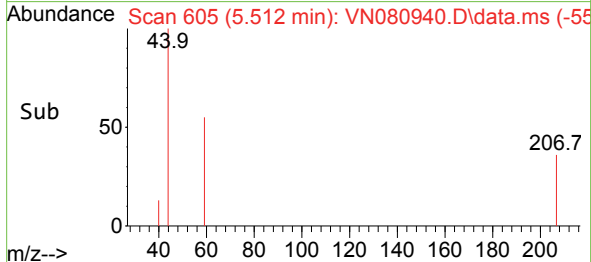

#13
Acrolein
Concen: 0.521 ug/l
RT: 4.177 min Scan# 378
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 56 Resp: 296
Ion Ratio Lower Upper
56 100
55 112.8 55.3 82.9#


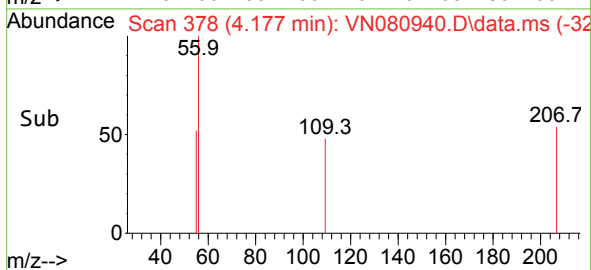

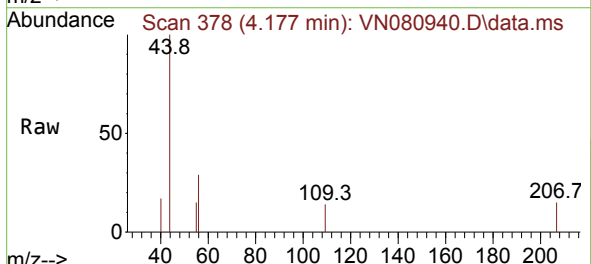




#16
Acetone
Concen: 40.727 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 43 Resp: 43853
Ion Ratio Lower Upper
43 100
58 33.9 24.8 37.2

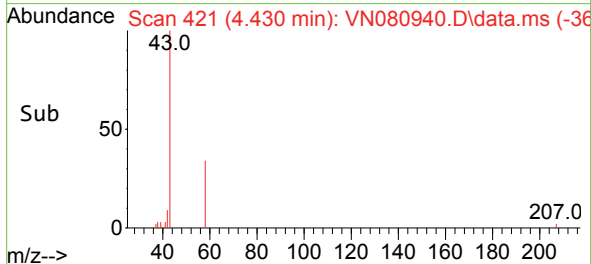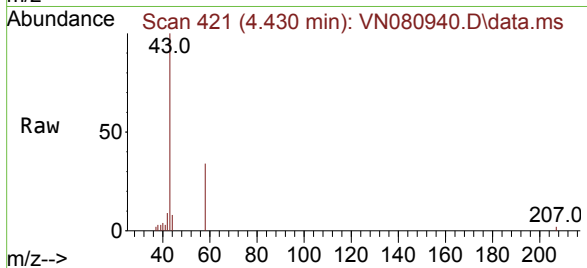

#18
Methyl Acetate
Concen: Below Cal
RT: 5.042 min Scan# 525
Delta R.T. 0.024 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 43 Resp: 5134
Ion Ratio Lower Upper
43 100
74 7.1 17.3 25.9#


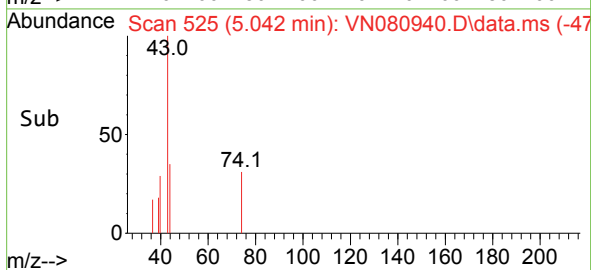

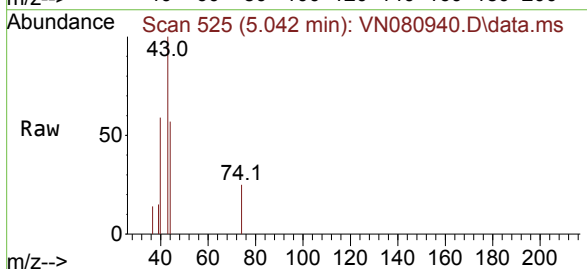




#20
Methylene Chloride
Concen: 2.584 ug/l
RT: 5.289 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion:	84	Resp:	8428
Ion	Ratio	Lower	Upper
84	100		
49	113.0	108.1	162.1
51	33.0	32.9	49.3
86	56.1	48.6	73.0

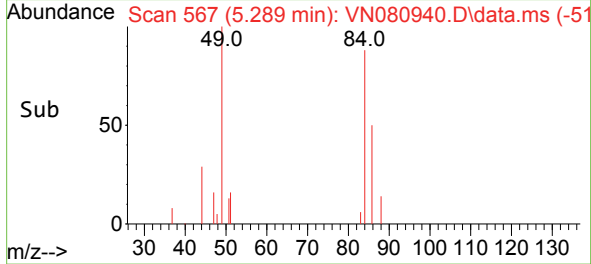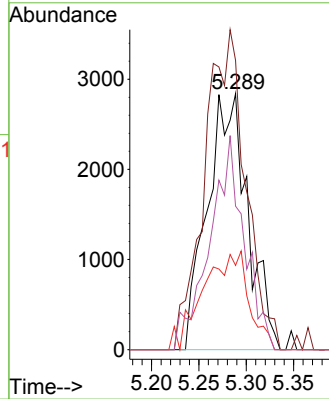

#25
2-Butanone
Concen: 3.600 ug/l
RT: 7.506 min Scan# 944
Delta R.T. 0.024 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion:	43	Resp:	6222
Ion	Ratio	Lower	Upper
43	100		
72	17.9	19.5	29.3#

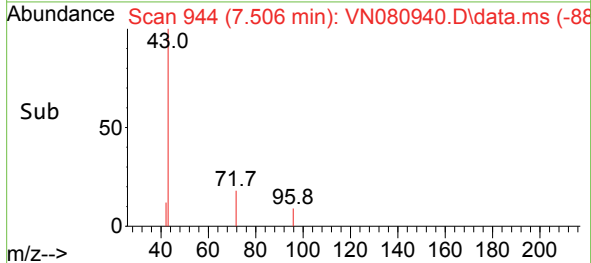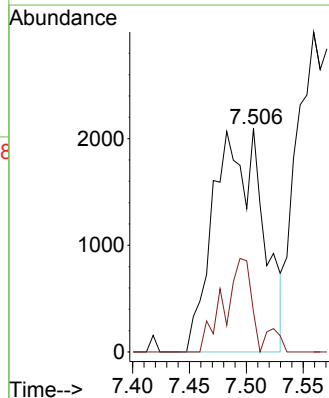



#29

Tetrahydrofuran

Concen: 0.498 ug/l

RT: 7.836 min Scan# 1000

Delta R.T. 0.000 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51





Instrument :

MSVOA_N

ClientSampleId :

PB158850ZHE#04

Tgt Ion:	42	Resp:	526
Ion	Ratio	Lower	Upper
42	100		
72	0.0	31.1	46.7#
71	0.0	28.3	42.5#



#31

Cyclohexane

Concen: 1.532 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.035 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51

Tgt Ion:	56	Resp:	6854
Ion	Ratio	Lower	Upper
56	100		
69	120.2	20.1	30.1#
84	168.5	56.9	85.3#

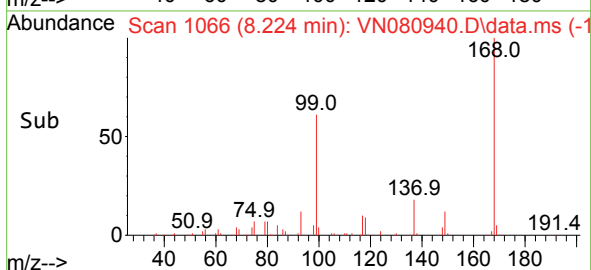



#33

1,2-Dichloroethane-d4

Concen: 58.639 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51

Instrument :

MSVOA_N

ClientSampleId :





PB158850ZHE#04

Tgt Ion: 65 Resp: 191914

Ion Ratio Lower Upper

65 100

67 51.0 0.0 102.4

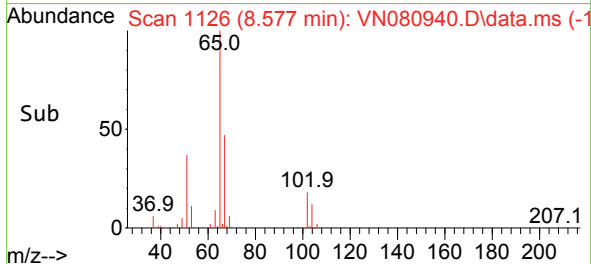

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.006 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51




Tgt Ion: 114 Resp: 563789


Ion Ratio Lower Upper

114 100

63 19.5 0.0 48.0

88 15.7 0.0 34.8









#35
Dibromofluoromethane
Concen: 58.442 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. 0.006 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion:113 Resp: 176804
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.4
192 15.9 12.5 18.7

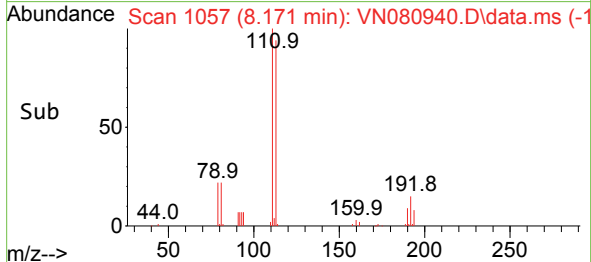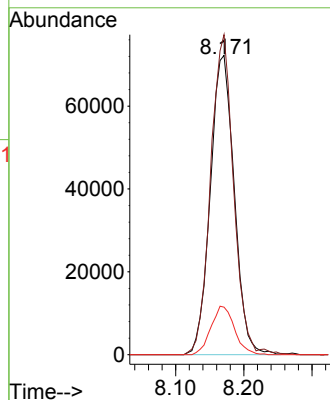

#36
1,1-Dichloropropene
Concen: 4.843 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.153 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 75 Resp: 21797
Ion Ratio Lower Upper
75 100
110 11.0 16.0 48.0#
77 0.0 25.8 38.6#


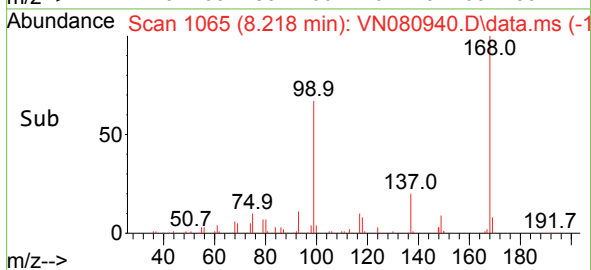
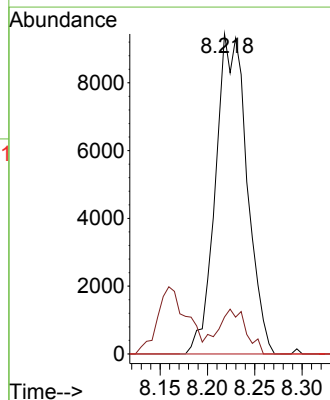
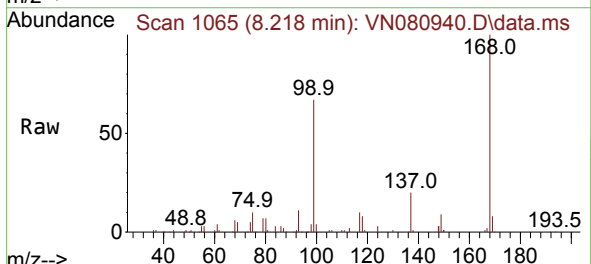




#37
Ethyl Acetate
Concen: 2.497 ug/l
RT: 7.559 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 43 Resp: 8504
Ion Ratio Lower Upper
43 100
61 17.7 10.6 15.8#
70 14.0 8.0 12.0#

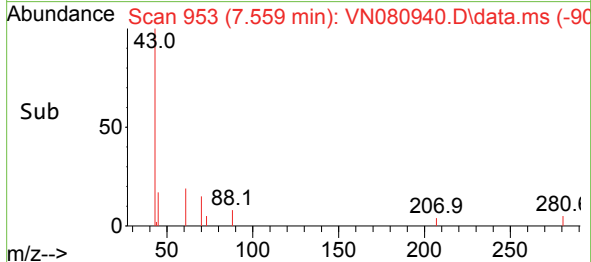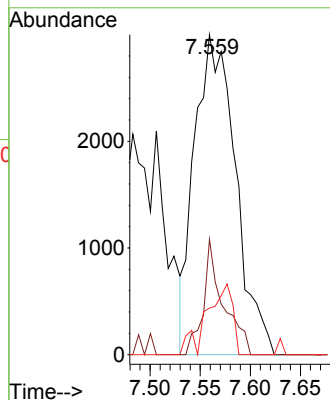

#38
Carbon Tetrachloride
Concen: 5.806 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.129 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 117 Resp: 26788
Ion Ratio Lower Upper
117 100
119 3.6 73.4 110.2#
121 0.0 24.4 36.6#

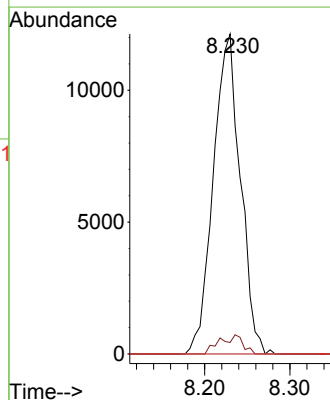



#42

1,2-Dichloroethane

Concen: 0.341 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.018 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51

Instrument :

MSVOA_N

ClientSampleId :





PB158850ZHE#04

Tgt Ion: 62 Resp: 1628

Ion Ratio Lower Upper

62 100

98 3.8 0.0 18.0

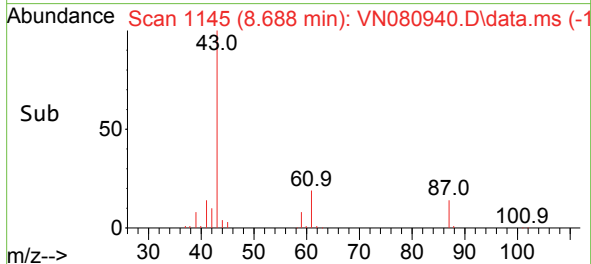

#43

Isopropyl Acetate

Concen: 46.379 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.000 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51




Tgt Ion: 43 Resp: 290435


Ion Ratio Lower Upper

43 100

61 18.9 19.9 29.9#

87 14.6 9.0 13.6#


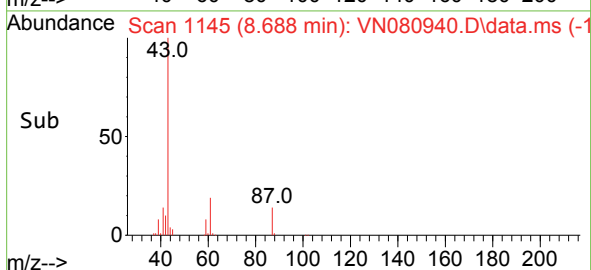






#48
Methyl methacrylate
Concen: 66.558 ug/l
RT: 9.741 min Scan# 1314
Delta R.T. 0.059 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 41 Resp: 234832
Ion Ratio Lower Upper
41 100
69 0.1 62.2 93.2#
39 57.3 47.6 71.4

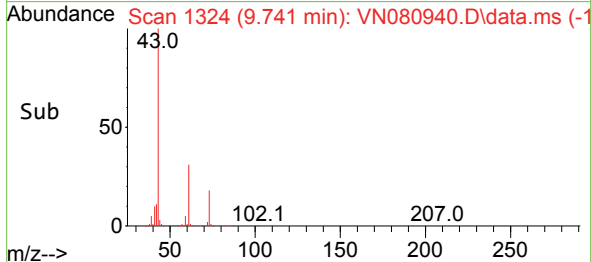

#49
1,4-Dioxane
Concen: 2.533 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.024 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 88 Resp: 165
Ion Ratio Lower Upper
88 100
43 0.0 30.1 45.1#
58 3338.2 63.9 95.9#




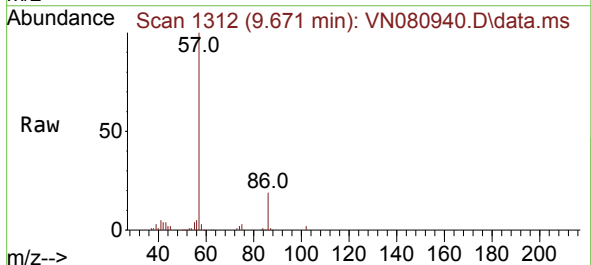


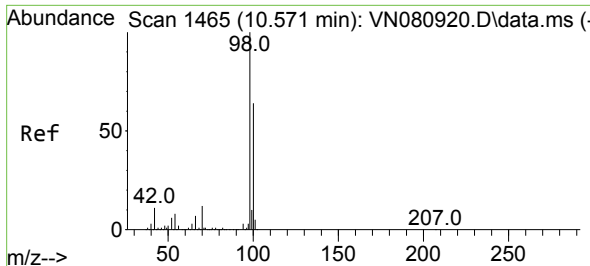

#50
Toluene-d8
Concen: 64.467 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 98 Resp: 705445
Ion Ratio Lower Upper
98 100
100 64.9 51.4 77.0

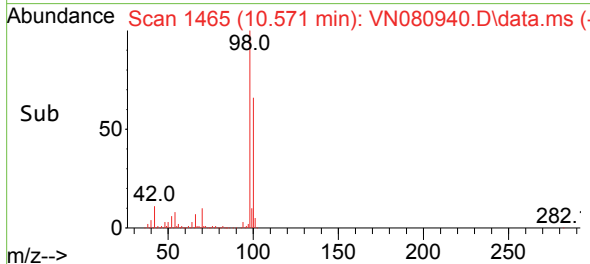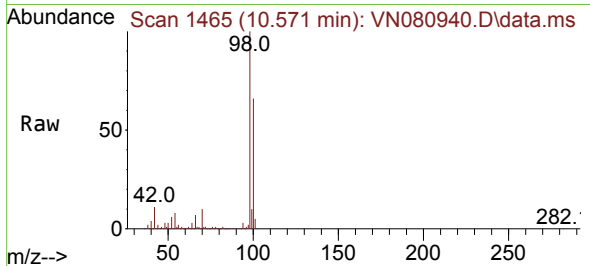

#51
4-Methyl-2-Pentanone
Concen: 2.966 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 43 Resp: 11195
Ion Ratio Lower Upper
43 100
58 44.1 29.4 44.0#


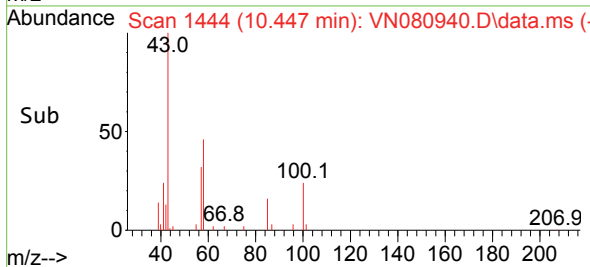

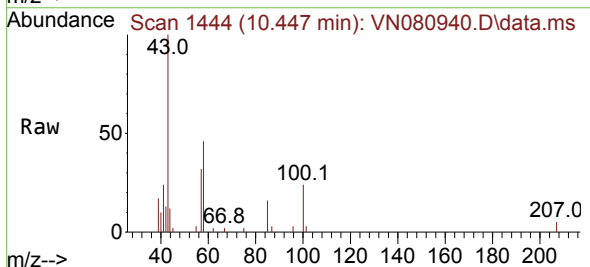


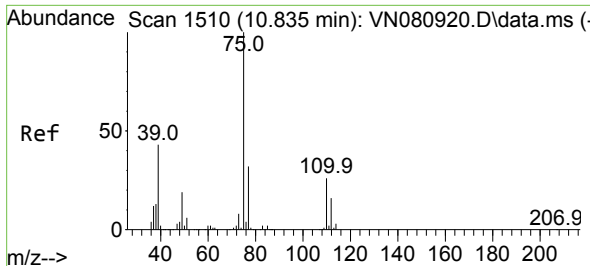

#53
 t-1,3-Dichloropropene
 Concen: 0.489 ug/l
 RT: 10.735 min Scan# 1493
 Delta R.T. -0.100 min
 Lab File: VN080940.D
 Acq: 07 Feb 2024 16:51




Instrument :
 MSVOA_N
 ClientSampleId :
 PB158850ZHE#04


Tgt Ion: 75 Resp: 2531
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.5 38.3#

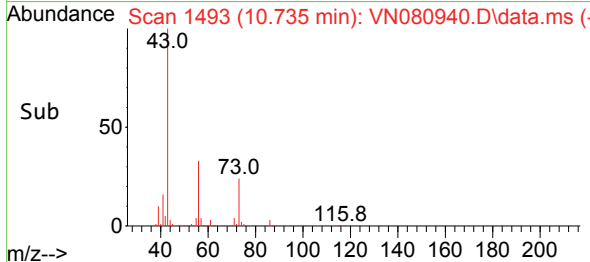

#54
 cis-1,3-Dichloropropene
 Concen: 19.333 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.047 min
 Lab File: VN080940.D
 Acq: 07 Feb 2024 16:51

Tgt Ion: 75 Resp: 112266
 Ion Ratio Lower Upper
 75 100
 77 0.5 23.3 34.9#
 39 29.6 44.6 66.8#


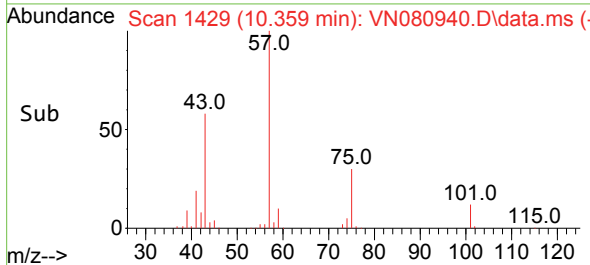

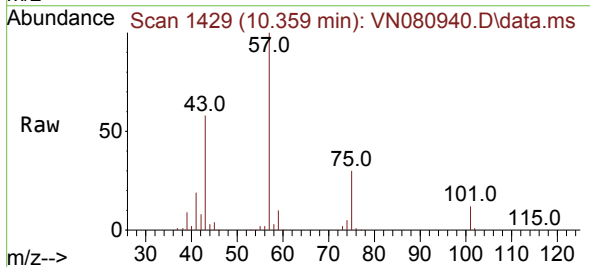


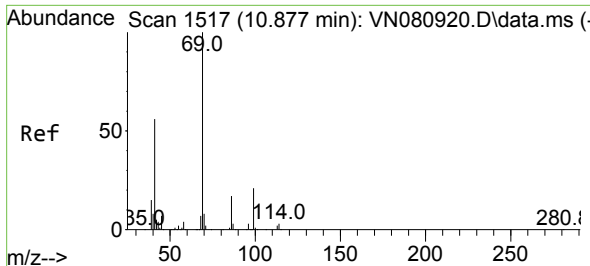

#56
Ethyl methacrylate
Concen: 0.644 ug/l
RT: 10.982 min Scan# 1535
Delta R.T. 0.105 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 69 Resp: 2732
Ion Ratio Lower Upper
69 100
41 5989.1 61.0 91.6#
39 2763.4 31.8 47.6#

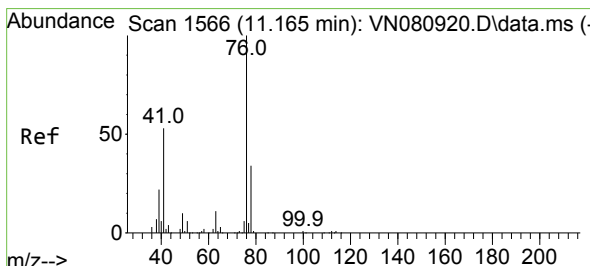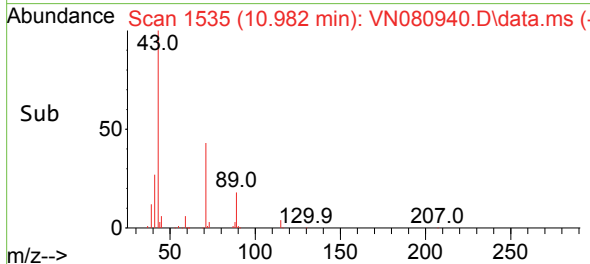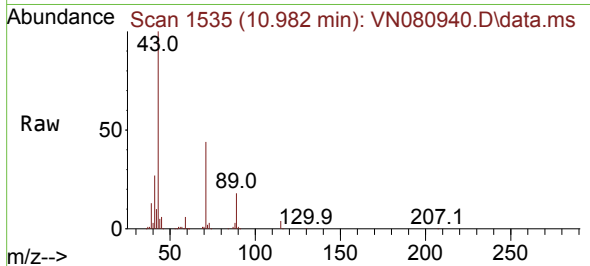

#57
1,3-Dichloropropane
Concen: 2.638 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.041 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 76 Resp: 15177
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#


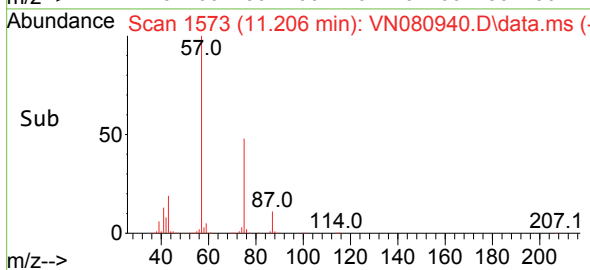

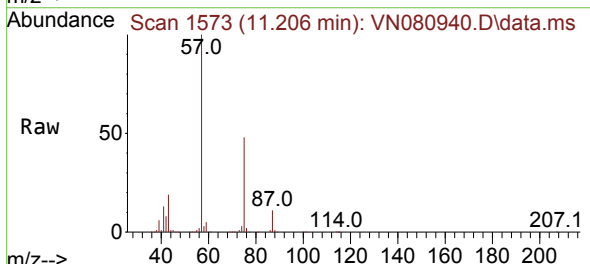


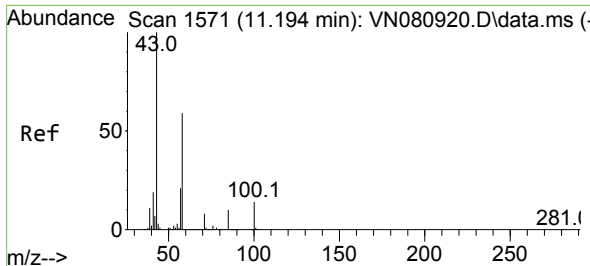

#59
2-Hexanone
Concen: 77.466 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.024 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 43 Resp: 221577
Ion Ratio Lower Upper
43 100
58 0.0 25.9 77.8#

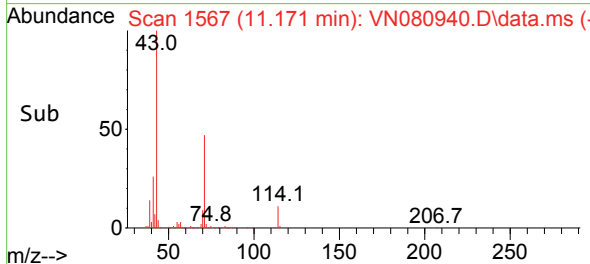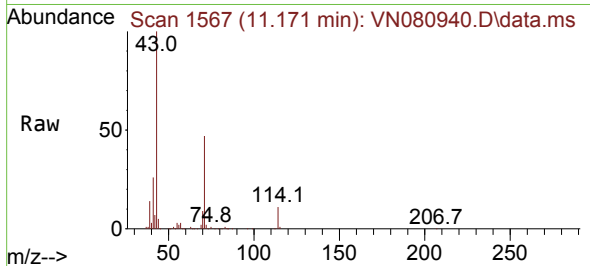

#62
4-Bromofluorobenzene
Concen: 73.862 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 95 Resp: 293620
Ion Ratio Lower Upper
95 100
174 73.8 0.0 120.4
176 71.7 0.0 121.0


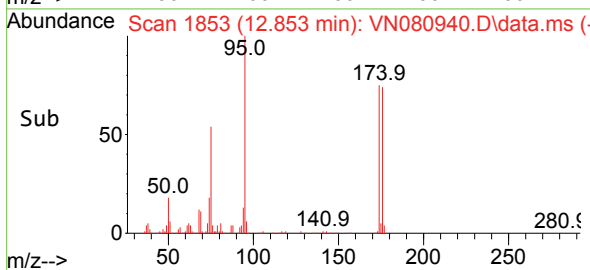

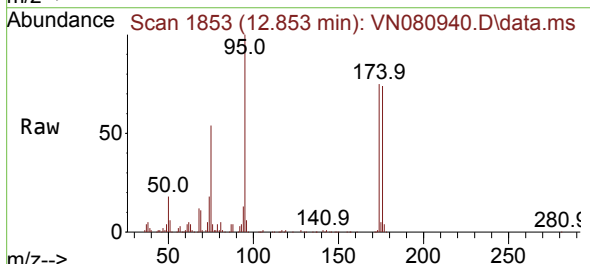


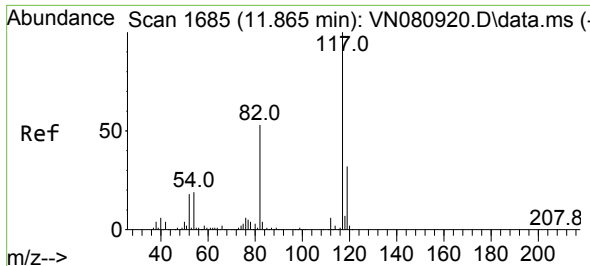

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion:117 Resp: 712562
Ion Ratio Lower Upper
117 100
82 56.6 52.7 79.1
119 33.3 25.3 37.9

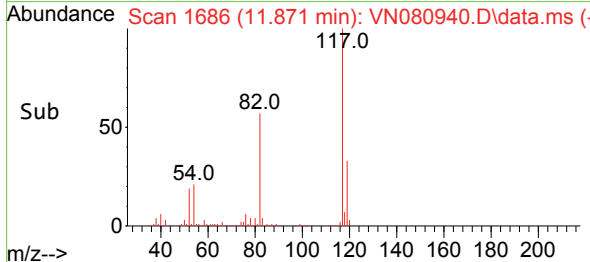

#65
Chlorobenzene
Concen: 0.227 ug/l
RT: 11.894 min Scan# 1690
Delta R.T. 0.000 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion:112 Resp: 3397
Ion Ratio Lower Upper
112 100
114 60.0 23.7 35.5#

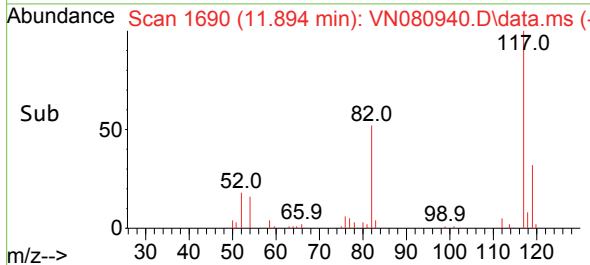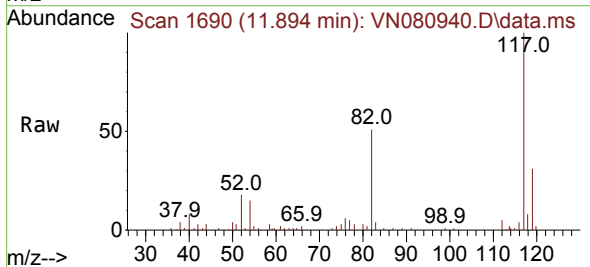



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51

Instrument :

MSVOA_N

ClientSampleId :

PB158850ZHE#04





Tgt Ion:152 Resp: 304100

Ion Ratio Lower Upper

152 100

115 61.8 32.3 96.8

150 156.1 0.0 339.8

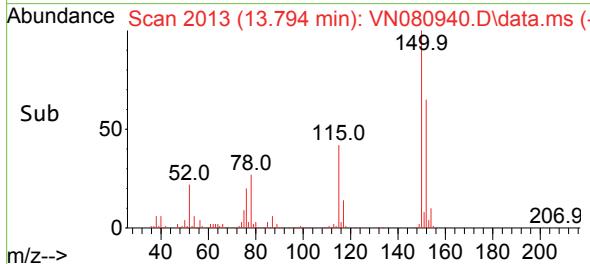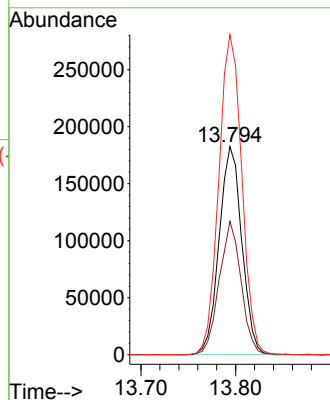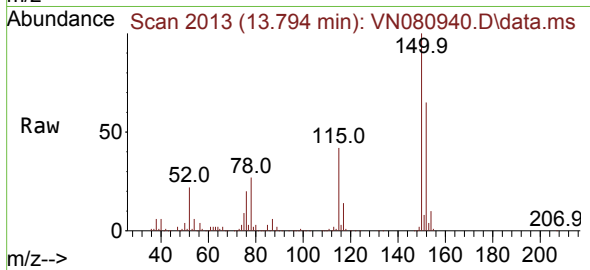

#74

N-ethyl acetate

Concen: 0.370 ug/l

RT: 12.488 min Scan# 1791

Delta R.T. -0.006 min

Lab File: VN080940.D

Acq: 07 Feb 2024 16:51

Tgt Ion: 43 Resp: 3157




Ion Ratio Lower Upper


43 100

70 0.0 30.1 45.1#

55 0.0 17.0 25.4#

61 0.0 17.5 26.3#



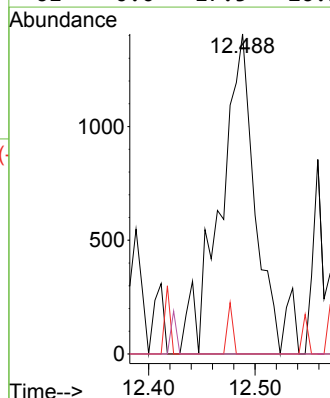
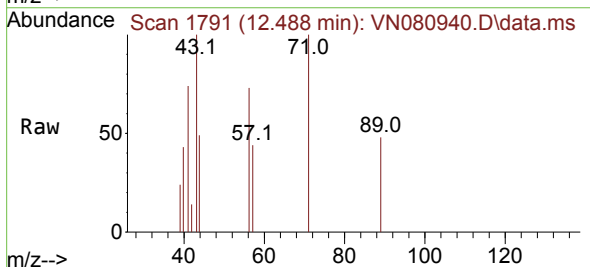




#76
1,2,3-Trichloropropane
Concen: 25.926 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51




Instrument :
MSVOA_N
ClientSampleId :
PB158850ZHE#04


Tgt Ion: 75 Resp: 160753
Ion Ratio Lower Upper
75 100
77 1.5 91.0 272.8#

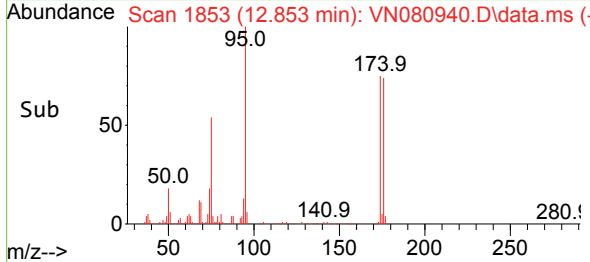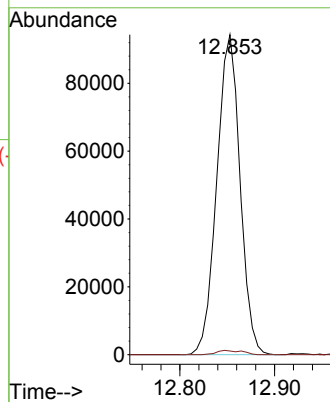

#81
trans-1,4-Dichloro-2-butene
Concen: 70.438 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN080940.D
Acq: 07 Feb 2024 16:51

Tgt Ion: 75 Resp: 160753
Ion Ratio Lower Upper
75 100
53 0.0 71.4 107.2#
89 0.0 33.4 50.0#

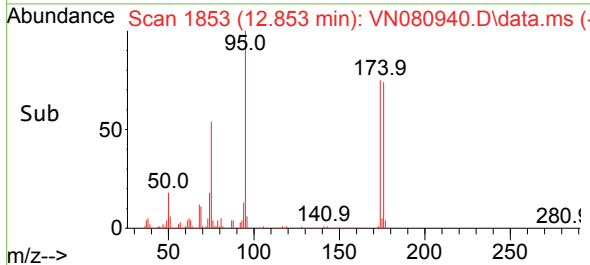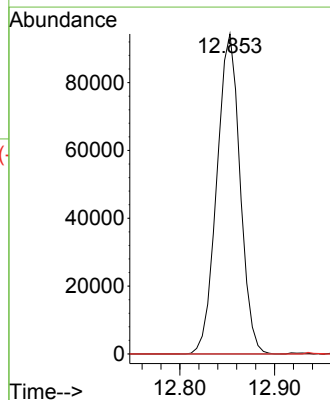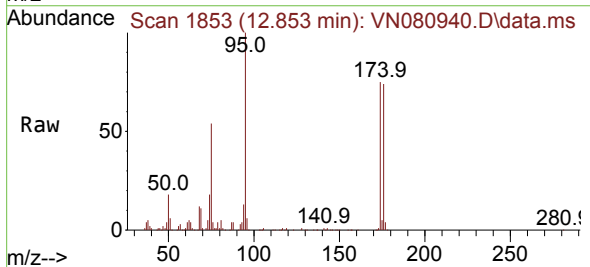

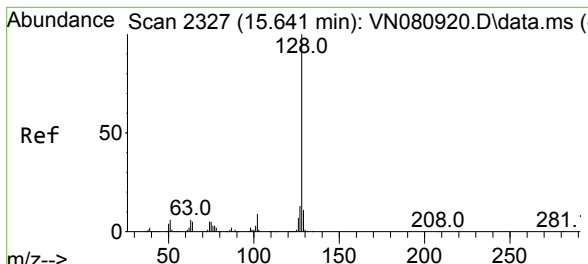

#95
 Naphthalene
 Concen: 0.214 ug/l
 RT: 15.647 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN080940.D
 Acq: 07 Feb 2024 16:51

Instrument :
 MSVOA_N
 ClientSampleId :
 PB158850ZHE#04

Tgt Ion:	128	Resp:	3559
Ion	Ratio	Lower	Upper
128	100		
127	10.3	10.0	15.0
129	2.4	8.7	13.1#

