
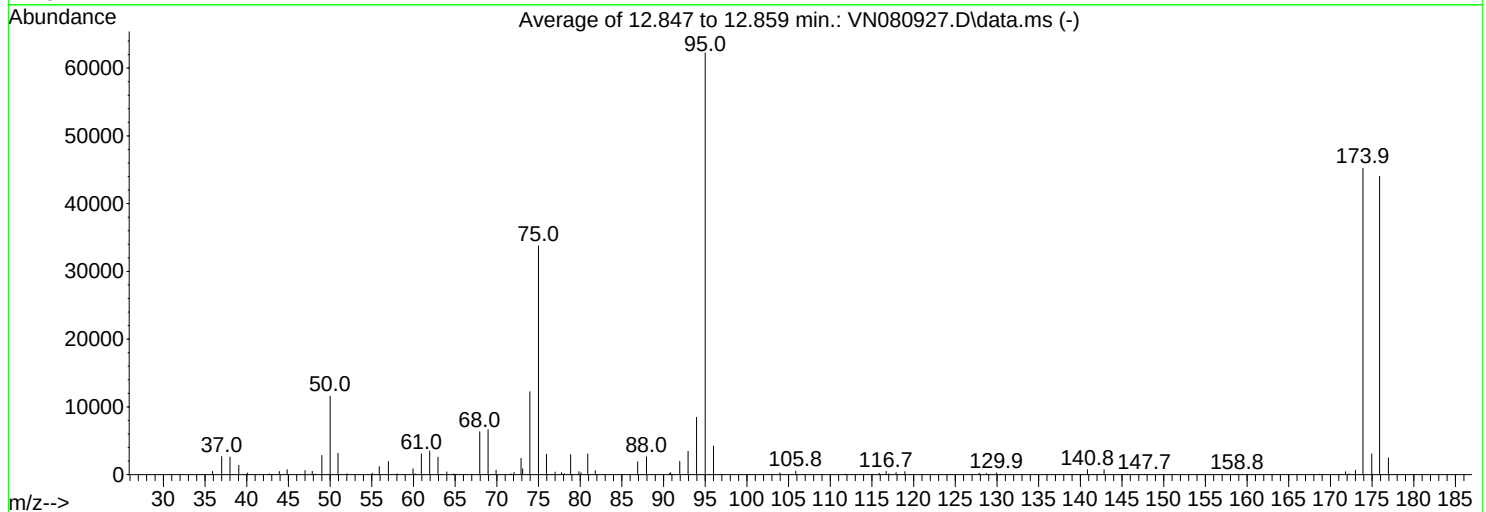


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN020724\  
Data File : VN080927.D  
Acq On : 07 Feb 2024 08:50  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N020624W.M  
Title : SW846 8260  
Last Update : Wed Feb 07 06:22:23 2024

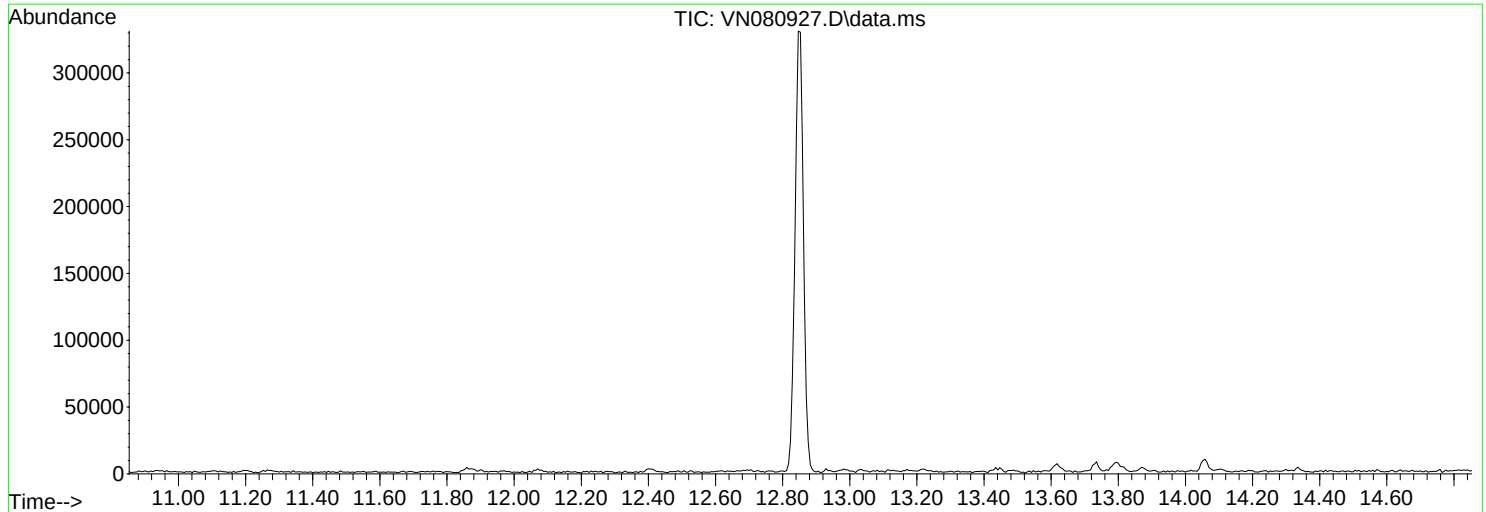

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1842

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.6  | 11607 | PASS      |
| 75     | 95      | 30     | 60     | 54.3  | 33779 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 62253 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 4214  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.4   | 630   | PASS      |
| 174    | 95      | 50     | 100    | 72.7  | 45227 | PASS      |
| 175    | 174     | 5      | 9      | 6.8   | 3072  | PASS      |
| 176    | 174     | 95     | 101    | 97.4  | 44035 | PASS      |
| 177    | 176     | 5      | 9      | 5.6   | 2481  | PASS      |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.90 | 480    | 48.20 | 86     | 60.95 | 3099   | 72.05 | 361    |
| 37.00 | 2672   | 49.00 | 2828   | 61.95 | 3483   | 72.90 | 241    |
| 38.00 | 2594   | 50.00 | 11607  | 62.95 | 2574   | 73.10 | 86     |
| 39.05 | 1373   | 50.95 | 3152   | 64.00 | 404    | 73.95 | 1223   |
| 39.85 | 13     | 52.05 | 152    | 64.80 | 128    | 75.00 | 33779  |
| 40.10 | 227    | 55.05 | 184    | 65.10 | 79     | 75.95 | 2997   |
| 42.70 | 121    | 55.90 | 1171   | 67.00 | 63     | 77.00 | 371    |
| 43.90 | 462    | 57.00 | 1932   | 67.95 | 6331   | 77.75 | 290    |
| 44.85 | 735    | 58.05 | 137    | 68.95 | 6634   | 78.10 | 134    |
| 47.00 | 624    | 59.95 | 886    | 69.90 | 655    | 78.85 | 2947   |
| 47.85 | 491    | 60.20 | 124    | 71.70 | 122    | 79.85 | 459    |

Average of 12.847 to 12.859 min.: VN080927.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|-------|--------|--------|--------|--------|--------|--------|--------|
| 80.10 | 281    | 96.00  | 4214   | 128.75 | 188    | 157.00 | 56     |
| 80.90 | 3057   | 96.90  | 63     | 129.95 | 258    | 158.80 | 81     |
| 81.80 | 580    | 103.95 | 254    | 130.40 | 61     | 168.70 | 64     |
| 86.90 | 1893   | 105.85 | 519    | 134.60 | 58     | 171.80 | 427    |
| 87.95 | 2619   | 111.80 | 75     | 140.85 | 741    | 172.20 | 113    |
| 90.70 | 172    | 115.85 | 215    | 141.60 | 52     | 173.00 | 630    |
| 90.85 | 289    | 116.70 | 466    | 142.85 | 737    | 173.90 | 45227  |
| 91.95 | 1964   | 117.00 | 130    | 145.60 | 62     | 174.95 | 3072   |
| 92.95 | 3459   | 117.90 | 305    | 147.70 | 77     | 175.90 | 44035  |
| 93.95 | 8459   | 118.95 | 455    | 154.50 | 58     | 176.95 | 2481   |
| 95.00 | 62253  | 127.85 | 205    | 155.00 | 55     |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB