
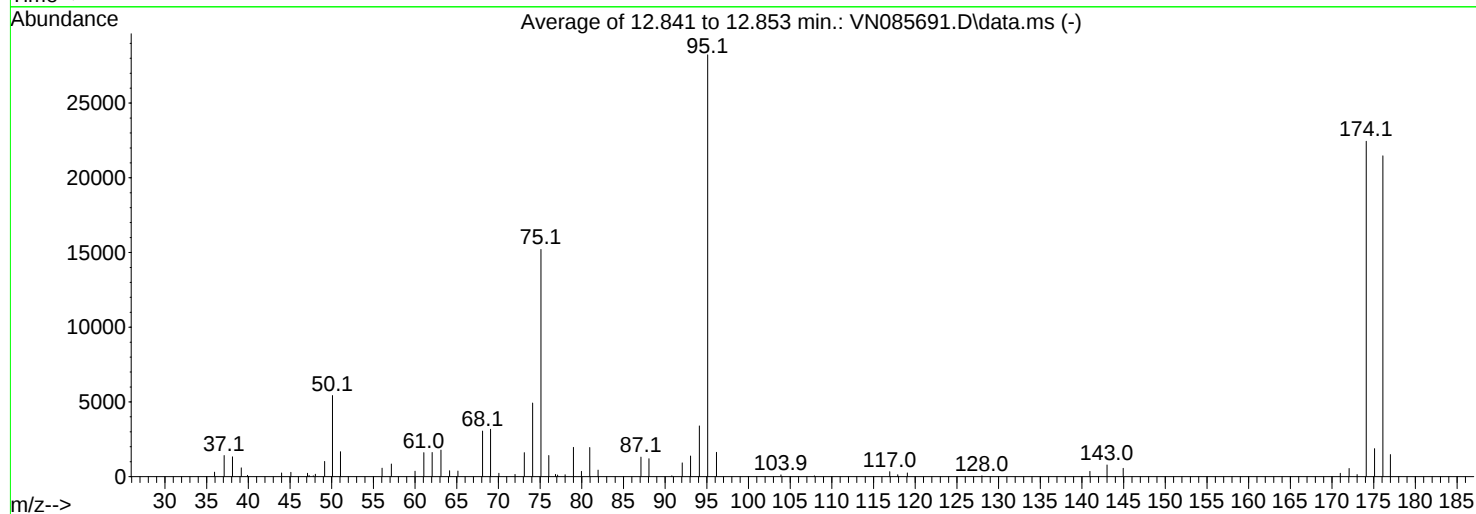


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020725\
Data File : VN085691.D
Acq On : 07 Feb 2025 11:54
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

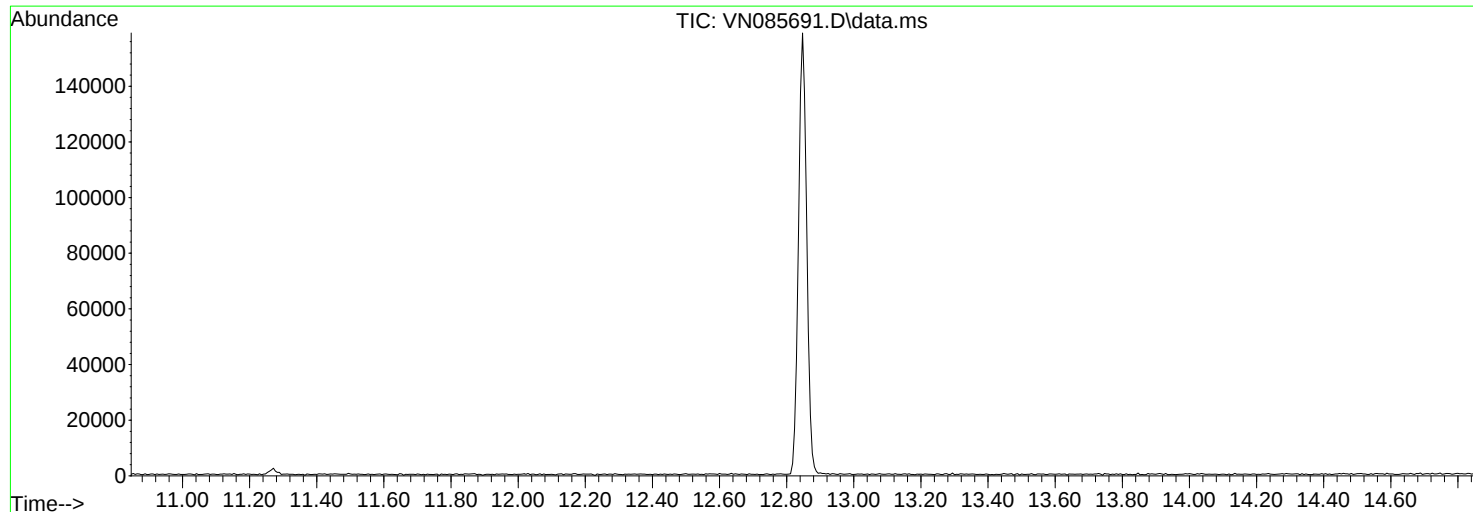

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	5426	PASS
75	95	30	60	53.9	15209	PASS
95	95	100	100	100.0	28229	PASS
96	95	5	9	5.8	1627	PASS
173	174	0.00	2	0.6	140	PASS
174	95	50	100	79.5	22443	PASS
175	174	5	9	8.3	1872	PASS
176	174	95	101	95.7	21475	PASS
177	176	5	9	6.9	1477	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	304	49.15	1016	68.10	3056	79.00	1961
37.10	1415	50.10	5426	69.05	3169	79.95	35
38.10	1326	51.05	1666	70.05	229	80.95	194
39.15	592	56.05	567	72.00	148	81.95	43
39.90	87	57.15	847	73.10	1611	87.10	1310
44.00	246	60.00	363	74.10	4921	88.05	1199
45.10	288	61.05	1610	75.10	15209	90.80	50
47.10	226	62.05	1612	76.05	1414	92.05	919
47.30	71	63.10	1777	76.85	147	93.05	1383
47.80	59	64.15	399	77.10	104	94.10	3396
48.05	157	65.15	378	78.00	134	95.10	28229

Average of 12.841 to 12.853 min.: VN085691.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.15	1627	172.05	544				
103.90	113	173.00	140				
107.90	52	174.10	22443				
116.95	332	175.10	1872				
117.90	127	176.10	21475				
119.05	251	177.00	1477				
128.00	57						
140.95	354						
143.00	785						
144.95	555						
171.00	227						

Instrument :

MSVOA_N

ClientSampleId :

BFB