
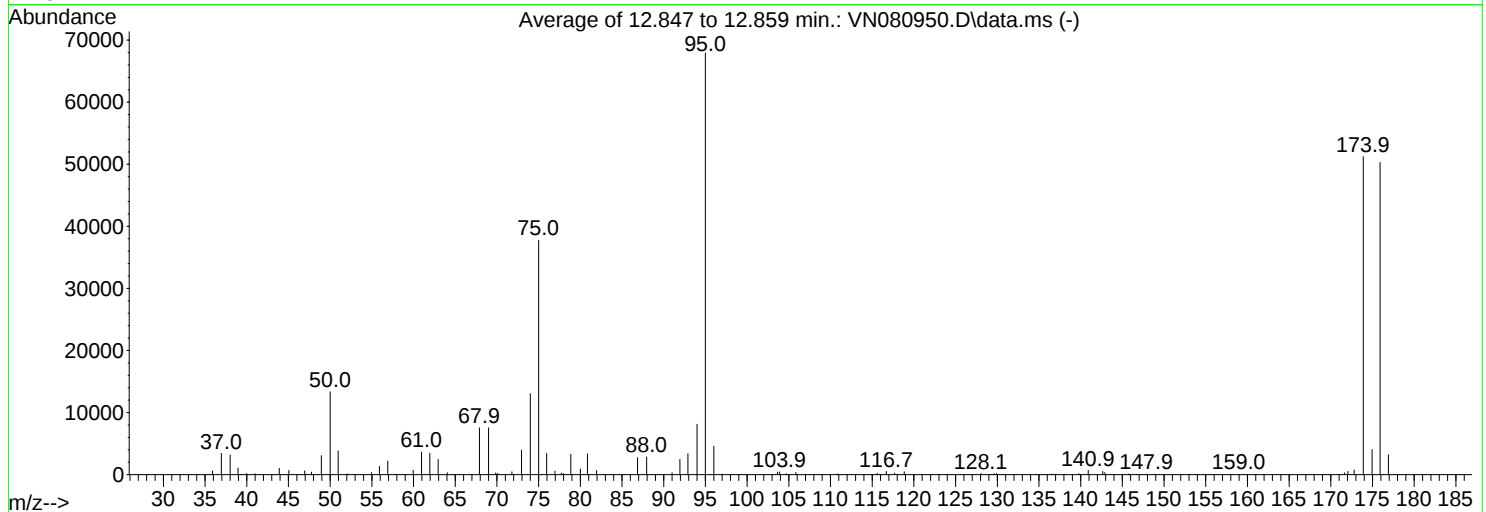


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020824\
Data File : VN080950.D
Acq On : 08 Feb 2024 09:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
Title : SW846 8260
Last Update : Wed Feb 07 06:22:23 2024

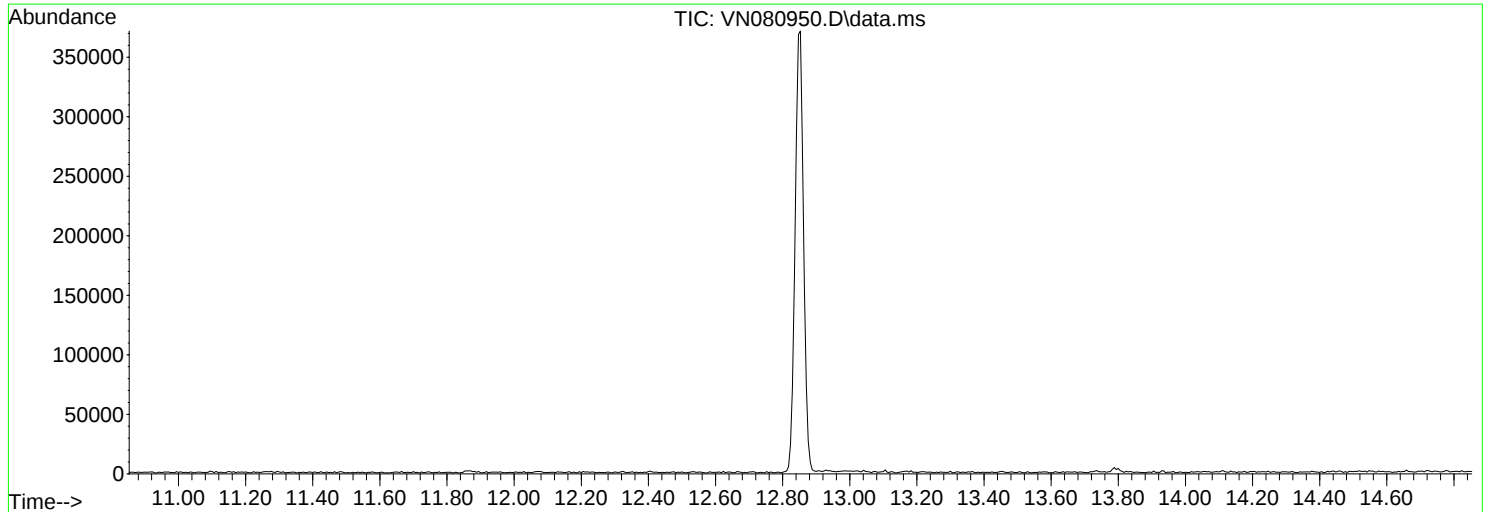

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	13356	PASS
75	95	30	60	55.6	37752	PASS
95	95	100	100	100.0	67949	PASS
96	95	5	9	6.8	4589	PASS
173	174	0.00	2	1.5	749	PASS
174	95	50	100	75.4	51251	PASS
175	174	5	9	7.9	4043	PASS
176	174	95	101	98.2	50315	PASS
177	176	5	9	6.3	3195	PASS

Average of 12.847 to 12.859 min.: VN080950.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	608	48.95	3080	62.95	2444	74.00	1307
36.95	3424	50.00	13356	64.05	302	75.00	3775
38.00	3166	50.95	3841	64.90	65	75.95	342
38.95	1051	52.10	123	66.70	62	76.95	56
39.95	182	54.95	324	67.00	65	77.75	230
41.00	148	55.90	1337	67.90	7527	78.00	183
43.90	1011	56.90	2189	69.00	7537	78.85	3286
45.05	704	57.80	59	69.85	283	80.00	913
46.95	622	59.95	705	70.10	206	80.85	3352
47.20	85	60.95	3636	71.80	458	81.95	668
47.75	417	61.95	3450	72.95	3932	86.85	2747

Average of 12.847 to 12.859 min.: VN080950.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	2843	105.85	359	129.60	154	145.90	79
91.00	308	107.00	84	129.90	193	146.70	52
91.95	2457	109.90	58	134.70	91	147.20	64
92.90	3383	110.85	142	136.50	81	147.90	76
94.00	8125	114.80	63	136.80	69	148.90	61
95.00	67949	115.60	246	139.80	129	159.00	58
96.00	4589	115.90	63	140.90	667	160.80	54
97.00	113	116.70	511	142.65	524	171.65	276
103.65	413	117.70	258	142.90	345	172.05	525
103.90	431	118.85	454	143.60	65	172.80	749
104.70	155	128.05	202	145.70	97	173.90	51251

Average of 12.847 to 12.859 min.: VN080950.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.95	4043						
175.90	50315						
176.90	3195						

Instrument :
MSVOA_N
ClientSampleId :
BFB