


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020921\
Data File : VN065770.D
Acq On : 9 Feb 2021 8:59
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Title : SW846 8260
Last Update : Mon Jan 25 13:47:28 2021

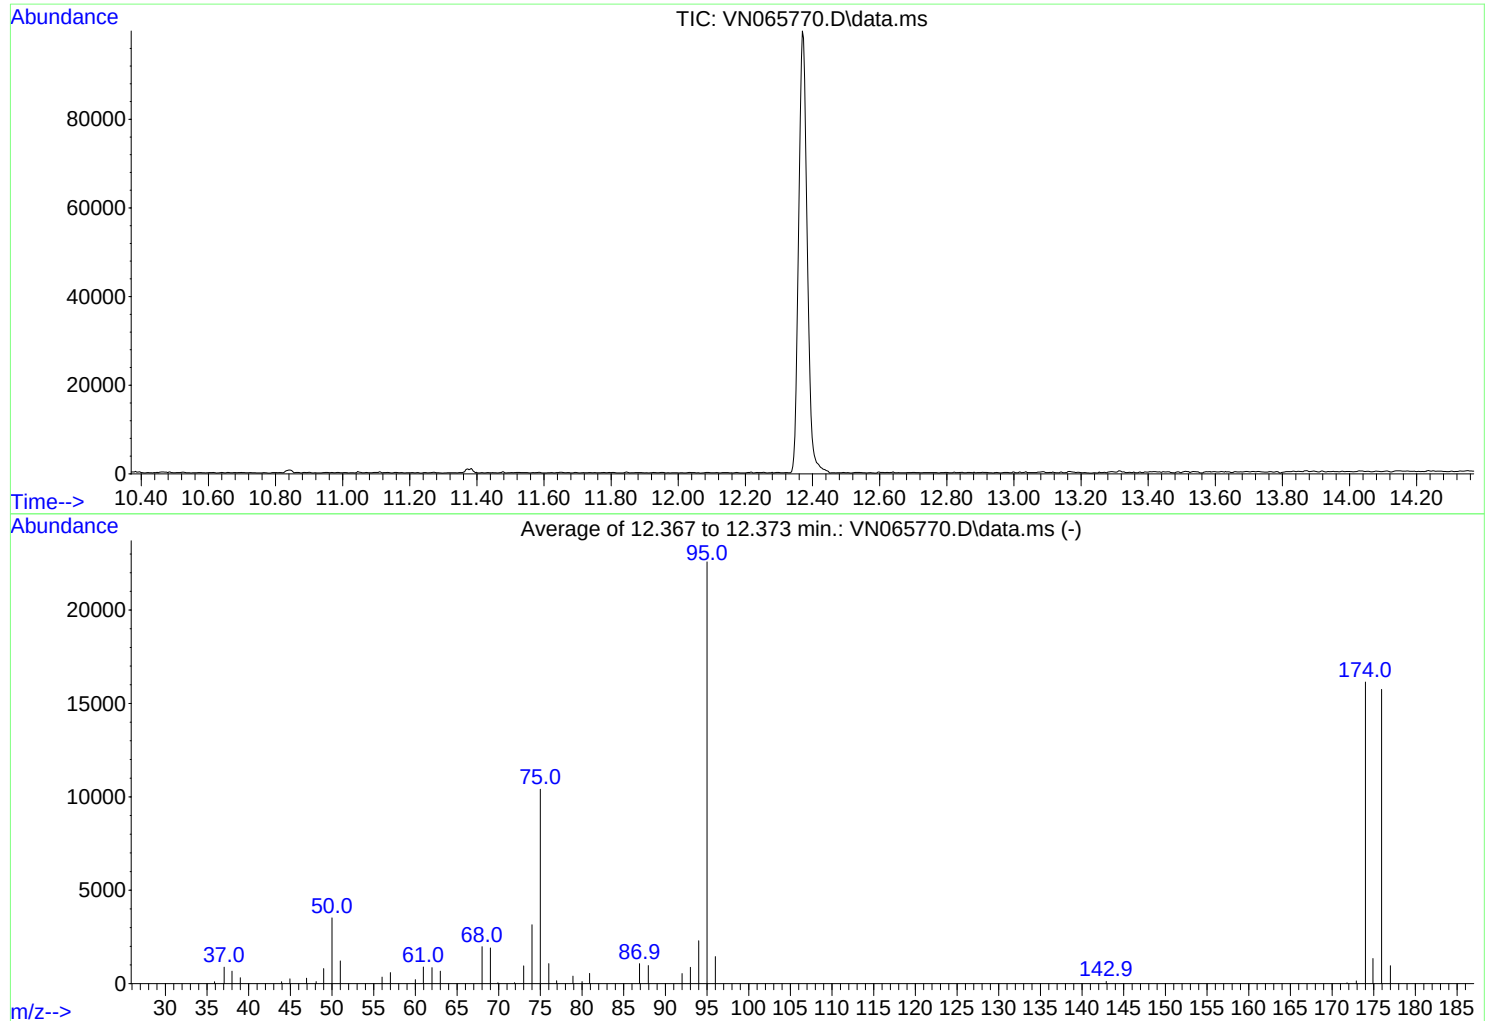

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	3521	PASS
75	95	30	60	46.1	10407	PASS
95	95	100	100	100.0	22581	PASS
96	95	5	9	6.4	1451	PASS
173	174	0.00	2	0.9	150	PASS
174	95	50	100	71.5	16147	PASS
175	174	5	9	8.3	1343	PASS
176	174	95	101	97.6	15755	PASS
177	176	5	9	6.1	958	PASS