


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020923\
Data File : VN076591.D
Acq On : 09 Feb 2023 15:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020923W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Feb 10 05:40:47 2023

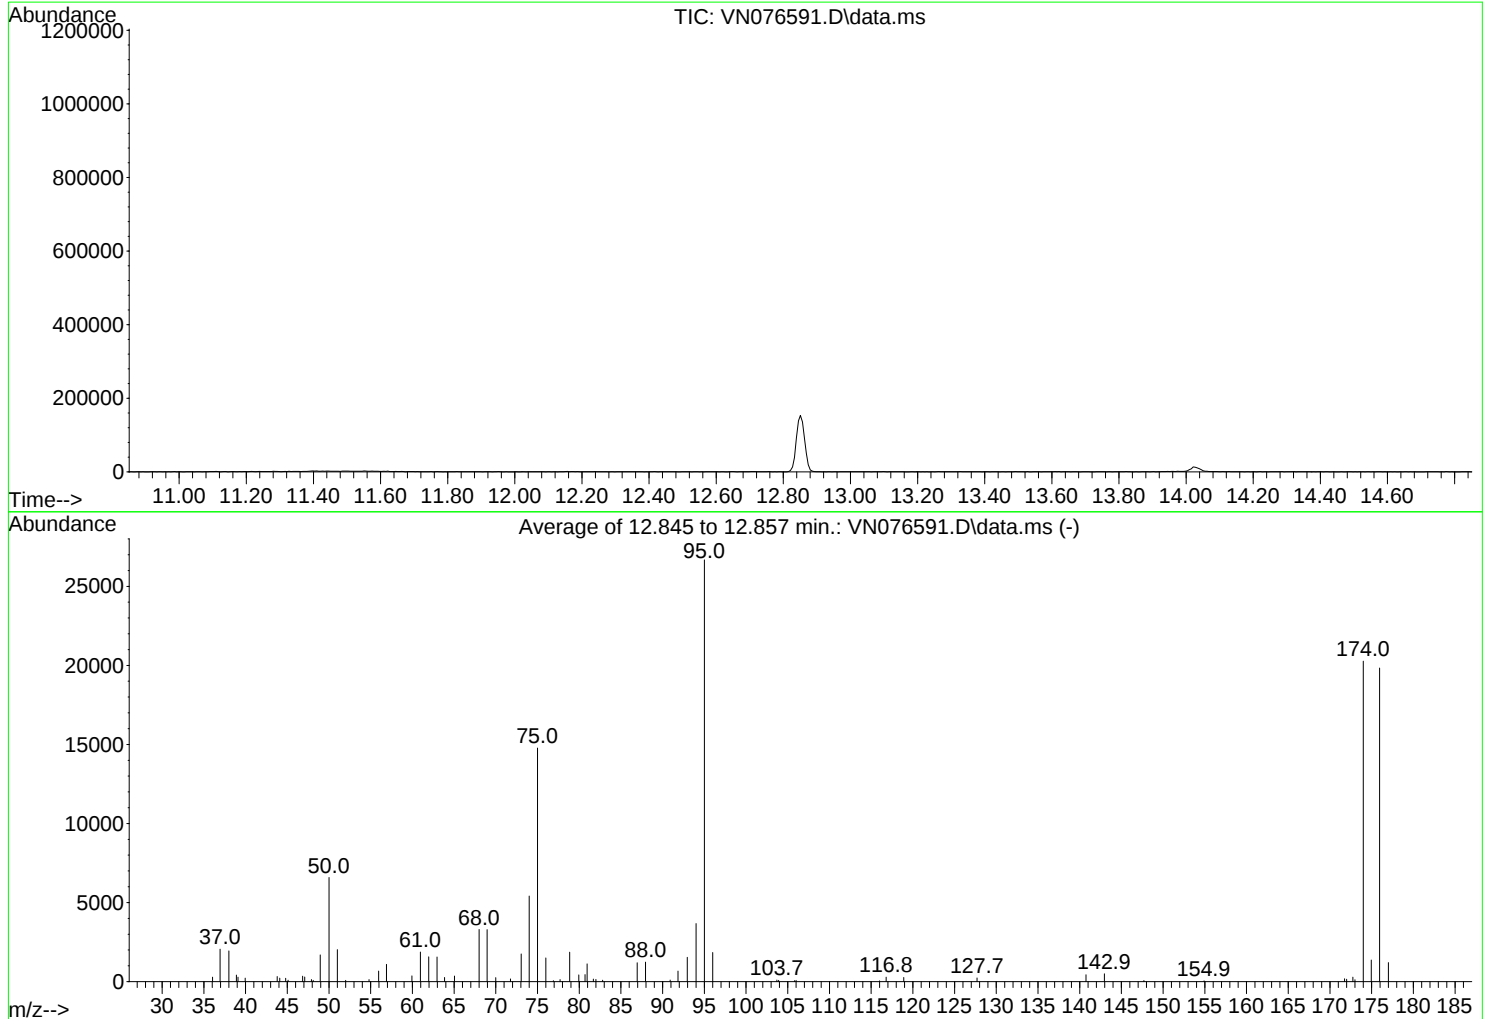

AutoFind: Scans 1863, 1864, 1865; Background Corrected with Scan 1856

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.7	6587	PASS
75	95	30	60	55.4	14771	PASS
95	95	100	100	100.0	26677	PASS
96	95	5	9	6.9	1846	PASS
173	174	0.00	2	1.4	280	PASS
174	95	50	100	76.0	20272	PASS
175	174	5	9	6.7	1364	PASS
176	174	95	101	97.9	19837	PASS
177	176	5	9	6.1	1209	PASS