


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020924\
Data File : VN080977.D
Acq On : 09 Feb 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020924W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Feb 10 01:55:02 2024

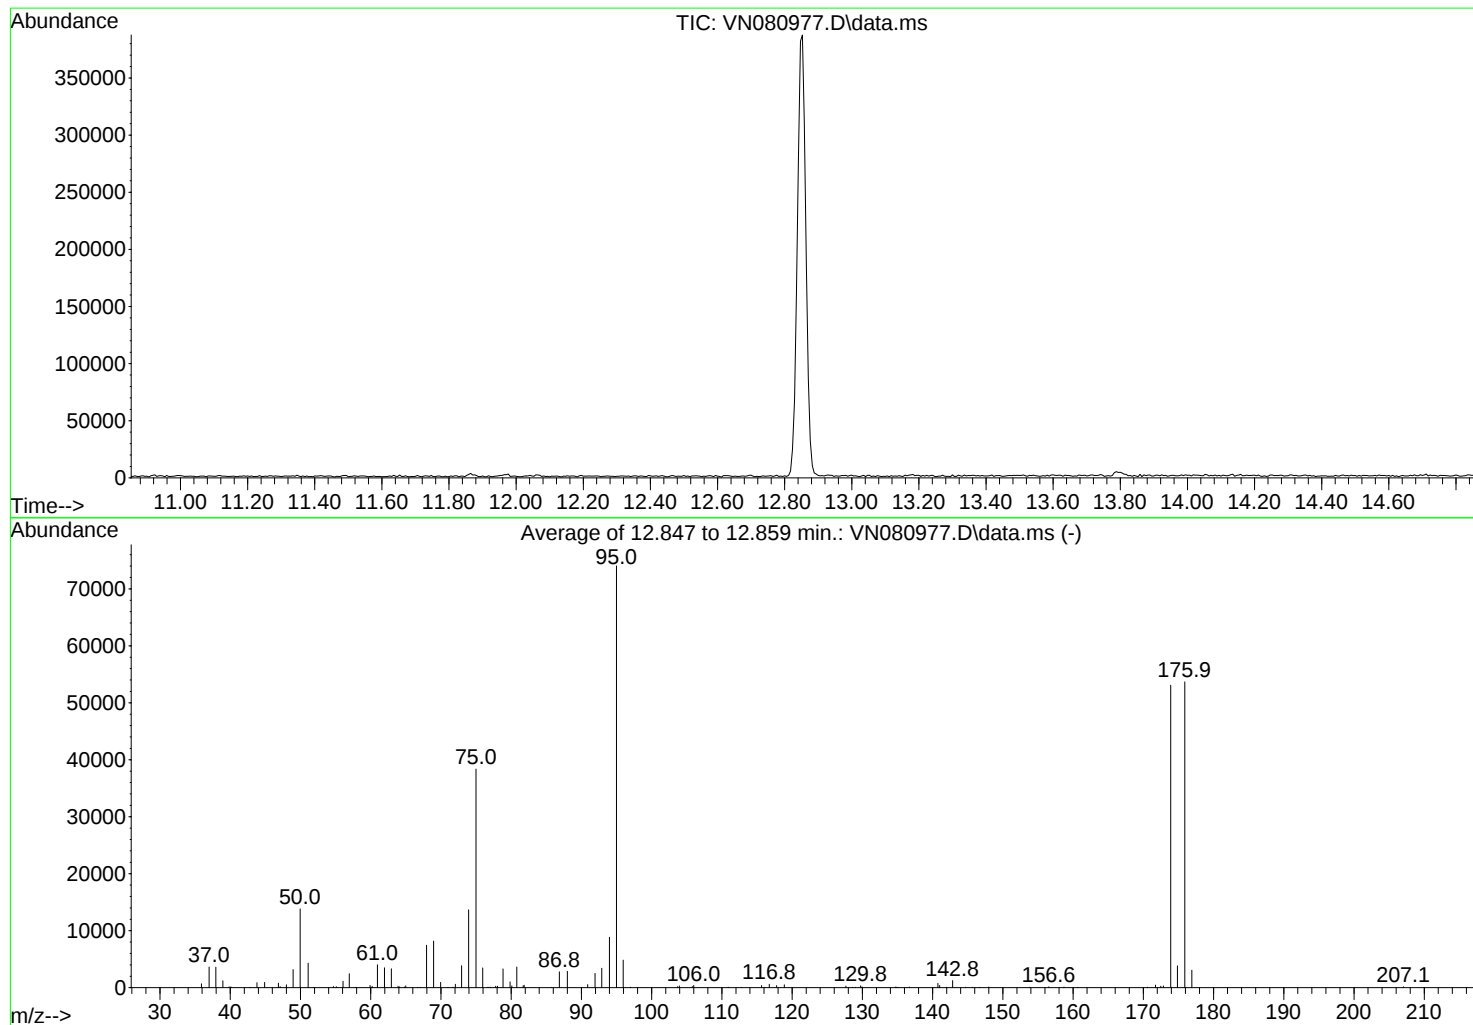

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	13833	PASS
75	95	30	60	51.8	38368	PASS
95	95	100	100	100.0	74040	PASS
96	95	5	9	6.5	4840	PASS
173	174	0.00	2	0.6	305	PASS
174	95	50	100	71.7	53093	PASS
175	174	5	9	7.2	3832	PASS
176	174	95	101	101.1	53675	FAIL*
177	176	5	9	5.7	3055	PASS