

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021020\
 Data File : VN060044.D
 Acq On : 10 Feb 2020 14:25
 Operator : JC/MD
 Sample : L1471-05
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Feb 11 07:08:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 18 03:09:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	199197	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	310902	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	294596	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	140001	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	115835	52.36	ug/l	0.00
Spiked Amount			Recovery	=	104.72%	
35) Dibromofluoromethane	7.57	113	94855	51.16	ug/l	0.00
Spiked Amount			Recovery	=	102.32%	
50) Toluene-d8	10.08	98	376532	52.42	ug/l	0.00
Spiked Amount			Recovery	=	104.84%	
62) 4-Bromofluorobenzene	12.40	95	138085	53.32	ug/l	0.00
Spiked Amount			Recovery	=	106.64%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.77	59	167	0.448	ug/l #	72
16) Acetone	3.81	43	64791	79.027	ug/l	98
18) Methyl Acetate	4.31	43	1321	0.511	ug/l #	54
20) Methylene Chloride	4.52	84	5595	1.541	ug/l	87
25) 2-Butanone	6.81	43	60469	48.270	ug/l	96
29) Tetrahydrofuran	6.91	42	2970	3.832	ug/l #	35
31) Cyclohexane	7.64	56	4205	1.285	ug/l #	19
36) 1,1-Dichloropropene	7.64	75	14225	5.254	ug/l #	50
37) Ethyl Acetate	6.90	43	45612	17.962	ug/l	98
38) Carbon Tetrachloride	7.64	117	18594	6.313	ug/l #	16
43) Isopropyl Acetate	8.14	43	50512	11.565	ug/l #	90
45) 1,2-Dichloropropane	9.25	63	1006	0.503	ug/l #	44
48) Methyl methacrylate	9.17	41	4719	2.415	ug/l #	33
51) 4-Methyl-2-Pentanone	9.97	43	3753	1.486	ug/l	90
52) Toluene	10.14	92	12006	2.354	ug/l	97
54) cis-1,3-Dichloropropene	9.89	75	22964	6.882	ug/l #	58
57) 1,3-Dichloropropane	10.75	76	3805	1.186	ug/l #	42
59) 2-Hexanone	10.75	43	51972	27.941	ug/l #	55
67) Ethyl Benzene	11.50	91	2275	0.216	ug/l	99
68) m/p-Xylenes	11.61	106	4819	1.214	ug/l	95
69) o-Xylene	11.94	106	2480	0.638	ug/l	94
74) N-amyl acetate	12.03	43	3824	0.960	ug/l #	46
76) 1,2,3-Trichloropropane	12.40	75	71210	30.224	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	71210	64.906	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	14.35	75	101	Below Cal	#	6
95) Naphthalene	15.13	128	1551	0.203	ug/l #	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

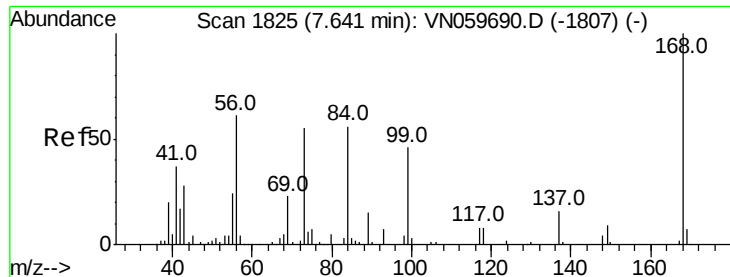

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. 0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25


Instrument :
MSVOA_N
ClientSampled :

Tot Ion:168 Resp: 199197

Ion Ratio Lower Upper




168 100

99 52.9 48.2 72.4

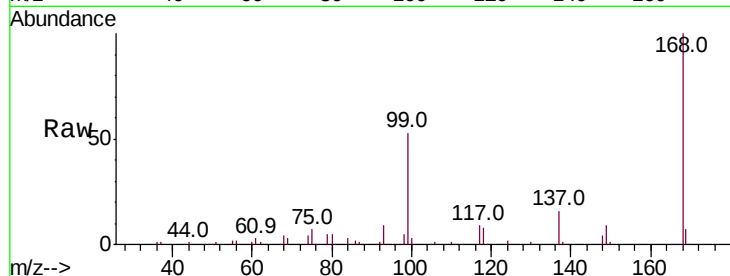

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

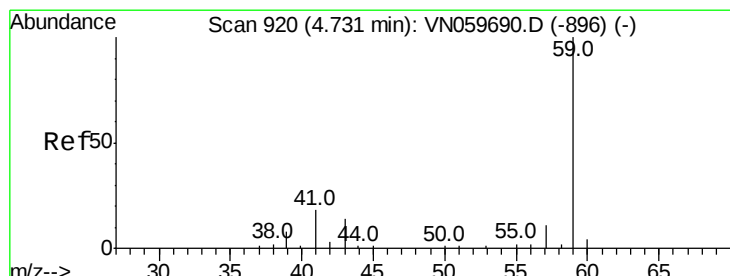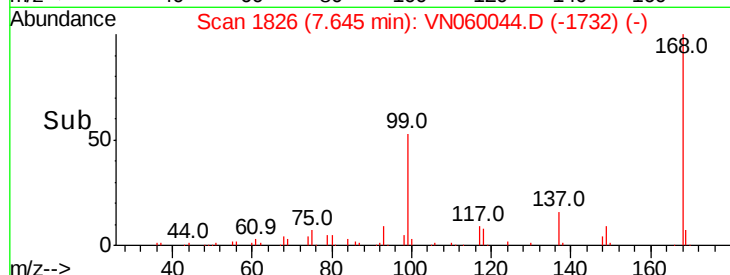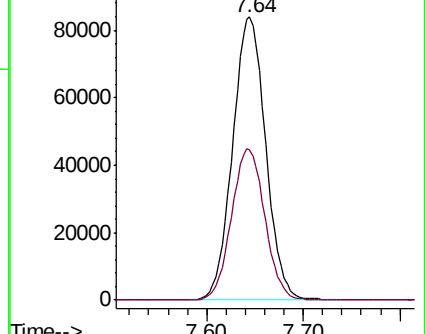

#11

Tert butyl alcohol

Concen: 0.448 ug/l

RT: 4.77 min Scan# 932

Delta R.T. 0.04 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 59 Resp: 167

Ion Ratio Lower Upper



59 100


57 0.0 8.6 12.8#

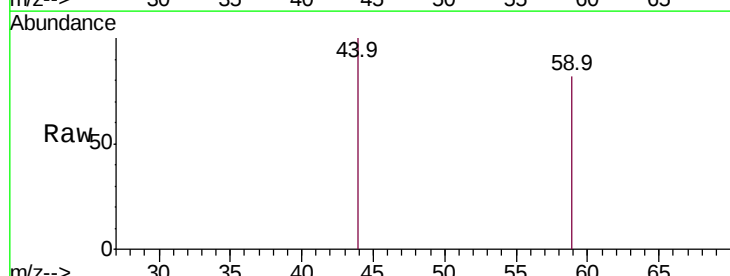

Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

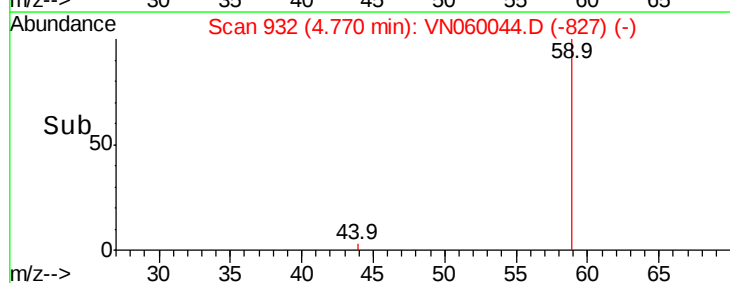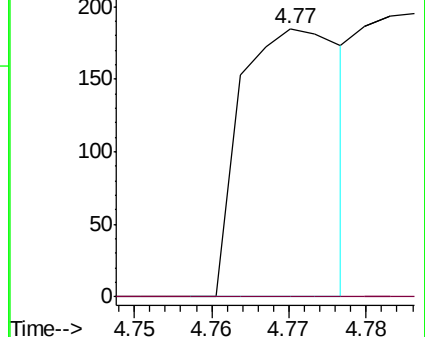



#16

Acetone

Concen: 79.027 ug/l

RT: 3.81 min Scan# 632

Delta R.T. 0.03 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N





ClientSampled :

Tot Ion: 43 Resp: 64791

Ion Ratio Lower Upper

43 100

58 30.4 23.6 35.4

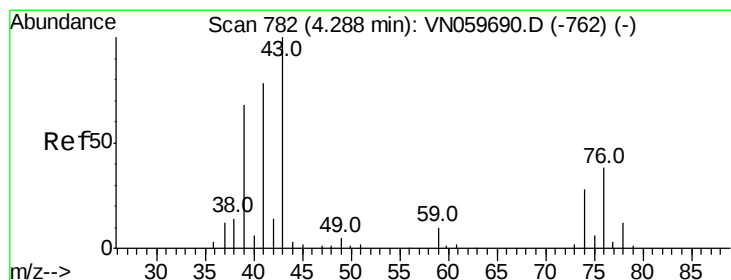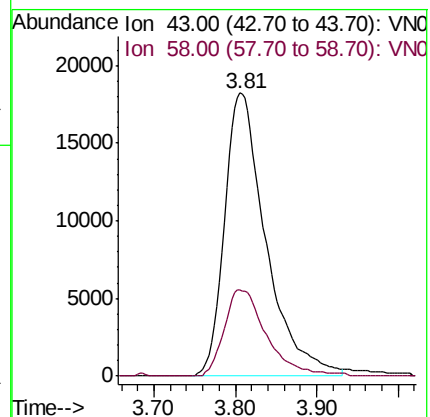

#18

Methyl Acetate

Concen: 0.511 ug/l

RT: 4.31 min Scan# 790

Delta R.T. 0.03 min

Lab File: VN060044.D




Acq: 10 Feb 2020 14:25


Tgt Ion: 43 Resp: 1321

Ion Ratio Lower Upper

43 100

74 0.0 17.5 26.3#

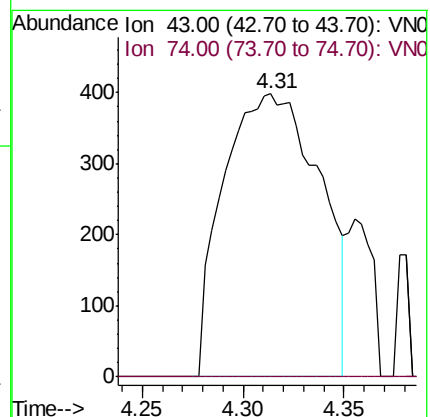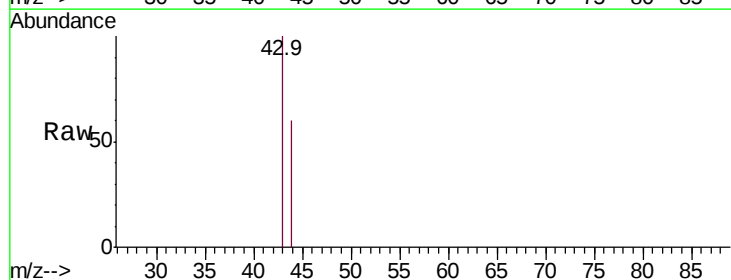



#20

Methvlene Chloride

Concen: 1.541 ug/l

RT: 4.52 min Scan# 854

Delta R.T. -0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 84 Resp: 5595


Ion Ratio Lower Upper

84 100




49 110.3 106.6 160.0

51 36.6 31.9 47.9

86 60.4 50.8 76.2



Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0

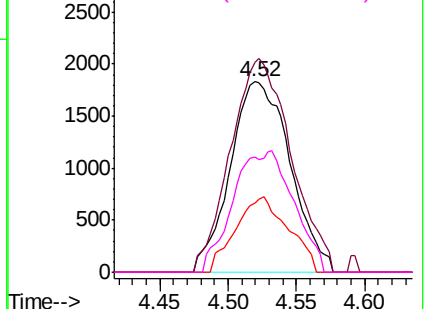

#25

2-Butanone

Concen: 48.270 ug/l

RT: 6.81 min Scan# 1567

Delta R.T. 0.01 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 43 Resp: 60469



Ion Ratio Lower Upper


43 100

72 26.8 19.9 29.9



Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 72.00 (71.70 to 72.70): VN0



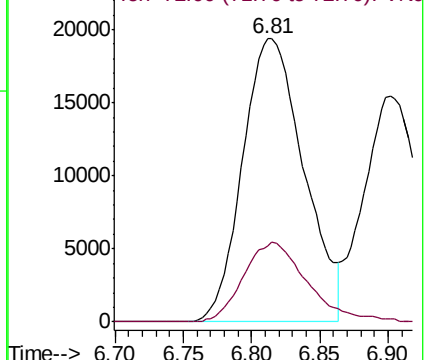



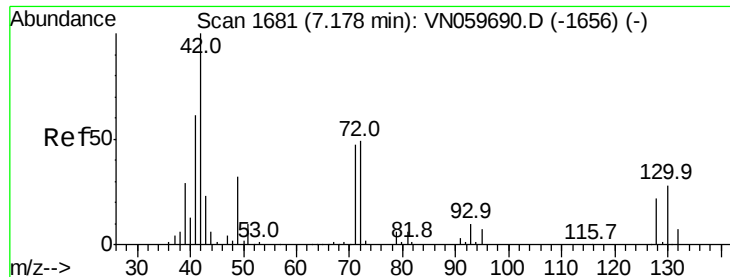

#29
Tetrahydrofuran
Concen: 3.832 ug/l
RT: 6.91 min Scan# 1596
Delta R.T. -0.27 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25




Instrument :
MSVOA_N
ClientSampled :


Tot Ion	Ratio	Lower	Upper
42	100		
72	0.0	33.1	49.7#
71	0.0	31.4	47.0#

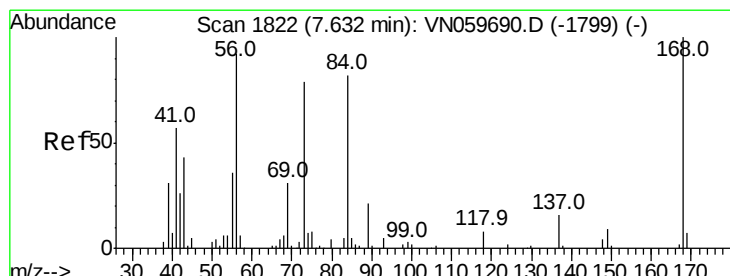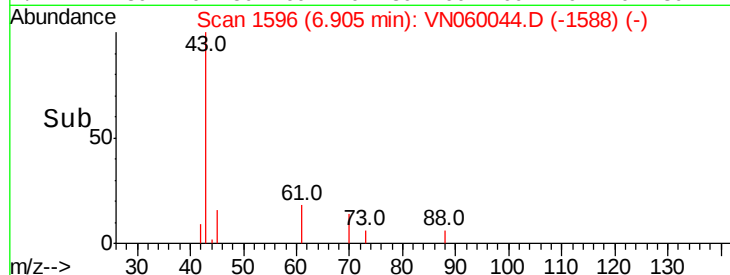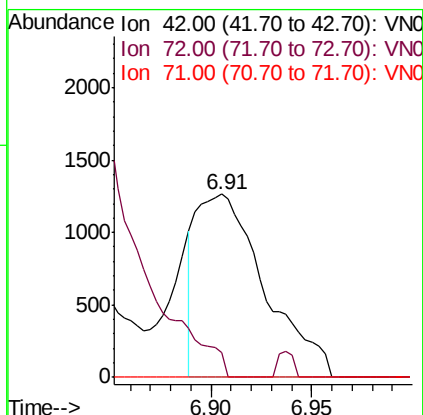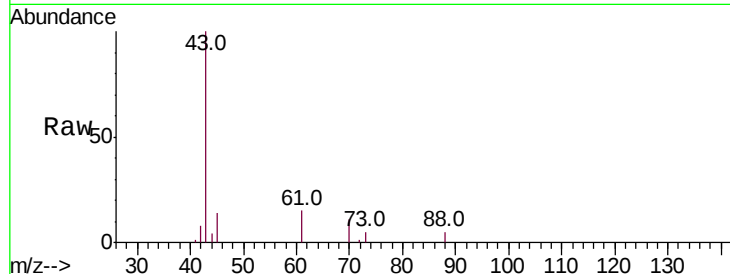

#31
Cyclohexane
Concen: 1.285 ug/l
RT: 7.64 min Scan# 1826
Delta R.T. 0.01 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Tgt Ion	Ratio	Lower	Upper
56	100		
69	144.0	26.5	39.7#
84	112.0	65.3	97.9#


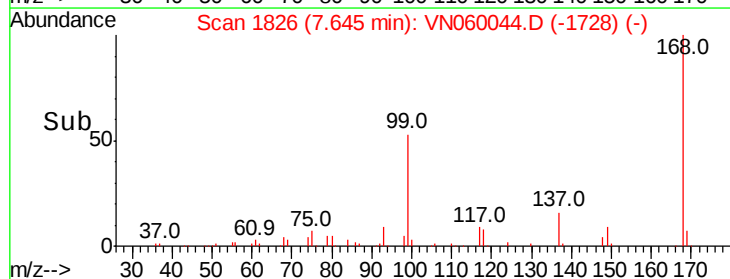
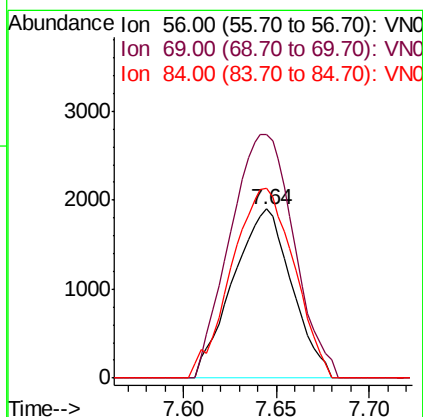
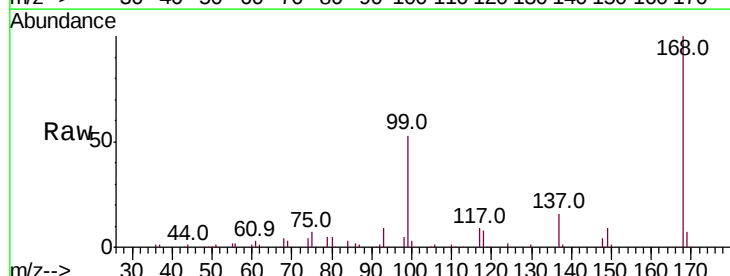




#33
 1,2-Dichloroethane-d4
 Concen: 52.363 ug/l
 RT: 8.00 min Scan# 1938
 Delta R.T. 0.00 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 65 Resp: 115835
 Ion Ratio Lower Upper
 65 100
 67 51.0 0.0 103.0

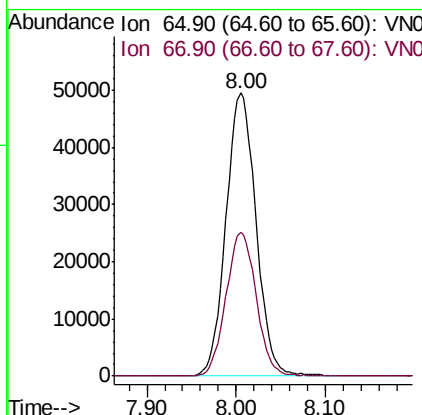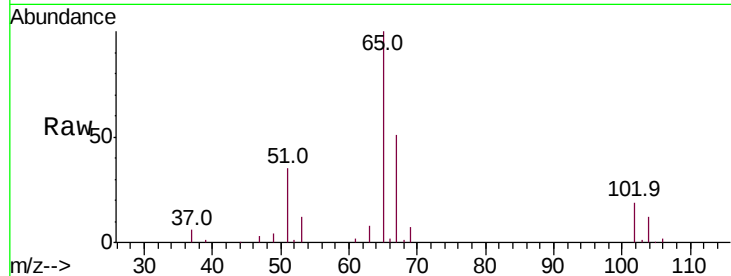

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25

Tgt Ion: 114 Resp: 310902
 Ion Ratio Lower Upper
 114 100
 63 20.3 0.0 43.6
 88 15.5 0.0 31.4



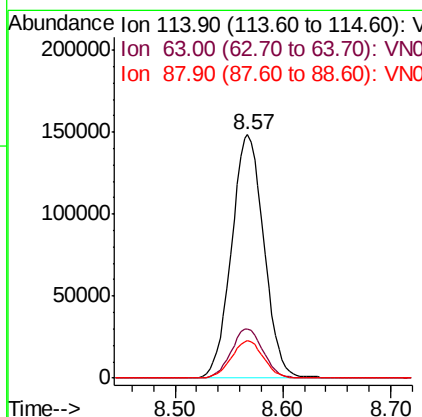





#35
 Dibromofluoromethane
 Concen: 51.161 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion:113 Resp: 94855
 Ion Ratio Lower Upper
 113 100
 111 103.7 83.5 125.3
 192 20.0 15.4 23.2

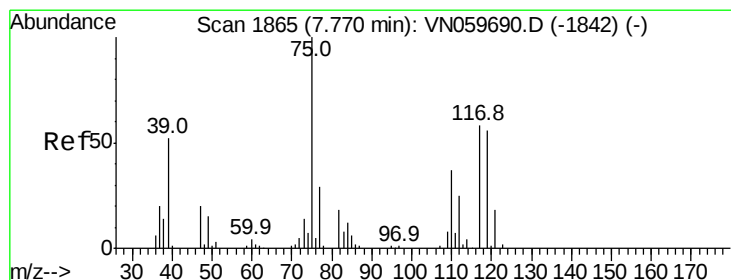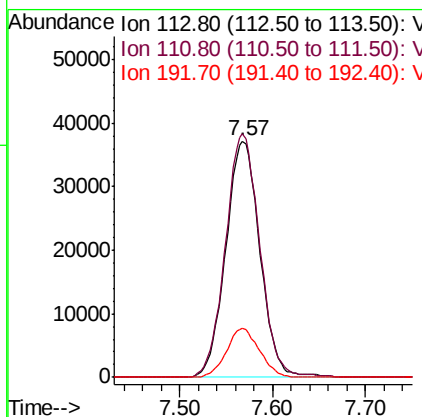

#36
 1,1-Dichloropropene
 Concen: 5.254 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.13 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25

Tgt Ion: 75 Resp: 14225
 Ion Ratio Lower Upper
 75 100
 110 8.2 16.6 49.7#
 77 0.0 25.1 37.7#

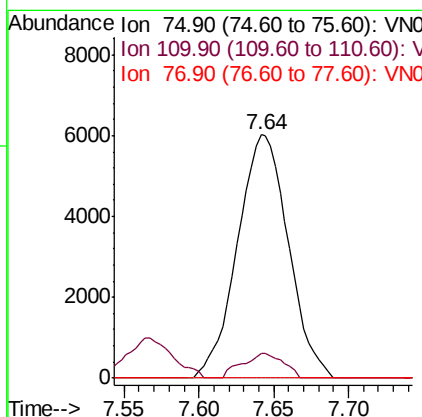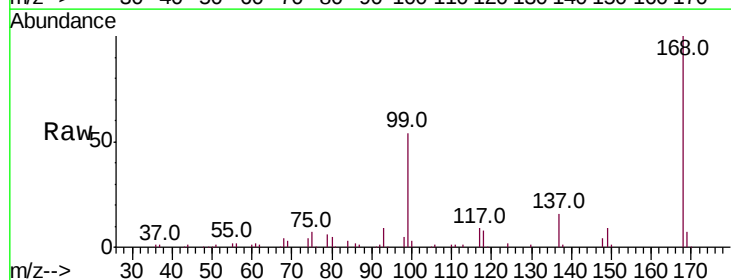


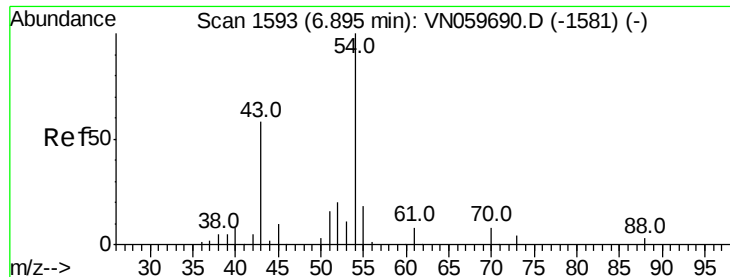




#37
Ethyl Acetate
Concen: 17.962 ug/l
RT: 6.90 min Scan# 1595
Delta R.T. 0.01 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 43 Resp: 45612
Ion Ratio Lower Upper
43 100
61 14.3 10.9 16.3
70 10.9 7.7 11.5

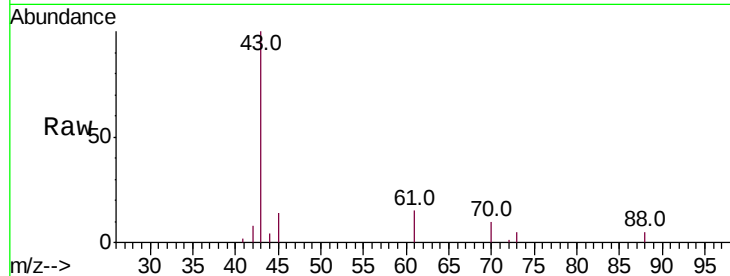


Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 60.90 (60.60 to 61.60): VN0
Ion 70.00 (69.70 to 70.70): VN0

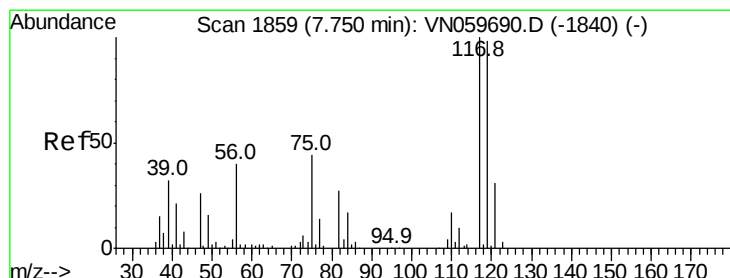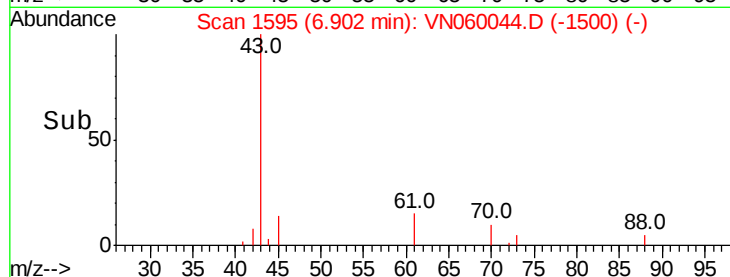
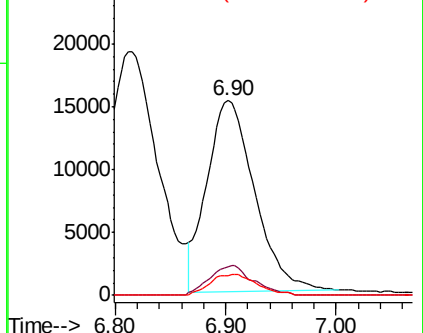



#38
Carbon Tetrachloride
Concen: 6.313 ug/l
RT: 7.64 min Scan# 1826
Delta R.T. -0.11 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Tgt Ion: 117 Resp: 18594
Ion Ratio Lower Upper
117 100
119 5.4 76.5 114.7#
121 0.0 25.1 37.7#

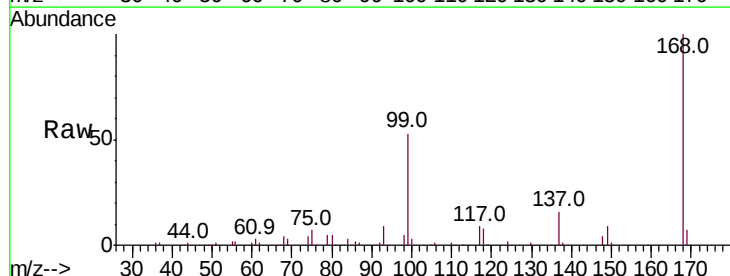

Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

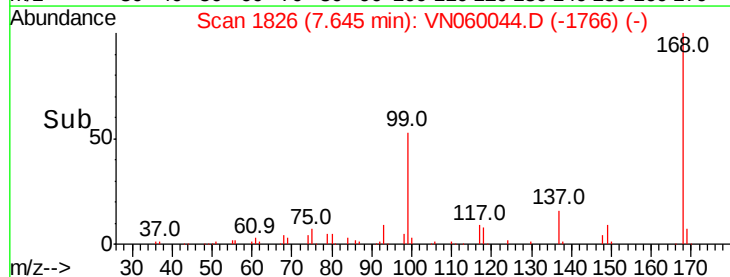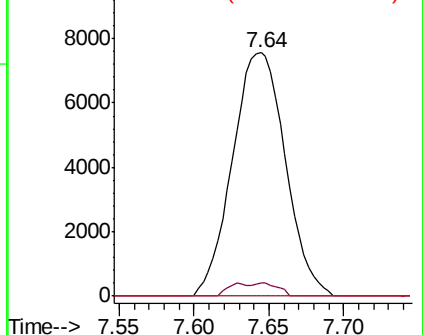



#43

Isopropyl Acetate

Concen: 11.565 ug/l

RT: 8.14 min Scan# 1981

Delta R.T. 0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 43 Resp: 50512

Ion Ratio Lower Upper

43 100

61 19.4 20.2 30.2#




87 14.2 9.5 14.3

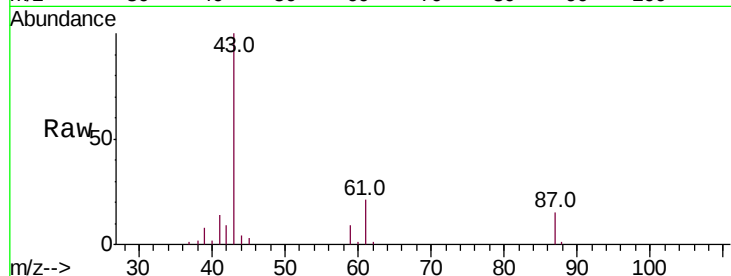

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

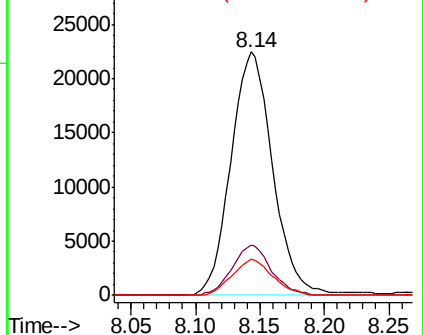

#45

1,2-Dichloropropane

Concen: 0.503 ug/l

RT: 9.25 min Scan# 2325

Delta R.T. 0.15 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 63 Resp: 1006

Ion Ratio Lower Upper



63 100


65 0.0 24.9 37.3#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0

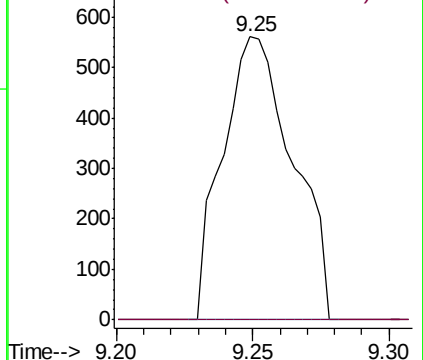



#48

Methvl methacrylate

Concen: 2.415 ug/l

RT: 9.17 min Scan# 2299

Delta R.T. -0.02 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 41 Resp: 4719

Ion Ratio Lower Upper

41 100

69 0.0 64.4 96.6#




39 35.3 51.3 76.9#

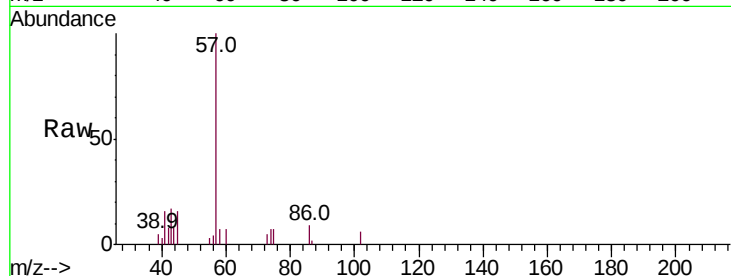

Abundance Ion 41.00 (40.70 to 41.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

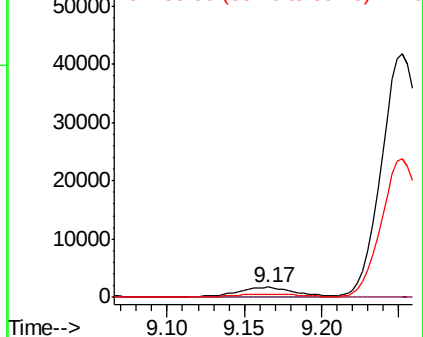

#50

Toluene-d8

Concen: 52.416 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. 0.00 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 98 Resp: 376532

Ion Ratio Lower Upper



98 100


100 65.0 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

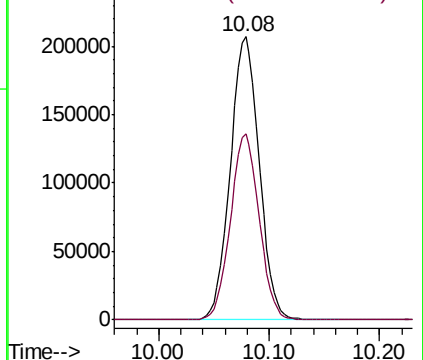



#51

4-Methyl-2-Pentanone

Concen: 1.486 ug/l

RT: 9.97 min Scan# 2550

Delta R.T. 0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 43 Resp: 3753

Ion Ratio Lower Upper




43 100

58 31.1 29.8 44.8

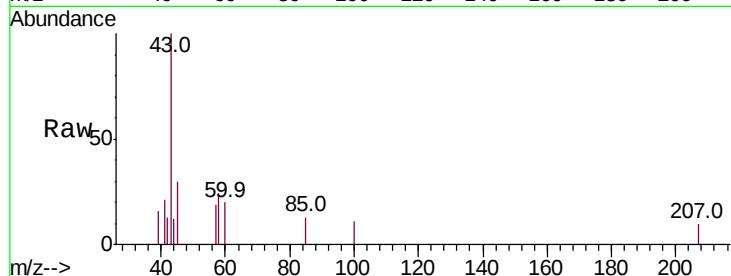

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

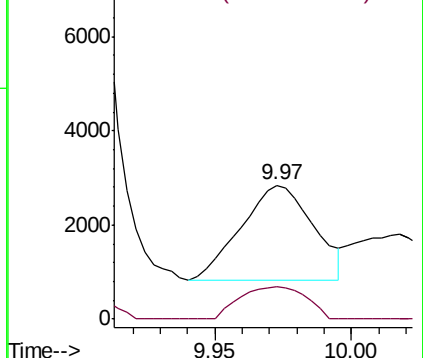

#52

Toluene

Concen: 2.354 ug/l

RT: 10.14 min Scan# 2603

Delta R.T. 0.00 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 92 Resp: 12006

Ion Ratio Lower Upper



92 100


91 179.2 140.4 210.6



Abundance Ion 92.00 (91.70 to 92.70): VN0

Ion 91.00 (90.70 to 91.70): VN0

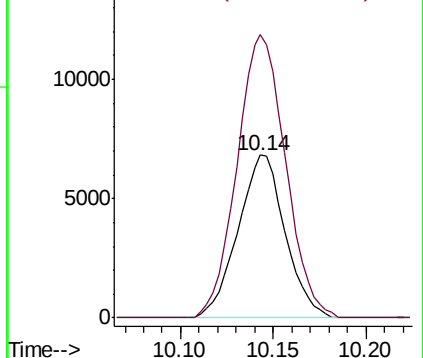



#54

cis-1,3-Dichloropropene

Concen: 6.882 ug/l

RT: 9.89 min Scan# 2524

Delta R.T. 0.06 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 75 Resp: 22964

Ion Ratio Lower Upper




75 100

77 0.0 25.1 37.7#

39 32.9 46.1 69.1#

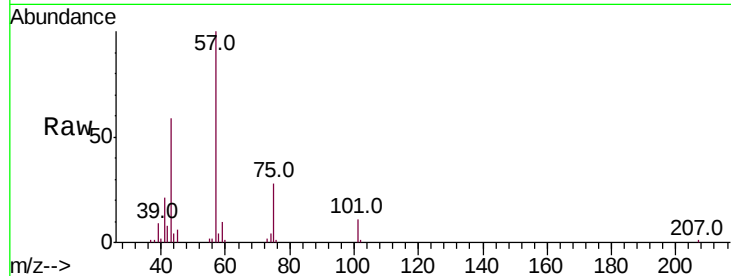

Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 76.90 (76.60 to 77.60): VN0
Ion 39.00 (38.70 to 39.70): VN0

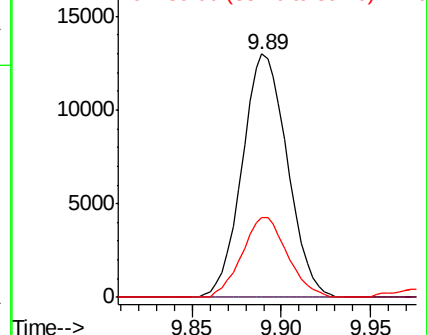

#57

1,3-Dichloropropane

Concen: 1.186 ug/l

RT: 10.75 min Scan# 2793

Delta R.T. 0.06 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion: 76 Resp: 3805



Ion Ratio Lower Upper


76 100

78 0.0 25.8 38.8#



Abundance Ion 75.90 (75.60 to 76.60): VN0
Ion 77.90 (77.60 to 78.60): VN0




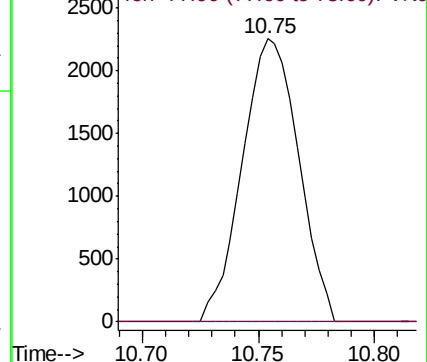




#59
2-Hexanone
Concen: 27.941 ug/l
RT: 10.75 min Scan# 2793
Delta R.T. 0.01 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 43 Resp: 51972
Ion Ratio Lower Upper
43 100
58 20.0 25.8 77.3#

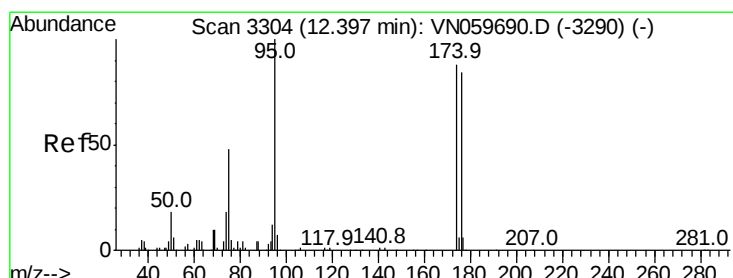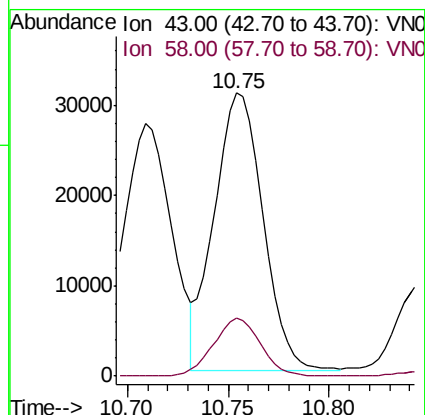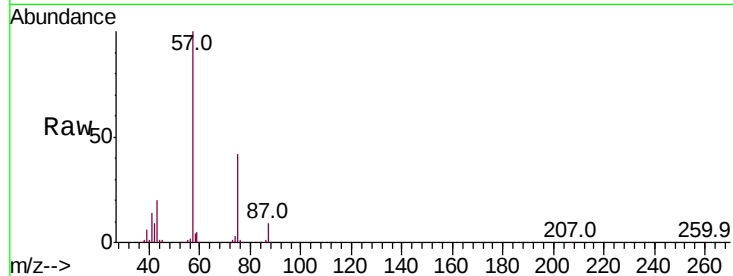

#62
4-Bromofluorobenzene
Concen: 53.322 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.00 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Tgt Ion: 95 Resp: 138085
Ion Ratio Lower Upper
95 100
174 86.9 0.0 151.4
176 83.4 0.0 146.0

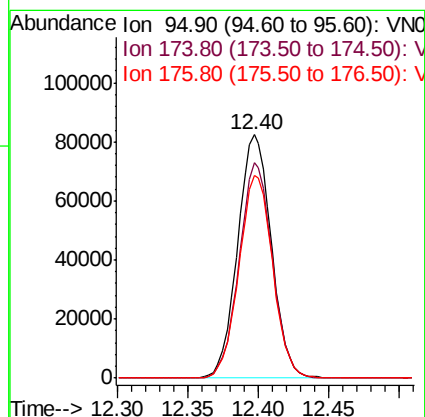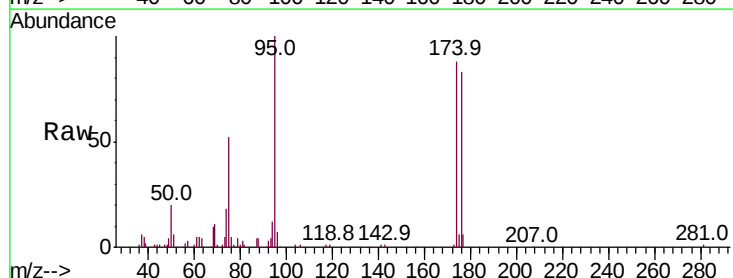







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Instrument :
MSVOA_N
ClientSampled :

Tot Ion:117 Resp: 294596
Ion Ratio Lower Upper
117 100
82 54.5 45.9 68.9
119 32.5 25.5 38.3

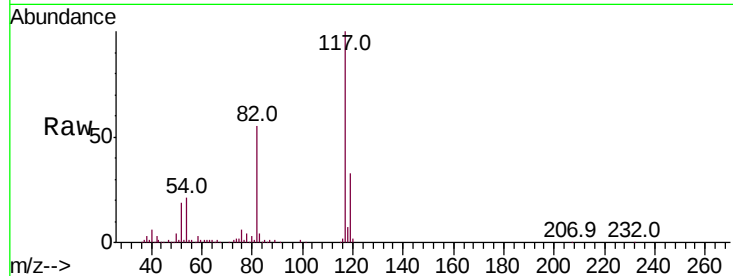


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN0
Ion 118.90 (118.60 to 119.60): V

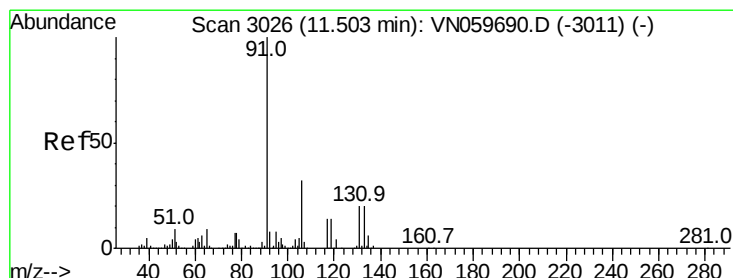
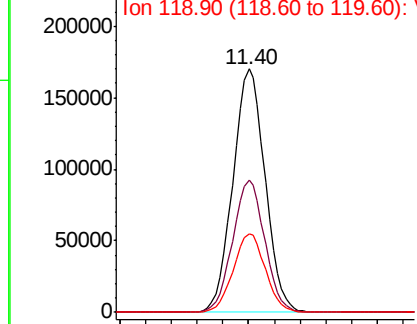



#67
Ethyl Benzene
Concen: 0.216 ug/l
RT: 11.50 min Scan# 3026
Delta R.T. 0.00 min
Lab File: VN060044.D
Acq: 10 Feb 2020 14:25

Tgt Ion: 91 Resp: 2275
Ion Ratio Lower Upper
91 100
106 29.5 24.1 36.1

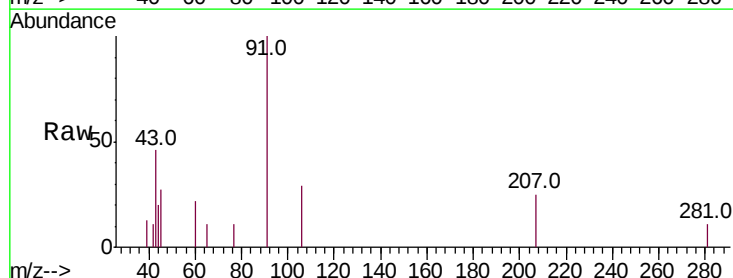

Abundance Ion 91.00 (90.70 to 91.70): VN0
Ion 106.00 (105.70 to 106.70): V

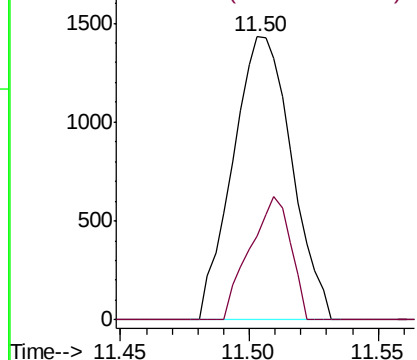



#68

m/p-Xylenes

Concen: 1.214 ug/l

RT: 11.61 min Scan# 3060

Delta R.T. -0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N


ClientSampled :

Tot Ion:106 Resp: 4819

Ion Ratio Lower Upper




106 100

91 201.9 167.9 251.9



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VN

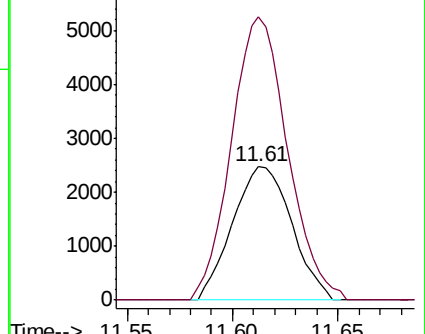

#69

o-Xylene

Concen: 0.638 ug/l

RT: 11.94 min Scan# 3162

Delta R.T. 0.00 min

Lab File: VN060044.D


Acq: 10 Feb 2020 14:25

Tgt Ion:106 Resp: 2480

Ion Ratio Lower Upper



106 100


91 211.6 110.3 330.9



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VN

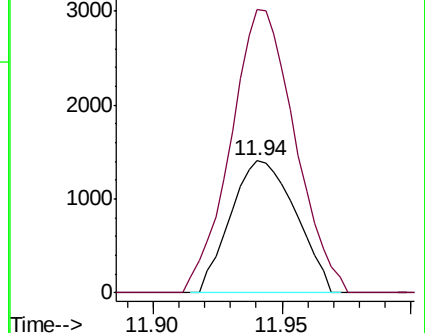

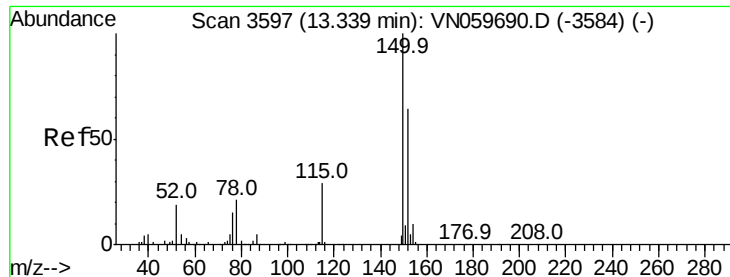

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. 0.00 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 140001

Ion Ratio Lower Upper

152 100

115 58.2 30.3 90.9




150 156.7 0.0 345.2

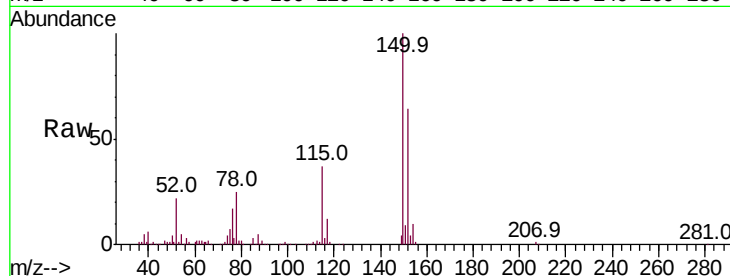

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

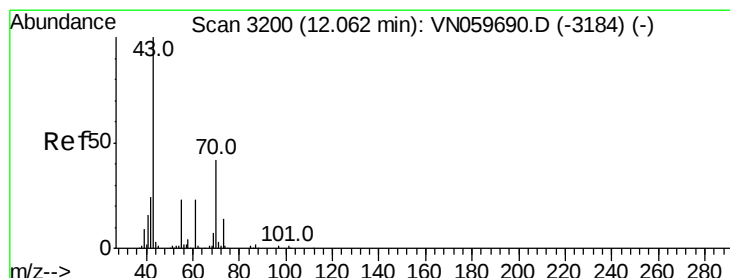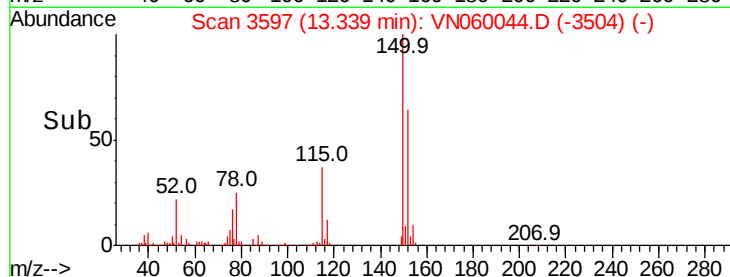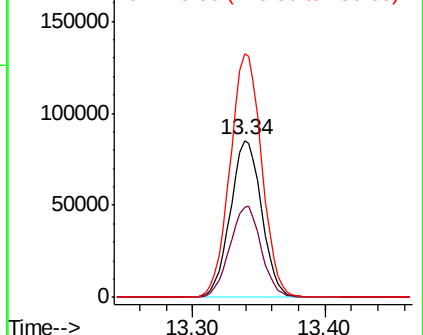

#74

N-ethyl acetate

Concen: 0.960 ug/l

RT: 12.03 min Scan# 3189

Delta R.T. -0.04 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Tgt Ion: 43 Resp: 3824


Ion Ratio Lower Upper

43 100

70 0.0 31.3 46.9#

55 2.5 19.8 29.6#

61 0.0 18.3 27.5#


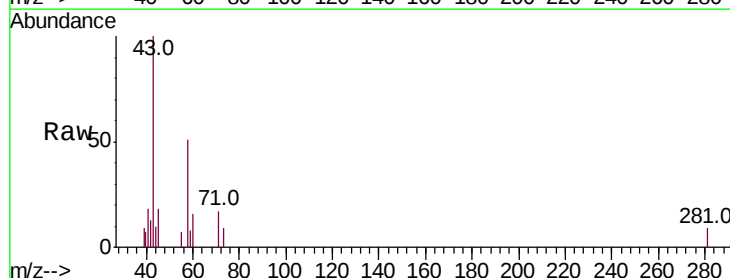



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

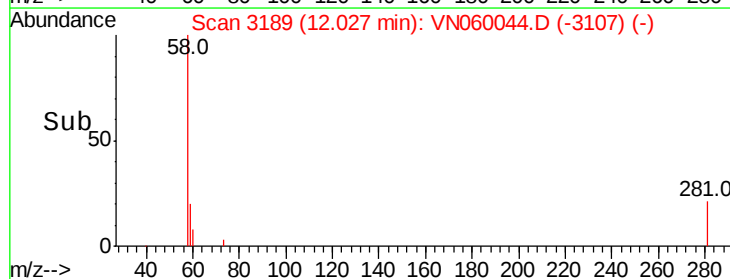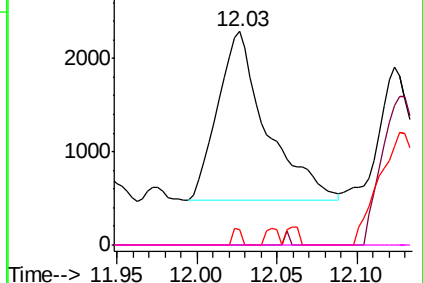



#76

1,2,3-Trichloropropane

Concen: 30.224 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25

Instrument :

MSVOA_N





ClientSampleId :

Tot Ion: 75 Resp: 71210

Ion Ratio Lower Upper

75 100

77 1.1 0.0 0.0#

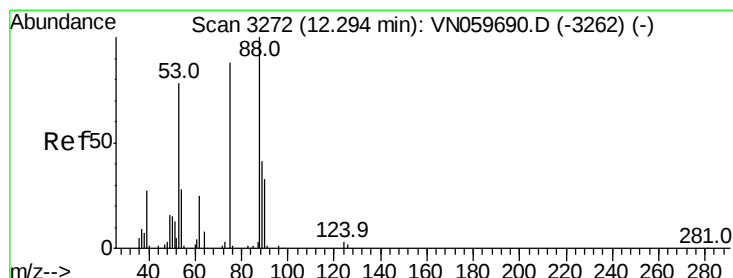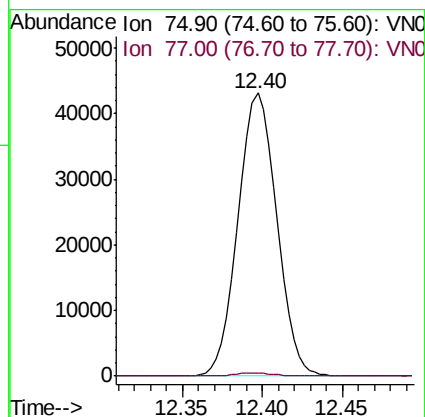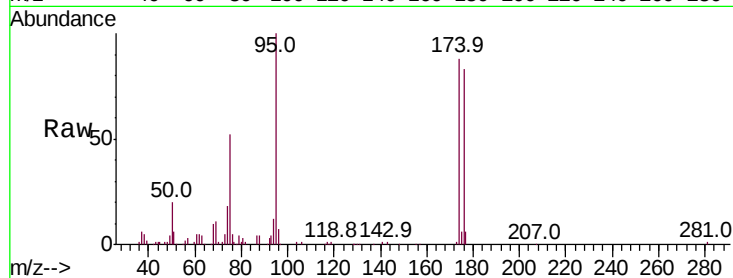

#81

trans-1,4-Dichloro-2-butene

Concen: 64.906 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.10 min

Lab File: VN060044.D

Acq: 10 Feb 2020 14:25




Tgt Ion: 75 Resp: 71210


Ion Ratio Lower Upper

75 100

53 0.0 78.1 117.1#

89 0.0 35.4 53.2#

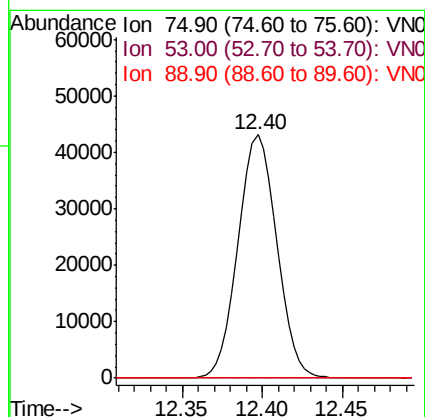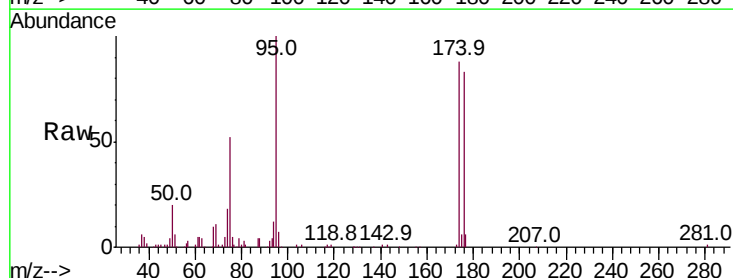







#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.35 min Scan# 3910
 Delta R.T. 0.08 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
75	100		
155	0.0	37.0	110.9#
157	0.0	48.4	145.2#

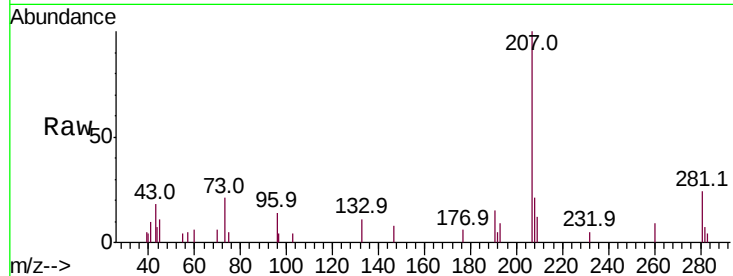


Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 154.80 (154.50 to 155.50): V
 Ion 156.80 (156.50 to 157.50): V

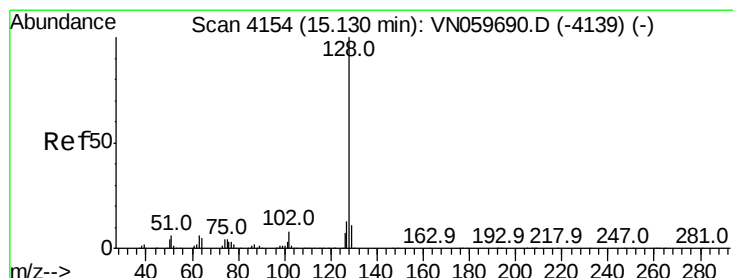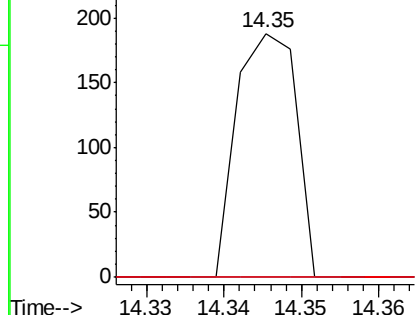

#95
 Naphthalene
 Concen: 0.203 ug/l
 RT: 15.13 min Scan# 4154
 Delta R.T. 0.00 min
 Lab File: VN060044.D
 Acq: 10 Feb 2020 14:25

Tgt Ion	Ratio	Lower	Upper
128	100		
127	6.3	10.4	15.6#
129	0.0	8.6	12.8#

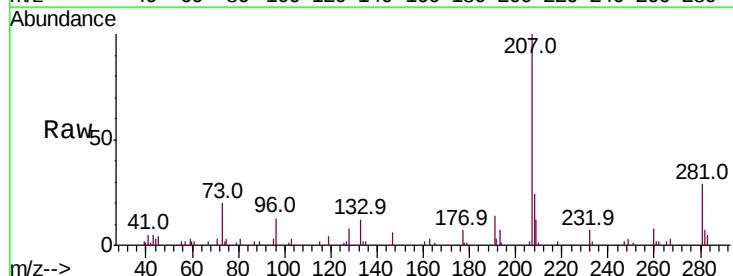

Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 127.00 (126.70 to 127.70): V
 Ion 129.00 (128.70 to 129.70): V

