


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021021\
 Data File : VN065790.D
 Acq On : 10 Feb 2021 9:56
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Feb 03 14:50:04 2021

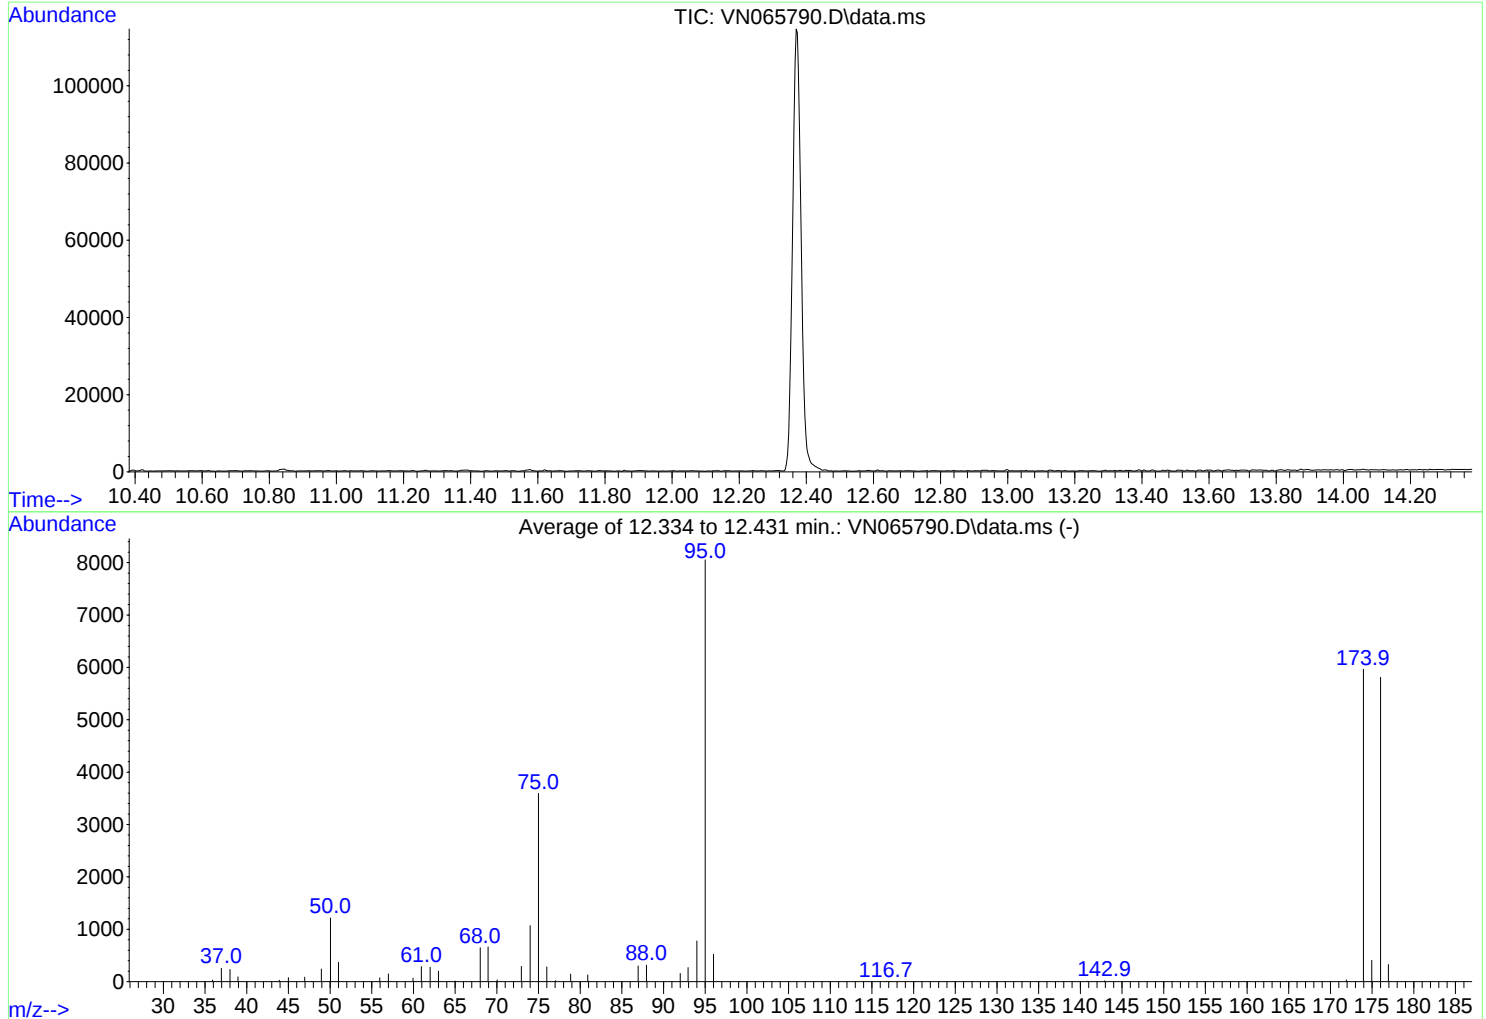

AutoFind: Averaged scan 3295 to 3325; Bkg corrected with scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	1217	PASS
75	95	30	60	44.6	3595	PASS
95	95	100	100	100.0	8053	PASS
96	95	5	9	6.5	521	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	5962	PASS
175	174	5	9	6.8	405	PASS
176	174	95	101	97.5	5810	PASS
177	176	5	9	5.6	328	PASS