

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021023\
 Data File : VN076614.D
 Acq On : 10 Feb 2023 17:09
 Operator : JC\MD
 Sample : 01500-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(FEB)

Quant Time: Feb 11 00:58:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020923W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Feb 10 05:40:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.822	128	23437	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.104	114	154627	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.869	117	176692	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.586	65	76349	27.639	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	92.133%
60) 4-Bromofluorobenzene	12.851	95	95860	24.031	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	80.100%
63) Toluene-d8	10.569	98	178296	27.482	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	91.600%
Target Compounds						
					Qvalue	
15) Acetone	4.440	58	170705	367.595	ug/l	77
30) 2-Butanone	7.498	43	39388	18.232	ug/l	99
58) 4-Methyl-2-Pentanone	10.451	43	9510	1.925	ug/l #	83
62) Toluene	10.633	91	27211	2.077	ug/l	100
67) m/p-Xylenes	12.074	106	2307	0.428	ug/l	85
80) 1,2,4-Trimethylbenzene	13.492	105	6473	0.494	ug/l	77
82) p-Isopropyltoluene	13.733	119	3432	0.271	ug/l	98
91) Naphthalene	15.645	128	56497	5.793	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021023\
Data File : VN076614.D
Acq On : 10 Feb 2023 17:09
Operator : JC\MD
Sample : 01500-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)

Quant Time: Feb 11 00:58:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N020923W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Feb 10 05:40:47 2023
Response via : Initial Calibration




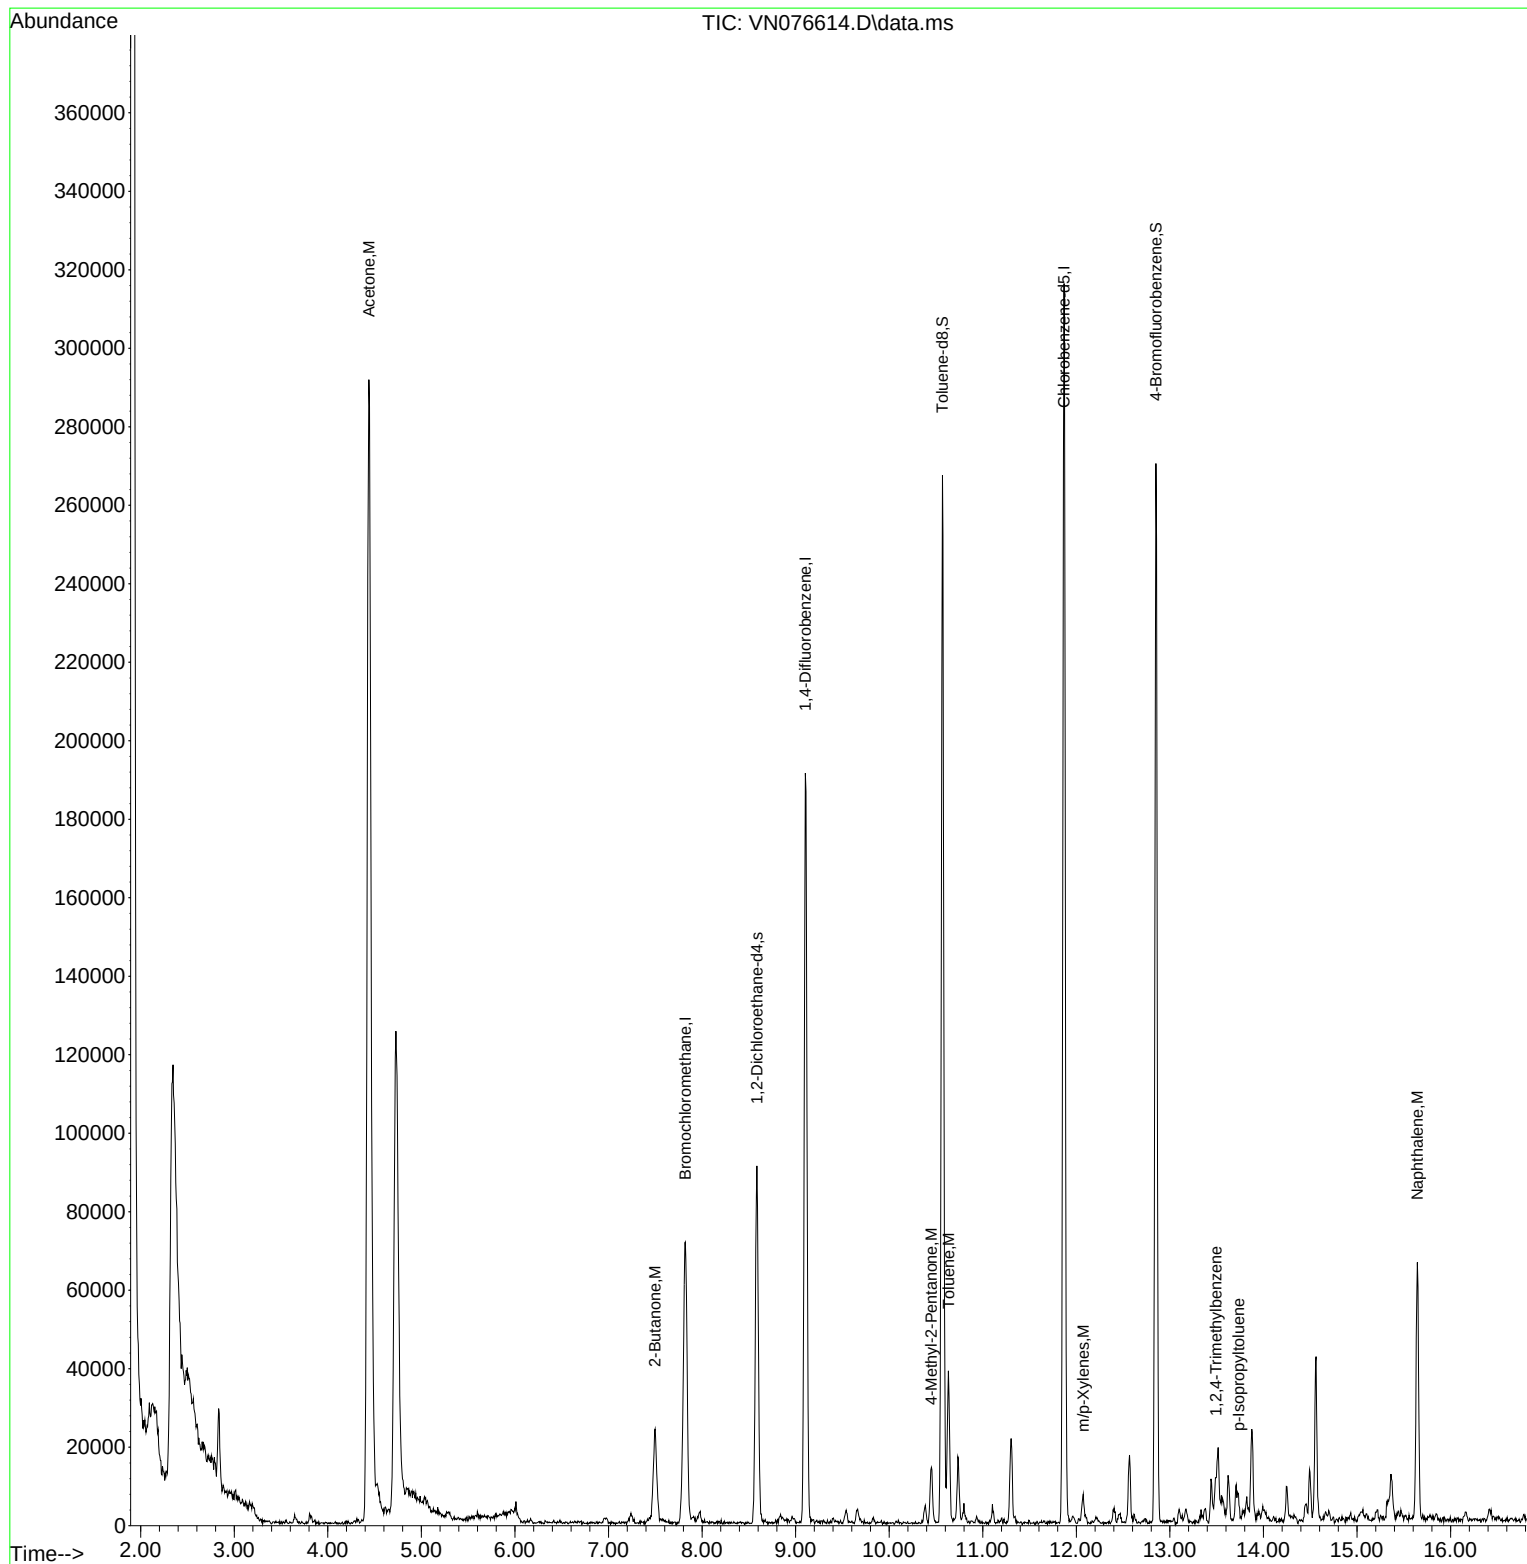


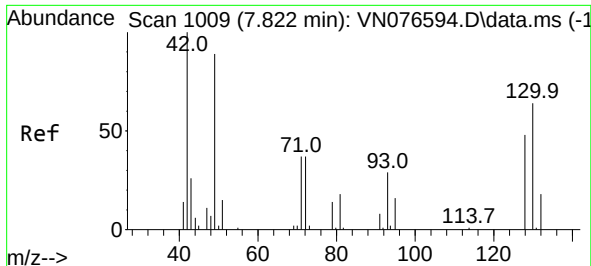

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.822 min Scan# 1009
Delta R.T. -0.008 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)


Tgt Ion:128 Resp: 23437
Ion Ratio Lower Upper
128 100
49 185.6 0.0 492.0
130 133.4 0.0 313.3

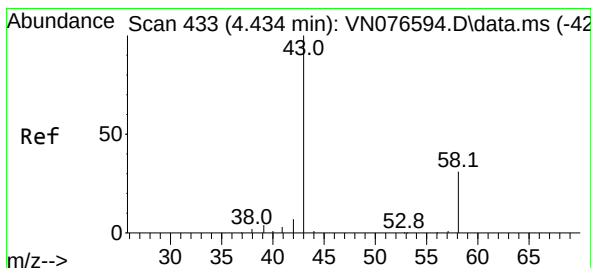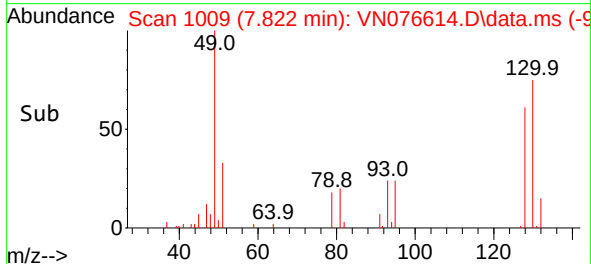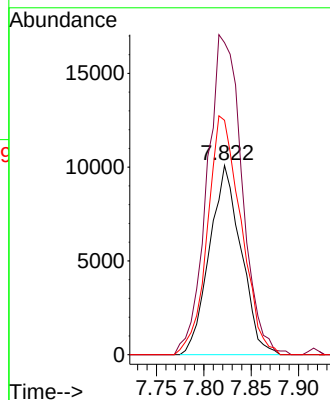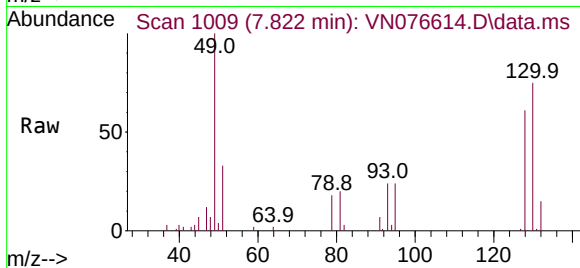

#15
Acetone
Concen: 367.595 ug/l
RT: 4.440 min Scan# 434
Delta R.T. -0.013 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09

Tgt Ion: 58 Resp: 170705
Ion Ratio Lower Upper
58 100
43 335.3 232.2 348.4

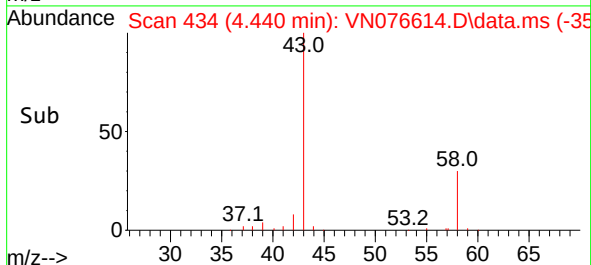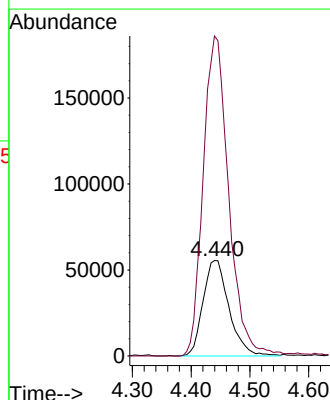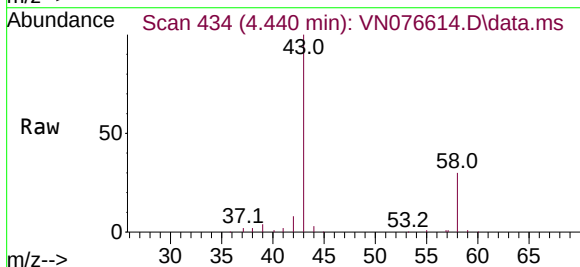

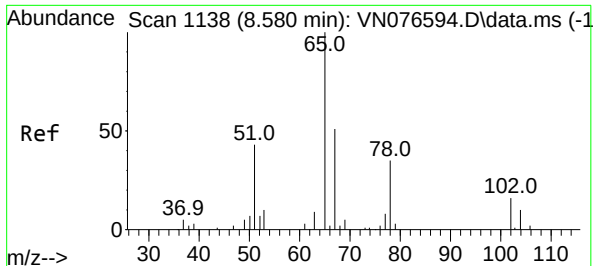

#27

1,2-Dichloroethane-d4

Concen: 27.639 ug/l

RT: 8.586 min Scan# 1139

Delta R.T. -0.002 min

Lab File: VN076614.D

Acq: 10 Feb 2023 17:09

Instrument :

MSVOA_N

ClientSampleId :





001-WILLETS-PT-BLVD(FEB)

Tgt Ion: 65 Resp: 76349

Ion Ratio Lower Upper

65 100

67 49.1 45.2 67.8

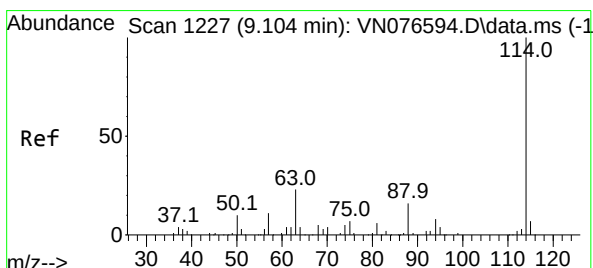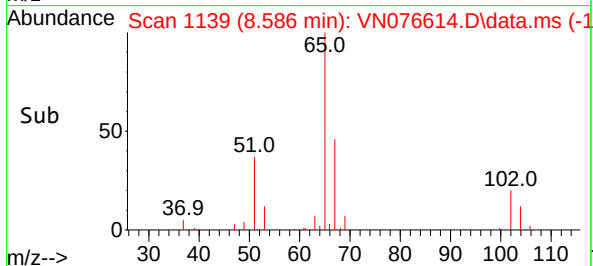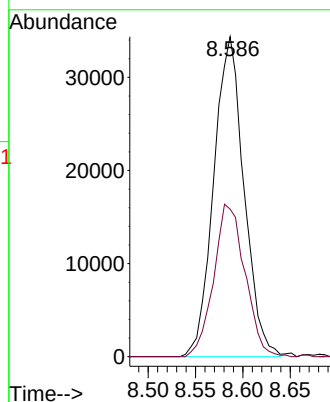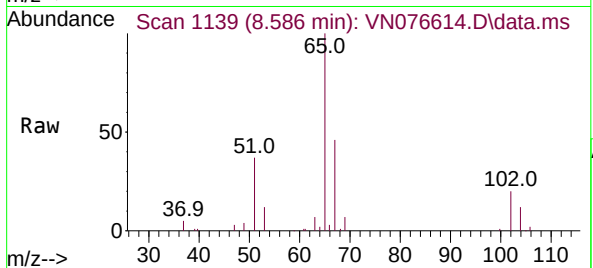

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.104 min Scan# 1227

Delta R.T. -0.002 min

Lab File: VN076614.D

Acq: 10 Feb 2023 17:09




Tgt Ion: 114 Resp: 154627


Ion Ratio Lower Upper

114 100

63 23.5 16.6 25.0

88 17.8 12.2 18.4


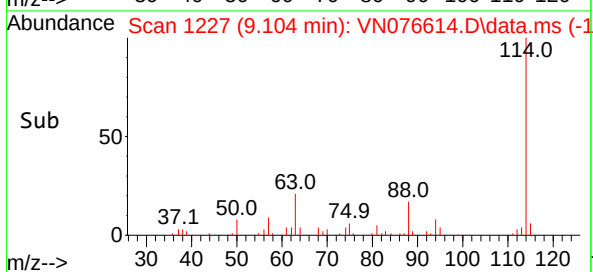
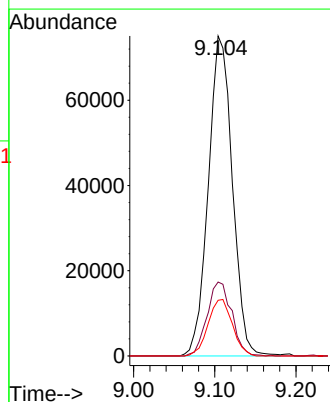
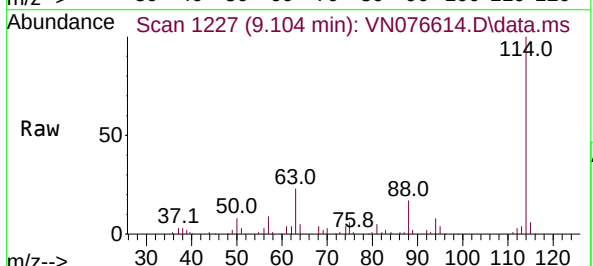


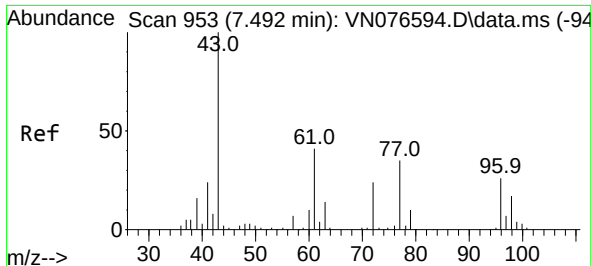

#30
2-Butanone
Concen: 18.232 ug/l
RT: 7.498 min Scan# 91
Delta R.T. -0.008 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)


Tgt Ion: 43 Resp: 39388
Ion Ratio Lower Upper
43 100
57 7.3 6.3 9.5
72 25.7 21.0 31.4

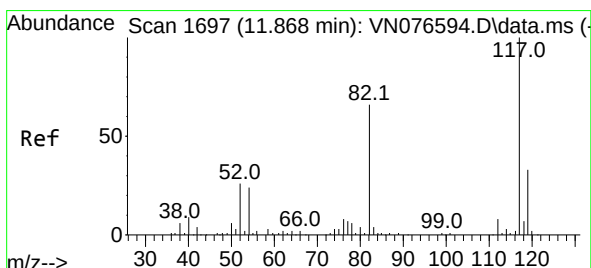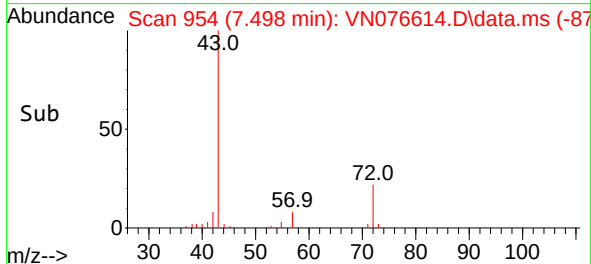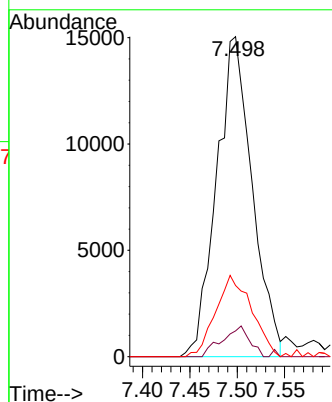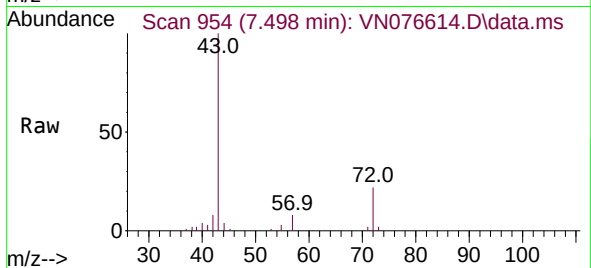

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.869 min Scan# 1697
Delta R.T. -0.002 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09

Tgt Ion: 117 Resp: 176692
Ion Ratio Lower Upper
117 100
82 58.1 44.6 67.0
119 30.8 25.6 38.4


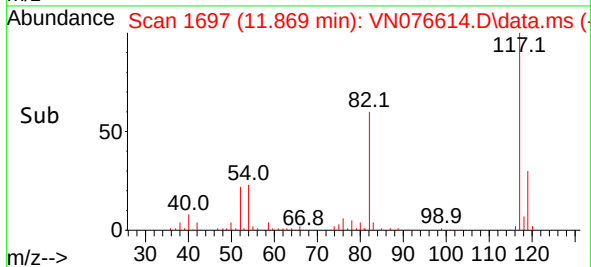
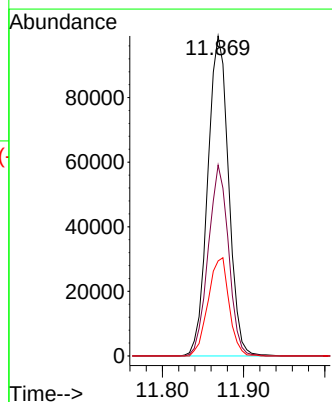
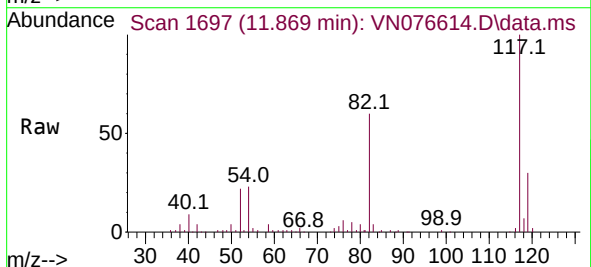


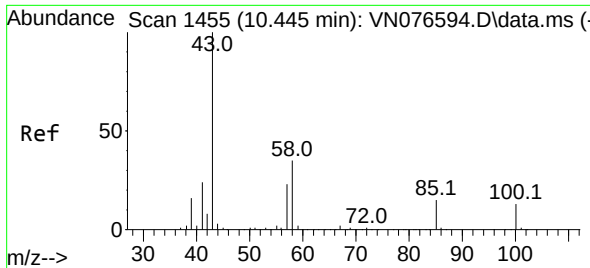

#58
4-Methyl-2-Pentanone
Concen: 1.925 ug/l
RT: 10.451 min Scan# 1455
Delta R.T. 0.004 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)


Tgt Ion: 43 Resp: 9510
Ion Ratio Lower Upper
43 100
58 24.0 30.8 46.2#
85 15.7 13.3 19.9

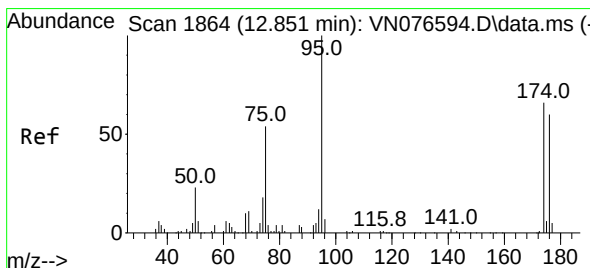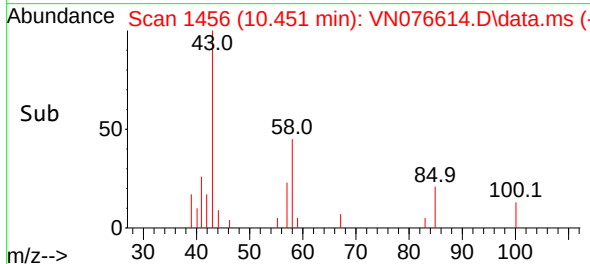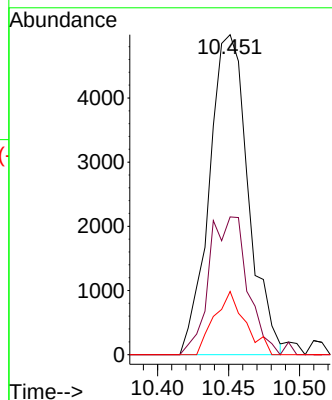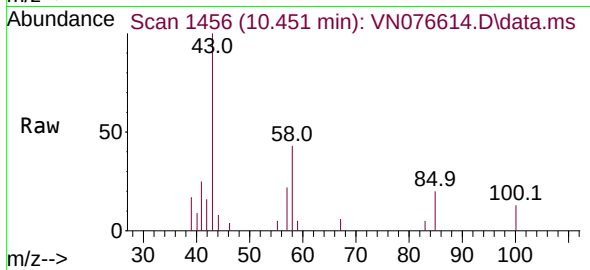

#60
4-Bromofluorobenzene
Concen: 24.031 ug/l
RT: 12.851 min Scan# 1864
Delta R.T. -0.002 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09

Tgt Ion: 95 Resp: 95860
Ion Ratio Lower Upper
95 100
174 70.9 57.8 86.8
176 67.6 57.0 85.4


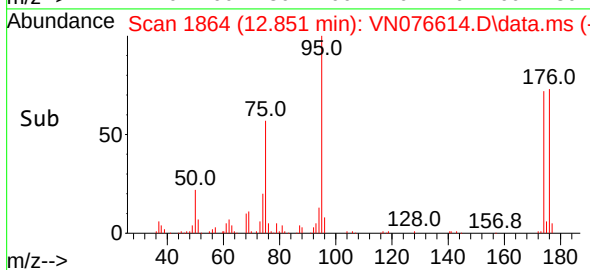
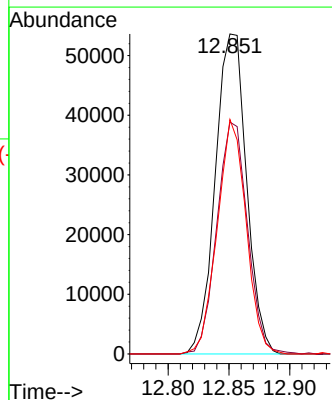
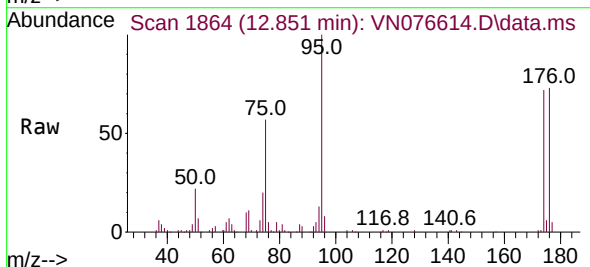


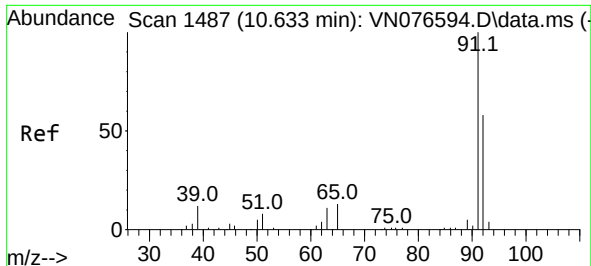

#62
Toluene
Concen: 2.077 ug/l
RT: 10.633 min Scan# 1487
Delta R.T. -0.002 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)


Tgt Ion: 91 Resp: 27211
Ion Ratio Lower Upper
91 100
92 57.2 46.0 69.0

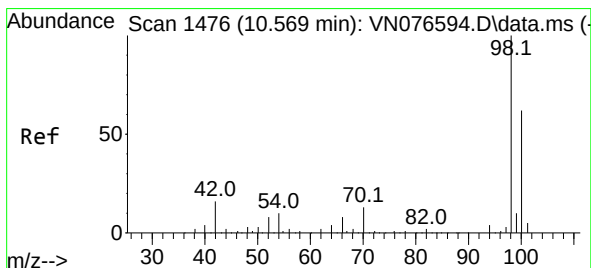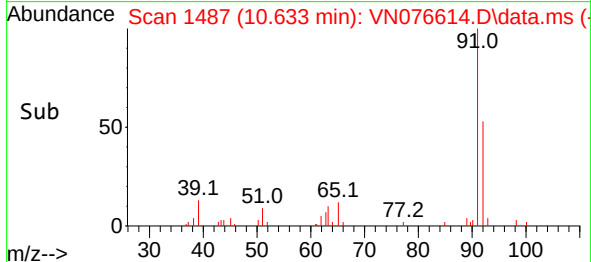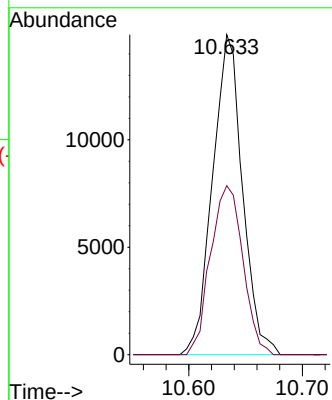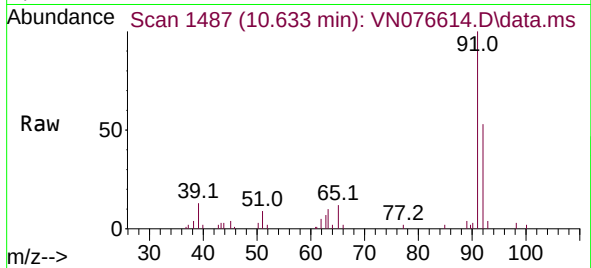

#63
Toluene-d8
Concen: 27.482 ug/l
RT: 10.569 min Scan# 1476
Delta R.T. -0.002 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09

Tgt Ion: 98 Resp: 178296
Ion Ratio Lower Upper
98 100
100 64.7 52.7 79.1


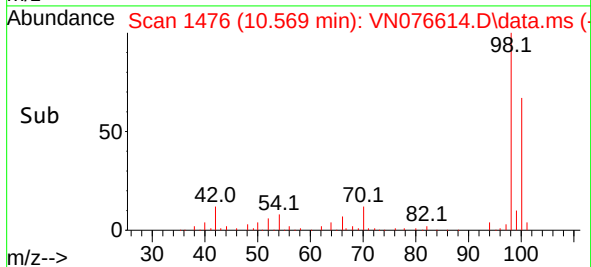
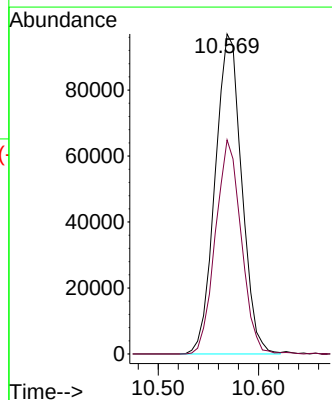
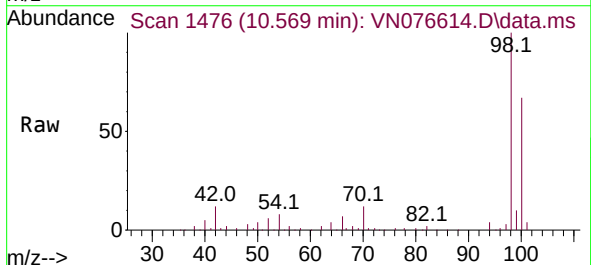


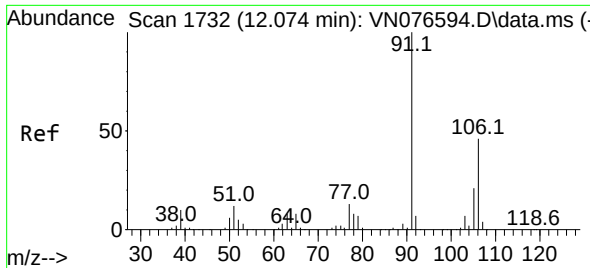

#67
m/p-Xylenes
Concen: 0.428 ug/l
RT: 12.074 min Scan# 11
Delta R.T. -0.002 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(FEB)


Tgt Ion:106 Resp: 2307
Ion Ratio Lower Upper
106 100
91 181.5 164.2 246.4

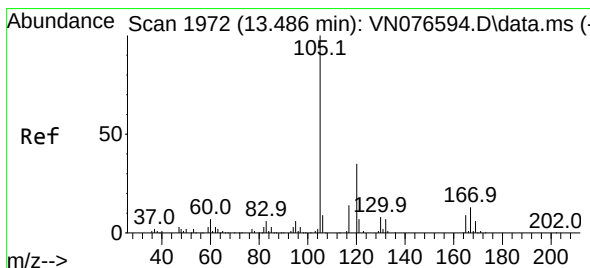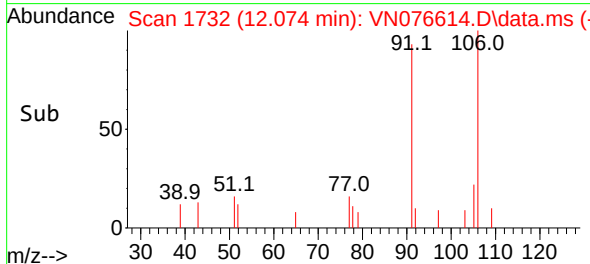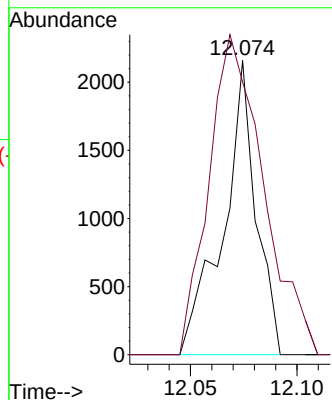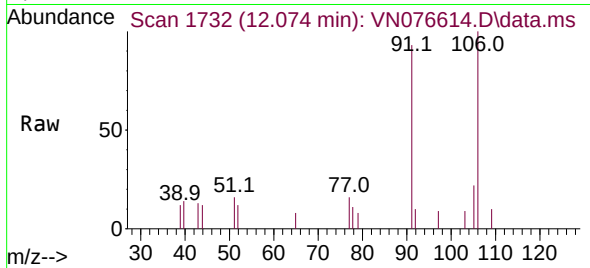

#80
1,2,4-Trimethylbenzene
Concen: 0.494 ug/l
RT: 13.492 min Scan# 1973
Delta R.T. 0.010 min
Lab File: VN076614.D
Acq: 10 Feb 2023 17:09

Tgt Ion:105 Resp: 6473
Ion Ratio Lower Upper
105 100
120 31.2 0.0 93.2

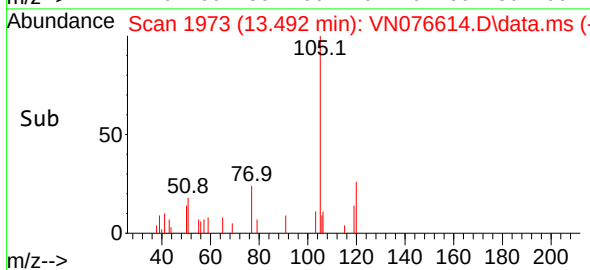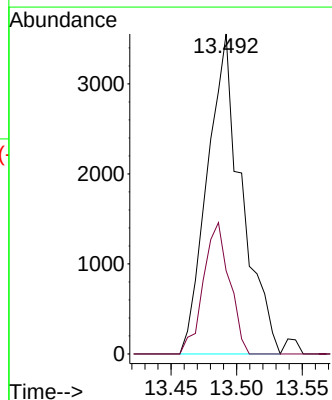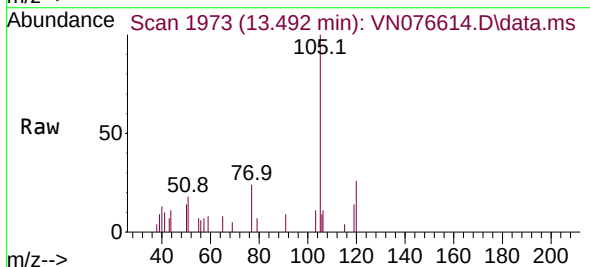

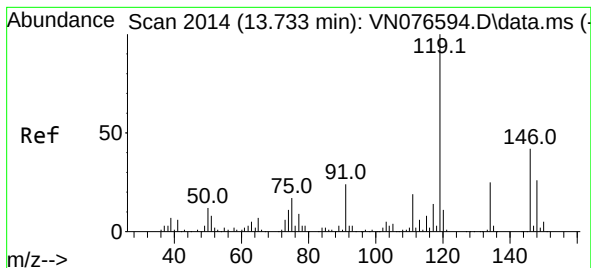

#82

p-Isopropyltoluene

Concen: 0.271 ug/l

RT: 13.733 min Scan# 2014

Delta R.T. 0.004 min

Lab File: VN076614.D

Acq: 10 Feb 2023 17:09

Instrument :

MSVOA_N

ClientSampleId :

001-WILLETS-PT-BLVD(FEB)





Tgt Ion:119 Resp: 3432

Ion Ratio Lower Upper

119 100

134 25.0 0.0 51.4

91 25.1 0.0 46.8

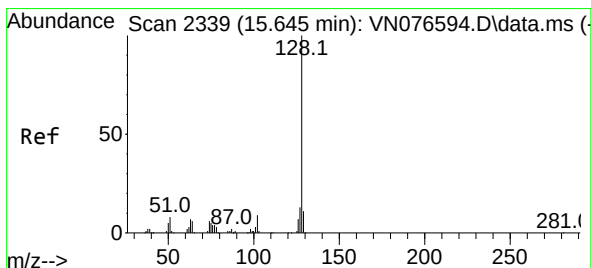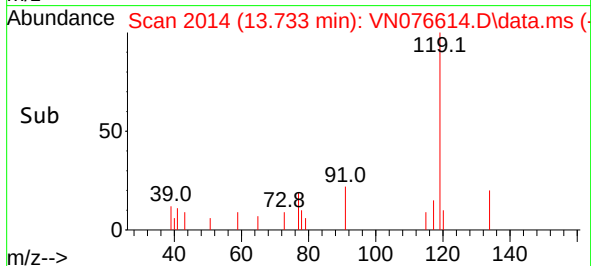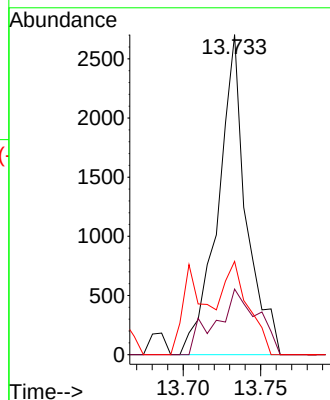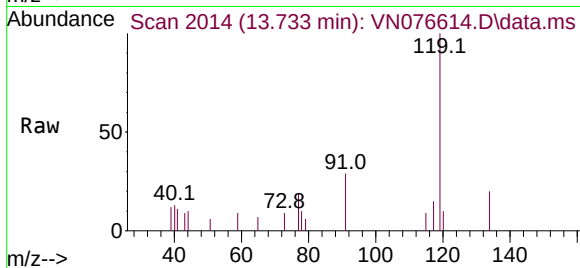

#91

Naphthalene

Concen: 5.793 ug/l

RT: 15.645 min Scan# 2339

Delta R.T. 0.004 min

Lab File: VN076614.D

Acq: 10 Feb 2023 17:09

Tgt Ion:128 Resp: 56497

Ion Ratio Lower Upper

128 100

127 13.6 10.7 16.1

129 10.5 8.9 13.3

