


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021023\  
Data File : VN076600.D  
Acq On : 10 Feb 2023 09:37  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N020923W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Fri Feb 10 05:40:47 2023

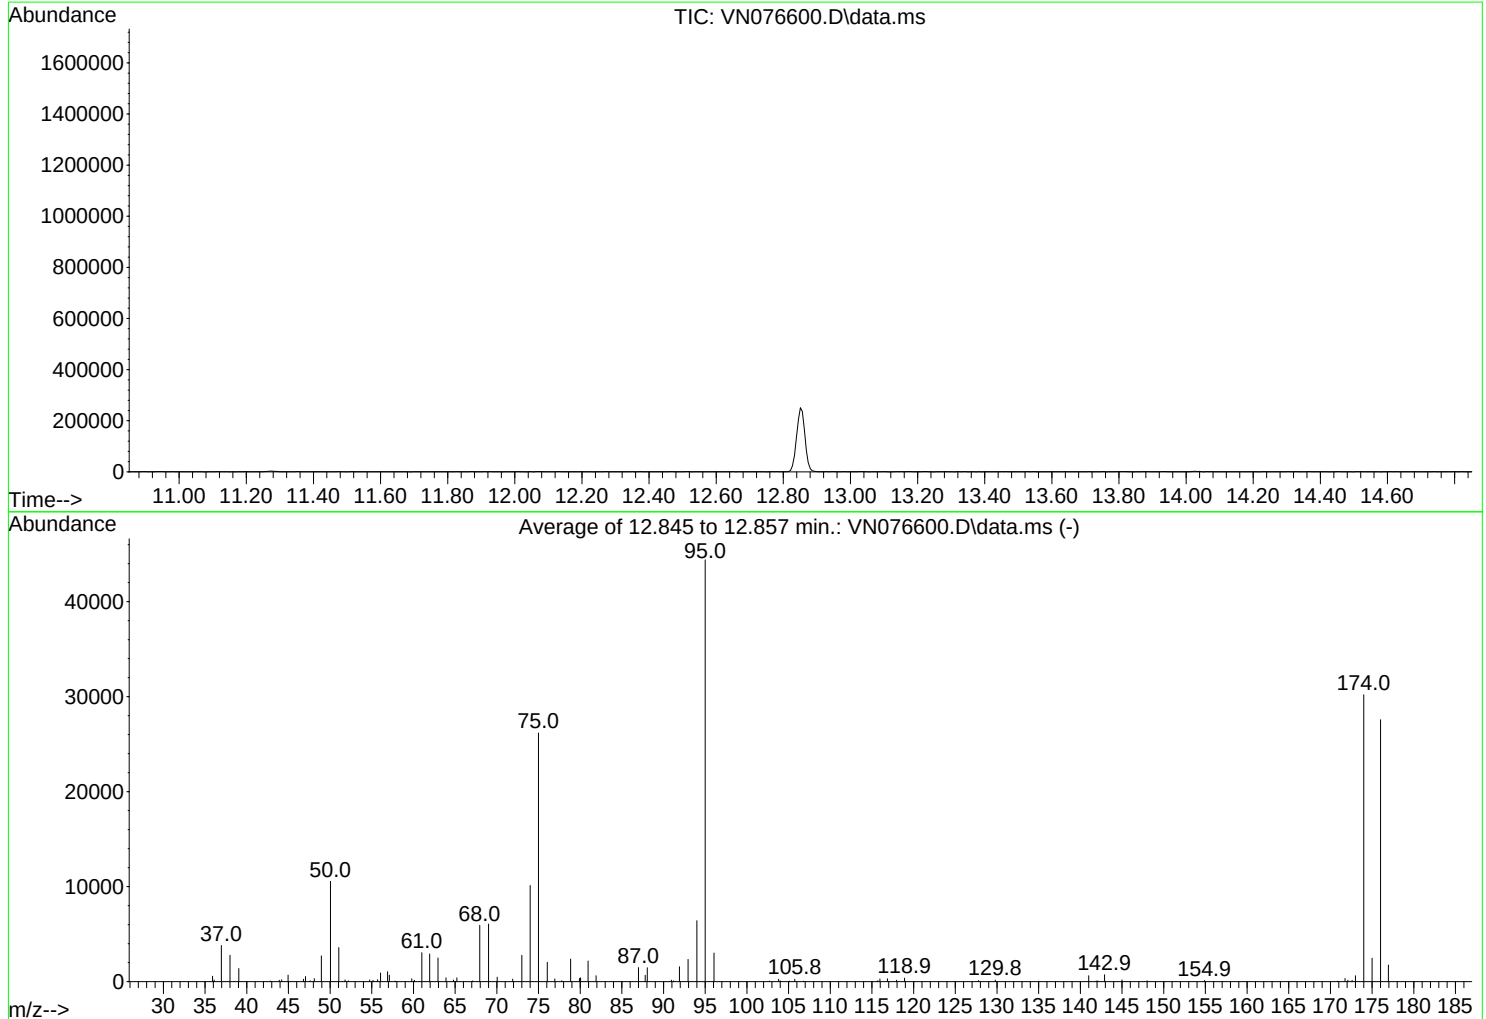

AutoFind: Scans 1863, 1864, 1865; Background Corrected with Scan 1856

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 23.8  | 10555 | PASS      |
| 75     | 95      | 30     | 60     | 58.9  | 26168 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 44400 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 3013  | PASS      |
| 173    | 174     | 0.00   | 2      | 2.0   | 616   | FAIL*     |
| 174    | 95      | 50     | 100    | 68.0  | 30192 | PASS      |
| 175    | 174     | 5      | 9      | 8.2   | 2464  | PASS      |
| 176    | 174     | 95     | 101    | 91.3  | 27565 | FAIL*     |
| 177    | 176     | 5      | 9      | 6.4   | 1754  | PASS      |