

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021025\
 Data File : VN085719.D
 Acq On : 10 Feb 2025 12:48
 Operator : JC\MD
 Sample : VN0210MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0210MBL01

Quant Time: Feb 11 03:19:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 15 02:16:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	221683	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	408756	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	350213	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	139593	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	176505	49.325	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.640%
35) Dibromofluoromethane	8.165	113	144684	51.021	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.040%
50) Toluene-d8	10.565	98	493624	48.993	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.980%
62) 4-Bromofluorobenzene	12.847	95	145081	42.095	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	84.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021025\
Data File : VN085719.D
Acq On : 10 Feb 2025 12:48
Operator : JC\MD
Sample : VN0210MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0210MBL01

Quant Time: Feb 11 03:19:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 02:16:08 2025
Response via : Initial Calibration




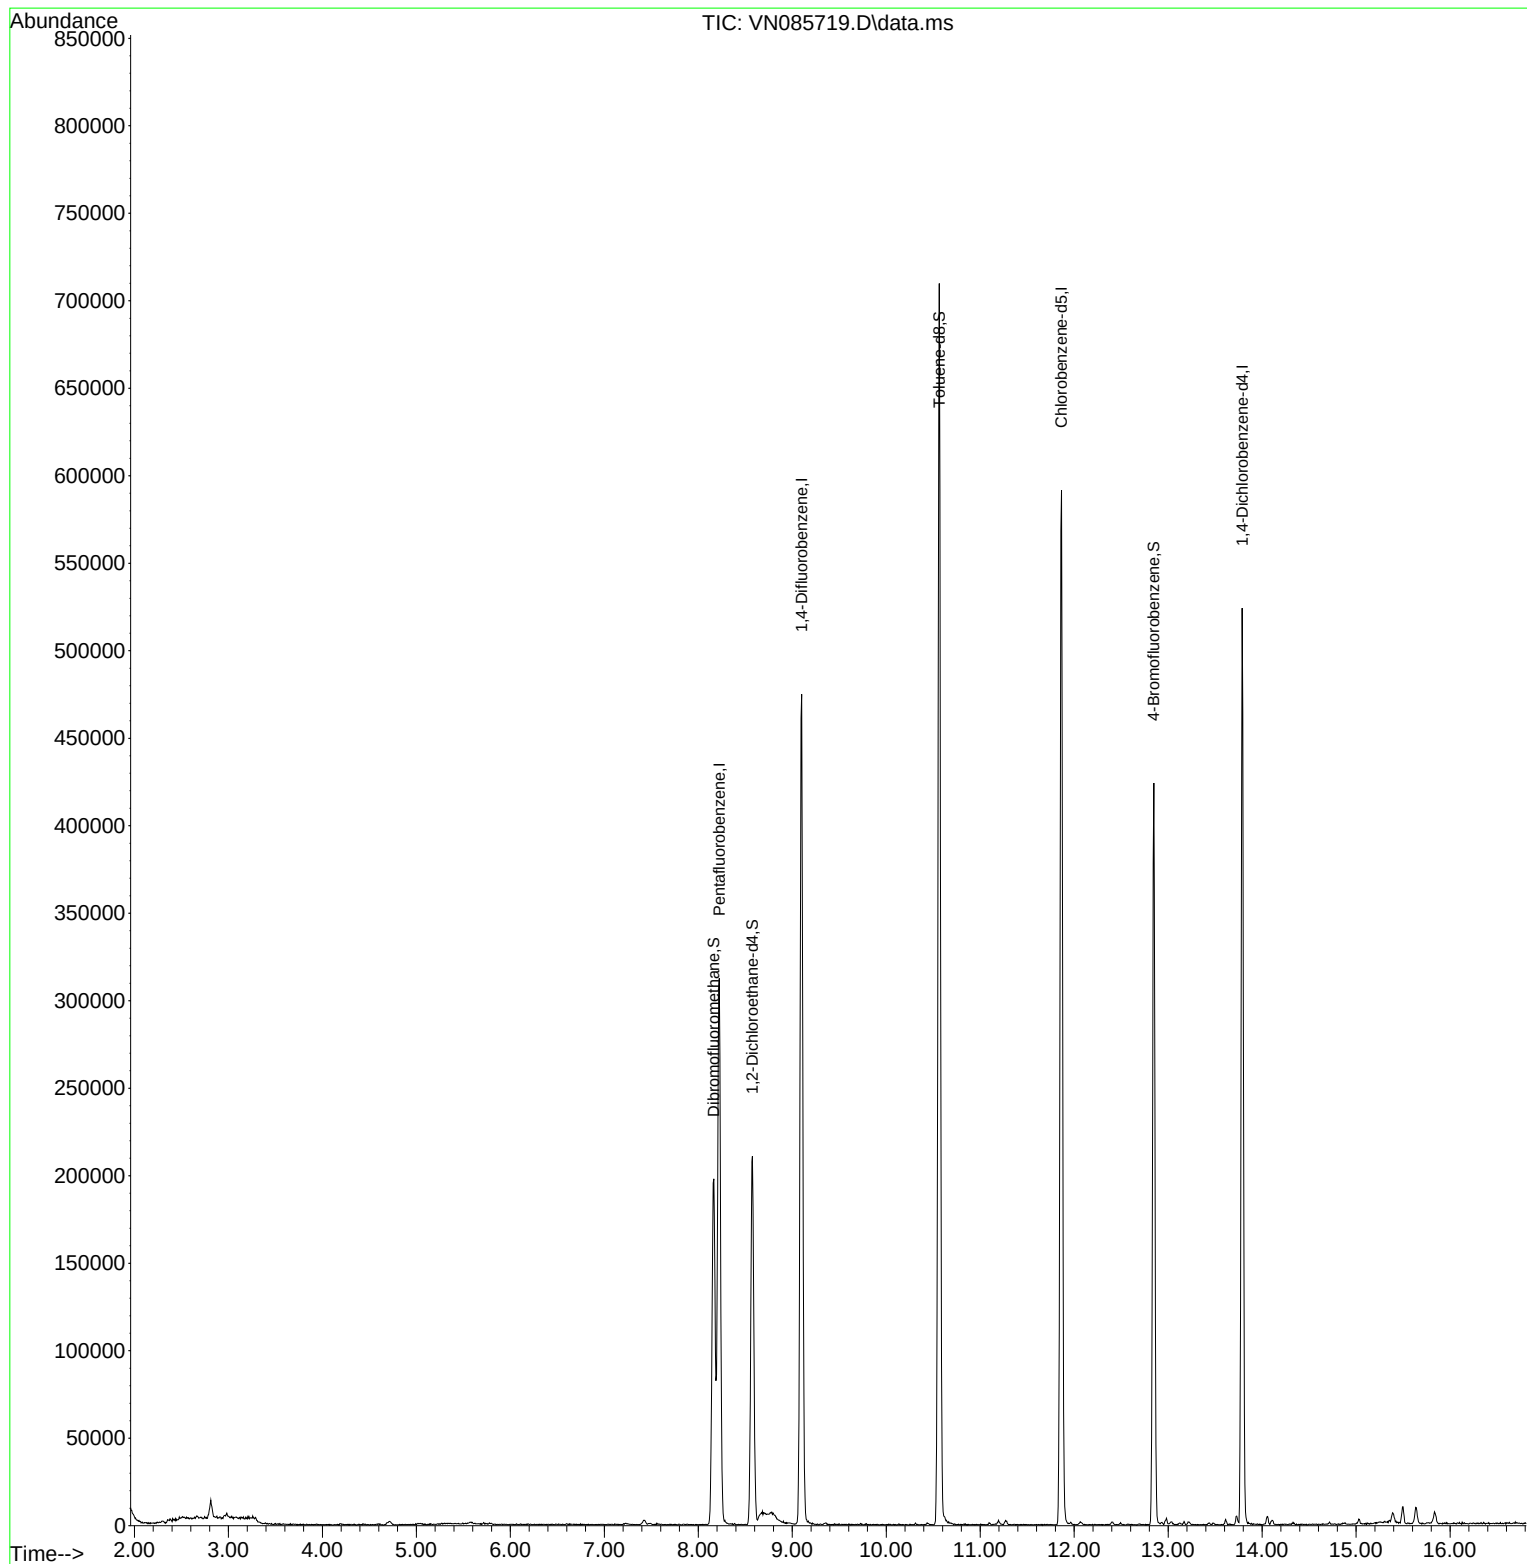


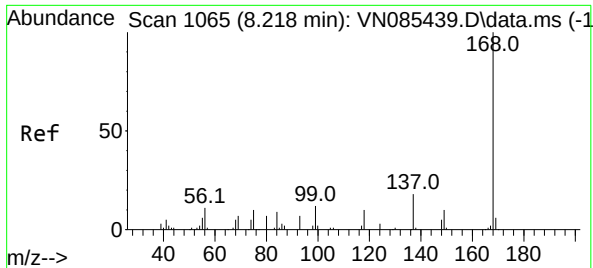

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1106
Delta R.T. 0.006 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48




Instrument :
MSVOA_N
ClientSampleId :
VN0210MBL01


Tgt Ion:168 Resp: 221683
Ion Ratio Lower Upper
168 100
99 61.7 53.6 80.4

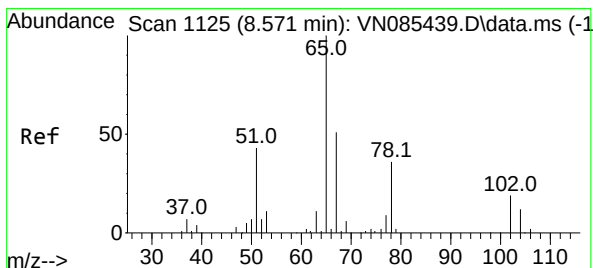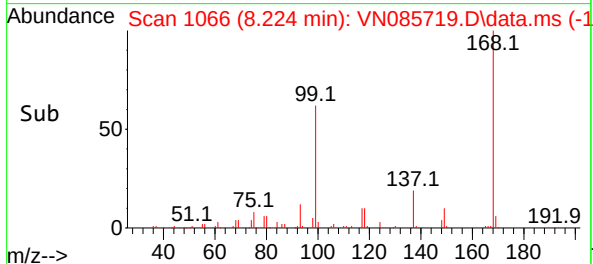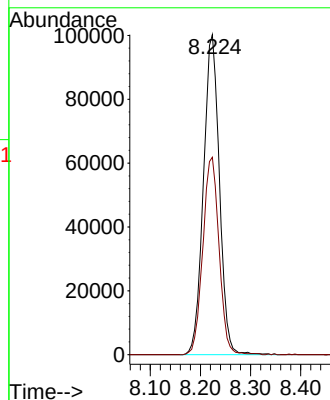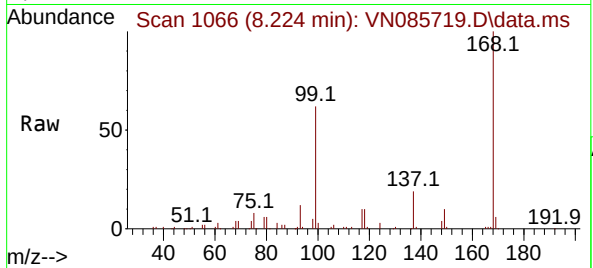

#33
1,2-Dichloroethane-d4
Concen: 49.325 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48

Tgt Ion: 65 Resp: 176505
Ion Ratio Lower Upper
65 100
67 50.9 0.0 101.6

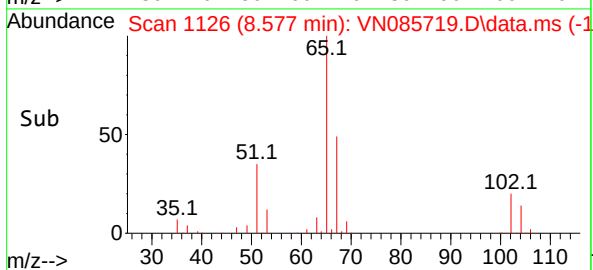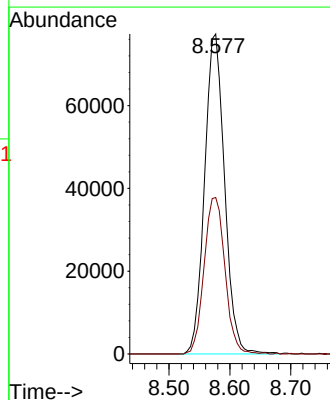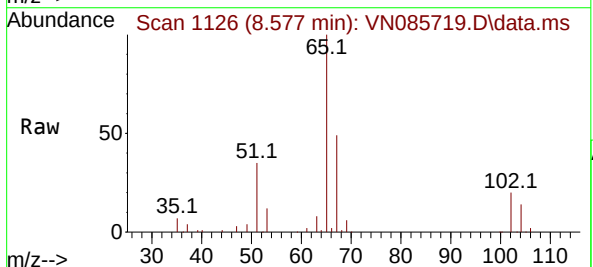

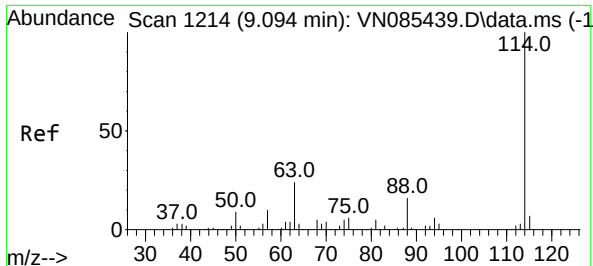

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085719.D

Acq: 10 Feb 2025 12:48

Instrument :

MSVOA_N

ClientSampleId :

VN0210MBL01





Tgt Ion:114 Resp: 408756

Ion Ratio Lower Upper

114 100

63 20.1 0.0 47.6

88 16.2 0.0 32.6

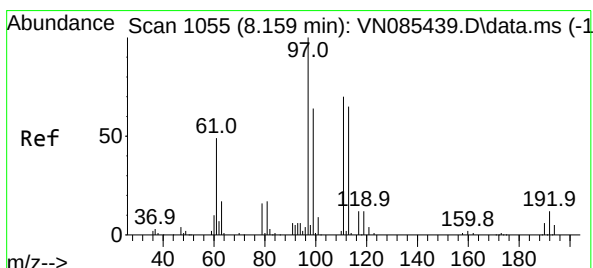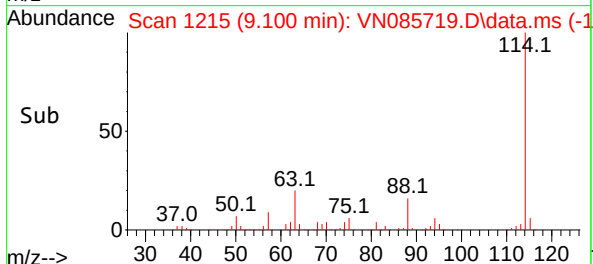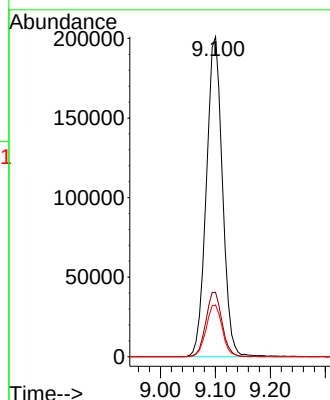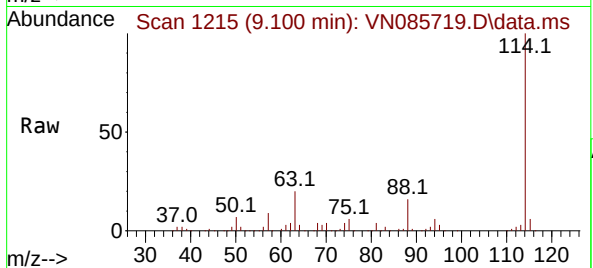

#35

Dibromofluoromethane

Concen: 51.021 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085719.D

Acq: 10 Feb 2025 12:48




Tgt Ion:113 Resp: 144684


Ion Ratio Lower Upper

113 100

111 102.5 82.7 124.1

192 18.3 14.3 21.5


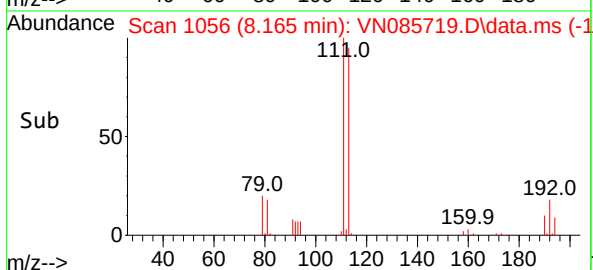
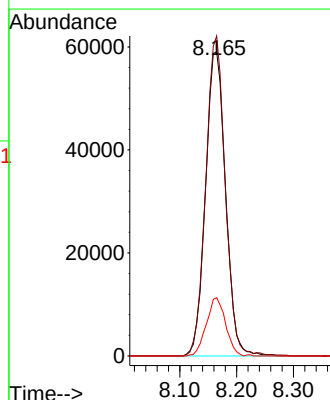
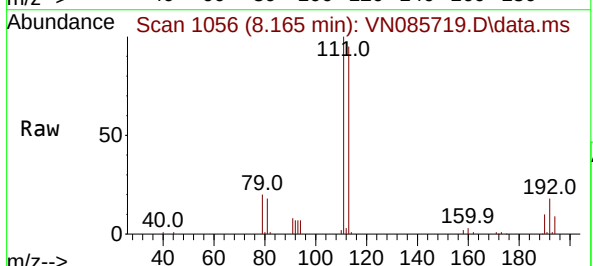


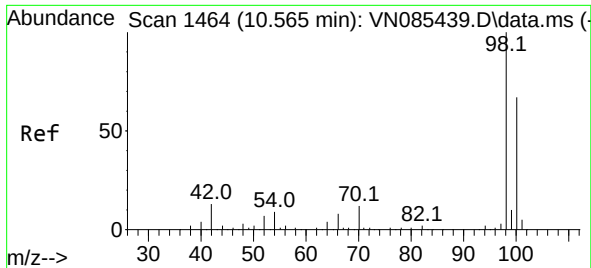

#50
Toluene-d8
Concen: 48.993 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48




Instrument :
MSVOA_N
ClientSampleId :
VN0210MBL01


Tgt Ion: 98 Resp: 493624
Ion Ratio Lower Upper
98 100
100 62.8 52.2 78.4

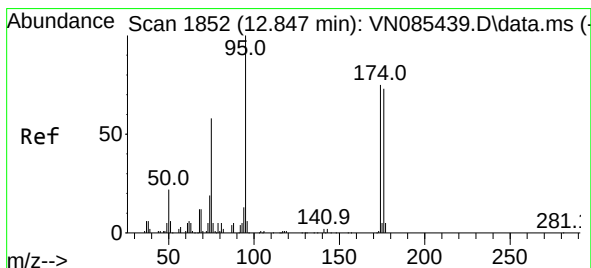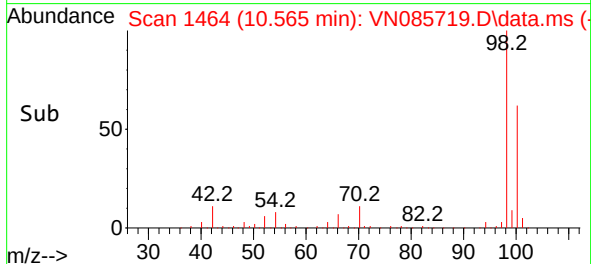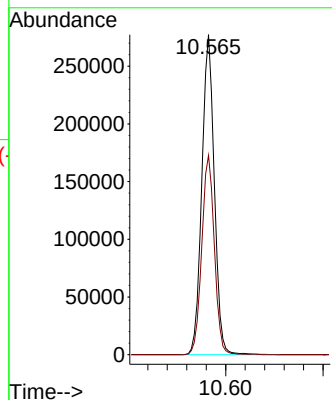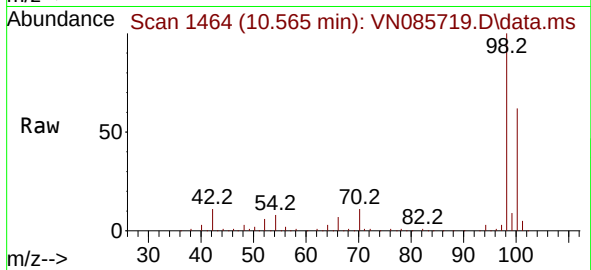

#62
4-Bromofluorobenzene
Concen: 42.095 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48

Tgt Ion: 95 Resp: 145081
Ion Ratio Lower Upper
95 100
174 77.9 0.0 145.0
176 74.0 0.0 142.4


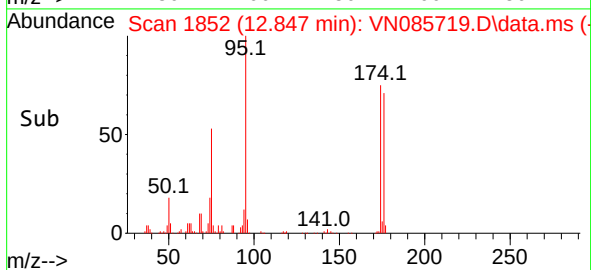
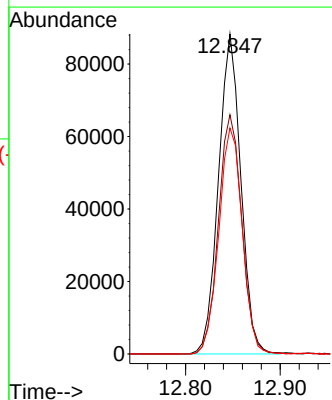
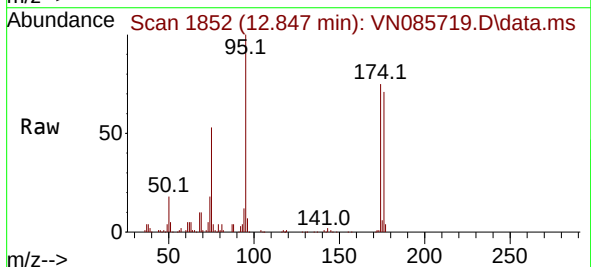


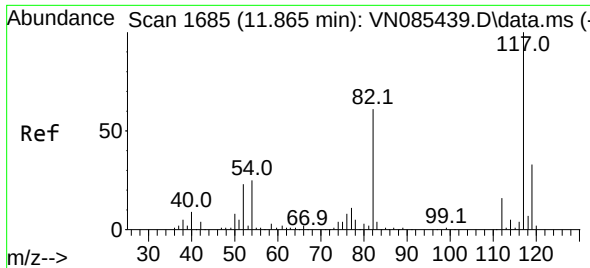

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48

Instrument :
MSVOA_N
ClientSampleId :
VN0210MBL01

Tgt Ion:117 Resp: 350213
Ion Ratio Lower Upper
117 100
82 56.9 48.6 72.8
119 32.2 26.6 39.8

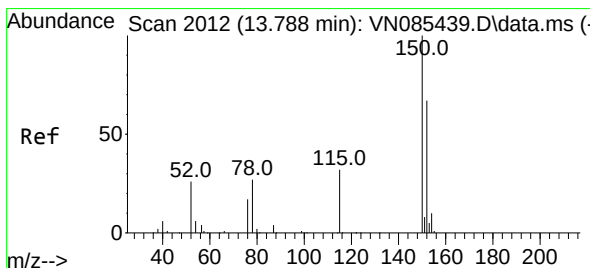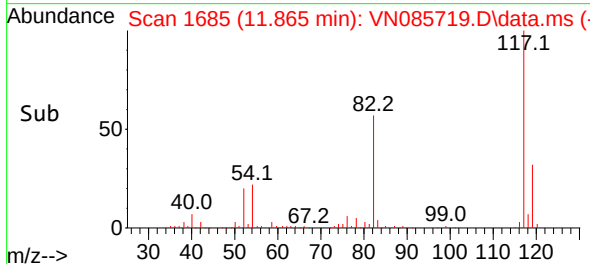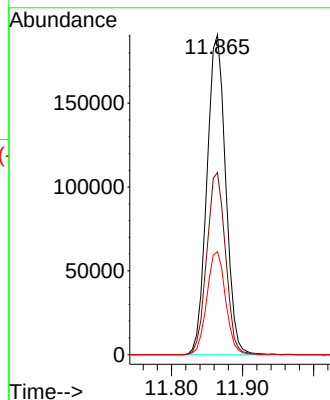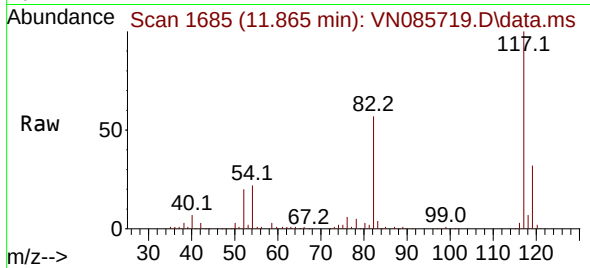

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN085719.D
Acq: 10 Feb 2025 12:48

Tgt Ion:152 Resp: 139593
Ion Ratio Lower Upper
152 100
115 59.3 31.1 93.3
150 157.5 0.0 343.6

