
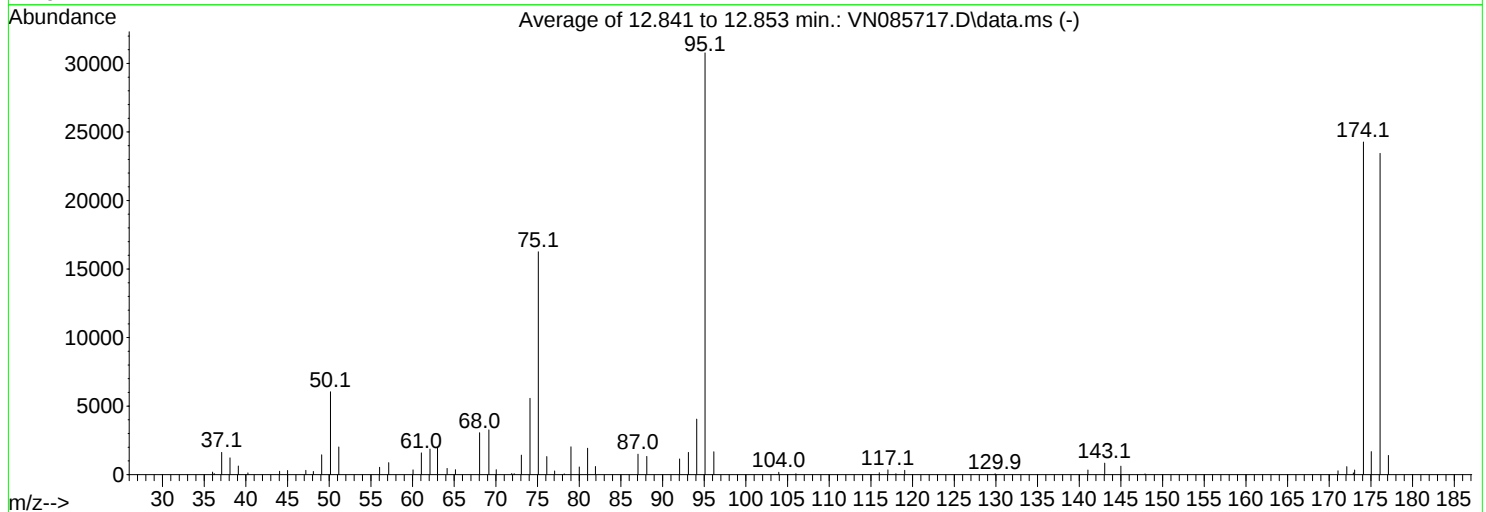


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021025\
Data File : VN085717.D
Acq On : 10 Feb 2025 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

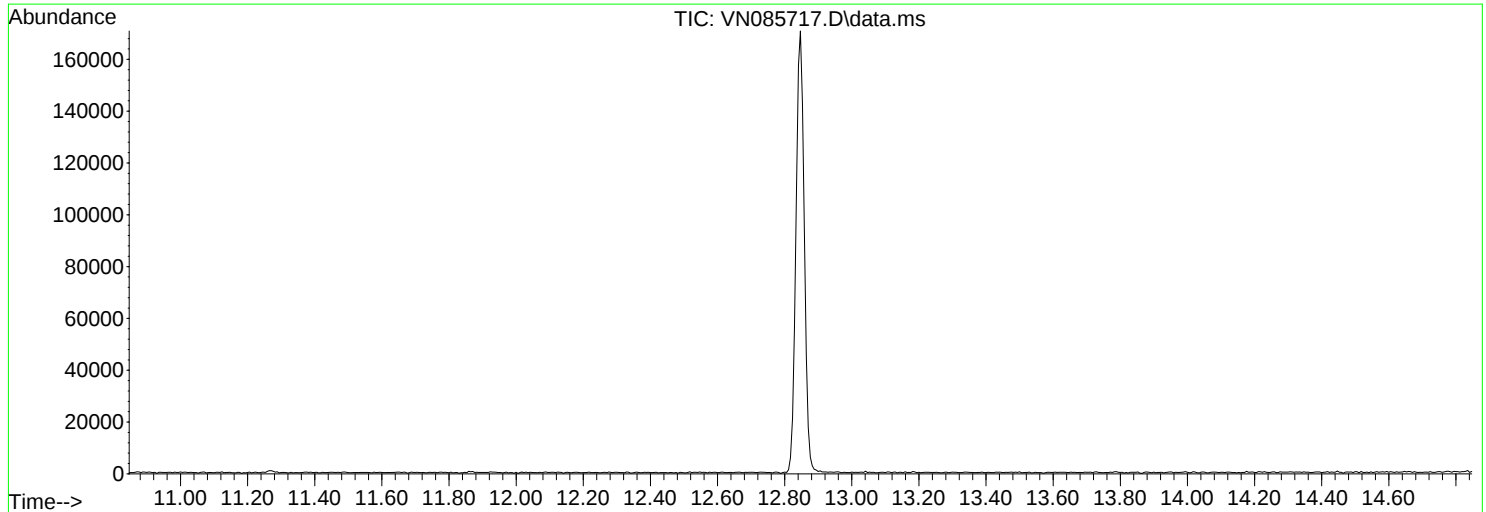

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	6047	PASS
75	95	30	60	52.8	16257	PASS
95	95	100	100	100.0	30773	PASS
96	95	5	9	5.4	1672	PASS
173	174	0.00	2	1.4	340	PASS
174	95	50	100	78.9	24269	PASS
175	174	5	9	6.9	1684	PASS
176	174	95	101	96.6	23435	PASS
177	176	5	9	6.0	1400	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	183	50.15	6047	69.15	3274	80.00	56
36.20	83	51.15	2022	70.05	359	81.00	193
37.10	1627	56.05	539	71.90	77	81.95	59
38.10	1224	57.15	873	72.20	67	87.05	149
39.10	630	60.05	352	73.05	1422	88.10	1333
40.25	123	61.05	1589	74.10	5567	92.05	1140
44.05	242	62.10	1871	75.10	16257	93.10	1625
45.00	308	63.00	1954	76.10	1320	94.10	4056
47.20	314	64.15	455	77.05	266	95.10	30773
48.10	236	65.15	366	78.20	55	96.15	1672
49.10	1449	68.05	3055	79.00	2034	103.95	175

Average of 12.841 to 12.853 min.: VN085717.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
106.00	66	172.10	586				
116.00	135	172.90	127				
117.05	349	173.05	340				
118.00	76	174.10	24269				
119.05	310	175.05	1684				
129.90	67	176.10	23435				
141.05	338	177.10	1400				
143.05	843						
145.00	623						
147.90	55						
171.05	275						

Instrument :

MSVOA_N

ClientSampleId :

BFB