
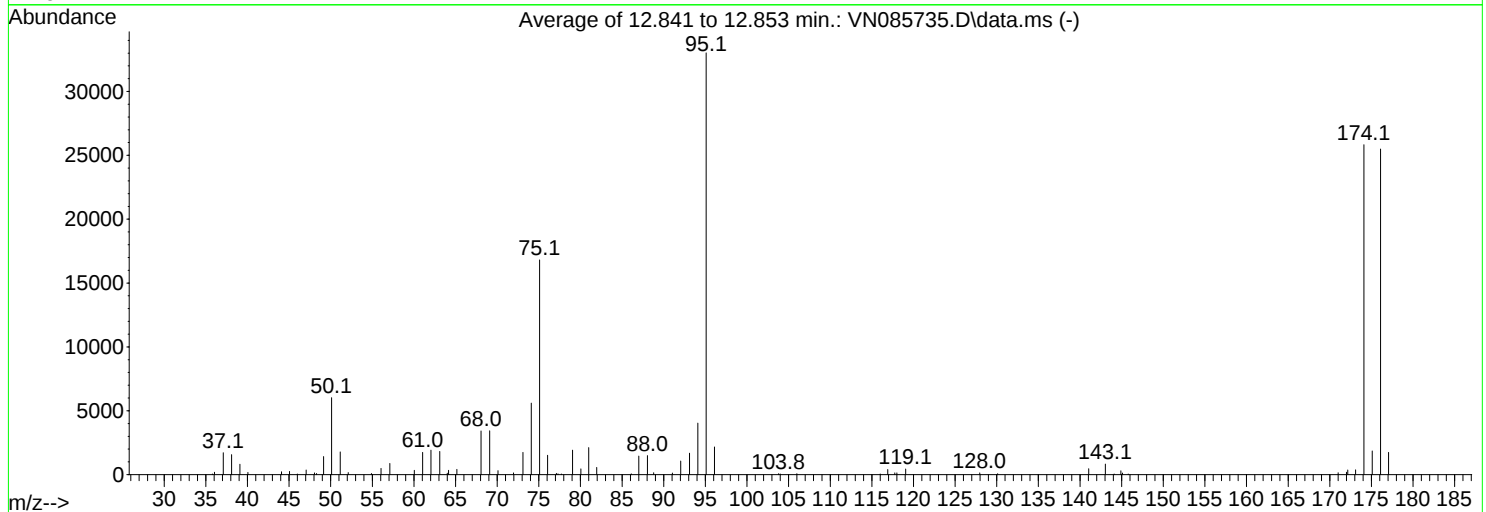


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021125\
Data File : VN085735.D
Acq On : 11 Feb 2025 10:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

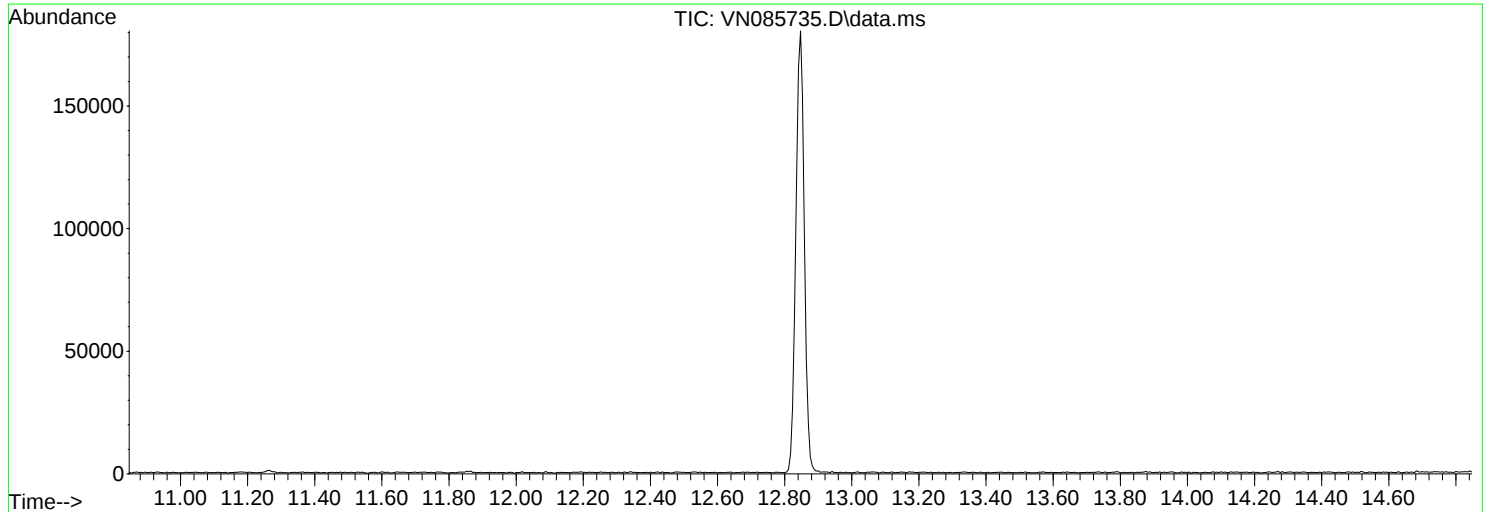

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	6020	PASS
75	95	30	60	50.9	16814	PASS
95	95	100	100	100.0	33024	PASS
96	95	5	9	6.6	2173	PASS
173	174	0.00	2	1.5	379	PASS
174	95	50	100	78.2	25837	PASS
175	174	5	9	7.2	1857	PASS
176	174	95	101	98.7	25491	PASS
177	176	5	9	6.8	1736	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	55	48.30	84	63.10	1820	76.05	1511
36.05	192	49.15	1413	64.00	113	77.10	104
37.10	1720	50.10	6020	64.15	340	77.30	6
38.10	1564	51.15	1779	65.15	414	77.70	5
39.10	820	52.10	169	68.05	3427	79.05	1923
40.05	177	54.90	92	69.10	3428	80.05	446
44.10	229	56.05	488	70.10	308	81.00	2115
45.05	247	57.10	878	71.95	132	81.95	564
46.00	56	60.05	342	73.10	1743	86.10	68
47.05	359	61.05	1747	74.10	5601	87.00	1454
48.05	141	62.05	1920	75.10	16814	88.05	1495

Average of 12.841 to 12.853 min.: VN085735.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.80	149	116.90	402	145.80	51		
91.05	130	117.75	145	171.00	151		
92.05	1065	118.00	141	172.00	188		
93.10	1679	119.05	438	172.15	369		
94.10	4036	127.95	141	173.10	379		
95.10	33024	130.10	70	174.10	25837		
96.10	2173	141.05	466	175.10	1857		
103.80	77	143.05	833	176.10	25491		
104.00	55	144.10	52	177.05	1736		
106.00	77	144.90	301				
116.00	55	145.10	122				

Instrument :

MSVOA_N

ClientSampleId :

BFB