


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021219\
Data File : VN053719.D
Acq On : 12 Feb 2019 9:44
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

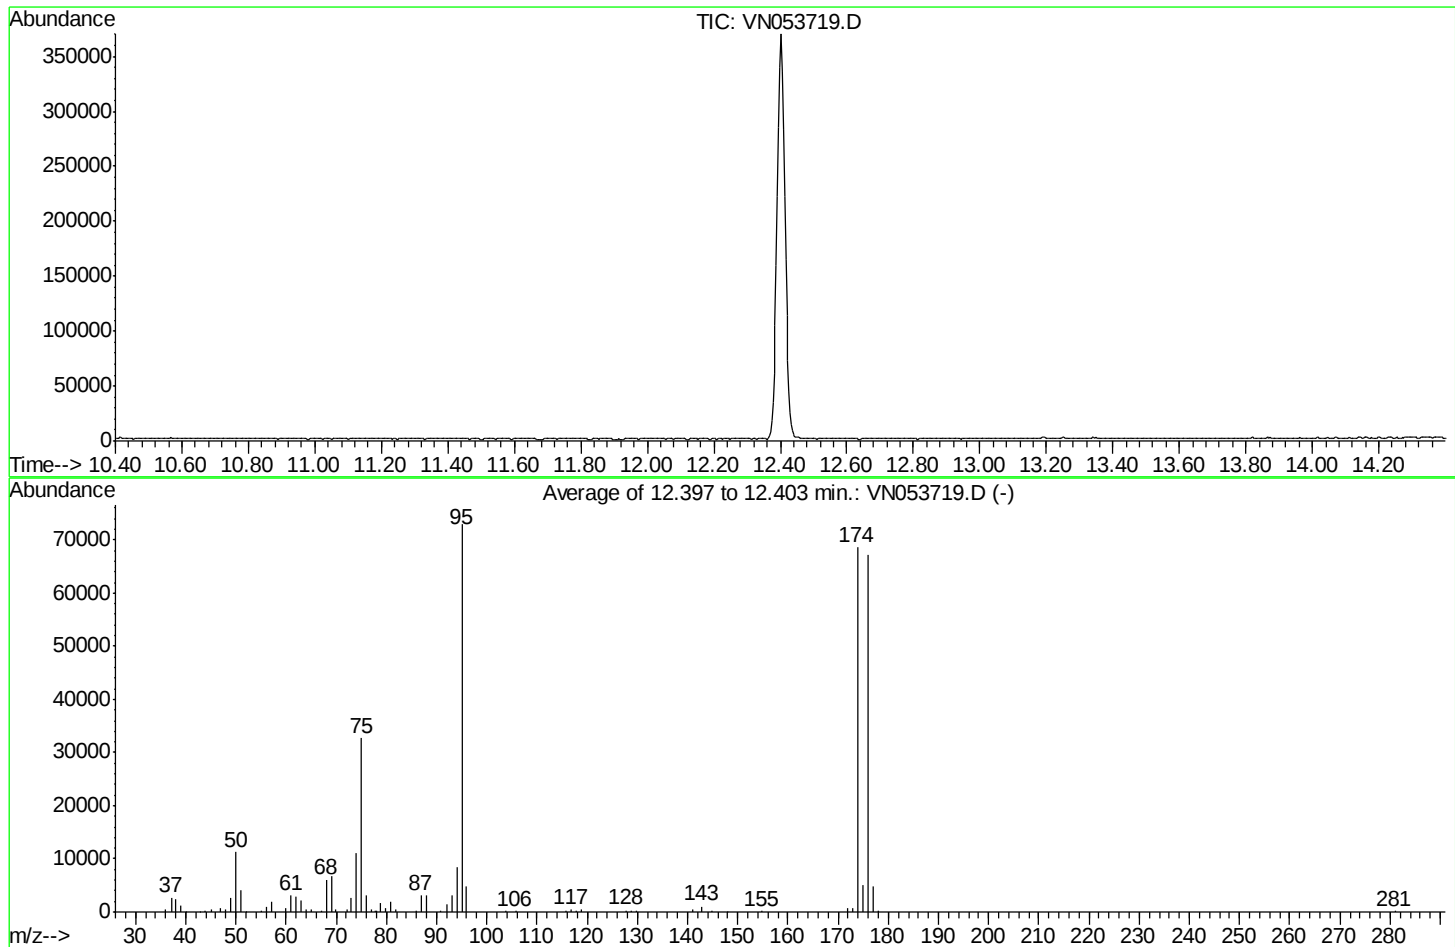

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	11222	PASS
75	95	30	60	44.9	32709	PASS
95	95	100	100	100.0	72917	PASS
96	95	5	9	6.6	4825	PASS
173	174	0.00	2	0.9	638	PASS
174	95	50	100	94.0	68517	PASS
175	174	5	9	7.3	4999	PASS
176	174	95	101	98.0	67136	PASS
177	176	5	9	7.2	4817	PASS