

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
 Data File : VN065838.D
 Acq On : 12 Feb 2021 15:04
 Operator : JC/MD
 Sample : M1341-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 13 00:48:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.624	168	127376	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	246387	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	251786	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	103183	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	78059	46.58	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.16%		
35) Dibromofluoromethane	7.547	113	70694	48.42	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	96.84%		
50) Toluene-d8	10.058	98	318201	55.44	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	110.88%		
62) 4-Bromofluorobenzene	12.373	95	121805	58.94	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	117.88%		
Target Compounds						
					Qvalue	
5) Bromomethane	2.544	94	260	0.21	ug/l #	74
11) Tert butyl alcohol	4.766	59	514	1.64	ug/l #	73
13) Acrolein	3.560	56	292	19.09	ug/l #	75
16) Acetone	3.782	43	13349	20.46	ug/l	93
17) Carbon Disulfide	4.000	76	3756	0.77	ug/l	96
20) Methylene Chloride	4.499	84	1842	1.02	ug/l	94
25) 2-Butanone	6.804	43	5943	5.81	ug/l	91
31) Cyclohexane	7.624	56	2321	0.74	ug/l #	1
36) 1,1-Dichloropropene	7.618	75	8926	3.60	ug/l #	48
37) Ethyl Acetate	6.804	43	5943	2.50	ug/l #	68
38) Carbon Tetrachloride	7.624	117	11842	5.80	ug/l #	17
48) Methyl methacrylate	9.135	41	962	0.48	ug/l #	28
51) 4-Methyl-2-Pentanone	9.955	43	1686	0.73	ug/l	99
59) 2-Hexanone	10.727	43	2431	1.51	ug/l	90
65) Chlorobenzene	11.405	112	5347	1.02	ug/l	99
68) m/p-Xylenes	11.592	106	1132	0.32	ug/l	82
74) N-amyl acetate	12.003	43	2170	0.57	ug/l #	42
76) 1,2,3-Trichloropropane	12.370	75	54954	20.37	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.370	75	54954	52.17	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.013	105	3293	0.43	ug/l	97
86) p-Isopropyltoluene	13.260	119	1894	0.25	ug/l	92
87) 1,3-Dichlorobenzene	13.257	146	1587	0.46	ug/l	92
88) 1,4-Dichlorobenzene	13.257	146	1587	0.45	ug/l	92
89) n-Butylbenzene	13.585	91	2285	0.33	ug/l	84
90) Hexachloroethane	13.965	117	316	0.24	ug/l #	12
91) 1,2-Dichlorobenzene	13.627	146	1062	0.31	ug/l	89
93) 1,2,4-Trichlorobenzene	14.881	180	1870	4.20	ug/l	98
94) Hexachlorobutadiene	14.981	225	599	0.91	ug/l	89
95) Naphthalene	15.100	128	11587	5.07	ug/l #	85
96) 1,2,3-Trichlorobenzene	15.280	180	2126	3.82	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
Data File : VN065838.D
Acq On : 12 Feb 2021 15:04
Operator : JC/MD
Sample : M1341-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 13 00:48:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration




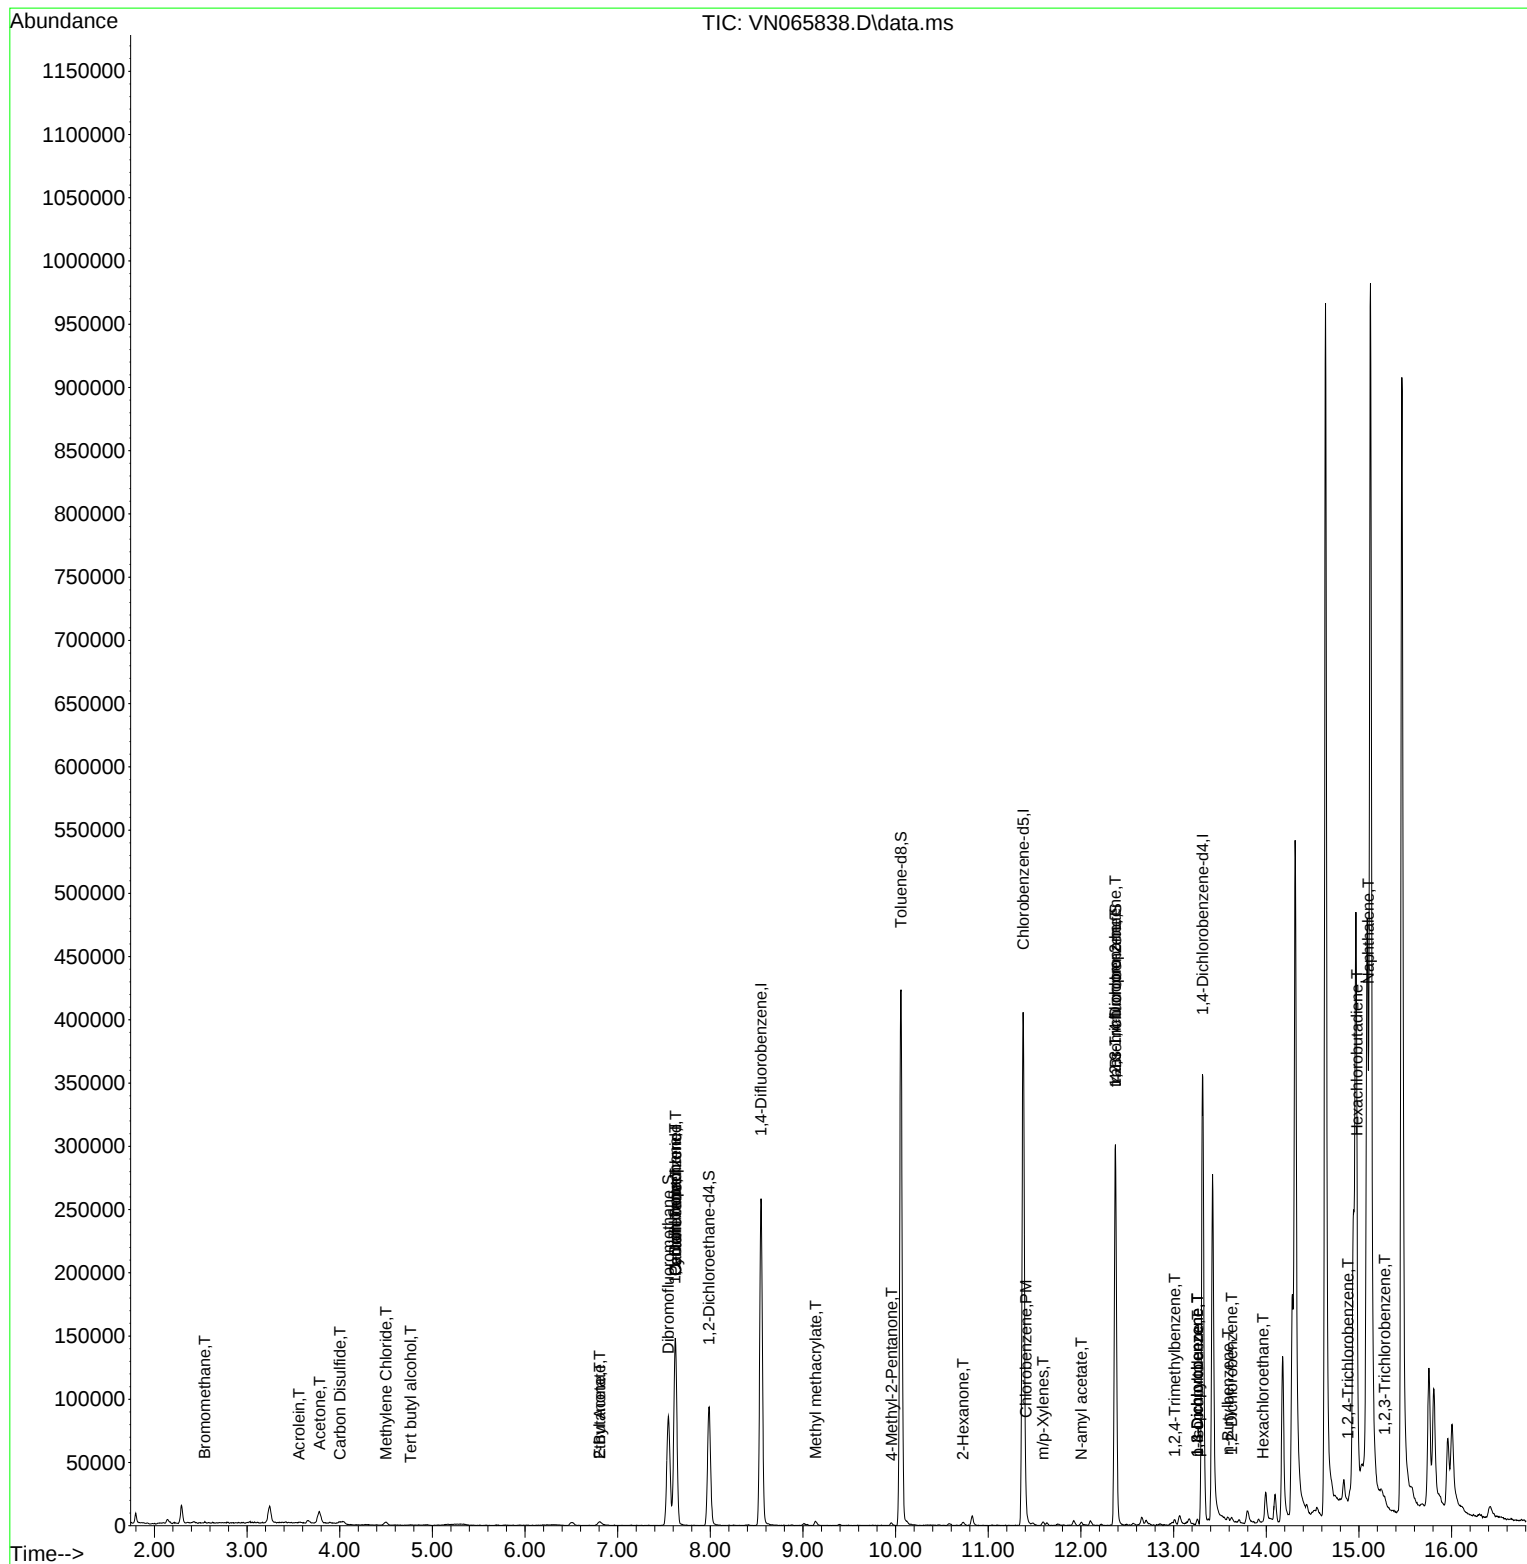




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 127376
Ion Ratio Lower Upper
168 100
99 56.6 42.6 63.8

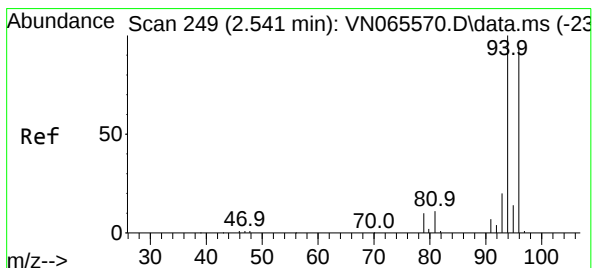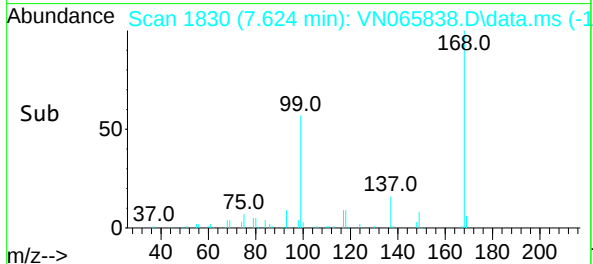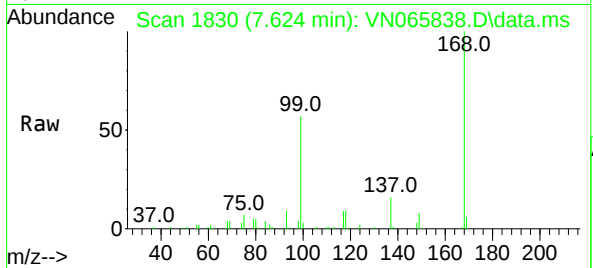

#5
Bromomethane
Concen: 0.21 ug/l
RT: 2.544 min Scan# 250
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion: 94 Resp: 260
Ion Ratio Lower Upper
94 100
96 66.8 73.0 109.4#

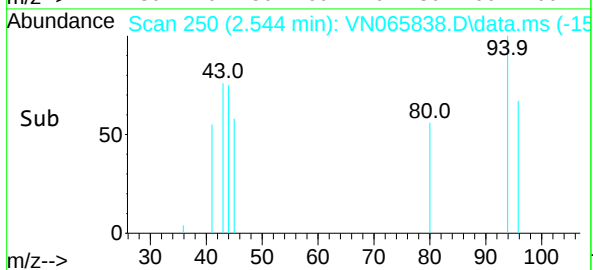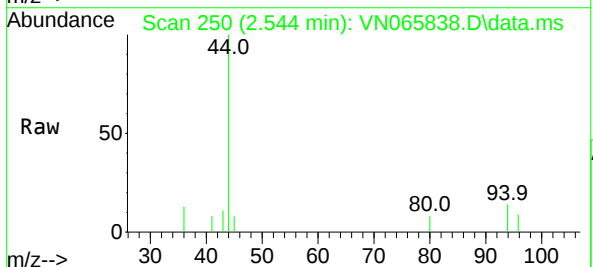






#11
Tert butyl alcohol
Concen: 1.64 ug/l
RT: 4.766 min Scan# 941
Delta R.T. 0.004 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampled :



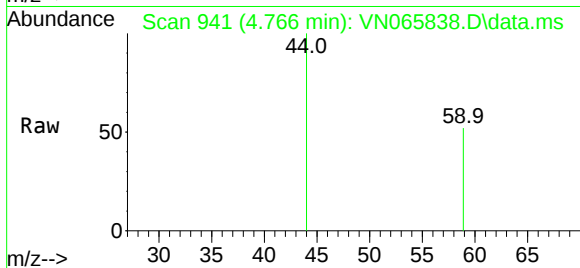



Tgt Ion: 59 Resp: 514
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#



#13
Acrolein
Concen: 19.09 ug/l
RT: 3.560 min Scan# 566
Delta R.T. -0.009 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion: 56 Resp: 292
Ion Ratio Lower Upper
56 100
55 90.8 56.0 84.0#

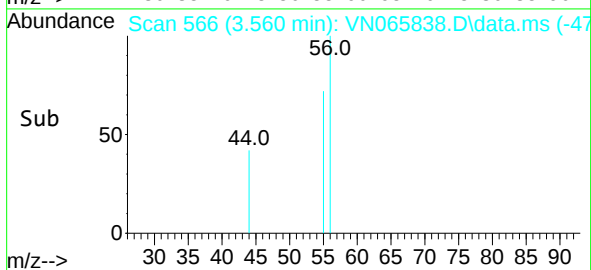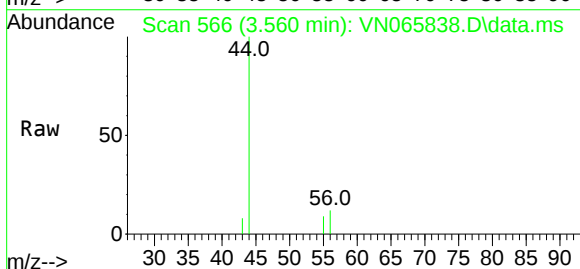






#16
Acetone
Concen: 20.46 ug/l
RT: 3.782 min Scan# 635
Delta R.T. -0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 43 Resp: 13349
Ion Ratio Lower Upper
43 100
58 38.0 27.0 40.6




#17
Carbon Disulfide
Concen: 0.77 ug/l
RT: 4.000 min Scan# 703
Delta R.T. -0.007 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Tgt Ion: 76 Resp: 3756
Ion Ratio Lower Upper
76 100
78 11.2 7.8 11.6

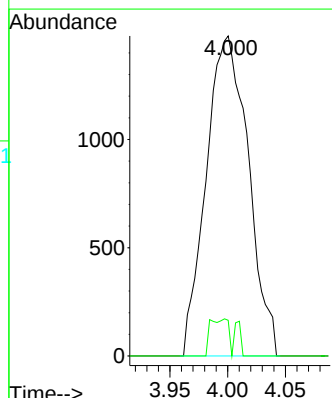






#20
Methylene Chloride
Concen: 1.02 ug/l
RT: 4.499 min Scan# 858
Delta R.T. -0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:	84	Resp:	1842
Ion	Ratio	Lower	Upper
84	100		
49	110.1	94.6	141.8
51	36.1	29.9	44.9
86	61.0	51.4	77.2

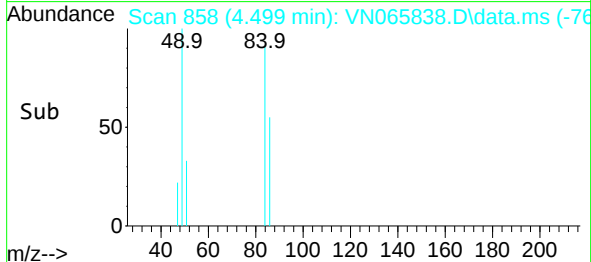

#25
2-Butanone
Concen: 5.81 ug/l
RT: 6.804 min Scan# 1575
Delta R.T. 0.013 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion:	43	Resp:	5943
Ion	Ratio	Lower	Upper
43	100		
72	24.3	23.1	34.7

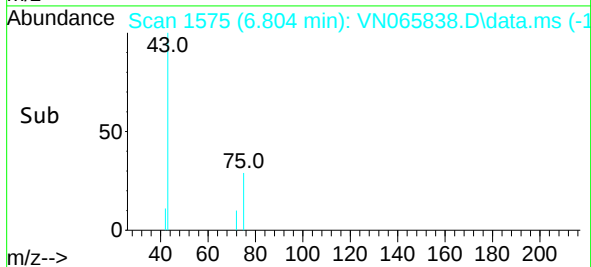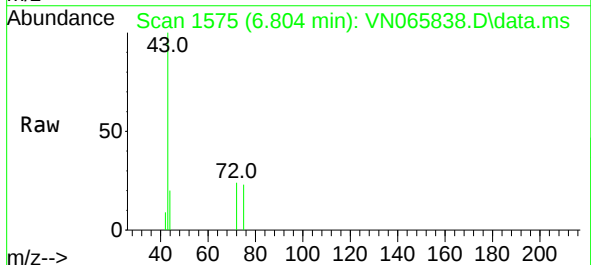



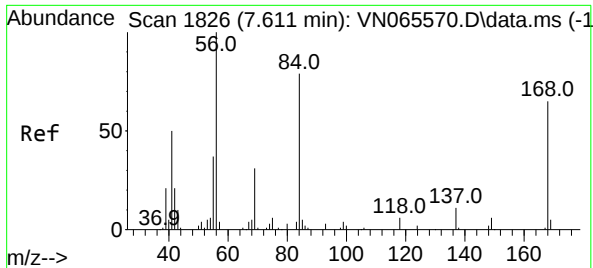


#31
Cyclohexane
Concen: 0.74 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.013 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampled :



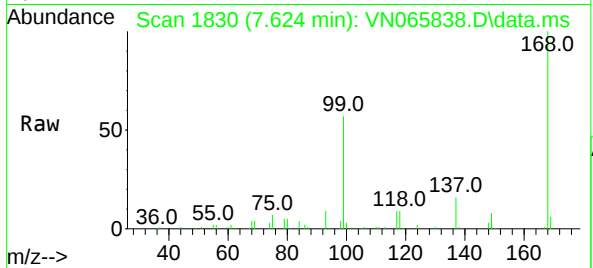



Tgt Ion: 56 Resp: 2321
Ion Ratio Lower Upper
56 100
69 206.9 26.6 39.8#
84 192.8 70.4 105.6#

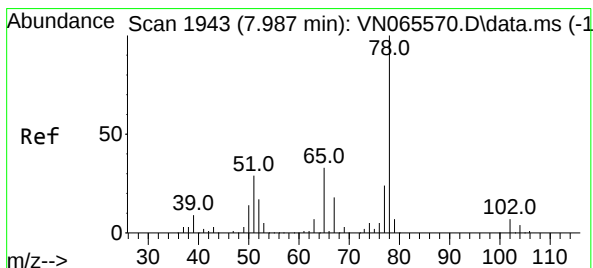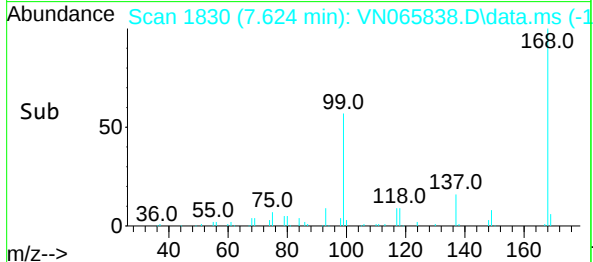

#33
1,2-Dichloroethane-d4
Concen: 46.58 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion: 65 Resp: 78059
Ion Ratio Lower Upper
65 100
67 56.6 0.0 107.2


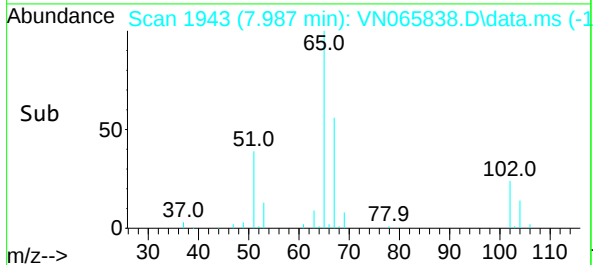

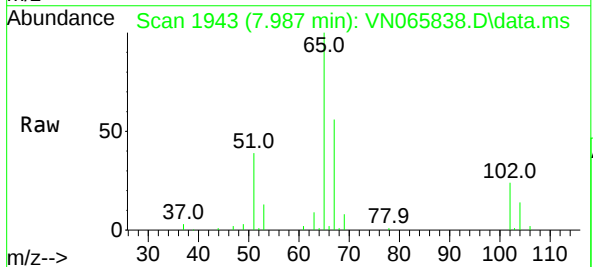




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:	114	Resp:	246387
Ion Ratio	Lower	Upper	
114	100		
63	19.8	0.0	38.6
88	16.4	0.0	30.6

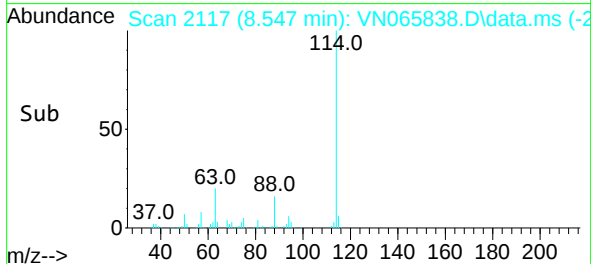

#35
Dibromofluoromethane
Concen: 48.42 ug/l
RT: 7.547 min Scan# 1806
Delta R.T. -0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:	113	Resp:	70694
Ion Ratio	Lower	Upper	
113	100		
111	103.7	82.2	123.2
192	18.2	15.4	23.0


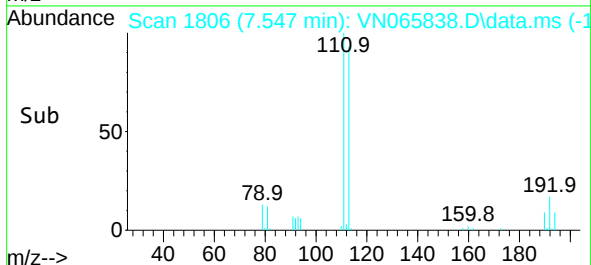

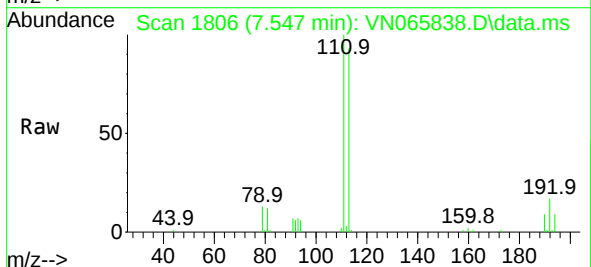


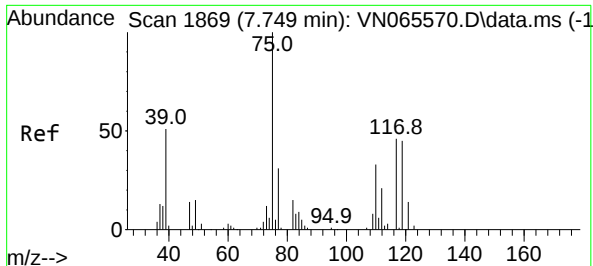

#36
1,1-Dichloropropene
Concen: 3.60 ug/l
RT: 7.618 min Scan# 1828
Delta R.T. -0.131 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 8926
Ion Ratio Lower Upper
75 100
110 7.9 18.2 54.6#
77 0.0 24.9 37.3#

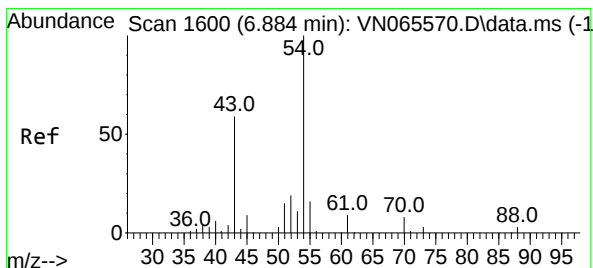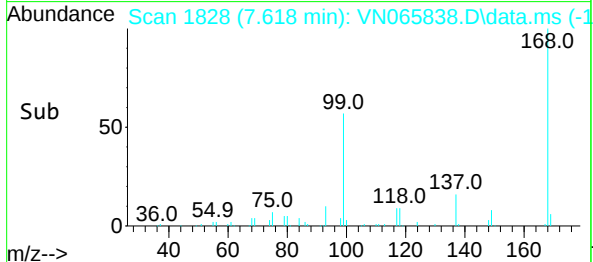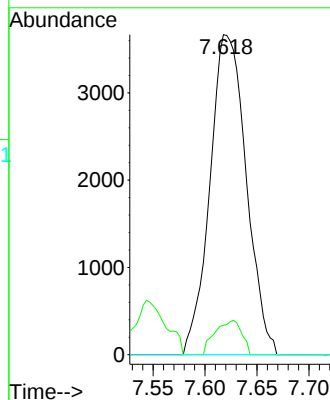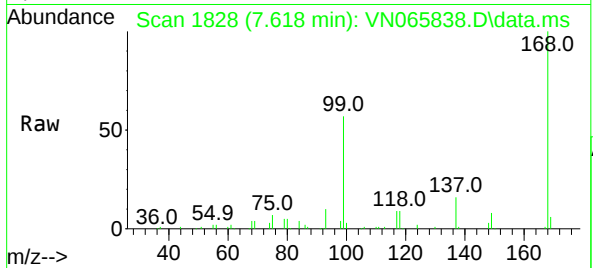

#37
Ethyl Acetate
Concen: 2.50 ug/l
RT: 6.804 min Scan# 1575
Delta R.T. -0.080 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion: 43 Resp: 5943
Ion Ratio Lower Upper
43 100
61 0.0 11.6 17.4#
70 0.0 8.6 13.0#

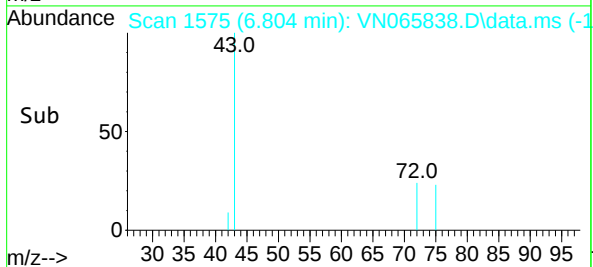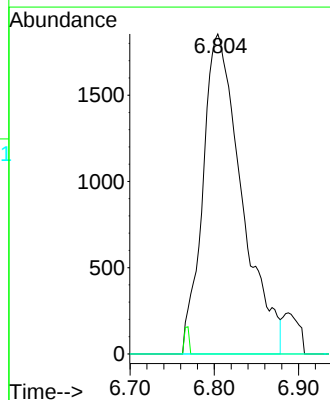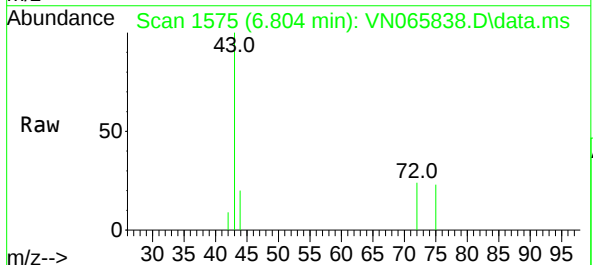



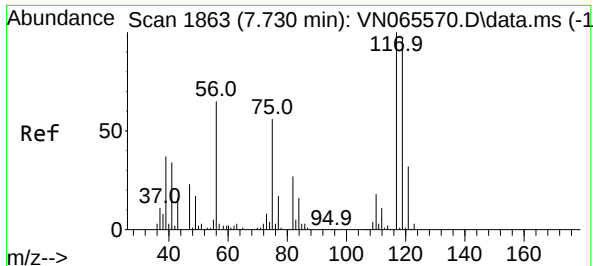


#38
Carbon Tetrachloride
Concen: 5.80 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.106 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampleId :



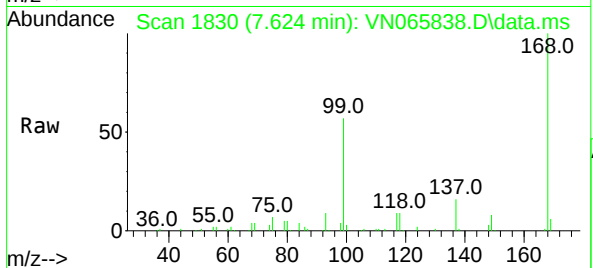



Tgt Ion:117 Resp: 11842
Ion Ratio Lower Upper
117 100
119 5.3 76.0 114.0#
121 0.0 24.5 36.7#

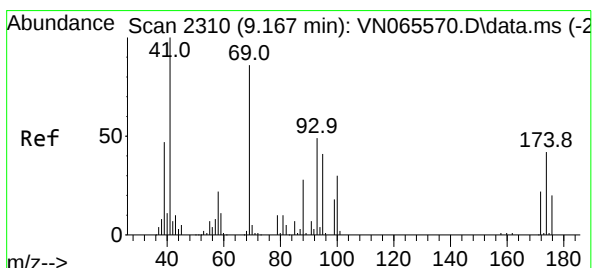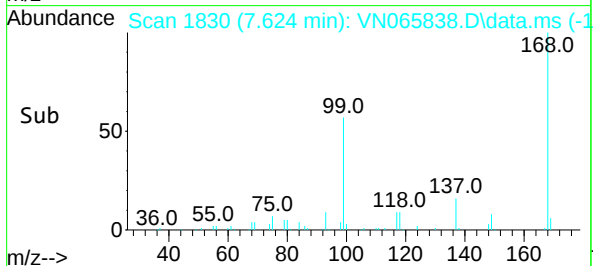

#48
Methyl methacrylate
Concen: 0.48 ug/l
RT: 9.135 min Scan# 2300
Delta R.T. -0.032 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion: 41 Resp: 962
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 36.8 46.6 69.8#


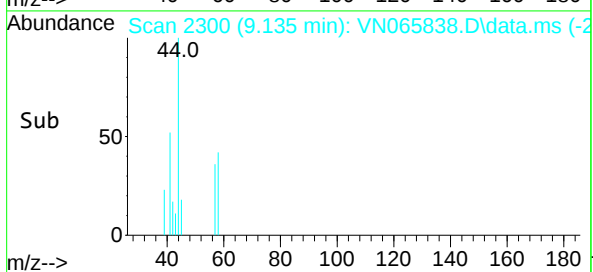

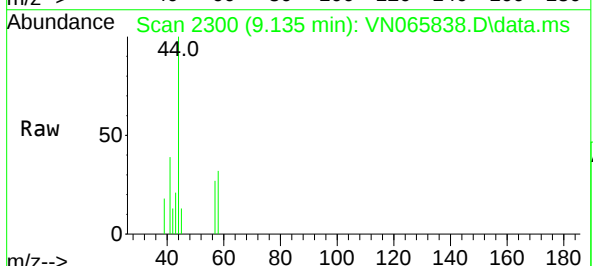




#50
Toluene-d8
Concen: 55.44 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 318201
Ion Ratio Lower Upper
98 100
100 64.1 50.5 75.7

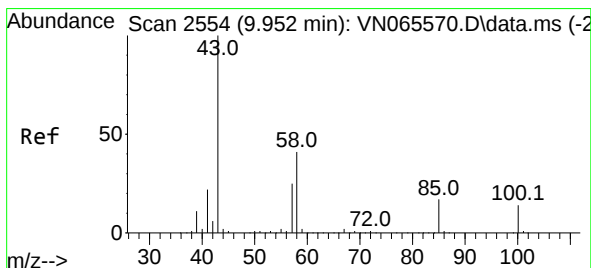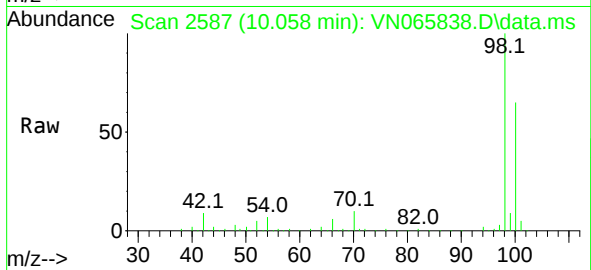

#51
4-Methyl-2-Pentanone
Concen: 0.73 ug/l
RT: 9.955 min Scan# 2555
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion: 43 Resp: 1686
Ion Ratio Lower Upper
43 100
58 41.3 32.5 48.7


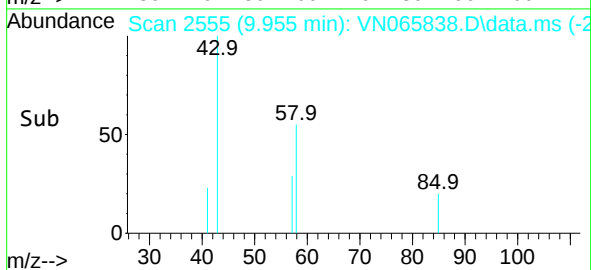

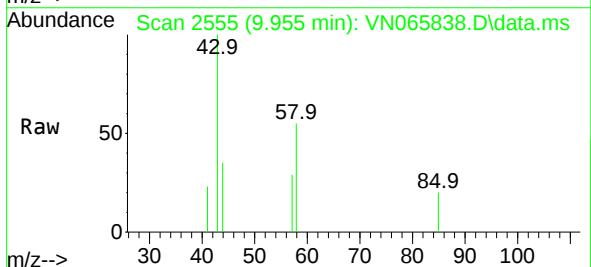




#59
2-Hexanone
Concen: 1.51 ug/l
RT: 10.727 min Scan# 2795
Delta R.T. 0.007 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2431
Ion Ratio Lower Upper
43 100
58 49.1 28.1 84.3

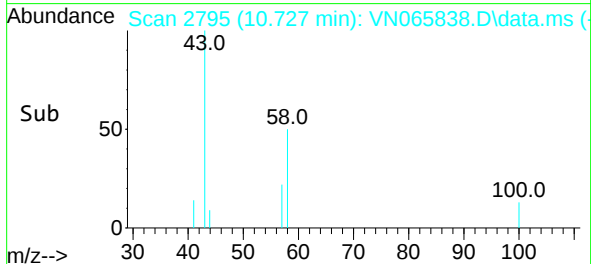

#62
4-Bromofluorobenzene
Concen: 58.94 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion: 95 Resp: 121805
Ion Ratio Lower Upper
95 100
174 71.8 0.0 169.0
176 70.2 0.0 162.4



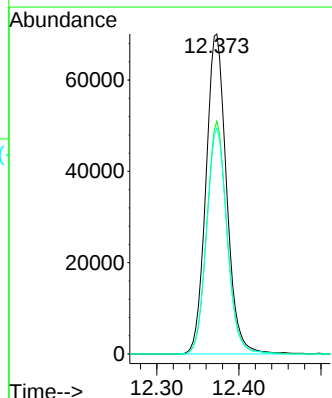
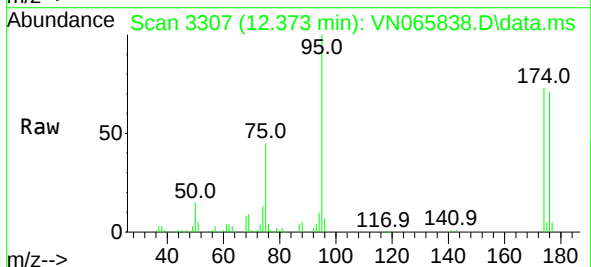




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 251786
Ion Ratio Lower Upper
117 100
82 57.9 43.7 65.5
119 31.9 26.1 39.1

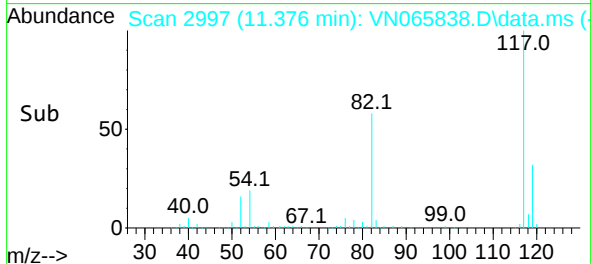

#65
Chlorobenzene
Concen: 1.02 ug/l
RT: 11.405 min Scan# 3006
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:112 Resp: 5347
Ion Ratio Lower Upper
112 100
114 33.2 26.1 39.1


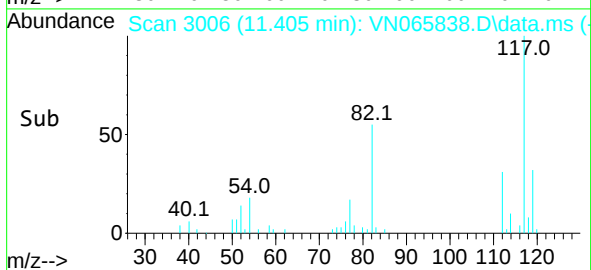

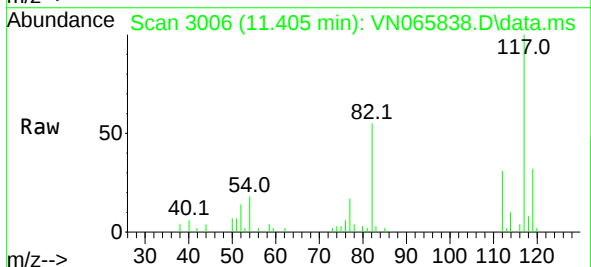


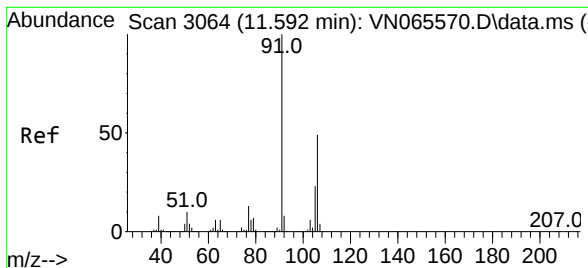

#68
m/p-Xylenes
Concen: 0.32 ug/l
RT: 11.592 min Scan# 3064
Delta R.T. -0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 1132
Ion Ratio Lower Upper
106 100
91 228.7 161.4 242.0

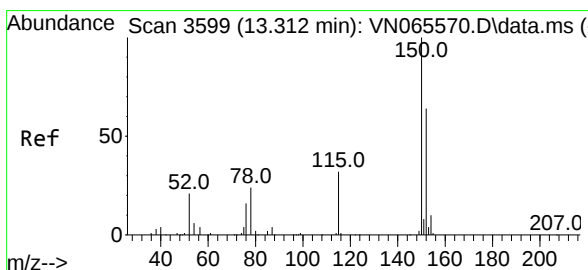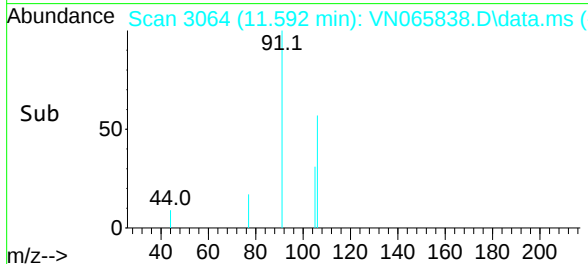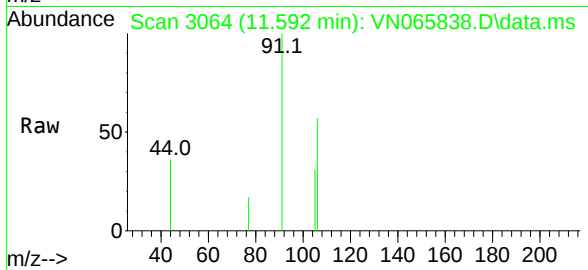

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:152 Resp: 103183
Ion Ratio Lower Upper
152 100
115 59.5 28.5 85.6
150 158.0 0.0 347.6


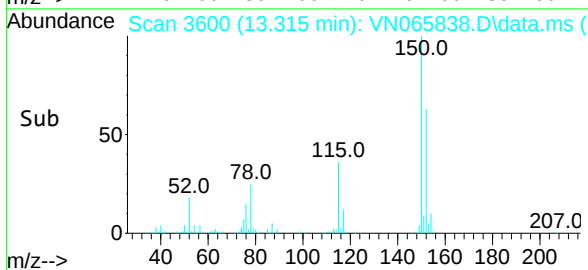

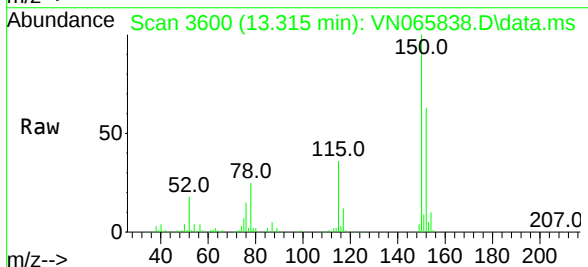




#74
N-amy1 acetate
Concen: 0.57 ug/l
RT: 12.003 min Scan# 3192
Delta R.T. -0.036 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43	Resp: 2170
Ion Ratio	Lower Upper
43 100	
70 0.0	34.4 51.6#
55 0.0	20.7 31.1#
61 0.0	19.1 28.7#

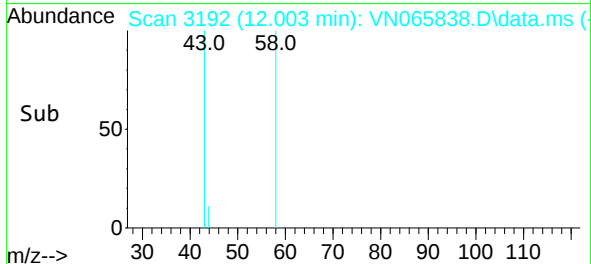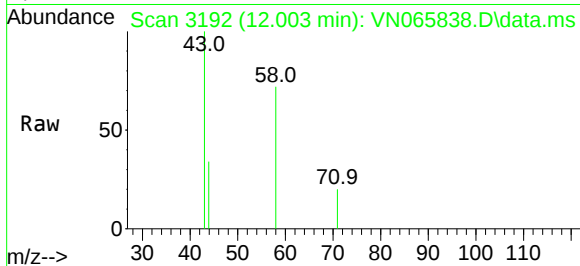

#76
1,2,3-Trichloropropane
Concen: 20.37 ug/l
RT: 12.370 min Scan# 3306
Delta R.T. -0.154 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion: 75	Resp: 54954
Ion Ratio	Lower Upper
75 100	
77 1.4	0.0 0.0#

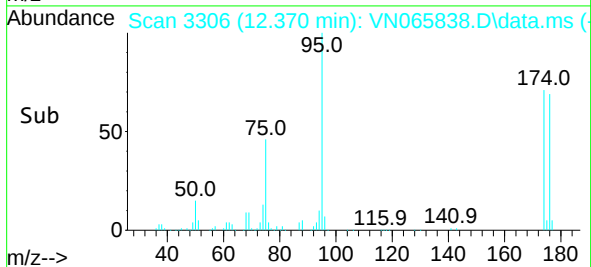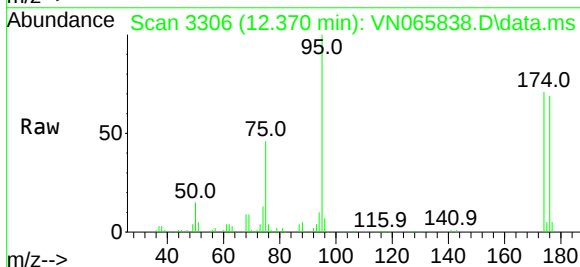



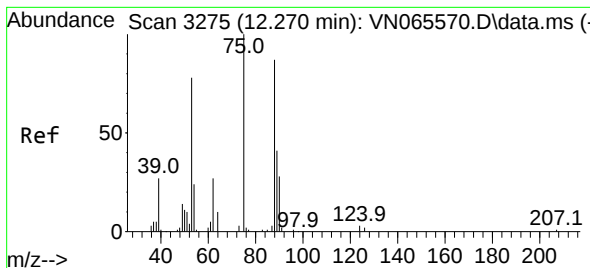


#81
trans-1,4-Dichloro-2-butene
Concen: 52.17 ug/l
RT: 12.370 min Scan# 3306
Delta R.T. 0.100 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampled :



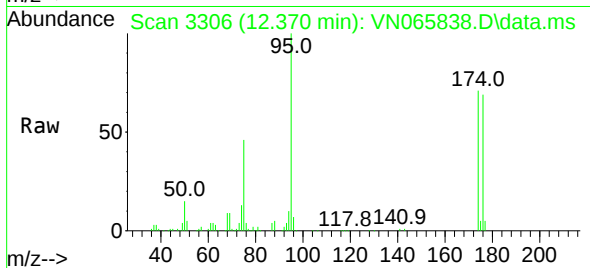



Tgt Ion: 75 Resp: 54954
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#

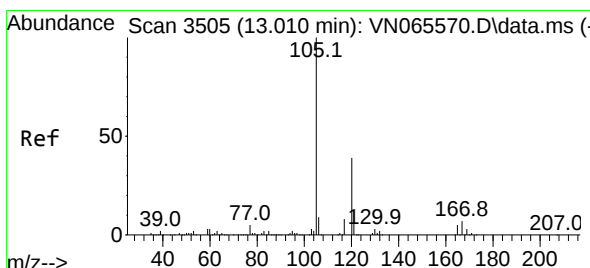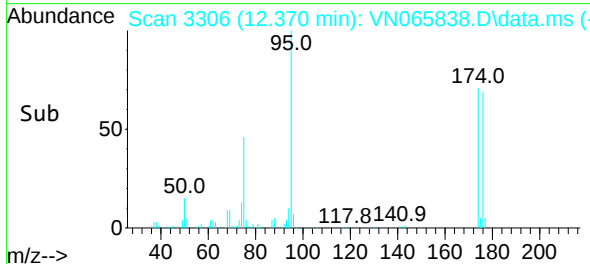

#84
1,2,4-Trimethylbenzene
Concen: 0.43 ug/l
RT: 13.013 min Scan# 3506
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Tgt Ion: 105 Resp: 3293
Ion Ratio Lower Upper
105 100
120 42.9 22.4 67.0

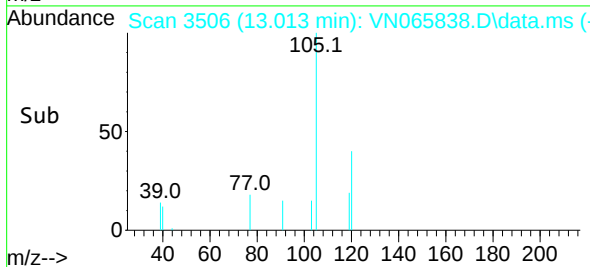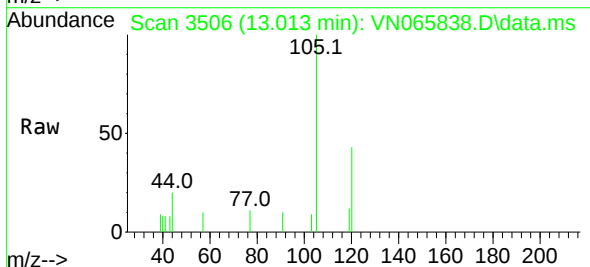






#86
p-Isopropyltoluene
Concen: 0.25 ug/l
RT: 13.260 min Scan# 3583
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04


Instrument :
MSVOA_N
ClientSampled :

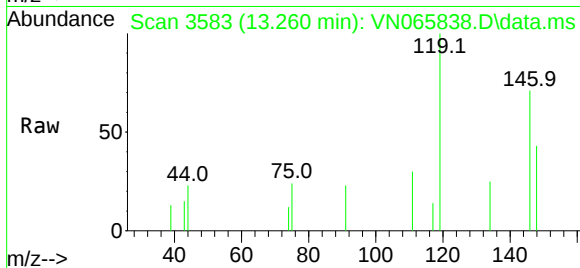



Tgt Ion:119 Resp: 1894
Ion Ratio Lower Upper
119 100
134 20.4 13.3 39.8
91 22.1 11.8 35.3

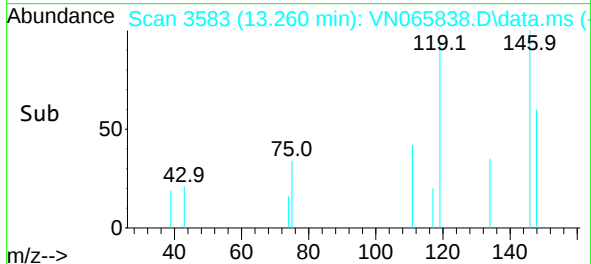


#87
1,3-Dichlorobenzene
Concen: 0.46 ug/l
RT: 13.257 min Scan# 3582
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

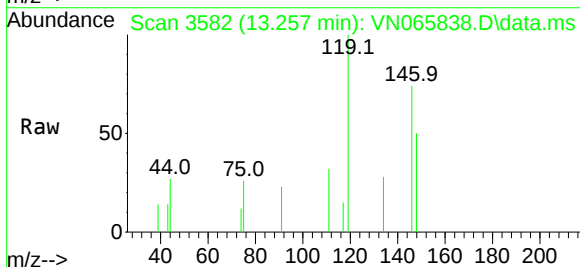

Tgt Ion:146 Resp: 1587
Ion Ratio Lower Upper
146 100
111 42.2 19.5 58.5
148 57.0 32.3 96.9



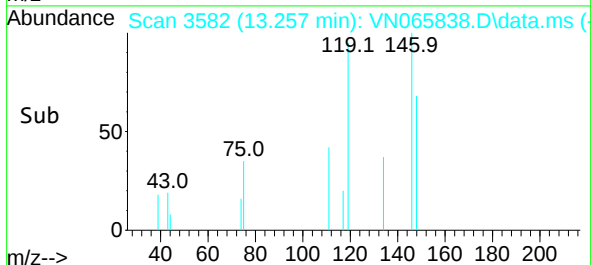





#88
1,4-Dichlorobenzene
Concen: 0.45 ug/l
RT: 13.257 min Scan# 3582
Delta R.T. -0.077 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:146 Resp: 1587
Ion Ratio Lower Upper
146 100
111 42.2 19.0 57.0
148 57.0 31.8 95.3

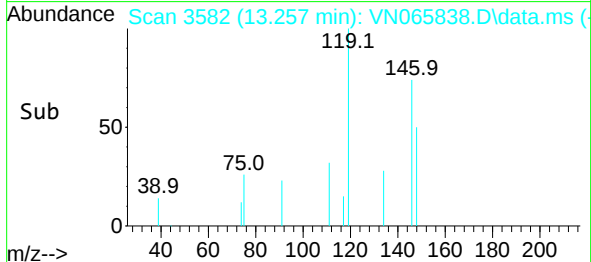

#89
n-Butylbenzene
Concen: 0.33 ug/l
RT: 13.585 min Scan# 3684
Delta R.T. 0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion: 91 Resp: 2285
Ion Ratio Lower Upper
91 100
92 42.8 26.1 78.3
134 15.4 13.0 38.9


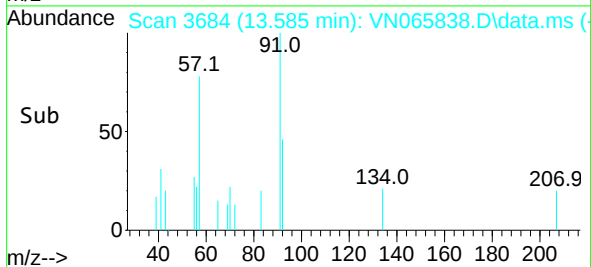

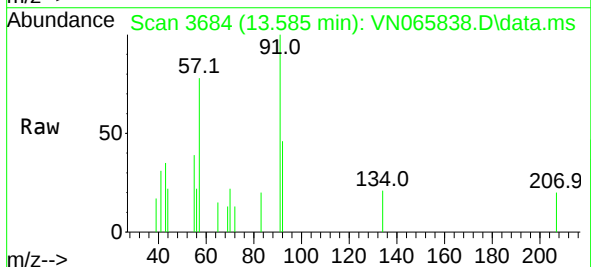


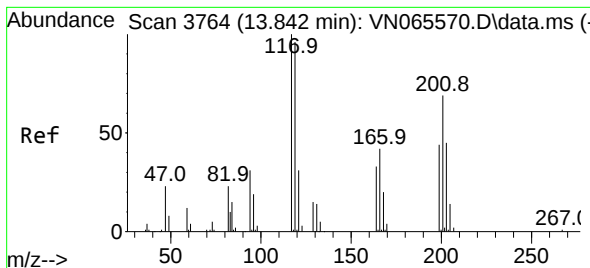

#90
Hexachloroethane
Concen: 0.24 ug/l
RT: 13.965 min Scan# 3802
Delta R.T. 0.123 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 316
Ion Ratio Lower Upper
117 100
201 0.0 37.8 113.3#

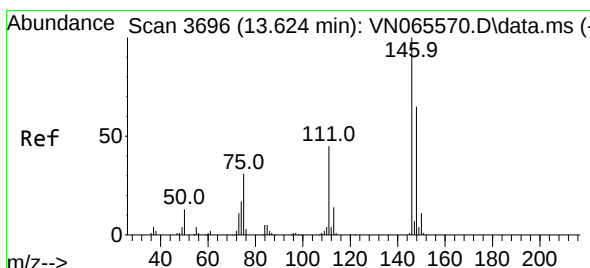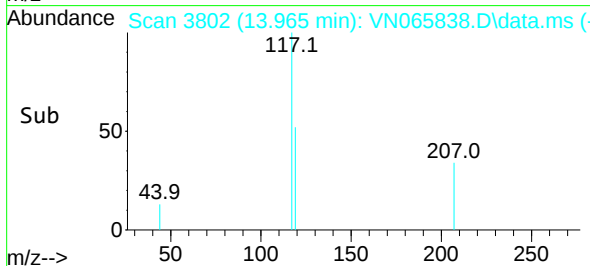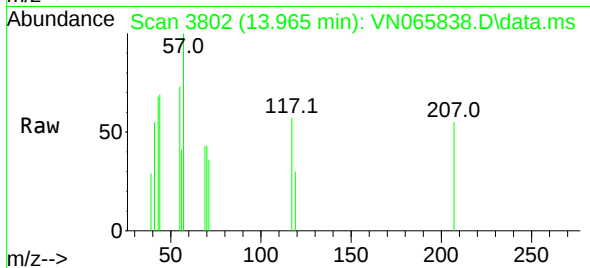

#91
1,2-Dichlorobenzene
Concen: 0.31 ug/l
RT: 13.627 min Scan# 3697
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:146 Resp: 1062
Ion Ratio Lower Upper
146 100
111 29.1 20.1 60.3
148 59.3 32.0 96.0


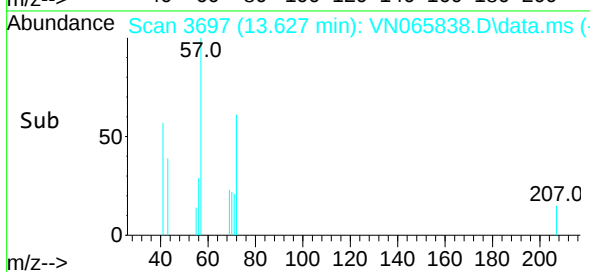

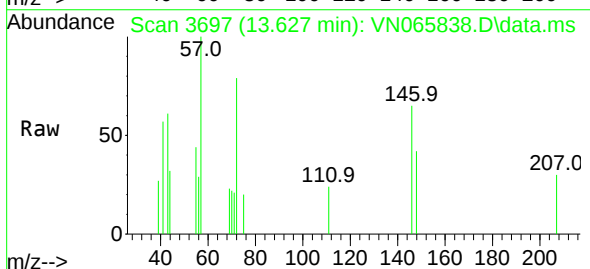


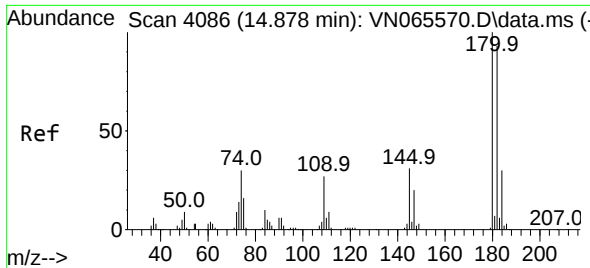

#93
1,2,4-Trichlorobenzene
Concen: 4.20 ug/l
RT: 14.881 min Scan# 4087
Delta R.T. 0.003 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:180 Resp: 1870
Ion Ratio Lower Upper
180 100
182 92.6 47.3 142.0
145 30.5 15.6 46.8

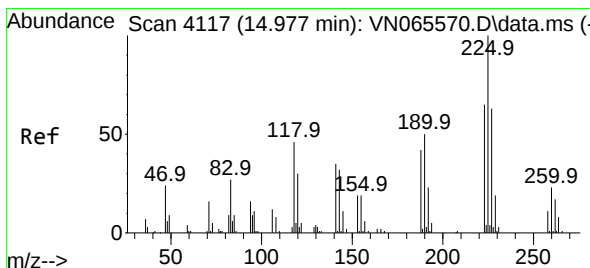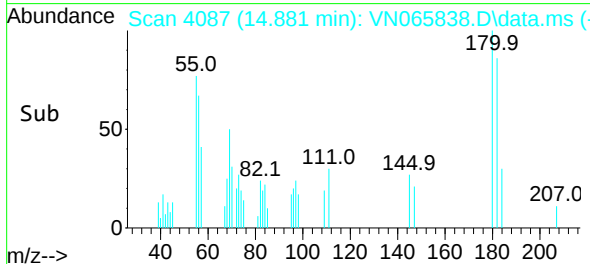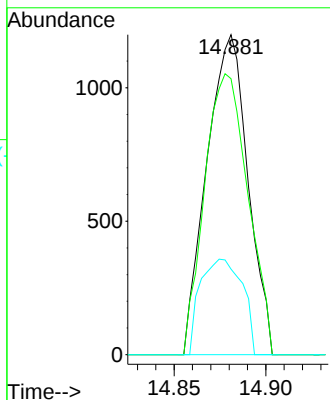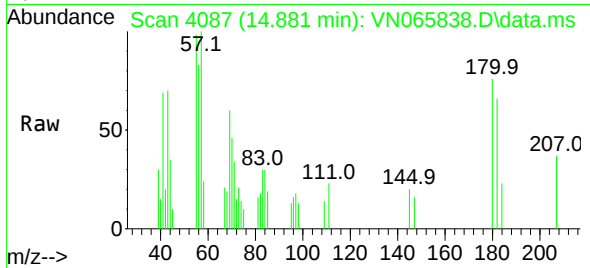

#94
Hexachlorobutadiene
Concen: 0.91 ug/l
RT: 14.981 min Scan# 4118
Delta R.T. 0.004 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:225 Resp: 599
Ion Ratio Lower Upper
225 100
223 61.3 31.9 95.9
227 49.1 31.6 95.0


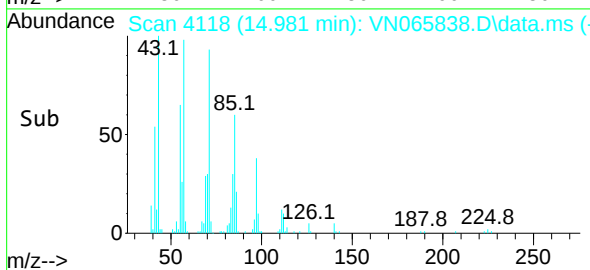
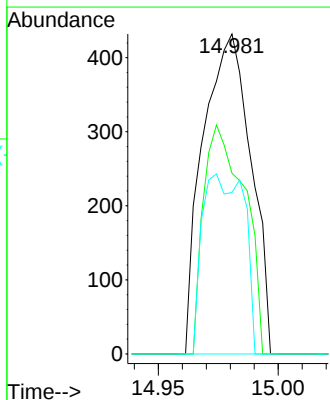
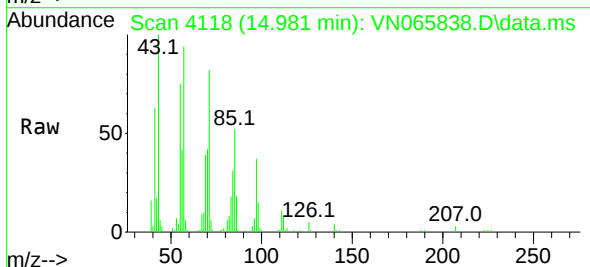




#95
Naphthalene
Concen: 5.07 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. -0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 11587
Ion Ratio Lower Upper
128 100
127 22.4 10.2 15.2#
129 11.8 8.6 13.0

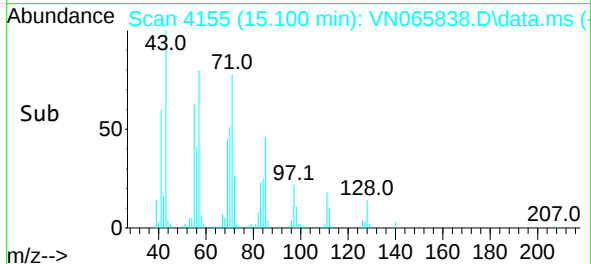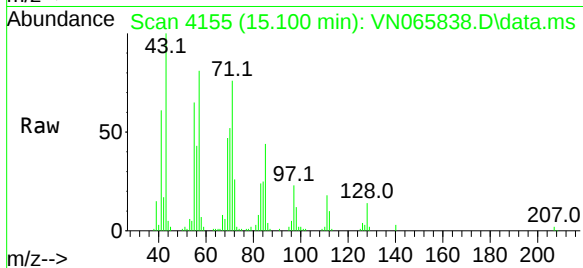

#96
1,2,3-Trichlorobenzene
Concen: 3.82 ug/l
RT: 15.280 min Scan# 4211
Delta R.T. -0.000 min
Lab File: VN065838.D
Acq: 12 Feb 2021 15:04

Tgt Ion:180 Resp: 2126
Ion Ratio Lower Upper
180 100
182 93.5 47.4 142.3
145 30.9 16.5 49.5

