

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
 Data File : VN065860.D
 Acq On : 13 Feb 2021 00:07
 Operator : JC/MD
 Sample : M1398-03ME 10X
 Misc : 3.43g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 13 03:38:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.624	168	110296	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	211272	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	228895	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.312	152	104694	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	65814	45.36	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 90.72%			
35) Dibromofluoromethane	7.544	113	60790	48.56	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.12%			
50) Toluene-d8	10.055	98	278504	56.59	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 113.18%			
62) 4-Bromofluorobenzene	12.370	95	115521	65.19	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 130.38%			
Target Compounds					Qvalue	
16) Acetone	3.778	43	265	0.47	ug/l #	41
18) Methyl Acetate	4.286	43	2955	1.87	ug/l #	80
31) Cyclohexane	7.614	56	2012	0.74	ug/l #	1
36) 1,1-Dichloropropene	7.621	75	7931	3.73	ug/l #	47
38) Carbon Tetrachloride	7.621	117	10094	5.77	ug/l #	17
39) Methylcyclohexane	9.039	83	8023	3.09	ug/l	93
48) Methyl methacrylate	9.103	41	527	0.31	ug/l #	10
51) 4-Methyl-2-Pentanone	10.055	43	2669	1.34	ug/l #	54
55) 1,1,2-Trichloroethane	10.498	97	15573	10.62	ug/l #	20
56) Ethyl methacrylate	10.399	69	3080	1.27	ug/l #	12
59) 2-Hexanone	10.688	43	14252	10.30	ug/l #	28
67) Ethyl Benzene	11.479	91	18963	2.11	ug/l	93
68) m/p-Xylenes	11.588	106	15488	4.76	ug/l	95
69) o-Xylene	11.920	106	2063	0.65	ug/l	98
73) Isopropylbenzene	12.219	105	47726	5.21	ug/l	99
74) N-amyl acetate	12.016	43	29843	7.70	ug/l #	60
75) 1,1,2,2-Tetrachloroethane	12.421	83	1194	0.44	ug/l #	37
76) 1,2,3-Trichloropropane	12.373	75	55051	20.11	ug/l #	100
77) Bromobenzene	12.418	156	69587	35.06	ug/l #	1
78) n-propylbenzene	12.559	91	139190	12.88	ug/l	100
79) 2-Chlorotoluene	12.627	91	9975	1.55	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.704	105	60847	7.80	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.373	75	55051	51.51	ug/l #	13
82) 4-Chlorotoluene	12.701	91	5768	0.88	ug/l #	51
83) tert-Butylbenzene	12.961	119	1669	0.26	ug/l #	26
84) 1,2,4-Trimethylbenzene	13.010	105	320597	41.18	ug/l	97
85) sec-Butylbenzene	13.141	105	102229	11.64	ug/l	88
86) p-Isopropyltoluene	13.257	119	34514	4.45	ug/l	99
89) n-Butylbenzene	13.582	91	121088	17.37	ug/l #	76
90) Hexachloroethane	13.858	117	25789	19.00	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.215	75	1101	2.05	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.878	180	928	3.77	ug/l #	80
95) Naphthalene	15.096	128	77269	14.06	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.305	180	1213	3.39	ug/l #	21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
Data File : VN065860.D
Acq On : 13 Feb 2021 00:07
Operator : JC/MD
Sample : M1398-03ME 10X
Misc : 3.43g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 13 03:38:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
Data File : VN065860.D
Acq On : 13 Feb 2021 00:07
Operator : JC/MD
Sample : M1398-03ME 10X
Misc : 3.43g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 13 03:38:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration




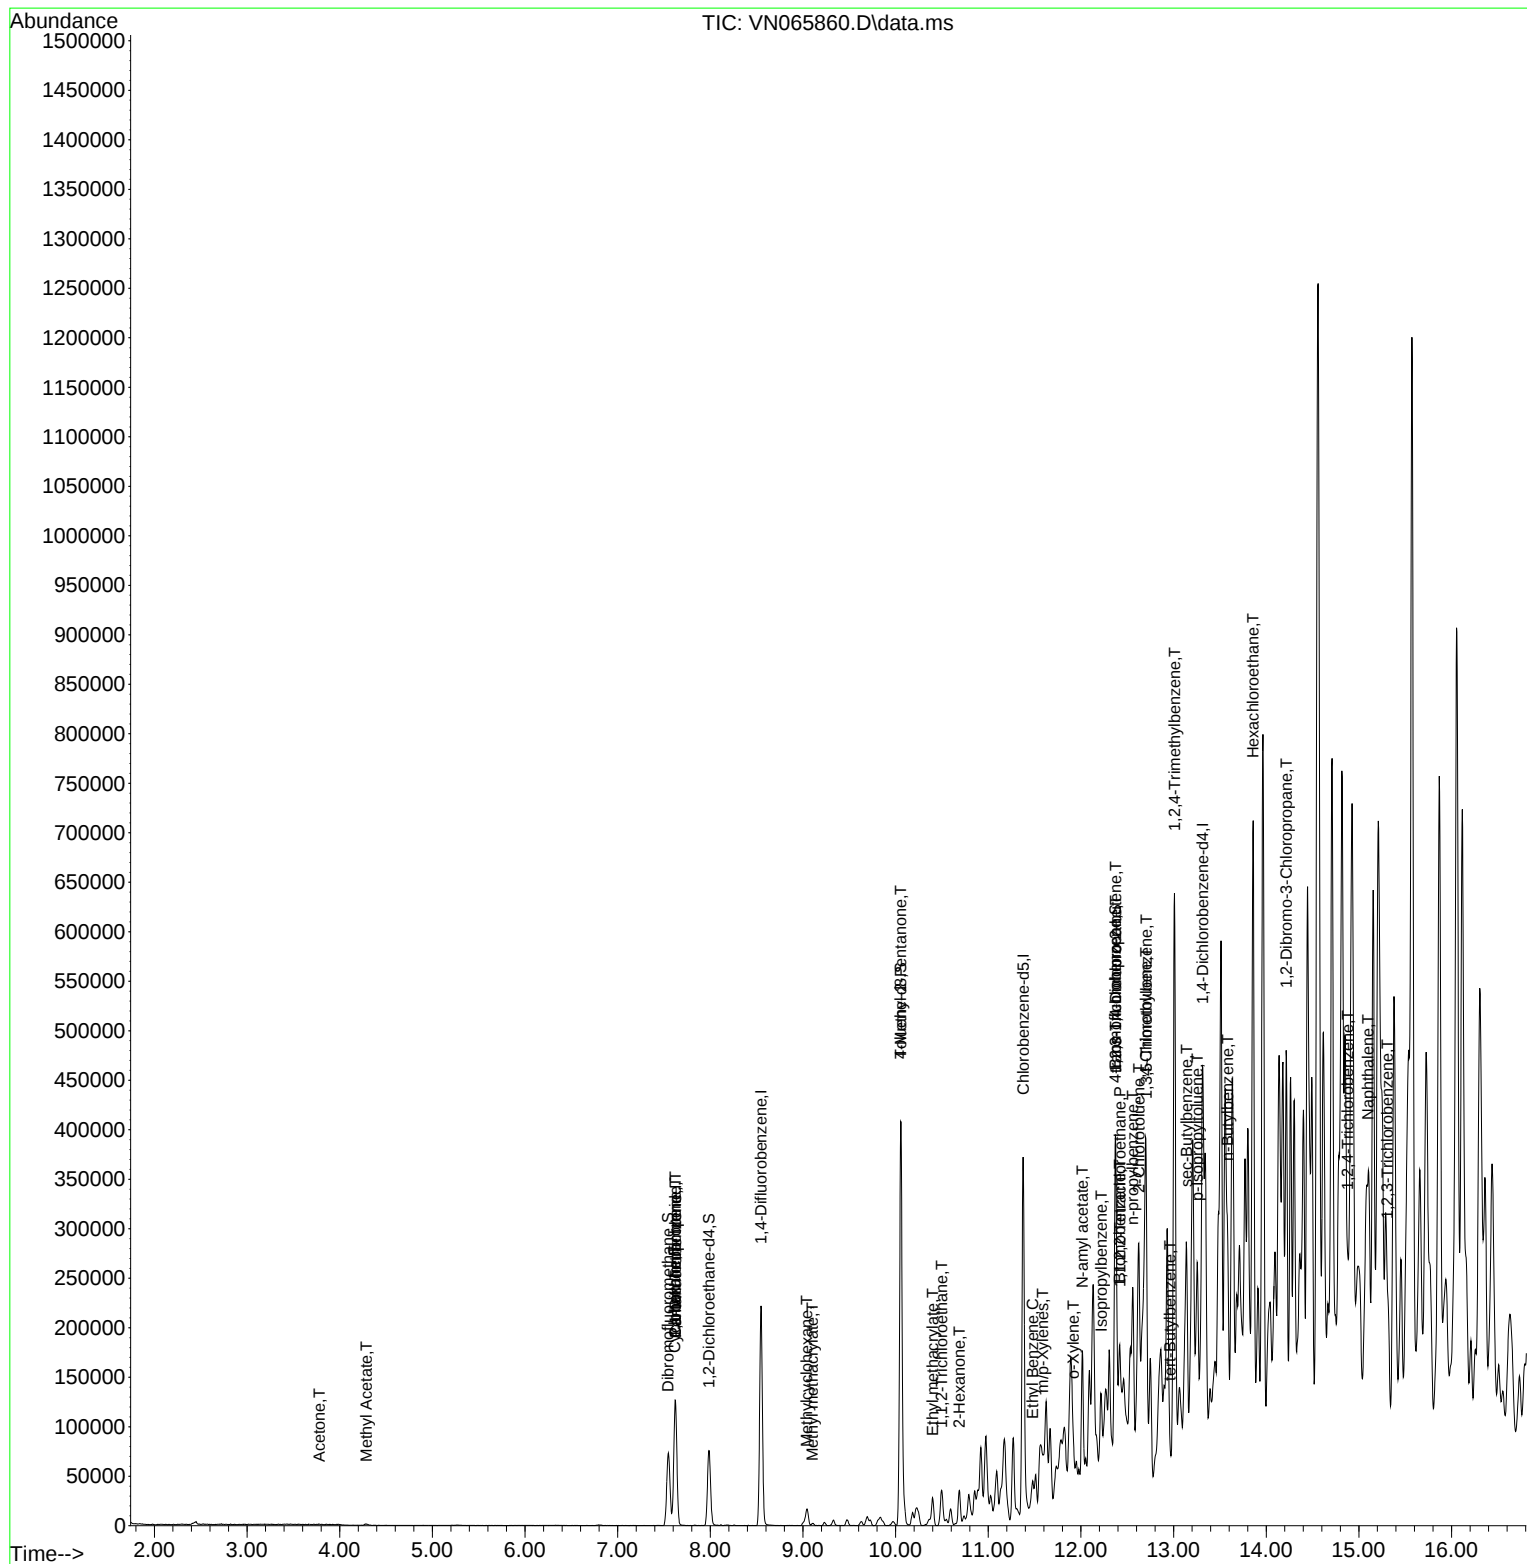




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 110296
Ion Ratio Lower Upper
168 100
99 56.8 42.6 63.8

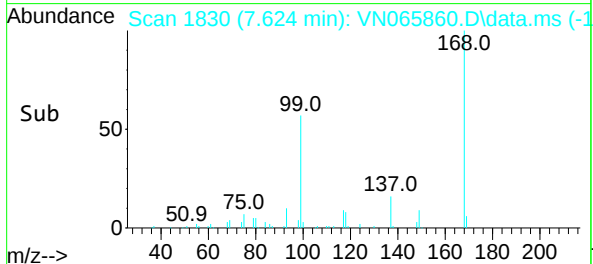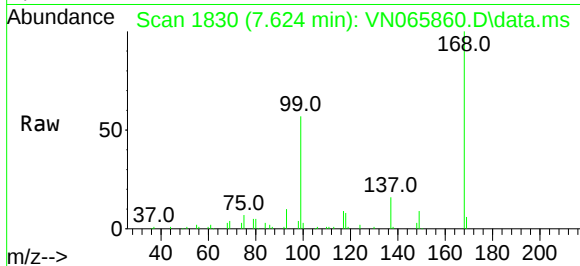

#16
Acetone
Concen: 0.47 ug/l
RT: 3.778 min Scan# 634
Delta R.T. -0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 43 Resp: 265
Ion Ratio Lower Upper
43 100
58 0.0 27.0 40.6#

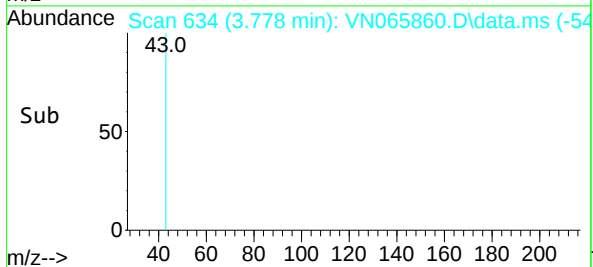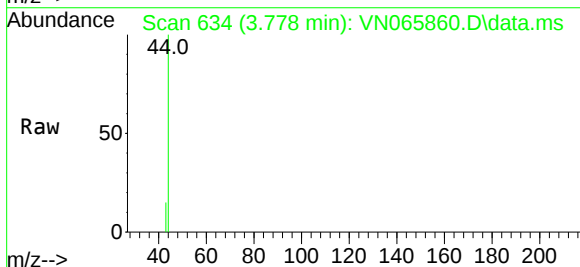

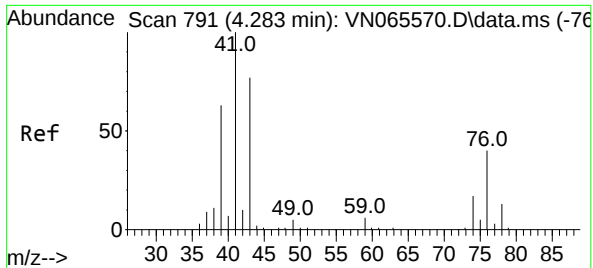

#18

Methyl Acetate


Concen: 1.87 ug/l

RT: 4.286 min Scan# 792

Delta R.T. 0.003 min

Lab File: VN065860.D

Acq: 13 Feb 2021 00:07



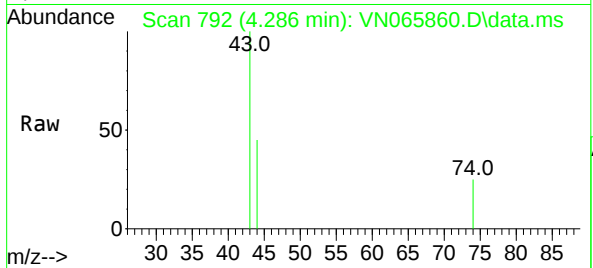


Tgt Ion: 43 Resp: 2955

Ion Ratio Lower Upper

43 100

74 14.6 19.5 29.3#

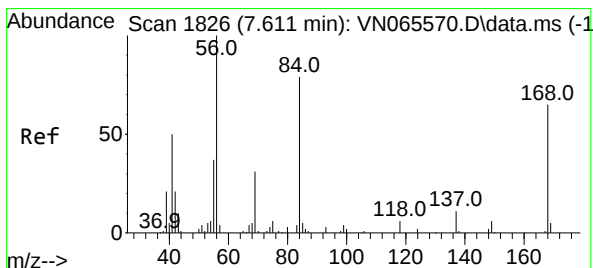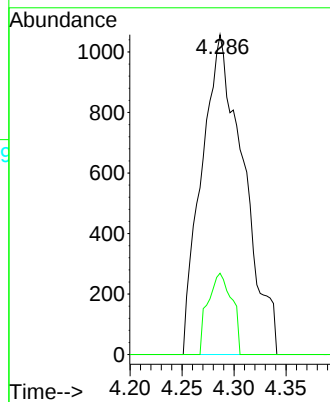

#31

Cyclohexane


Concen: 0.74 ug/l

RT: 7.614 min Scan# 1827

Delta R.T. 0.003 min

Lab File: VN065860.D

Acq: 13 Feb 2021 00:07

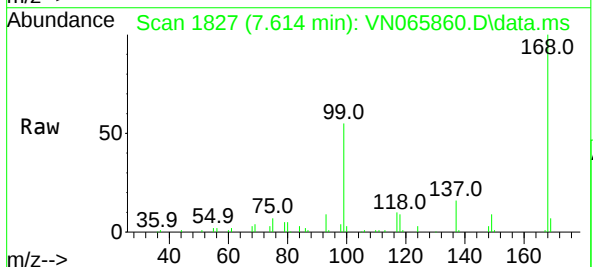



Tgt Ion: 56 Resp: 2012


Ion Ratio Lower Upper

56 100

69 183.2 26.6 39.8#

84 139.4 70.4 105.6#



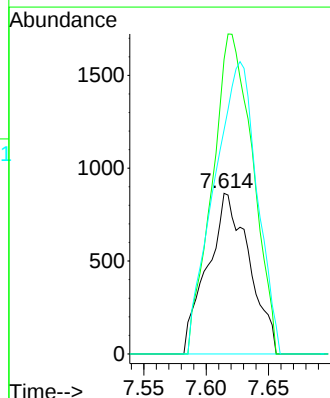
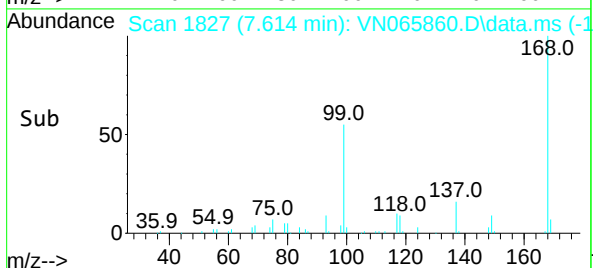




#33
1,2-Dichloroethane-d4
Concen: 45.36 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 65 Resp: 65814
Ion Ratio Lower Upper
65 100
67 54.9 0.0 107.2

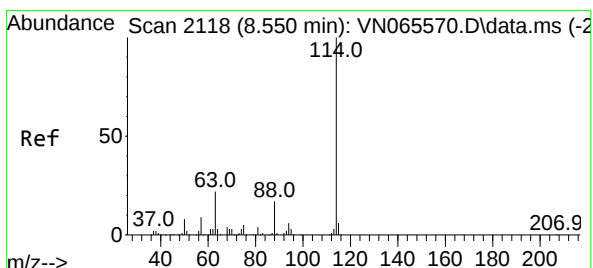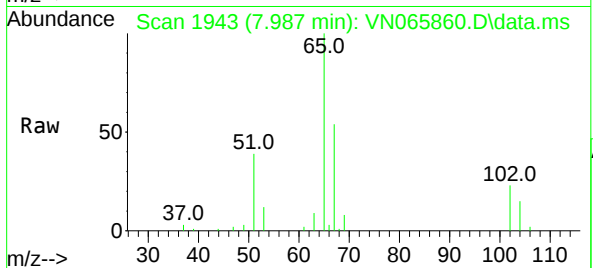

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 114 Resp: 211272
Ion Ratio Lower Upper
114 100
63 19.9 0.0 38.6
88 16.7 0.0 30.6


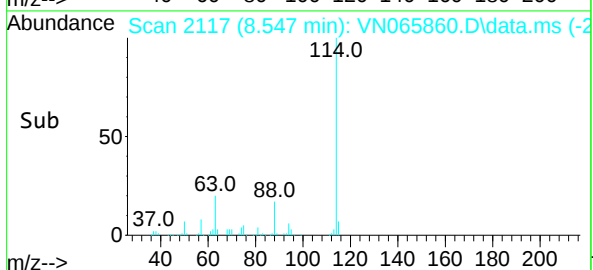






#35
Dibromofluoromethane
Concen: 48.56 ug/l
RT: 7.544 min Scan# 1805
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 60790
Ion Ratio Lower Upper
113 100
111 101.0 82.2 123.2
192 18.9 15.4 23.0

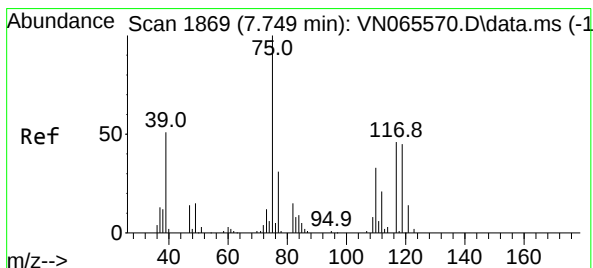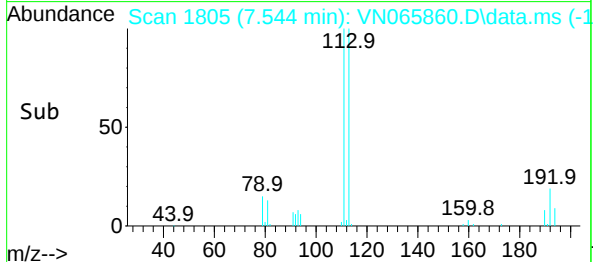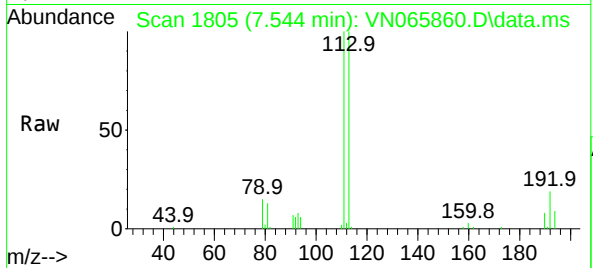

#36
1,1-Dichloropropene
Concen: 3.73 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. -0.128 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07


Tgt Ion: 75 Resp: 7931
Ion Ratio Lower Upper
75 100
110 6.8 18.2 54.6#
77 0.0 24.9 37.3#

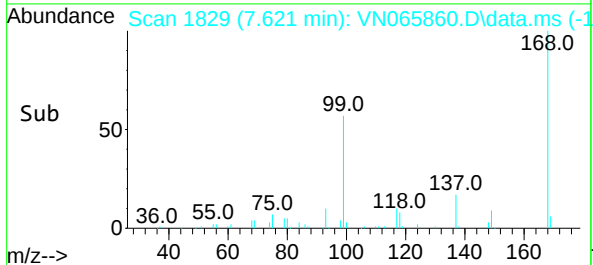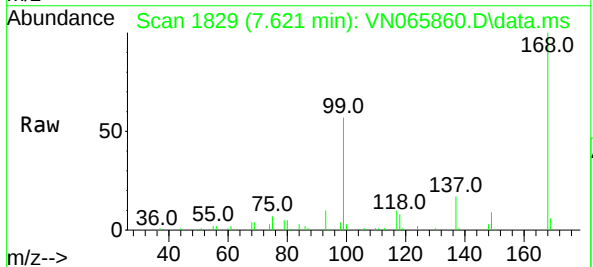






#38
Carbon Tetrachloride
Concen: 5.77 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. -0.109 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Instrument :
MSVOA_N
ClientSampled :



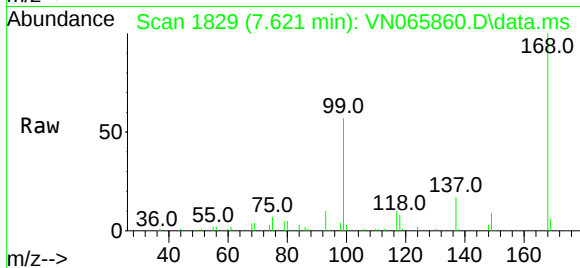



Tgt Ion: 117 Resp: 10094
Ion Ratio Lower Upper
117 100
119 5.4 76.0 114.0#
121 0.0 24.5 36.7#

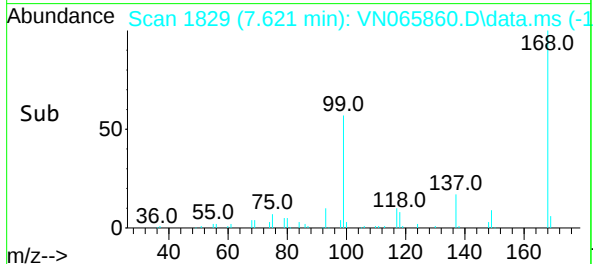

#39
Methylcyclohexane
Concen: 3.09 ug/l
RT: 9.039 min Scan# 2270
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 83 Resp: 8023
Ion Ratio Lower Upper
83 100
55 66.8 58.9 88.3
98 40.8 35.9 53.9


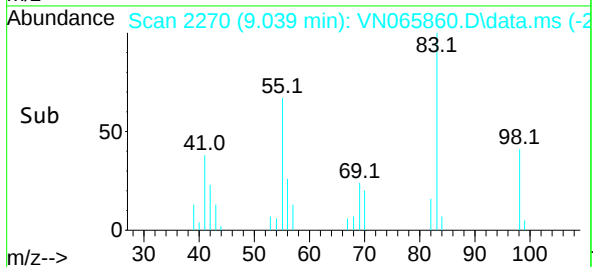

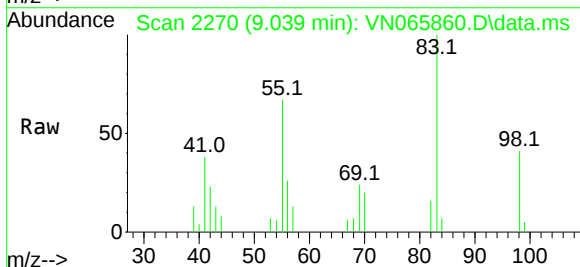




#48
Methyl methacrylate
Concen: 0.31 ug/l
RT: 9.103 min Scan# 2290
Delta R.T. -0.064 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 527
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 46.6 69.8#

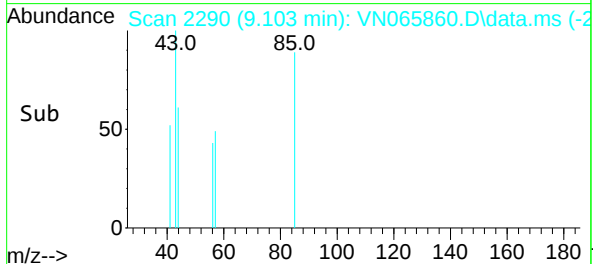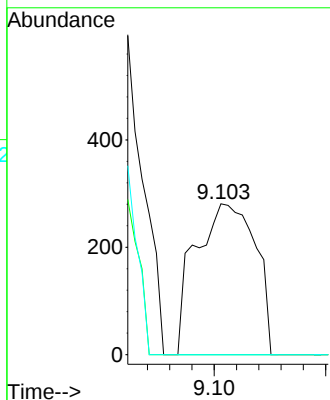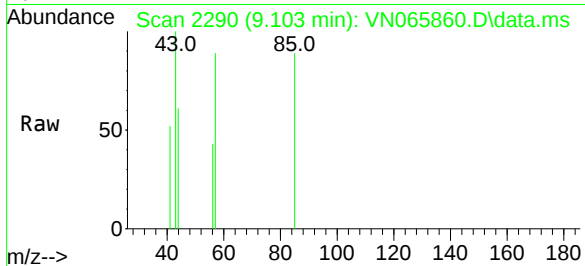

#50
Toluene-d8
Concen: 56.59 ug/l
RT: 10.055 min Scan# 2586
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 98 Resp: 278504
Ion Ratio Lower Upper
98 100
100 64.5 50.5 75.7


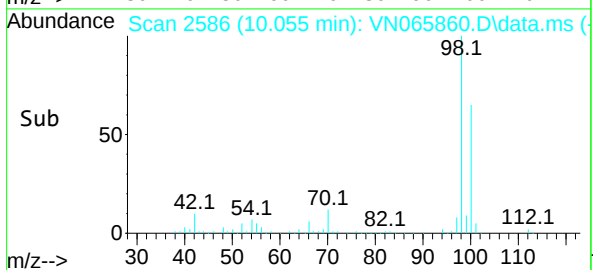
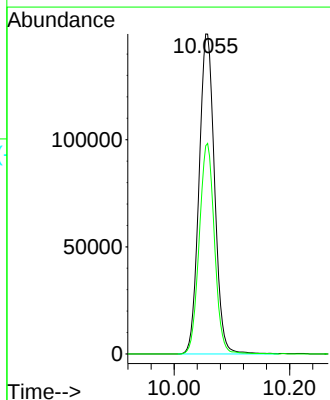
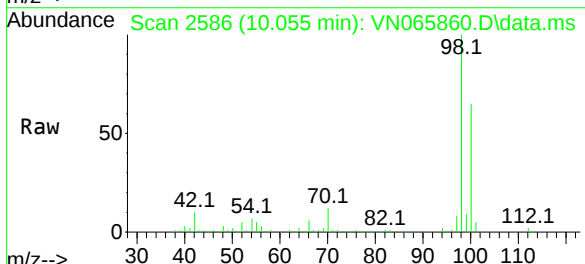


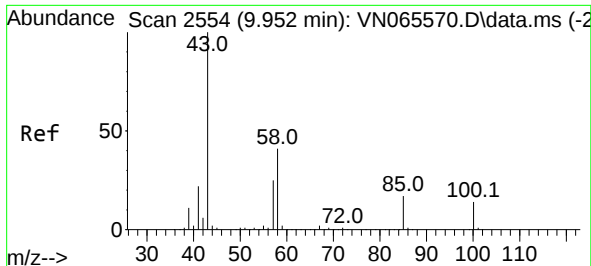

#51
4-Methyl-2-Pentanone
Concen: 1.34 ug/l
RT: 10.055 min Scan# 2586
Delta R.T. 0.103 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2669
Ion Ratio Lower Upper
43 100
58 69.1 32.5 48.7#

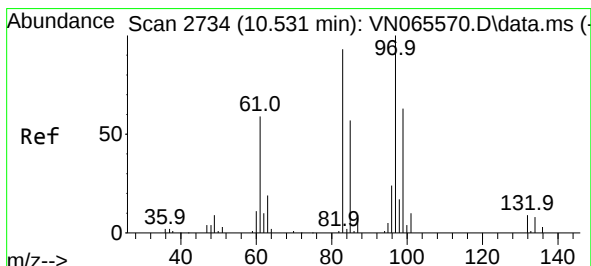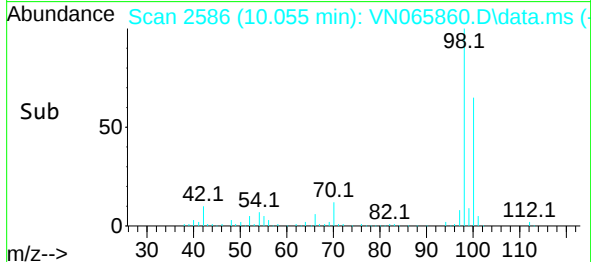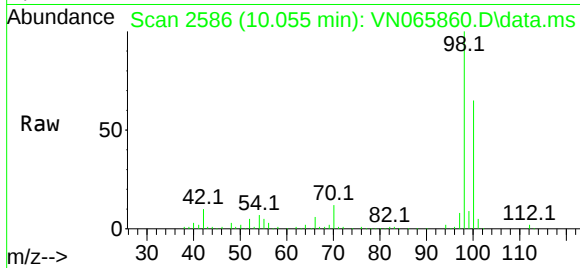

#55
1,1,2-Trichloroethane
Concen: 10.62 ug/l
RT: 10.498 min Scan# 2724
Delta R.T. -0.033 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 97 Resp: 15573
Ion Ratio Lower Upper
97 100
83 8.9 67.7 101.5#
85 0.0 44.5 66.7#
99 0.0 49.4 74.0#


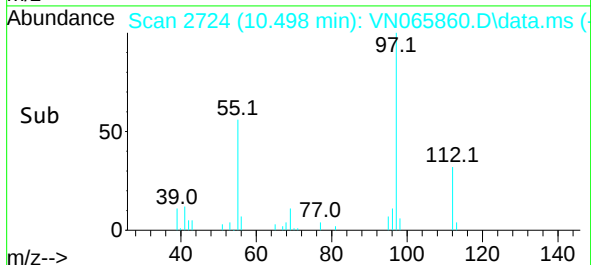
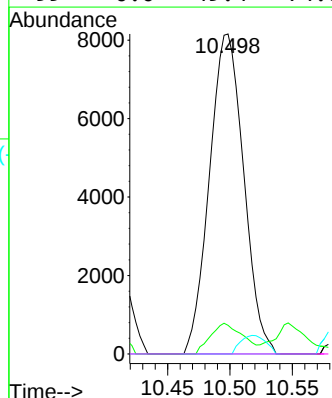
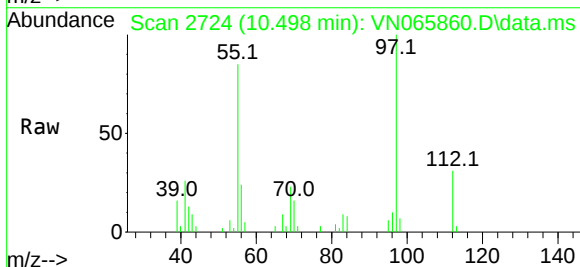


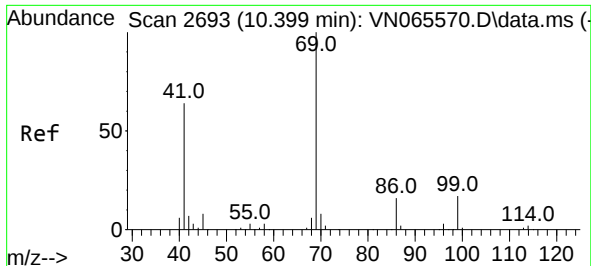

#56
Ethyl methacrylate
Concen: 1.27 ug/l
RT: 10.399 min Scan# 2693
Delta R.T. -0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 3080
Ion Ratio Lower Upper
69 100
41 155.1 49.6 74.4#
39 53.0 28.0 42.0#

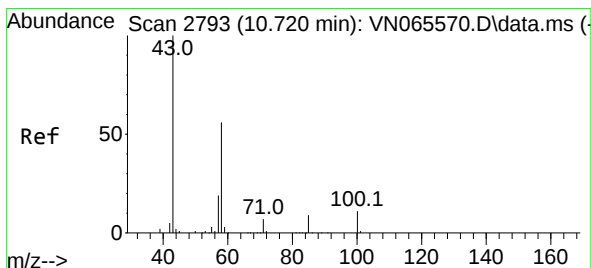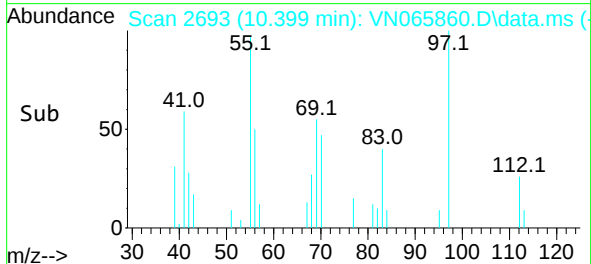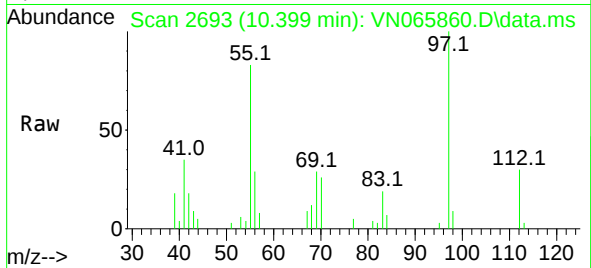

#59
2-Hexanone
Concen: 10.30 ug/l
RT: 10.688 min Scan# 2783
Delta R.T. -0.032 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 43 Resp: 14252
Ion Ratio Lower Upper
43 100
58 3.4 28.1 84.3#


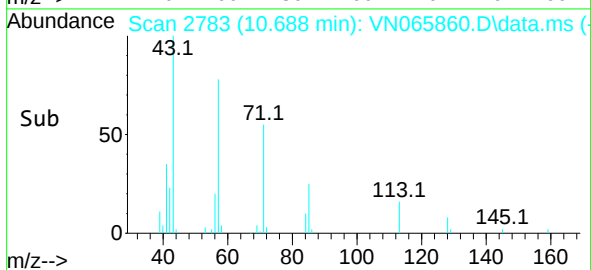

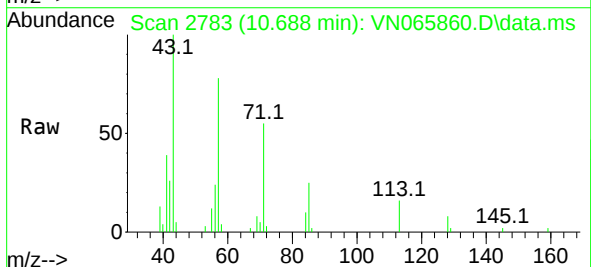


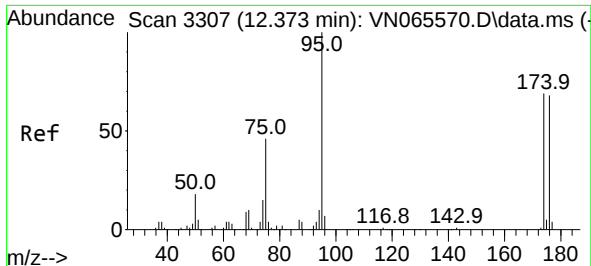

#62
4-Bromofluorobenzene
Concen: 65.19 ug/l
RT: 12.370 min Scan# 3306
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 95 Resp: 115521
Ion Ratio Lower Upper
95 100
174 75.2 0.0 169.0
176 71.5 0.0 162.4

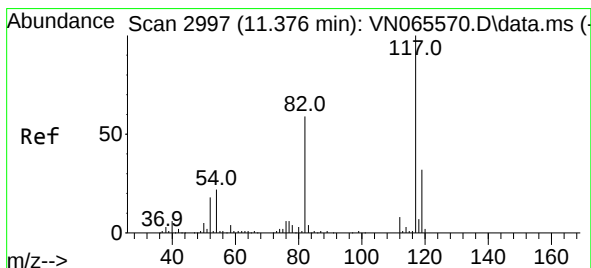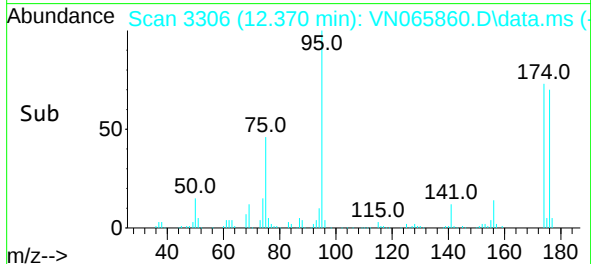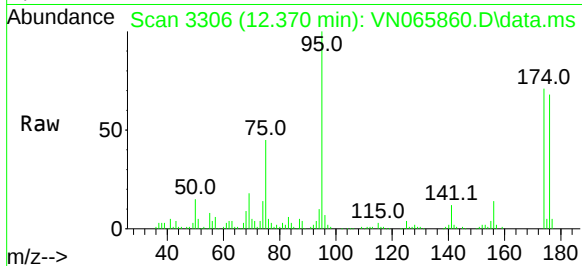

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 117 Resp: 228895
Ion Ratio Lower Upper
117 100
82 54.9 43.7 65.5
119 32.0 26.1 39.1


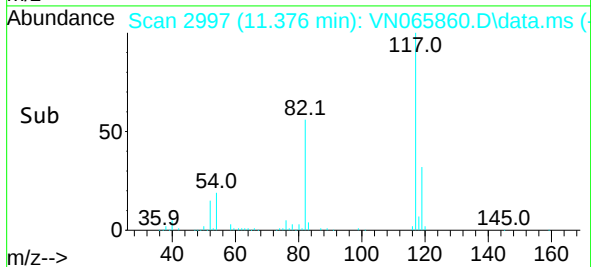

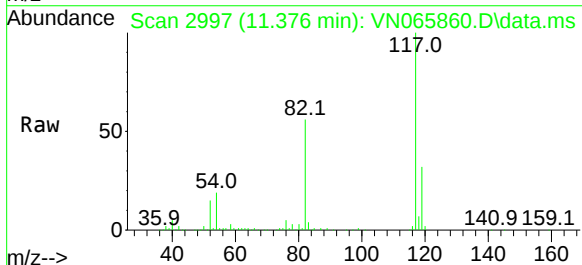




#67
Ethyl Benzene
Concen: 2.11 ug/l
RT: 11.479 min Scan# 3029
Delta R.T. 0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 18963
Ion Ratio Lower Upper
91 100
106 28.0 25.5 38.3

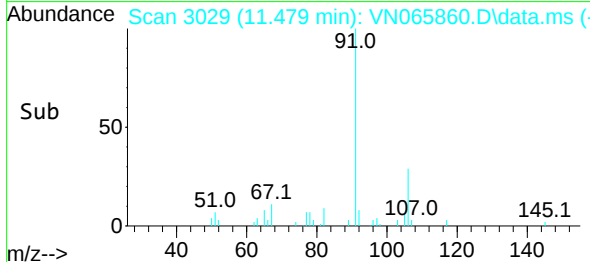

#68
m/p-Xylenes
Concen: 4.76 ug/l
RT: 11.588 min Scan# 3063
Delta R.T. -0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion:106 Resp: 15488
Ion Ratio Lower Upper
106 100
91 194.0 161.4 242.0


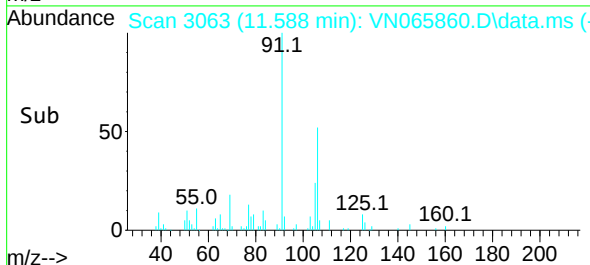
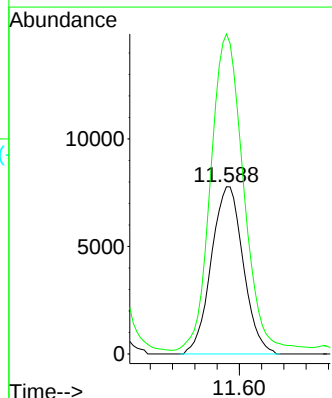
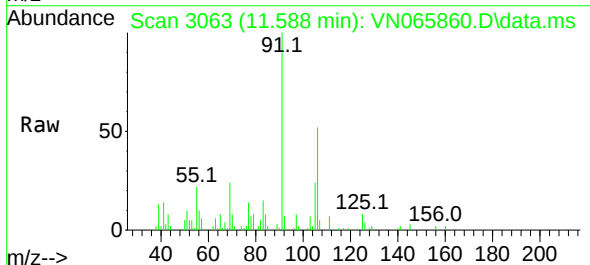




#69
o-Xylene
Concen: 0.65 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. 0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 2063
Ion Ratio Lower Upper
106 100
91 216.1 106.8 320.4

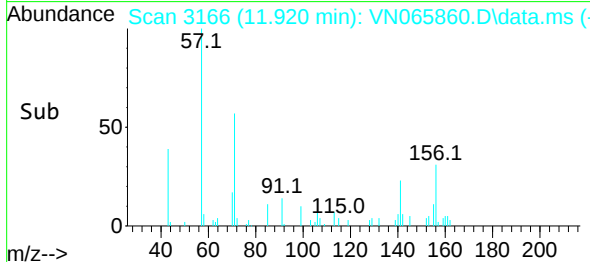

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.312 min Scan# 3599
Delta R.T. -0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion:152 Resp: 104694
Ion Ratio Lower Upper
152 100
115 63.8 28.5 85.6
150 156.0 0.0 347.6


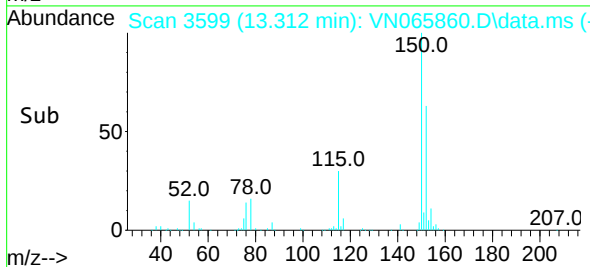

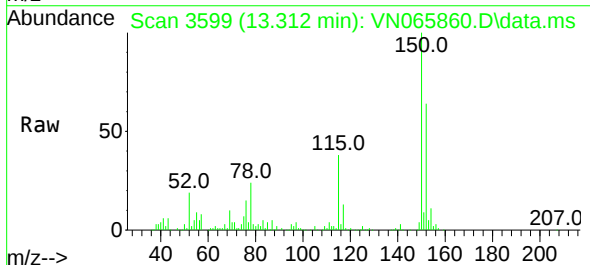




#73
Isopropylbenzene
Concen: 5.21 ug/l
RT: 12.219 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 47726
Ion Ratio Lower Upper
105 100
120 27.0 13.3 39.9

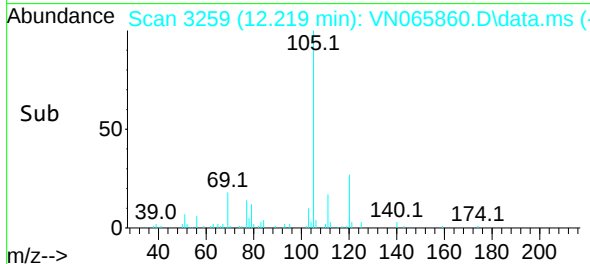

#74
N-ethyl acetate
Concen: 7.70 ug/l
RT: 12.016 min Scan# 3196
Delta R.T. -0.023 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 43 Resp: 29843
Ion Ratio Lower Upper
43 100
70 15.3 34.4 51.6#
55 11.9 20.7 31.1#
61 0.0 19.1 28.7#


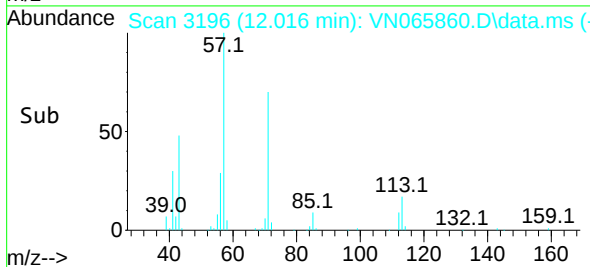

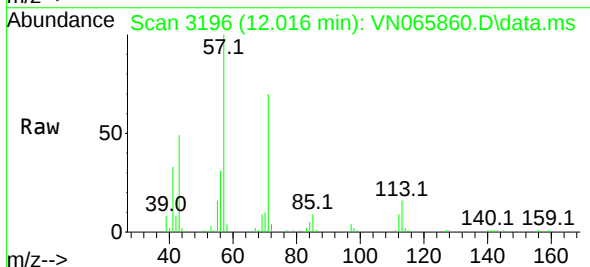


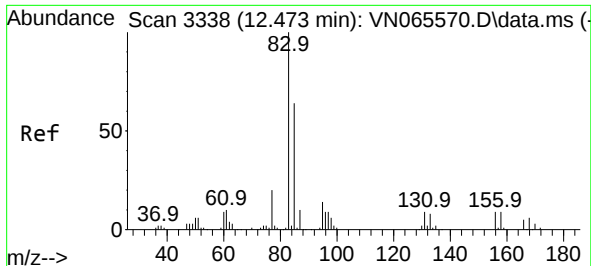

#75
1,1,2,2-Tetrachloroethane
Concen: 0.44 ug/l
RT: 12.421 min Scan# 3322
Delta R.T. -0.052 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 83 Resp: 1194
Ion Ratio Lower Upper
83 100
131 11.7 5.3 15.8
85 120.9 32.0 96.0#

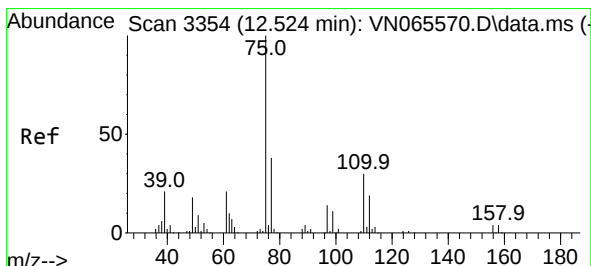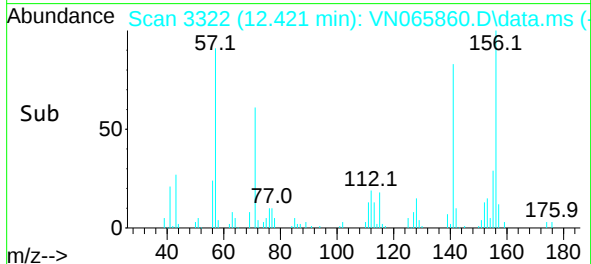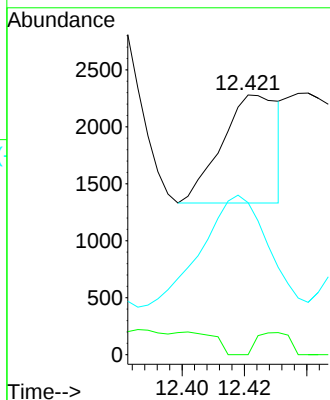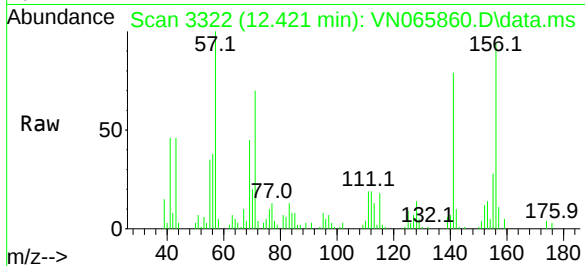

#76
1,2,3-Trichloropropane
Concen: 20.11 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 75 Resp: 55051
Ion Ratio Lower Upper
75 100
77 5.3 0.0 0.0#


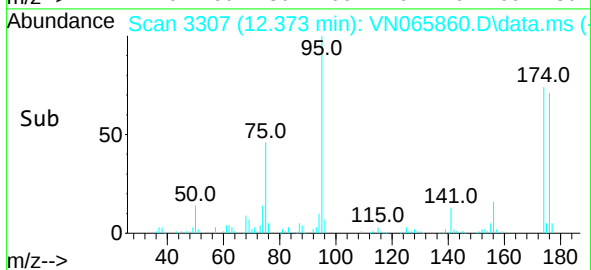
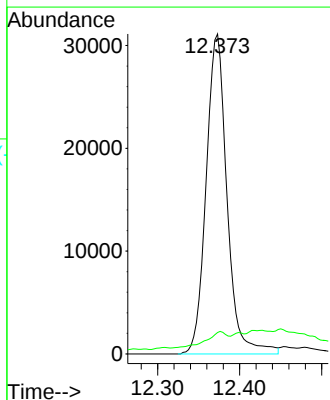
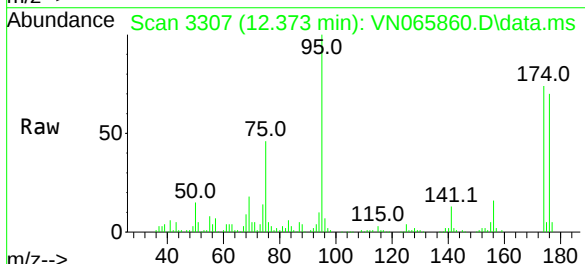


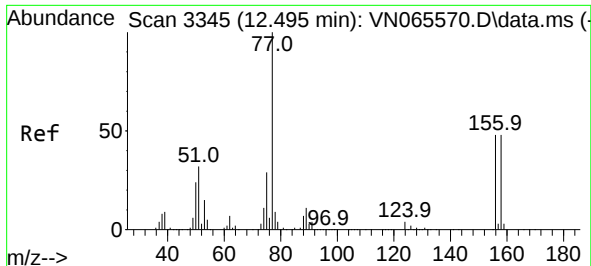

#77
Bromobenzene
Concen: 35.06 ug/l
RT: 12.418 min Scan# 3321
Delta R.T. -0.077 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:156 Resp: 69587
Ion Ratio Lower Upper
156 100
77 0.0 96.3 288.8#
158 0.0 49.0 147.0#

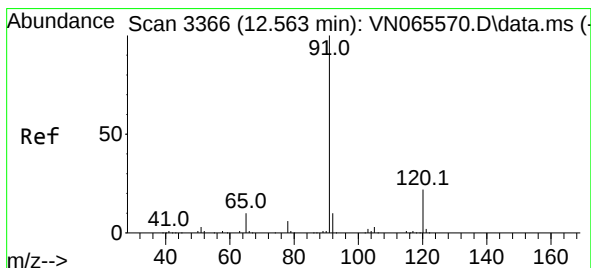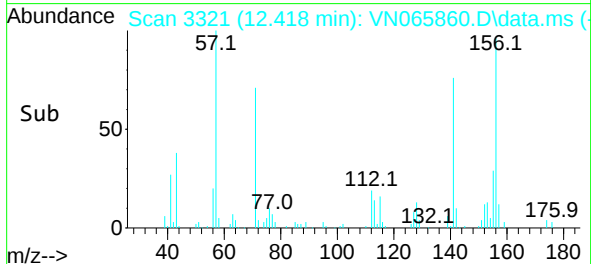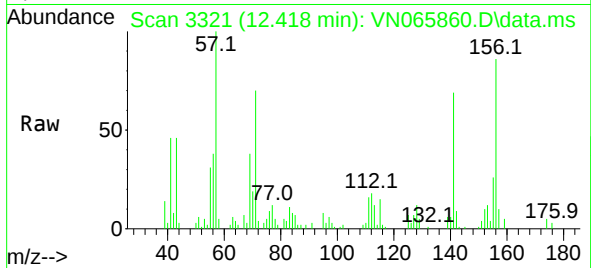

#78
n-propylbenzene
Concen: 12.88 ug/l
RT: 12.559 min Scan# 3365
Delta R.T. -0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion: 91 Resp: 139190
Ion Ratio Lower Upper
91 100
120 23.5 11.8 35.3


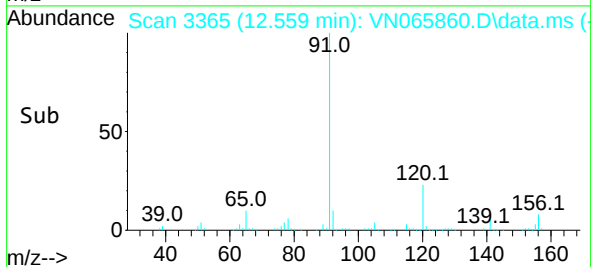

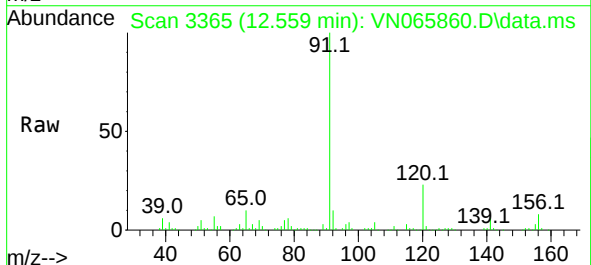




#79
2-Chlorotoluene
Concen: 1.55 ug/l
RT: 12.627 min Scan# 3386
Delta R.T. -0.016 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 9975
Ion Ratio Lower Upper
91 100
126 0.9 17.4 52.3#

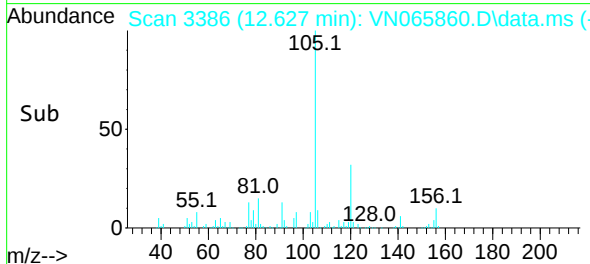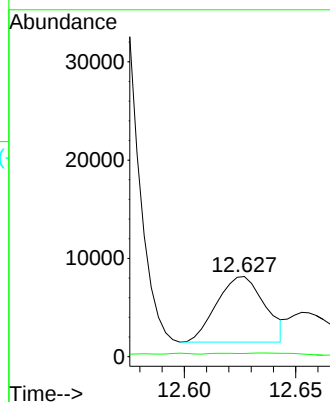

#80
1,3,5-Trimethylbenzene
Concen: 7.80 ug/l
RT: 12.704 min Scan# 3410
Delta R.T. 0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07


Tgt Ion: 105 Resp: 60847
Ion Ratio Lower Upper
105 100
120 49.0 24.3 72.8

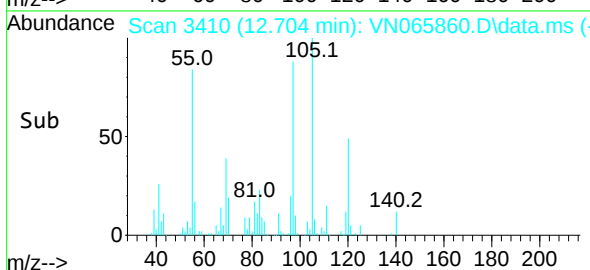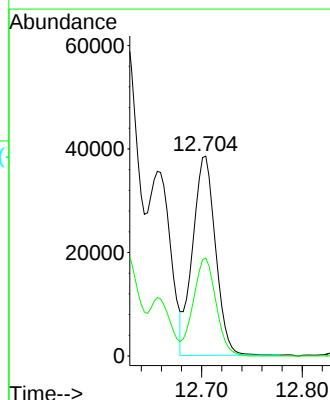






#81
trans-1,4-Dichloro-2-butene
Concen: 51.51 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 75 Resp: 55051
Ion Ratio Lower Upper
75 100
53 0.4 74.6 111.8#
89 0.0 35.8 53.8#

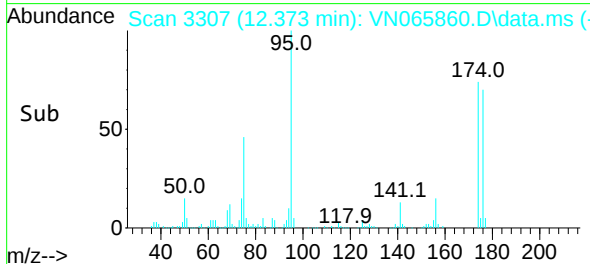


#82
4-Chlorotoluene
Concen: 0.88 ug/l
RT: 12.701 min Scan# 3409
Delta R.T. -0.042 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

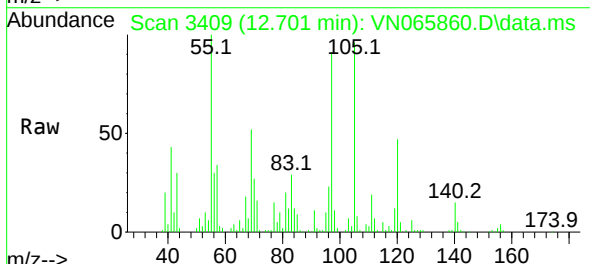

Tgt Ion: 91 Resp: 5768
Ion Ratio Lower Upper
91 100
126 6.1 17.2 51.6#









#83
tert-Butylbenzene
Concen: 0.26 ug/l
RT: 12.961 min Scan# 3490
Delta R.T. -0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:119 Resp: 1669
Ion Ratio Lower Upper
119 100
91 0.0 33.0 98.9#
134 0.0 12.7 38.1#

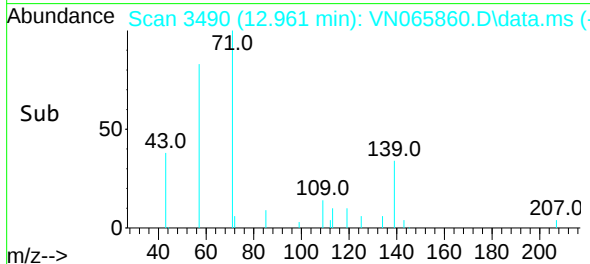

#84
1,2,4-Trimethylbenzene
Concen: 41.18 ug/l
RT: 13.010 min Scan# 3505
Delta R.T. -0.000 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion:105 Resp: 320597
Ion Ratio Lower Upper
105 100
120 46.5 22.4 67.0


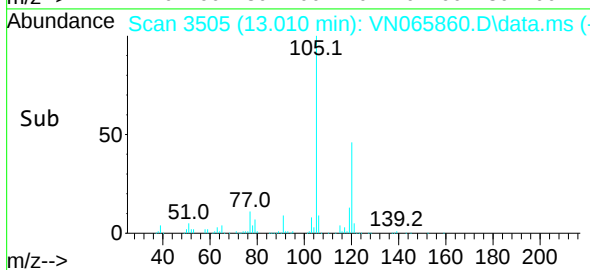

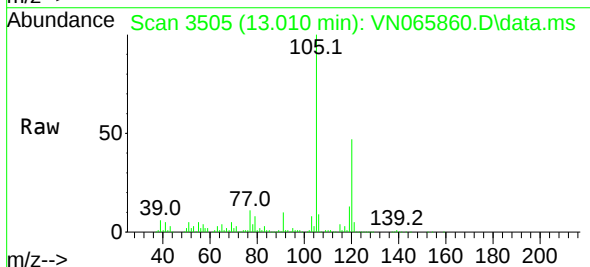


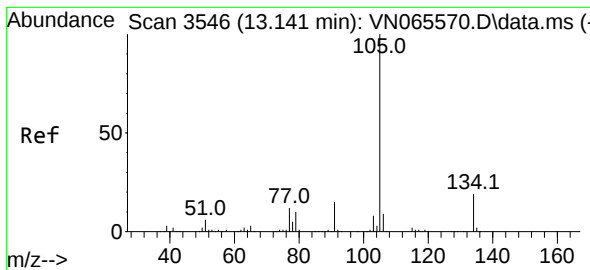

#85
 sec-Butylbenzene
 Concen: 11.64 ug/l
 RT: 13.141 min Scan# 3546
 Delta R.T. 0.000 min
 Lab File: VN065860.D
 Acq: 13 Feb 2021 00:07




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:105 Resp: 102229
 Ion Ratio Lower Upper
 105 100
 134 25.4 10.0 30.0

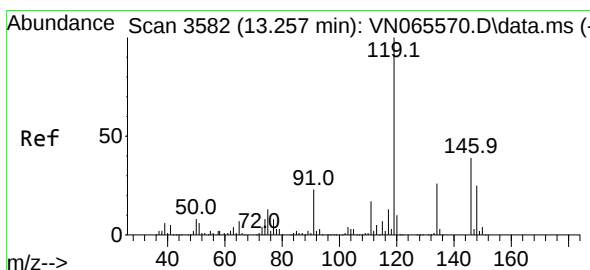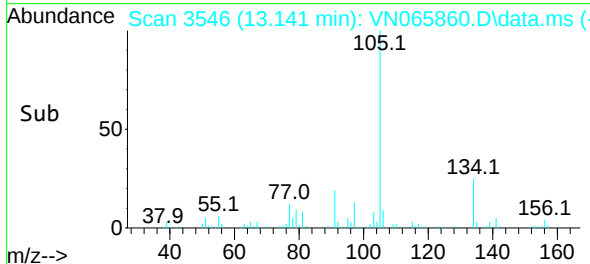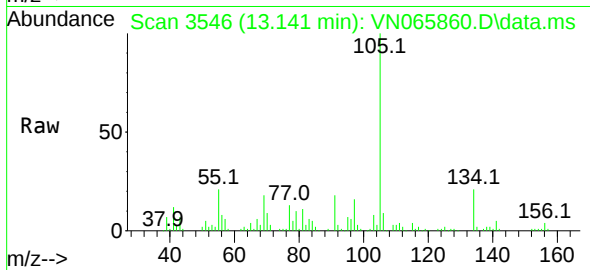

#86
 p-Isopropyltoluene
 Concen: 4.45 ug/l
 RT: 13.257 min Scan# 3582
 Delta R.T. 0.000 min
 Lab File: VN065860.D
 Acq: 13 Feb 2021 00:07

Tgt Ion:119 Resp: 34514
 Ion Ratio Lower Upper
 119 100
 134 25.9 13.3 39.8
 91 22.7 11.8 35.3


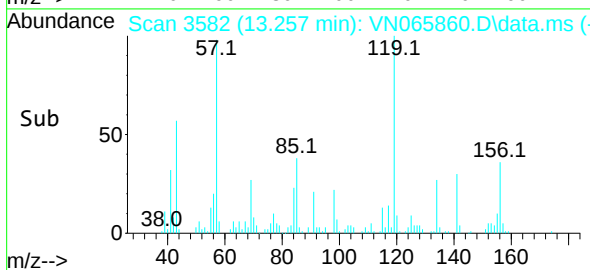

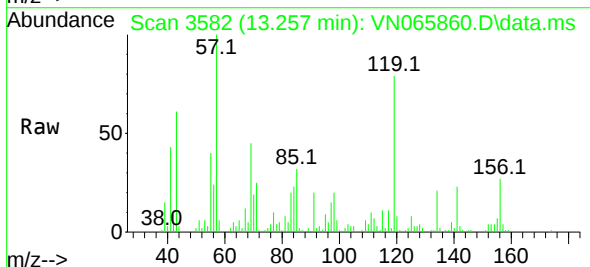




#89
n-Butylbenzene
Concen: 17.37 ug/l
RT: 13.582 min Scan# 3683
Delta R.T. -0.003 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 121088
Ion Ratio Lower Upper
91 100
92 44.7 26.1 78.3
134 0.0 13.0 38.9#

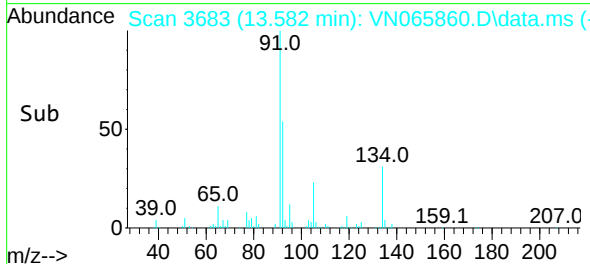

#90
Hexachloroethane
Concen: 19.00 ug/l
RT: 13.858 min Scan# 3769
Delta R.T. 0.016 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07


Tgt Ion: 117 Resp: 25789
Ion Ratio Lower Upper
117 100
201 0.0 37.8 113.3#

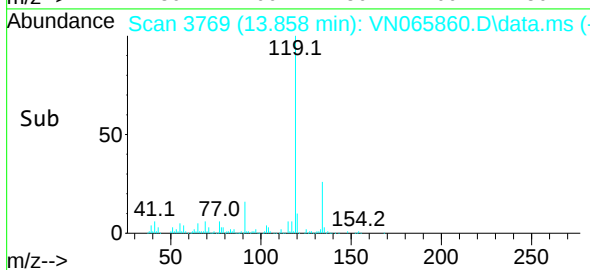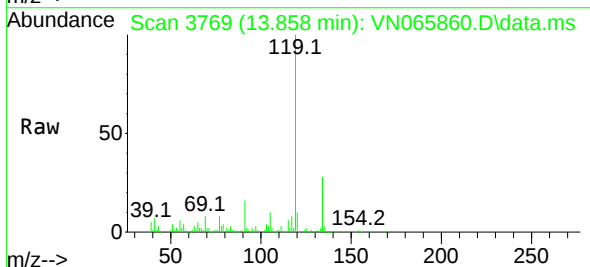






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.05 ug/l
 RT: 14.215 min Scan# 3880
 Delta R.T. -0.023 min
 Lab File: VN065860.D
 Acq: 13 Feb 2021 00:07

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 75 Resp: 1101
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.1 132.4#
 157 0.0 56.0 168.2#

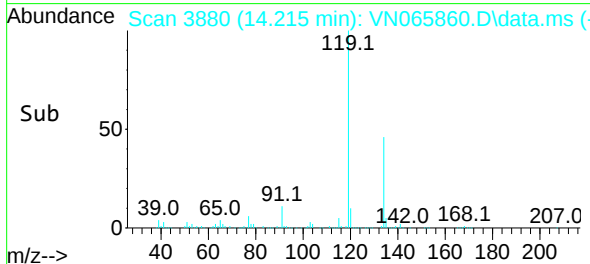

#93
 1,2,4-Trichlorobenzene
 Concen: 3.77 ug/l
 RT: 14.878 min Scan# 4086
 Delta R.T. -0.000 min
 Lab File: VN065860.D
 Acq: 13 Feb 2021 00:07

Tgt Ion: 180 Resp: 928
 Ion Ratio Lower Upper
 180 100
 182 86.5 47.3 142.0
 145 0.0 15.6 46.8#


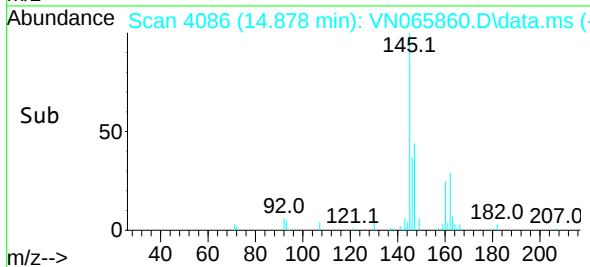

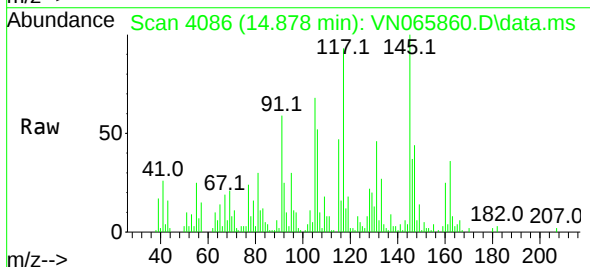




#95
Naphthalene
Concen: 14.06 ug/l
RT: 15.096 min Scan# 4154
Delta R.T. -0.004 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 77269
Ion Ratio Lower Upper
128 100
127 14.1 10.2 15.2
129 14.9 8.6 13.0#

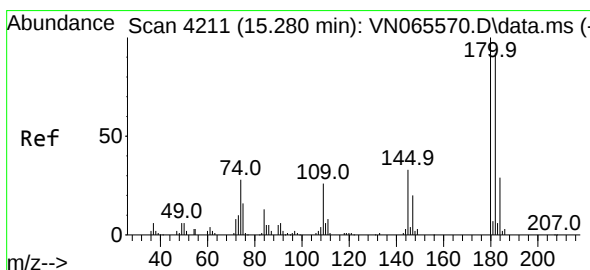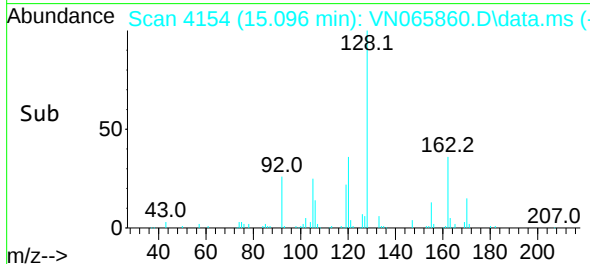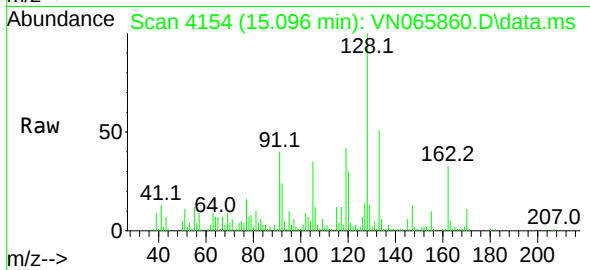

#96
1,2,3-Trichlorobenzene
Concen: 3.39 ug/l
RT: 15.305 min Scan# 4219
Delta R.T. 0.025 min
Lab File: VN065860.D
Acq: 13 Feb 2021 00:07

Tgt Ion:180 Resp: 1213
Ion Ratio Lower Upper
180 100
182 11.5 47.4 142.3#
145 0.0 16.5 49.5#

