

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
 Data File : VN065861.D
 Acq On : 13 Feb 2021 00:32
 Operator : JC/MD
 Sample : M1398-04ME 10X
 Misc : 3.44g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 32 Sample Multiplier: 1


Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 13 03:39:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.624	168	116078	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	226435	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	241747	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.312	152	109068	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.984	65	68913	45.13	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 90.26%			
35) Dibromofluoromethane	7.547	113	65308	48.67	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.34%			
50) Toluene-d8	10.055	98	297472	56.40	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 112.80%			
62) 4-Bromofluorobenzene	12.373	95	123193	64.86	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 129.72%			
Target Compounds						Qvalue
18) Methyl Acetate	4.283	43	646	0.39	ug/l #	51
31) Cyclohexane	7.618	56	1798	0.63	ug/l #	1
36) 1,1-Dichloropropene	7.618	75	8105	3.56	ug/l #	47
38) Carbon Tetrachloride	7.621	117	10756	5.73	ug/l #	18
39) Methylcyclohexane	9.042	83	2023	0.73	ug/l #	85
55) 1,1,2-Trichloroethane	10.495	97	4908	3.12	ug/l #	20
56) Ethyl methacrylate	10.399	69	1198	0.46	ug/l #	57
59) 2-Hexanone	10.688	43	4916	3.31	ug/l #	23
67) Ethyl Benzene	11.479	91	16892	1.78	ug/l #	88
68) m/p-Xylenes	11.589	106	17792	5.17	ug/l	86
69) o-Xylene	11.920	106	2798	0.84	ug/l	83
73) Isopropylbenzene	12.219	105	16270	1.70	ug/l #	68
74) N-amyl acetate	12.016	43	12663	3.13	ug/l #	58
75) 1,1,2,2-Tetrachloroethane	12.418	83	1051	0.37	ug/l #	38
76) 1,2,3-Trichloropropane	12.373	75	59686	20.93	ug/l #	100
77) Bromobenzene	12.434	156	165791	80.18	ug/l #	1
78) n-propylbenzene	12.560	91	48412	4.30	ug/l	98
79) 2-Chlorotoluene	12.624	91	12005	1.80	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.701	105	53464	6.58	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.373	75	59686	53.60	ug/l #	13
82) 4-Chlorotoluene	12.701	91	5430	0.80	ug/l #	45
83) tert-Butylbenzene	13.010	119	27522	4.06	ug/l #	73
84) 1,2,4-Trimethylbenzene	13.010	105	227885	28.10	ug/l	100
85) sec-Butylbenzene	13.142	105	38079	4.16	ug/l	89
86) p-Isopropyltoluene	13.257	119	21983	2.72	ug/l	98
89) n-Butylbenzene	13.582	91	33843	4.66	ug/l #	74
90) Hexachloroethane	13.855	117	12237	8.65	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.219	75	915	1.63	ug/l #	25
93) 1,2,4-Trichlorobenzene	14.884	180	661	3.64	ug/l #	53
95) Naphthalene	15.097	128	41908	8.97	ug/l #	77
96) 1,2,3-Trichlorobenzene	15.306	180	881	3.23	ug/l #	63





(#) = qualifier out of range (m) = manual integration (+) = signals summed

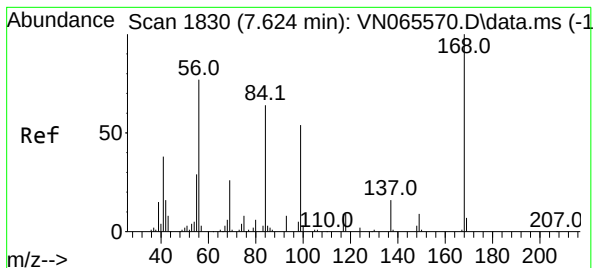

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 116078
Ion Ratio Lower Upper
168 100
99 55.4 42.6 63.8

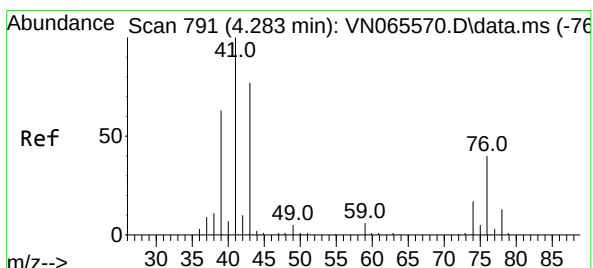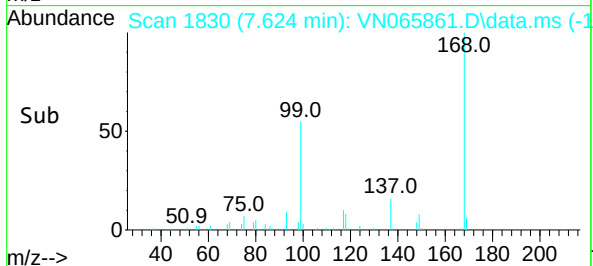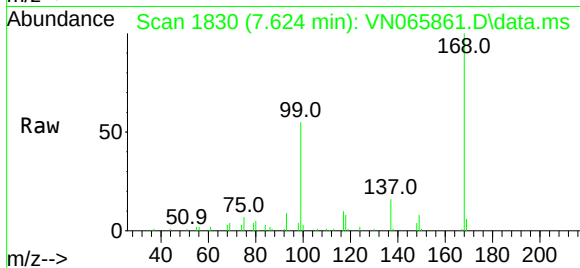

#18
Methyl Acetate
Concen: 0.39 ug/l
RT: 4.283 min Scan# 791
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 43 Resp: 646
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#


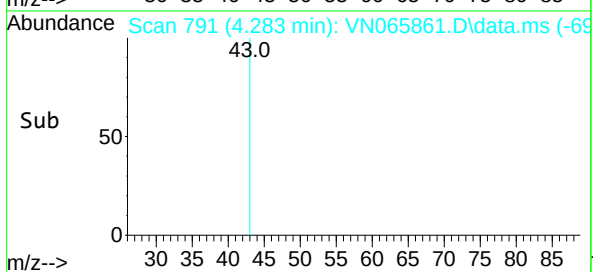

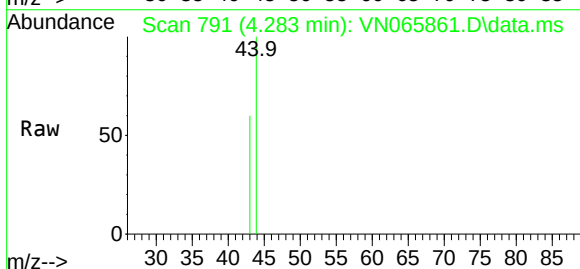


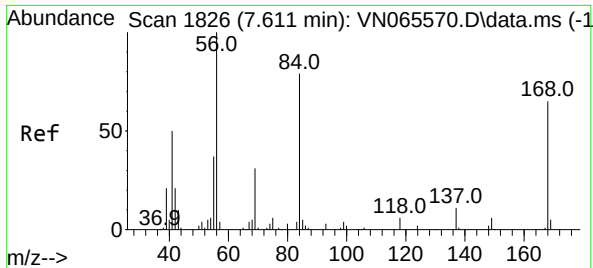

#31
Cyclohexane
Concen: 0.63 ug/l
RT: 7.618 min Scan# 1828
Delta R.T. 0.007 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 1798
Ion Ratio Lower Upper
56 100
69 235.4 26.6 39.8#
84 175.0 70.4 105.6#

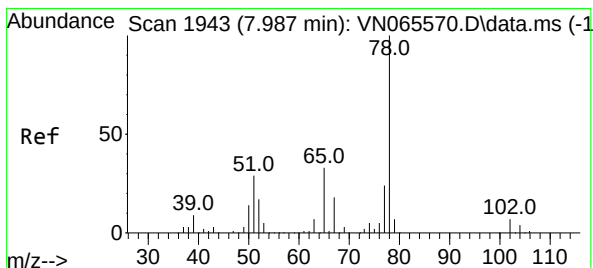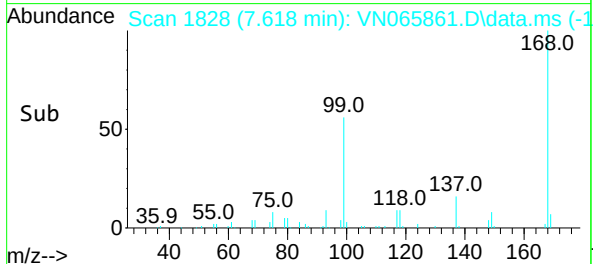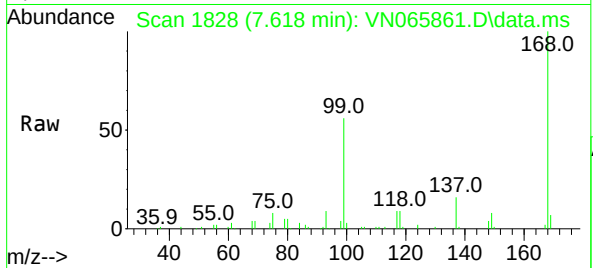

#33
1,2-Dichloroethane-d4
Concen: 45.13 ug/l
RT: 7.984 min Scan# 1942
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 65 Resp: 68913
Ion Ratio Lower Upper
65 100
67 57.7 0.0 107.2

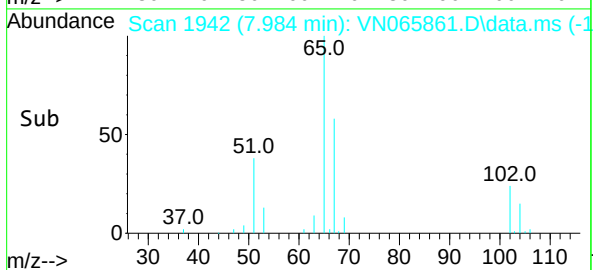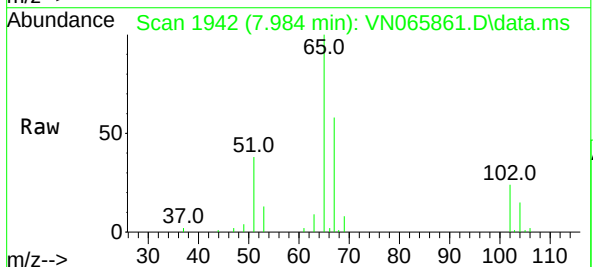




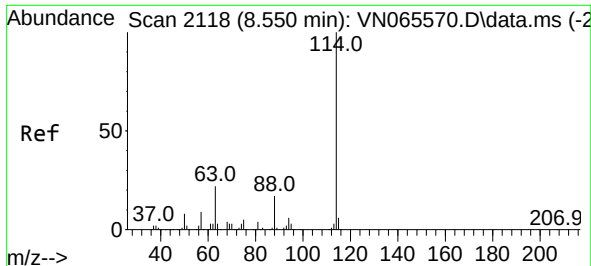


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Instrument :
MSVOA_N
ClientSampleId :




Tgt Ion:114 Resp: 226435
Ion Ratio Lower Upper
114 100
63 19.7 0.0 38.6
88 16.7 0.0 30.6

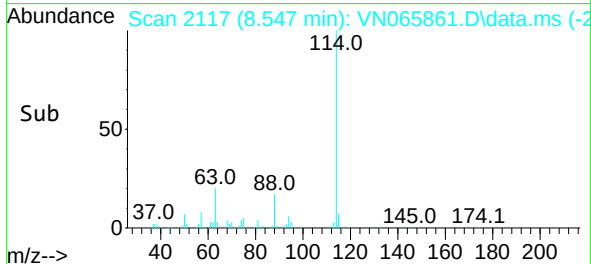


#35

Dibromofluoromethane
Concen: 48.67 ug/l
RT: 7.547 min Scan# 1806
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32


Tgt Ion:113 Resp: 65308
Ion Ratio Lower Upper
113 100
111 100.8 82.2 123.2
192 17.6 15.4 23.0

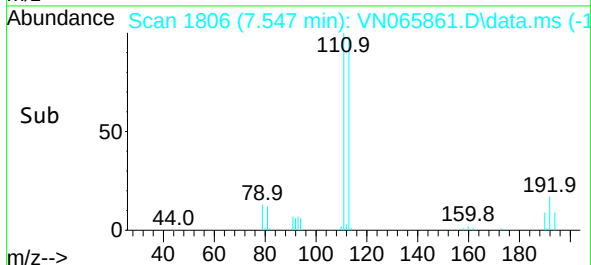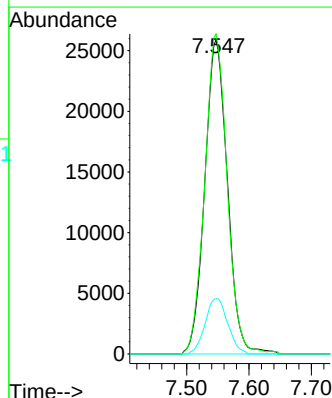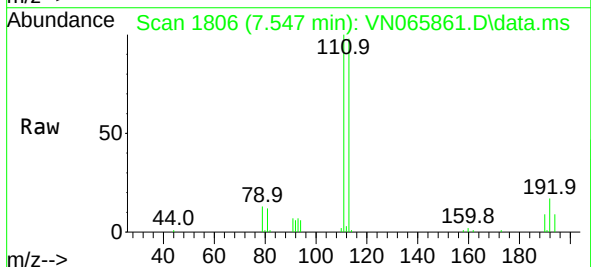



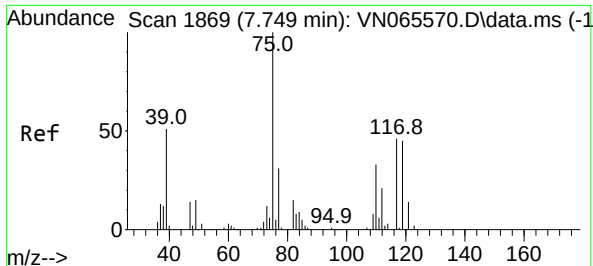


#36
1,1-Dichloropropene
Concen: 3.56 ug/l
RT: 7.618 min Scan# 1828
Delta R.T. -0.131 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Instrument :
MSVOA_N
ClientSampled :



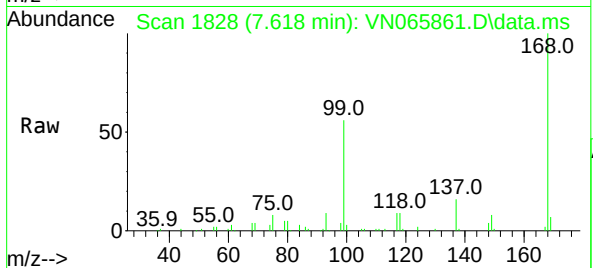



Tgt Ion: 75 Resp: 8105
Ion Ratio Lower Upper
75 100
110 7.0 18.2 54.6#
77 0.0 24.9 37.3#

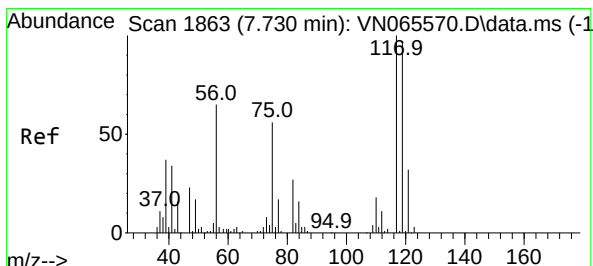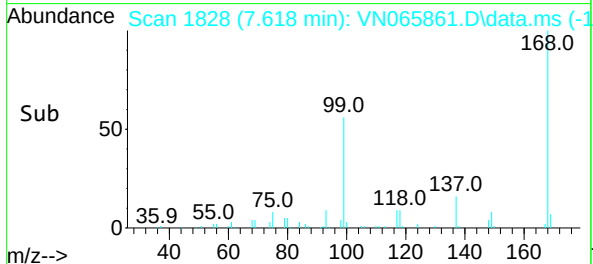

#38
Carbon Tetrachloride
Concen: 5.73 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. -0.109 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 117 Resp: 10756
Ion Ratio Lower Upper
117 100
119 7.0 76.0 114.0#
121 0.0 24.5 36.7#


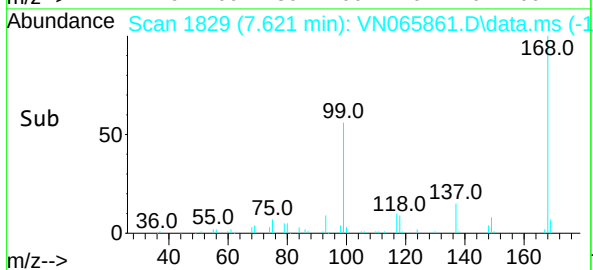

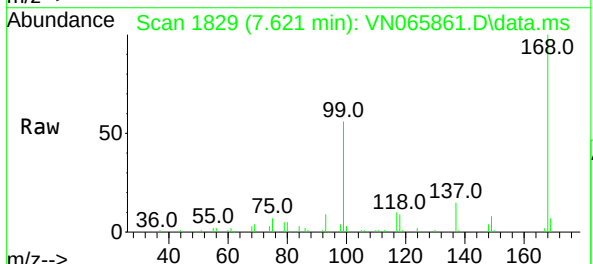


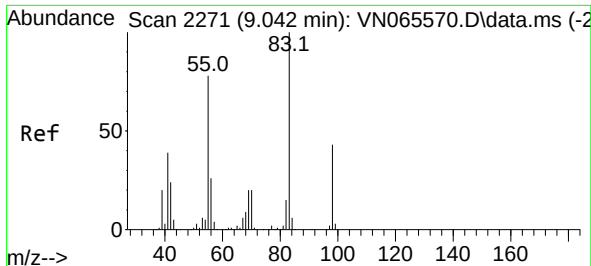

#39
Methylcyclohexane
Concen: 0.73 ug/l
RT: 9.042 min Scan# 2271
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 83 Resp: 2023
Ion Ratio Lower Upper
83 100
55 91.8 58.9 88.3#
98 42.4 35.9 53.9

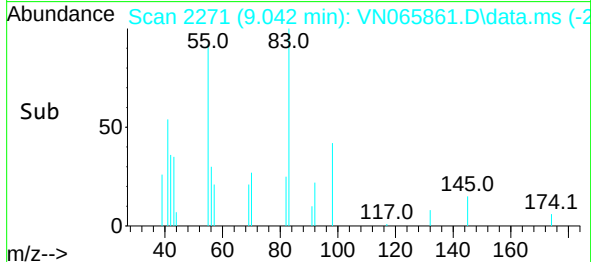

#50
Toluene-d8
Concen: 56.40 ug/l
RT: 10.055 min Scan# 2586
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 98 Resp: 297472
Ion Ratio Lower Upper
98 100
100 64.9 50.5 75.7


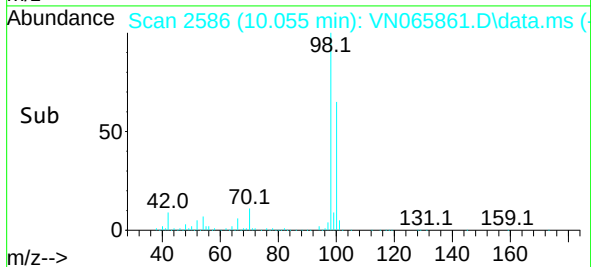

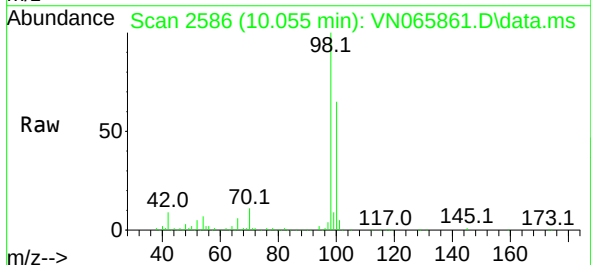


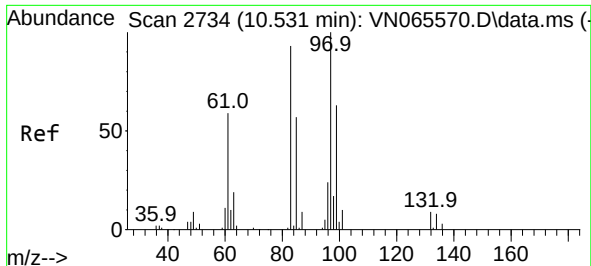

#55
1,1,2-Trichloroethane
Concen: 3.12 ug/l
RT: 10.495 min Scan# 2723
Delta R.T. -0.036 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	97	Resp:	4908
Ion	Ratio	Lower	Upper
97	100		
83	9.0	67.7	101.5#
85	0.0	44.5	66.7#
99	0.0	49.4	74.0#

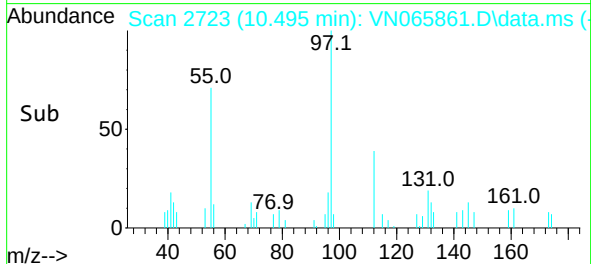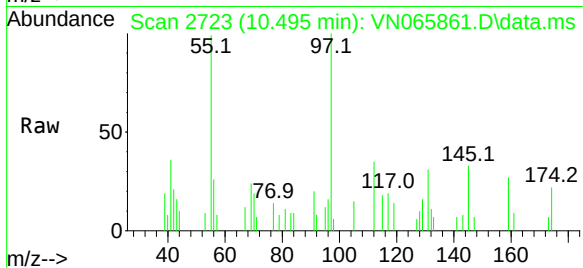

#56
Ethyl methacrylate
Concen: 0.46 ug/l
RT: 10.399 min Scan# 2693
Delta R.T. -0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion:	69	Resp:	1198
Ion	Ratio	Lower	Upper
69	100		
41	87.8	49.6	74.4#
39	69.9	28.0	42.0#


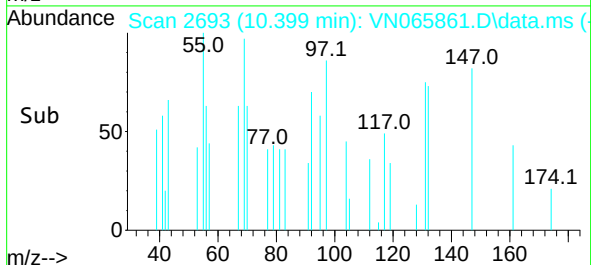

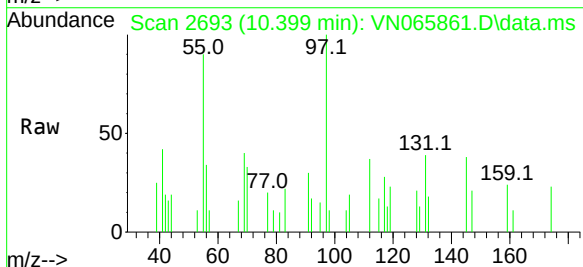


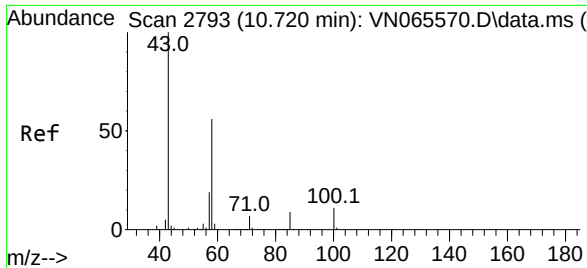

#59
2-Hexanone
Concen: 3.31 ug/l
RT: 10.688 min Scan# 2783
Delta R.T. -0.032 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 4916
Ion Ratio Lower Upper
43 100
58 0.0 28.1 84.3#

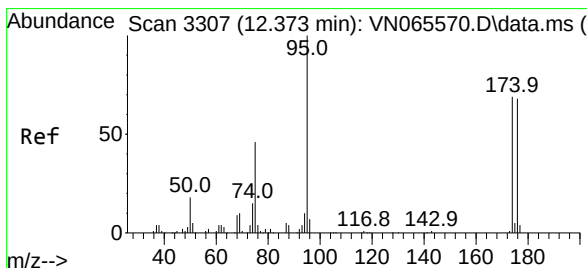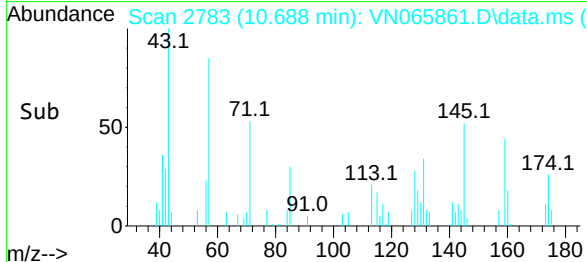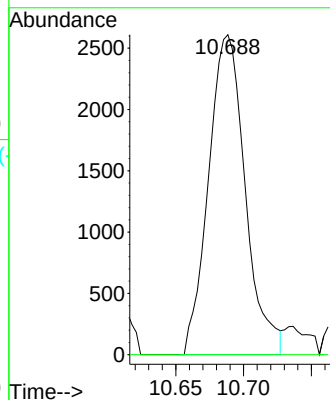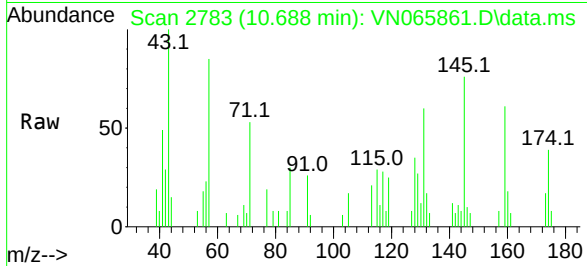

#62
4-Bromofluorobenzene
Concen: 64.86 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 95 Resp: 123193
Ion Ratio Lower Upper
95 100
174 78.0 0.0 169.0
176 71.2 0.0 162.4


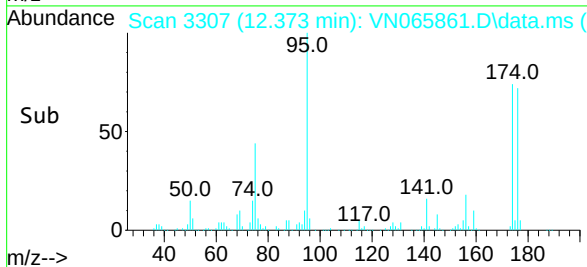
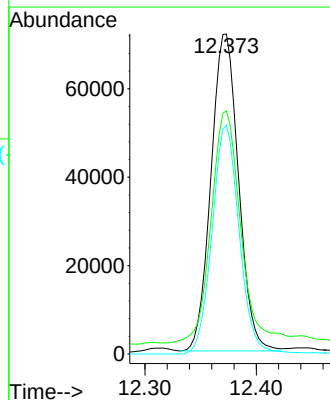
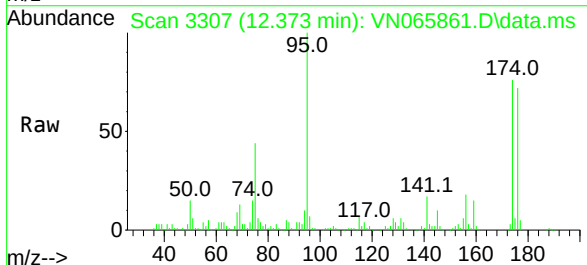




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 241747
Ion Ratio Lower Upper
117 100
82 56.2 43.7 65.5
119 32.2 26.1 39.1

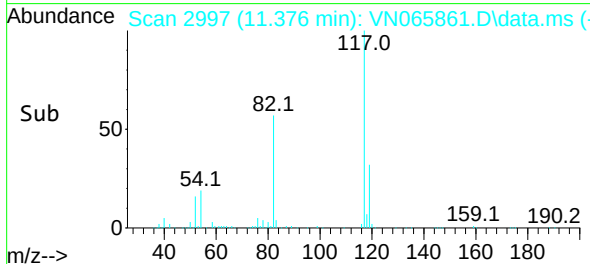

#67
Ethyl Benzene
Concen: 1.78 ug/l
RT: 11.479 min Scan# 3029
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 91 Resp: 16892
Ion Ratio Lower Upper
91 100
106 38.4 25.5 38.3#


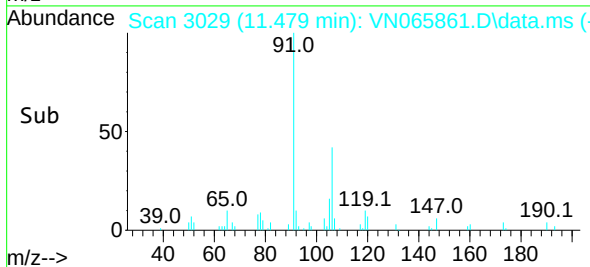

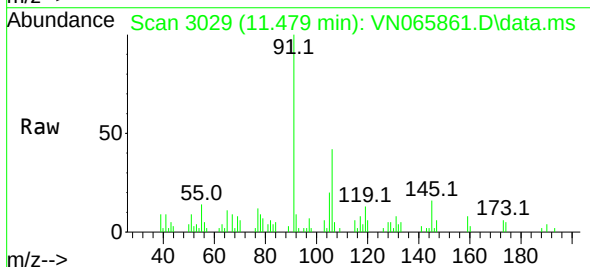




#68
m/p-Xylenes
Concen: 5.17 ug/l
RT: 11.589 min Scan# 3063
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 17792
Ion Ratio Lower Upper
106 100
91 180.7 161.4 242.0

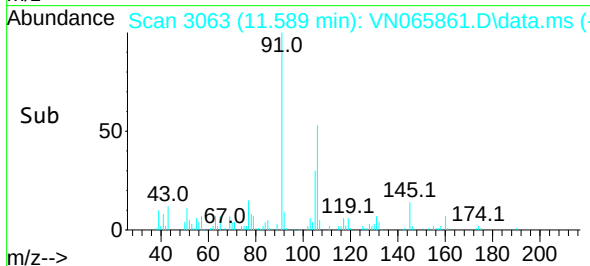

#69
o-Xylene
Concen: 0.84 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. 0.004 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion:106 Resp: 2798
Ion Ratio Lower Upper
106 100
91 187.3 106.8 320.4


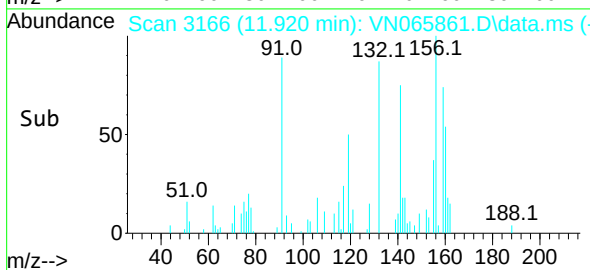

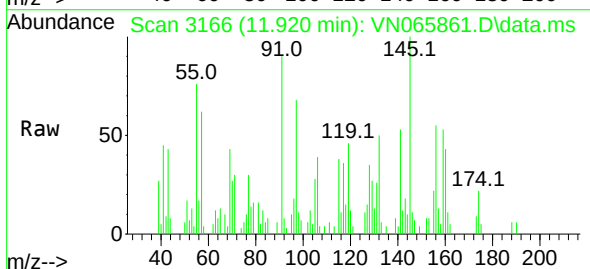




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.312 min Scan# 3599
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 109068
Ion Ratio Lower Upper
152 100
115 62.3 28.5 85.6
150 158.0 0.0 347.6

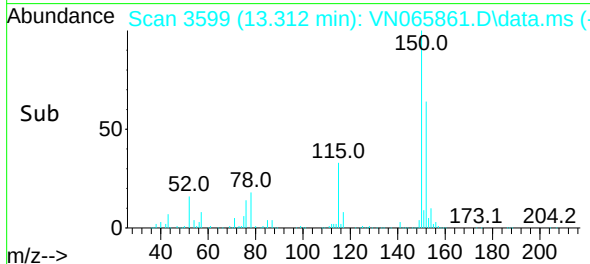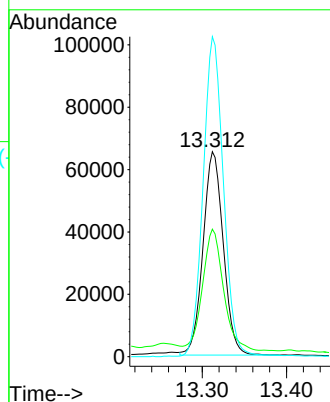

#73
Isopropylbenzene
Concen: 1.70 ug/l
RT: 12.219 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32


Tgt Ion:105 Resp: 16270
Ion Ratio Lower Upper
105 100
120 43.0 13.3 39.9#

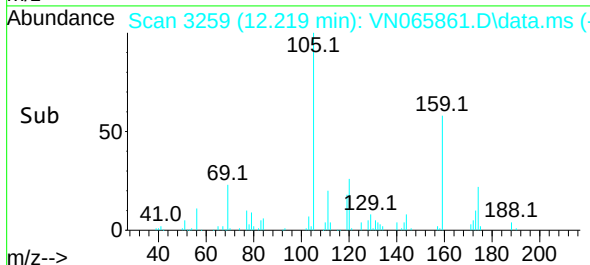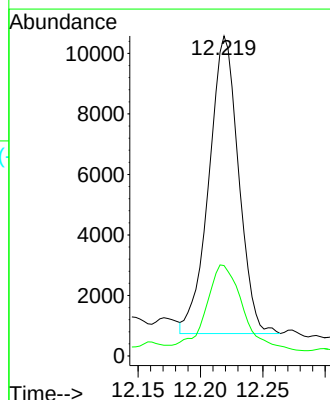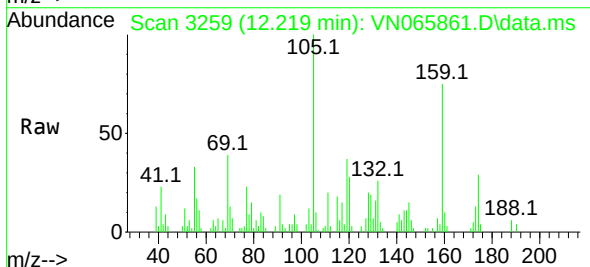






#74
N-amy1 acetate
Concen: 3.13 ug/l
RT: 12.016 min Scan# 3196
Delta R.T. -0.023 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 12663
Ion Ratio Lower Upper
43 100
70 14.4 34.4 51.6#
55 9.7 20.7 31.1#
61 0.0 19.1 28.7#

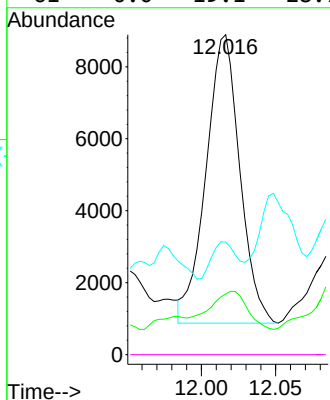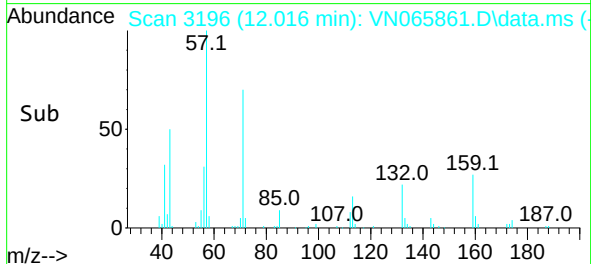


#75
1,1,2,2-Tetrachloroethane
Concen: 0.37 ug/l
RT: 12.418 min Scan# 3321
Delta R.T. -0.055 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

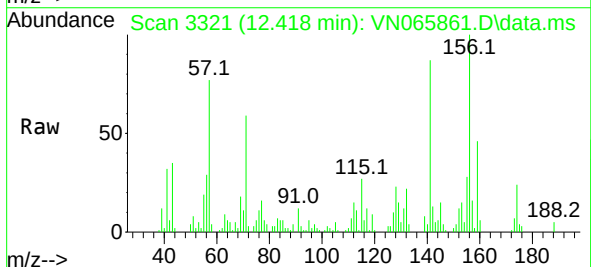

Tgt Ion: 83 Resp: 1051
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.8#
85 116.7 32.0 96.0#



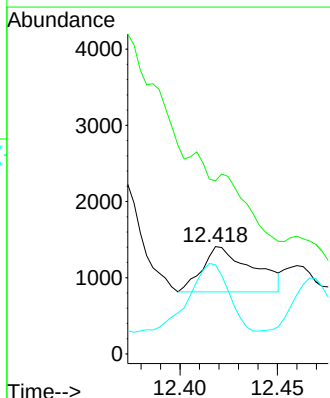



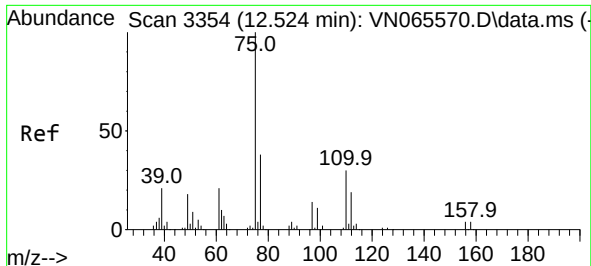

#76
1,2,3-Trichloropropane
Concen: 20.93 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 59686
Ion Ratio Lower Upper
75 100
77 14.3 0.0 0.0#

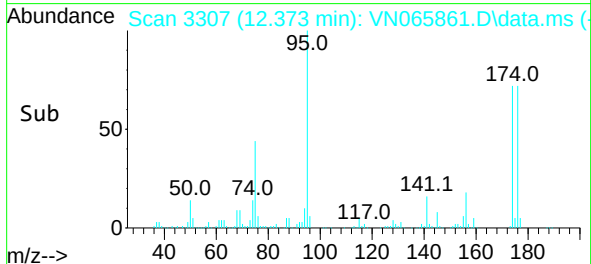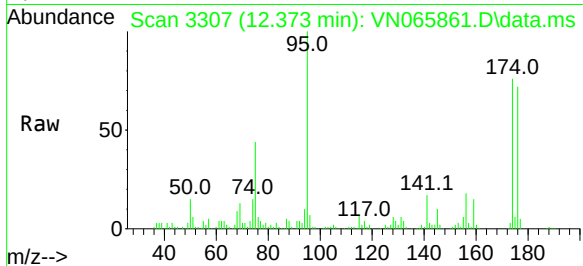

#77
Bromobenzene
Concen: 80.18 ug/l
RT: 12.434 min Scan# 3326
Delta R.T. -0.061 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 156 Resp: 165791
Ion Ratio Lower Upper
156 100
77 0.0 96.3 288.8#
158 0.1 49.0 147.0#


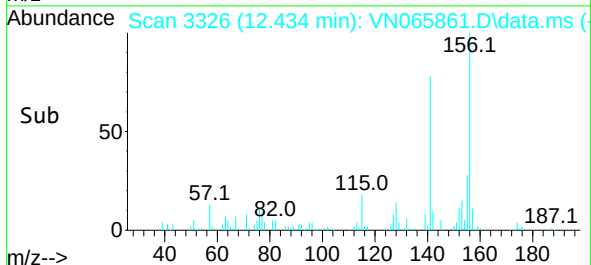

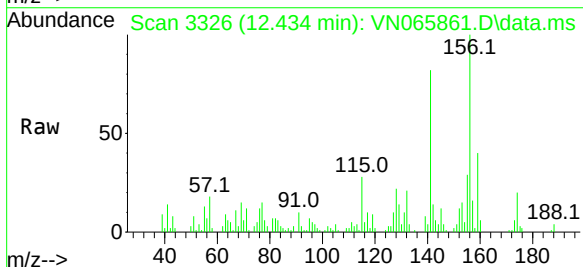


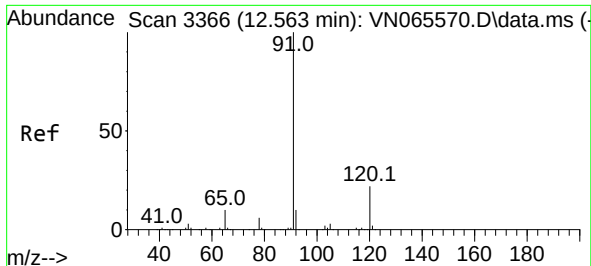

#78
n-propylbenzene
Concen: 4.30 ug/l
RT: 12.560 min Scan# 3365
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 48412
Ion Ratio Lower Upper
91 100
120 22.5 11.8 35.3

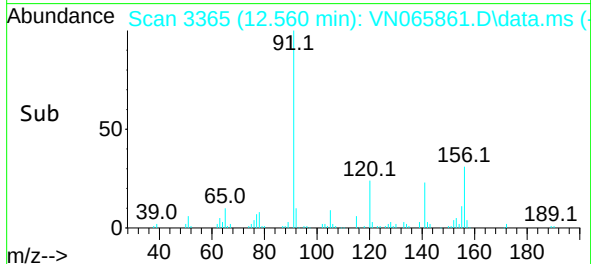

#79
2-Chlorotoluene
Concen: 1.80 ug/l
RT: 12.624 min Scan# 3385
Delta R.T. -0.019 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 91 Resp: 12005
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#




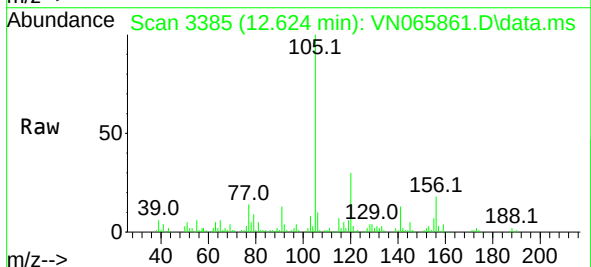


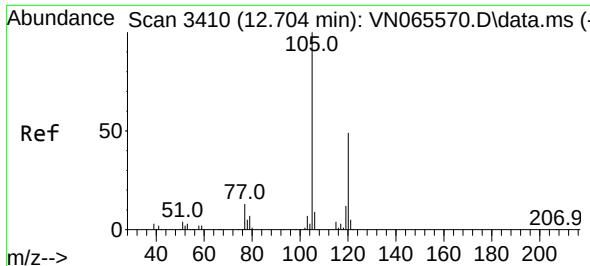

#80
1,3,5-Trimethylbenzene
Concen: 6.58 ug/l
RT: 12.701 min Scan# 3409
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 53464
Ion Ratio Lower Upper
105 100
120 51.9 24.3 72.8

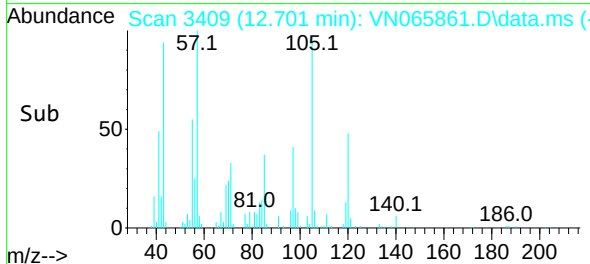

#81
trans-1,4-Dichloro-2-butene
Concen: 53.60 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 75 Resp: 59686
Ion Ratio Lower Upper
75 100
53 0.8 74.6 111.8#
89 0.6 35.8 53.8#


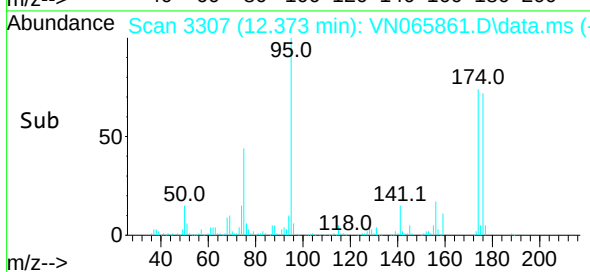

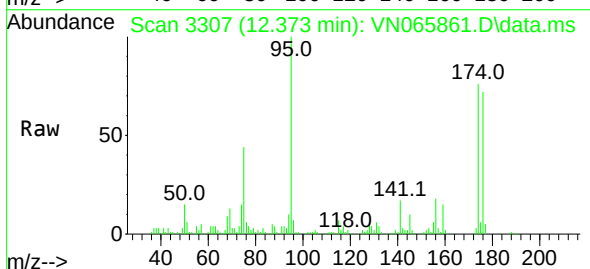


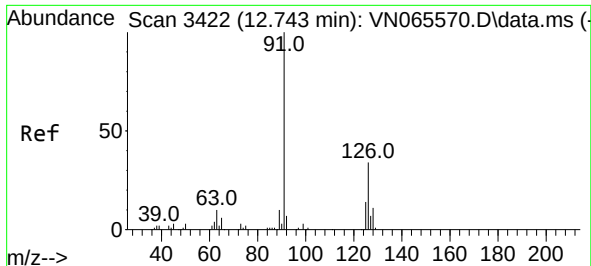

#82
4-Chlorotoluene
Concen: 0.80 ug/l
RT: 12.701 min Scan# 3409
Delta R.T. -0.042 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 5430
Ion Ratio Lower Upper
91 100
126 2.8 17.2 51.6#

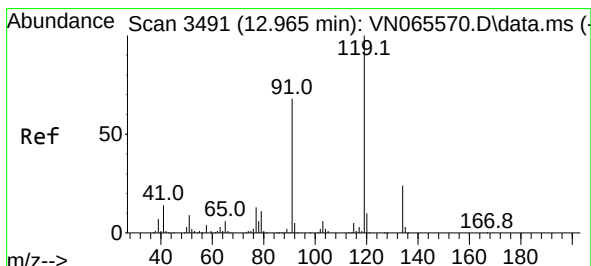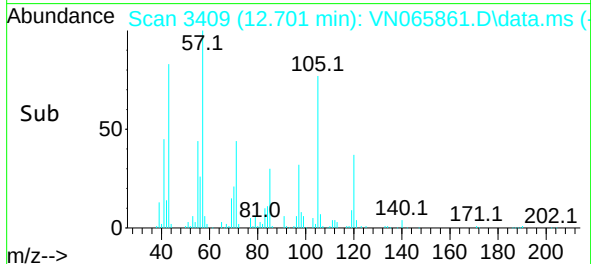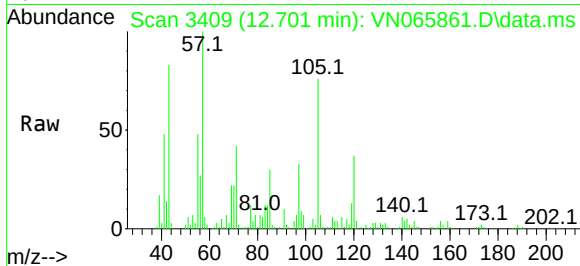

#83
tert-Butylbenzene
Concen: 4.06 ug/l
RT: 13.010 min Scan# 3505
Delta R.T. 0.045 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 119 Resp: 27522
Ion Ratio Lower Upper
119 100
91 80.5 33.0 98.9
134 0.0 12.7 38.1#


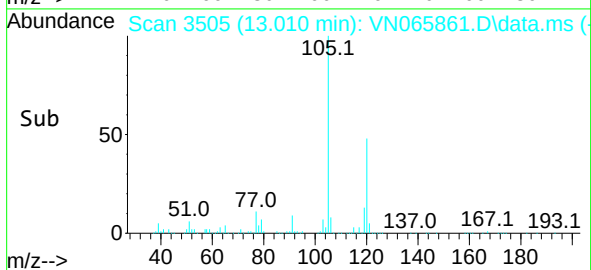

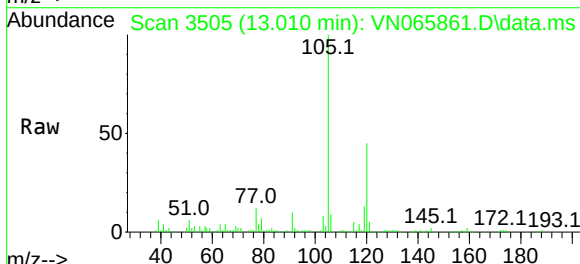


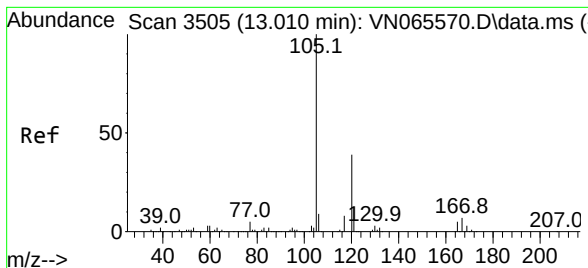

#84
1,2,4-Trimethylbenzene
Concen: 28.10 ug/l
RT: 13.010 min Scan# 3505
Delta R.T. -0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 227885
Ion Ratio Lower Upper
105 100
120 44.8 22.4 67.0

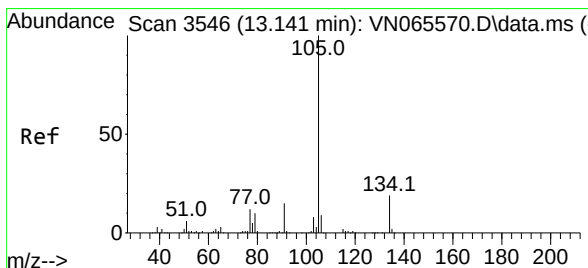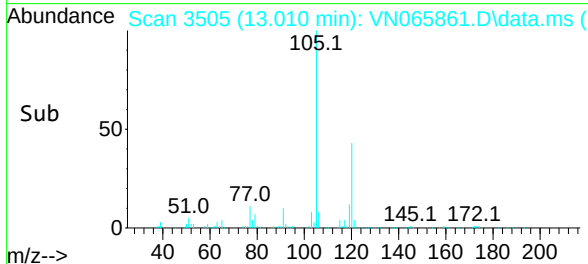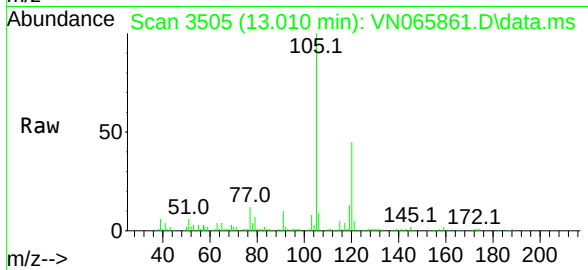

#85
sec-Butylbenzene
Concen: 4.16 ug/l
RT: 13.142 min Scan# 3546
Delta R.T. 0.001 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion:105 Resp: 38079
Ion Ratio Lower Upper
105 100
134 25.3 10.0 30.0


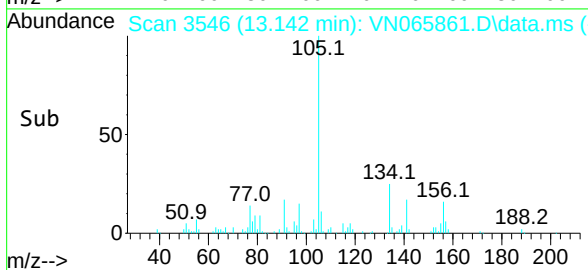

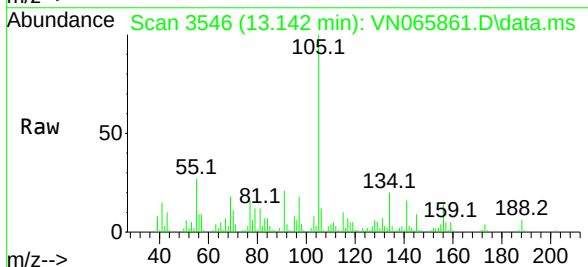


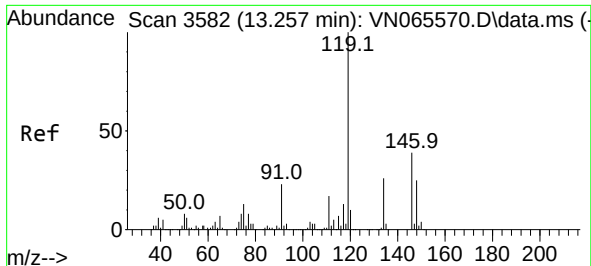

#86
p-Isopropyltoluene
Concen: 2.72 ug/l
RT: 13.257 min Scan# 3582
Delta R.T. 0.000 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:119 Resp: 21983
Ion Ratio Lower Upper
119 100
134 25.5 13.3 39.8
91 24.8 11.8 35.3

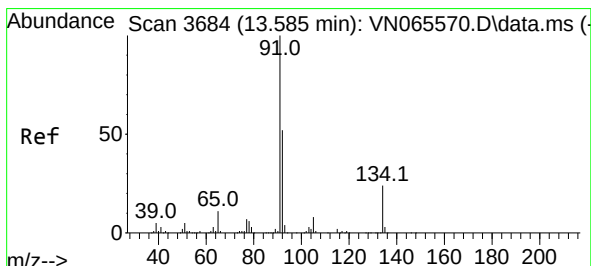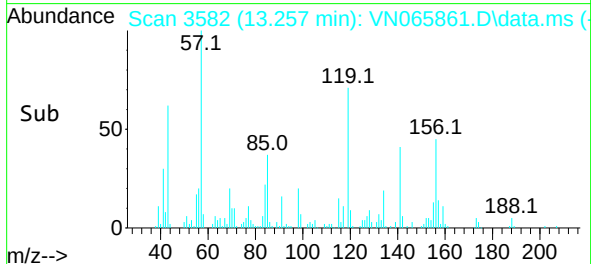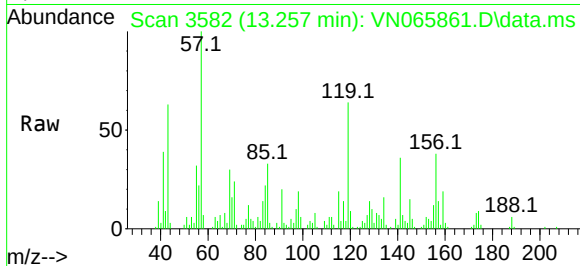

#89
n-Butylbenzene
Concen: 4.66 ug/l
RT: 13.582 min Scan# 3683
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32

Tgt Ion: 91 Resp: 33843
Ion Ratio Lower Upper
91 100
92 61.7 26.1 78.3
134 0.0 13.0 38.9#

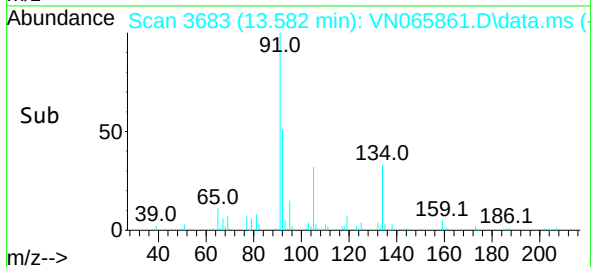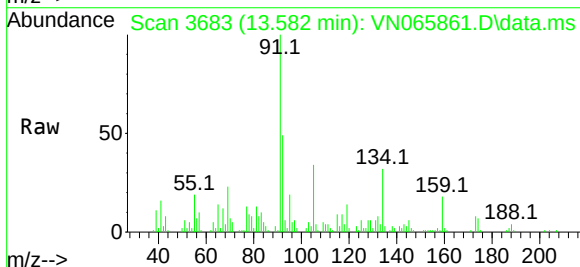



#90

Hexachloroethane

Concen: 8.65 ug/l

RT: 13.855 min Scan# 3768

Delta R.T. 0.013 min

Lab File: VN065861.D





Acq: 13 Feb 2021 00:32

Tgt Ion:117 Resp: 12237

Ion Ratio Lower Upper

117 100

201 0.0 37.8 113.3#

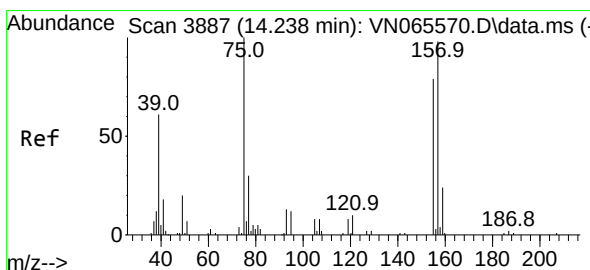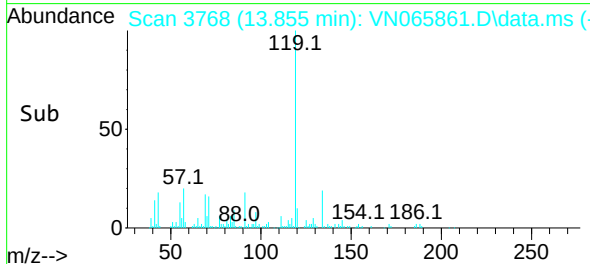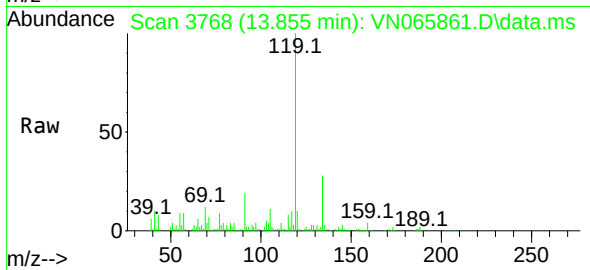

#92

1,2-Dibromo-3-Chloropropane

Concen: 1.63 ug/l

RT: 14.219 min Scan# 3881

Delta R.T. -0.019 min

Lab File: VN065861.D

Acq: 13 Feb 2021 00:32




Tgt Ion: 75 Resp: 915


Ion Ratio Lower Upper

75 100

155 54.0 44.1 132.4

157 0.0 56.0 168.2#


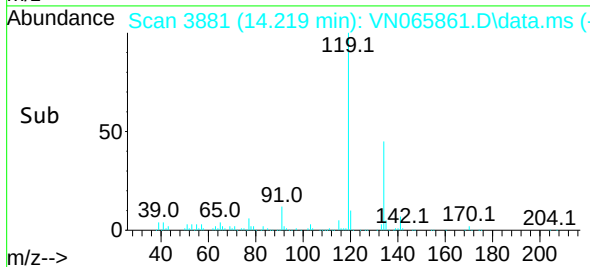

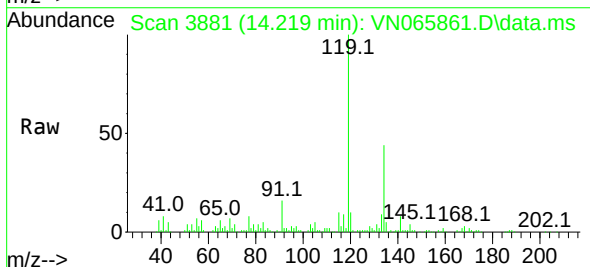


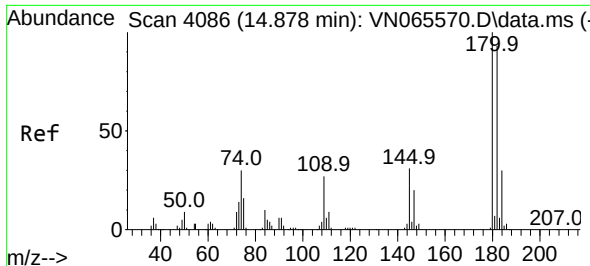

#93
1,2,4-Trichlorobenzene
Concen: 3.64 ug/l
RT: 14.884 min Scan# 4088
Delta R.T. 0.006 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:180 Resp: 661
Ion Ratio Lower Upper
180 100
182 136.9 47.3 142.0
145 0.0 15.6 46.8#

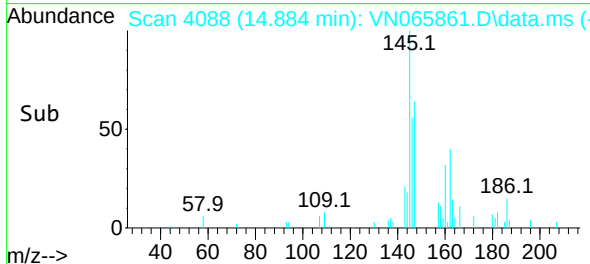

#95
Naphthalene
Concen: 8.97 ug/l
RT: 15.097 min Scan# 4154
Delta R.T. -0.003 min
Lab File: VN065861.D
Acq: 13 Feb 2021 00:32


Tgt Ion:128 Resp: 41908
Ion Ratio Lower Upper
128 100
127 18.9 10.2 15.2#
129 22.4 8.6 13.0#

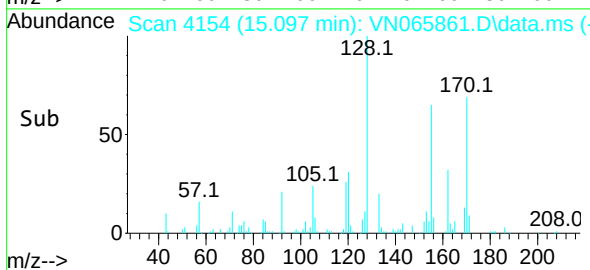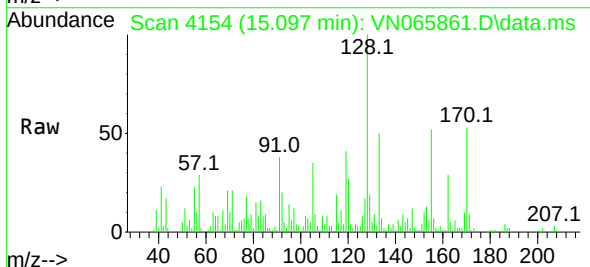

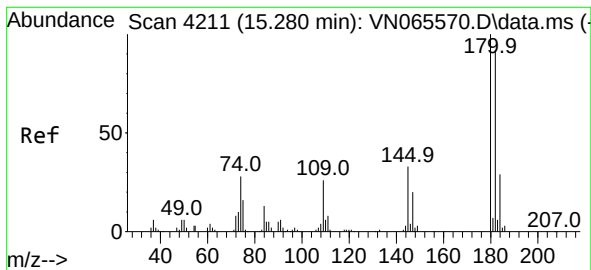

#96
 1,2,3-Trichlorobenzene
 Concen: 3.23 ug/l
 RT: 15.306 min Scan# 4219
 Delta R.T. 0.026 min
 Lab File: VN065861.D
 Acq: 13 Feb 2021 00:32

Instrument :
 MSVOA_N
 ClientSampled :

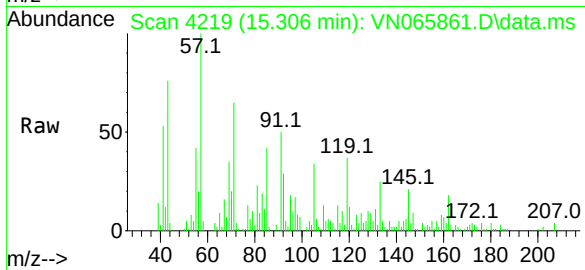

Tgt Ion:180 Resp: 881
 Ion Ratio Lower Upper
 180 100
 182 66.5 47.4 142.3
 145 0.0 16.5 49.5#

