


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
Data File : VN065830.D
Acq On : 12 Feb 2021 9:37
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Title : SW846 8260
Last Update : Mon Feb 15 10:57:01 2021

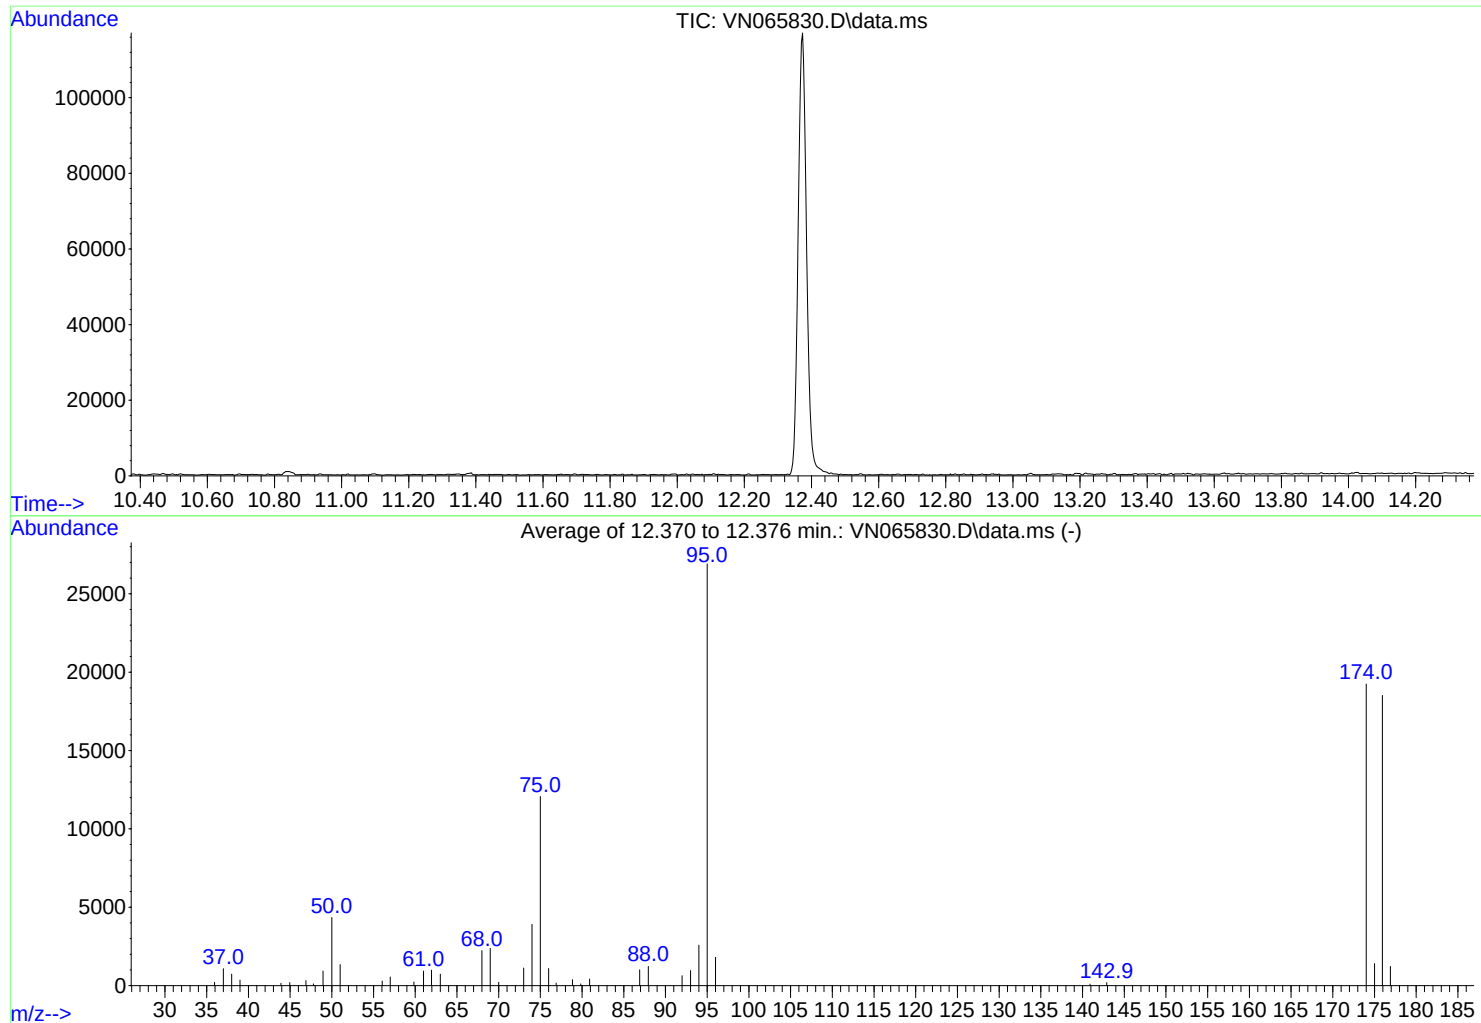

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	4346	PASS
75	95	30	60	44.8	12066	PASS
95	95	100	100	100.0	26912	PASS
96	95	5	9	6.7	1805	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.5	19240	PASS
175	174	5	9	7.3	1411	PASS
176	174	95	101	96.2	18517	PASS
177	176	5	9	6.6	1221	PASS