


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021221\
Data File : VN065854.D
Acq On : 12 Feb 2021 21:40
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Title : SW846 8260
Last Update : Mon Feb 15 10:57:01 2021

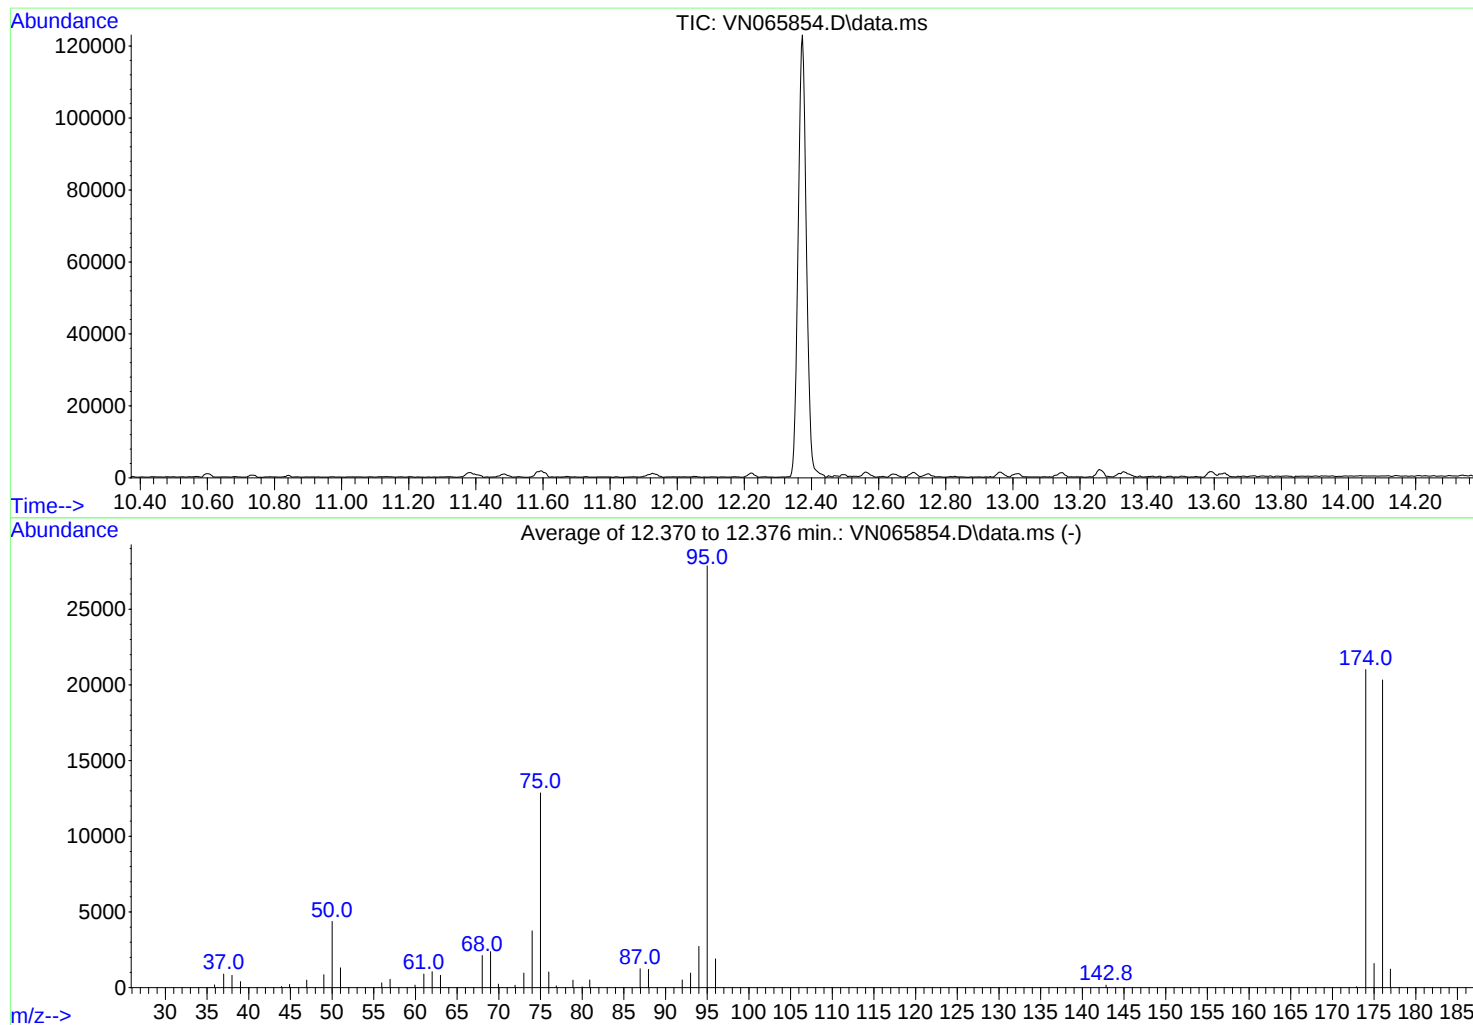

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	4371	PASS
75	95	30	60	46.2	12860	PASS
95	95	100	100	100.0	27864	PASS
96	95	5	9	6.8	1904	PASS
173	174	0.00	2	0.3	61	PASS
174	95	50	100	75.4	21013	PASS
175	174	5	9	7.6	1599	PASS
176	174	95	101	96.8	20331	PASS
177	176	5	9	6.0	1230	PASS