
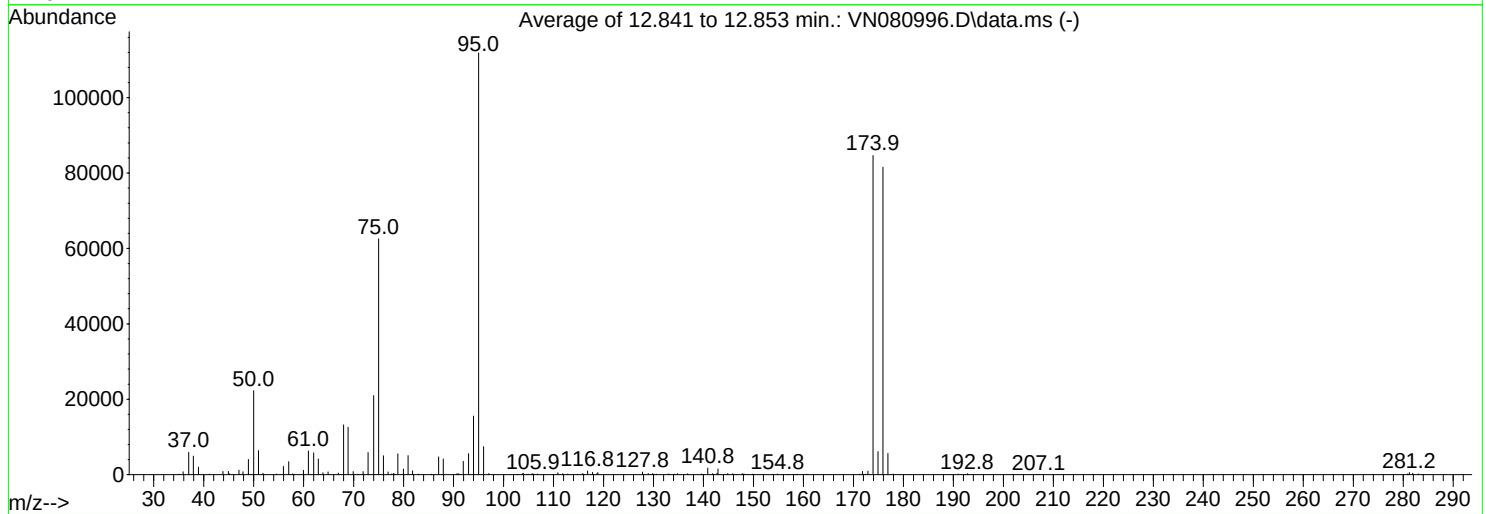


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021224\
Data File : VN080996.D
Acq On : 12 Feb 2024 08:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N020624W.M
Title : SW846 8260
Last Update : Wed Feb 07 06:22:23 2024

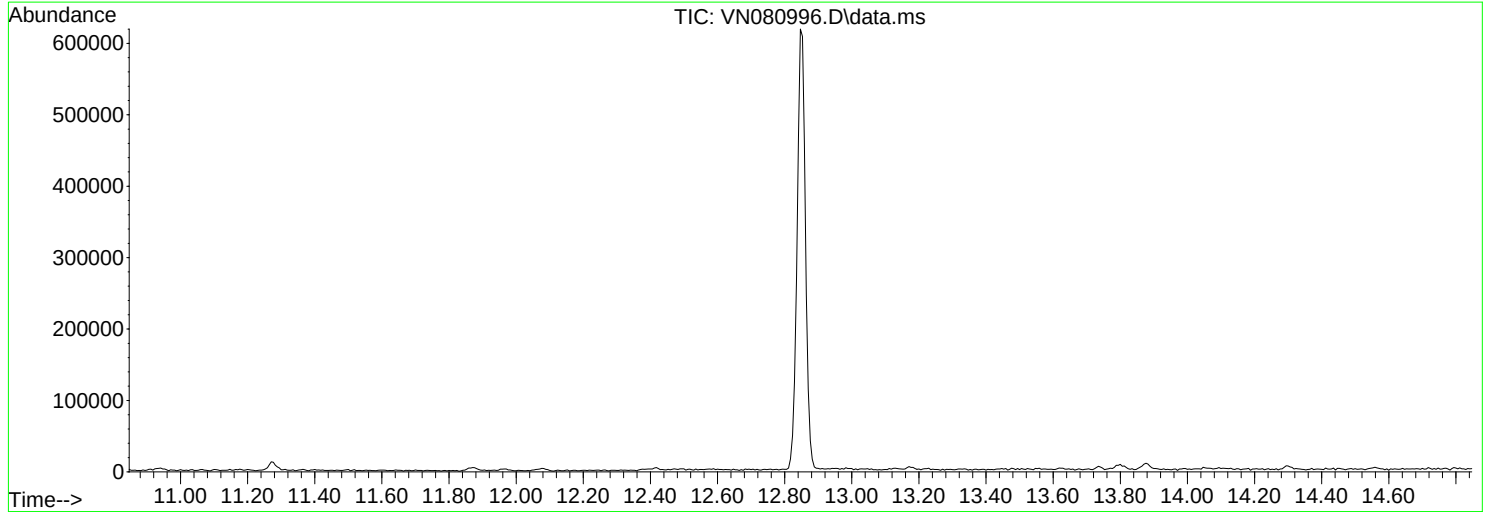

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	22275	PASS
75	95	30	60	55.9	62547	PASS
95	95	100	100	100.0	111888	PASS
96	95	5	9	6.6	7429	PASS
173	174	0.00	2	1.1	949	PASS
174	95	50	100	75.7	84693	PASS
175	174	5	9	7.2	6115	PASS
176	174	95	101	96.3	81595	PASS
177	176	5	9	6.9	5654	PASS

Average of 12.841 to 12.853 min.: VN080996.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	144	47.85	760	60.95	6277	72.90	586
35.90	756	48.95	4027	62.00	5781	74.00	2097
37.00	5927	50.00	22275	62.95	4174	75.00	6254
37.95	4919	50.95	6349	63.85	521	75.95	502
38.95	2007	51.85	401	64.90	724	76.90	722
39.90	68	54.60	186	66.95	428	77.60	177
41.15	131	55.95	2187	68.00	13207	77.95	322
43.85	839	57.00	3463	68.90	12558	78.20	186
44.95	861	57.80	200	69.90	815	78.85	5542
45.20	229	58.10	51	70.85	121	79.95	1479
47.05	1172	59.95	1162	71.90	830	80.90	5033

Average of 12.841 to 12.853 min.: VN080996.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	1002	96.00	7429	106.75	168	118.70	289
83.00	114	97.05	297	109.90	57	118.85	547
85.55	109	102.70	51	110.85	509	127.80	701
87.00	4699	102.90	55	111.85	260	128.95	296
87.95	4140	103.70	124	112.85	184	129.85	314
90.70	319	103.80	216	114.80	87	130.10	56
91.05	257	103.95	372	115.75	253	130.60	142
91.95	3509	104.70	64	115.90	155	132.90	188
93.00	5567	104.90	122	116.10	56	133.15	133
94.00	15556	105.70	272	116.80	990	134.15	121
95.00	111888	105.90	202	117.80	594	134.80	256

Average of 12.841 to 12.853 min.: VN080996.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
136.85	259	148.10	170	171.30	128	192.80	275
139.65	176	148.90	62	171.80	863	193.10	76
140.85	1730	149.85	123	172.40	114	206.70	81
141.85	297	153.95	144	172.90	949	207.10	85
142.70	389	154.85	185	173.90	84693	280.90	219
142.90	1522	156.90	50	174.90	6115	281.20	550
144.85	280	157.10	64	175.90	81595	281.90	396
145.85	262	158.00	51	176.90	5654	283.05	152
146.60	57	158.60	69	177.95	187	283.70	68
147.75	241	158.80	107	190.95	173		
147.90	124	160.70	111	192.40	81		